

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
 Data File : VU062974.D
 Acq On : 23 Jan 2025 18:28
 Operator : MD/SY
 Sample : Q1137-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 24 02:21:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 24 00:16:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	8666	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	10507	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3456	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2217	0.480	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	96.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3891	0.513	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.687	67	2656	0.469	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	94.000%		
8) Toluene-d8	7.887	98	7739	0.495	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	2561	0.549	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	110.000%		
Target Compounds						
6) Trichloroethene	6.544	95	173	0.021	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
Data File : VU062974.D
Acq On : 23 Jan 2025 18:28
Operator : MD/SY
Sample : Q1137-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 24 02:21:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 24 00:16:16 2025
Response via : Initial Calibration

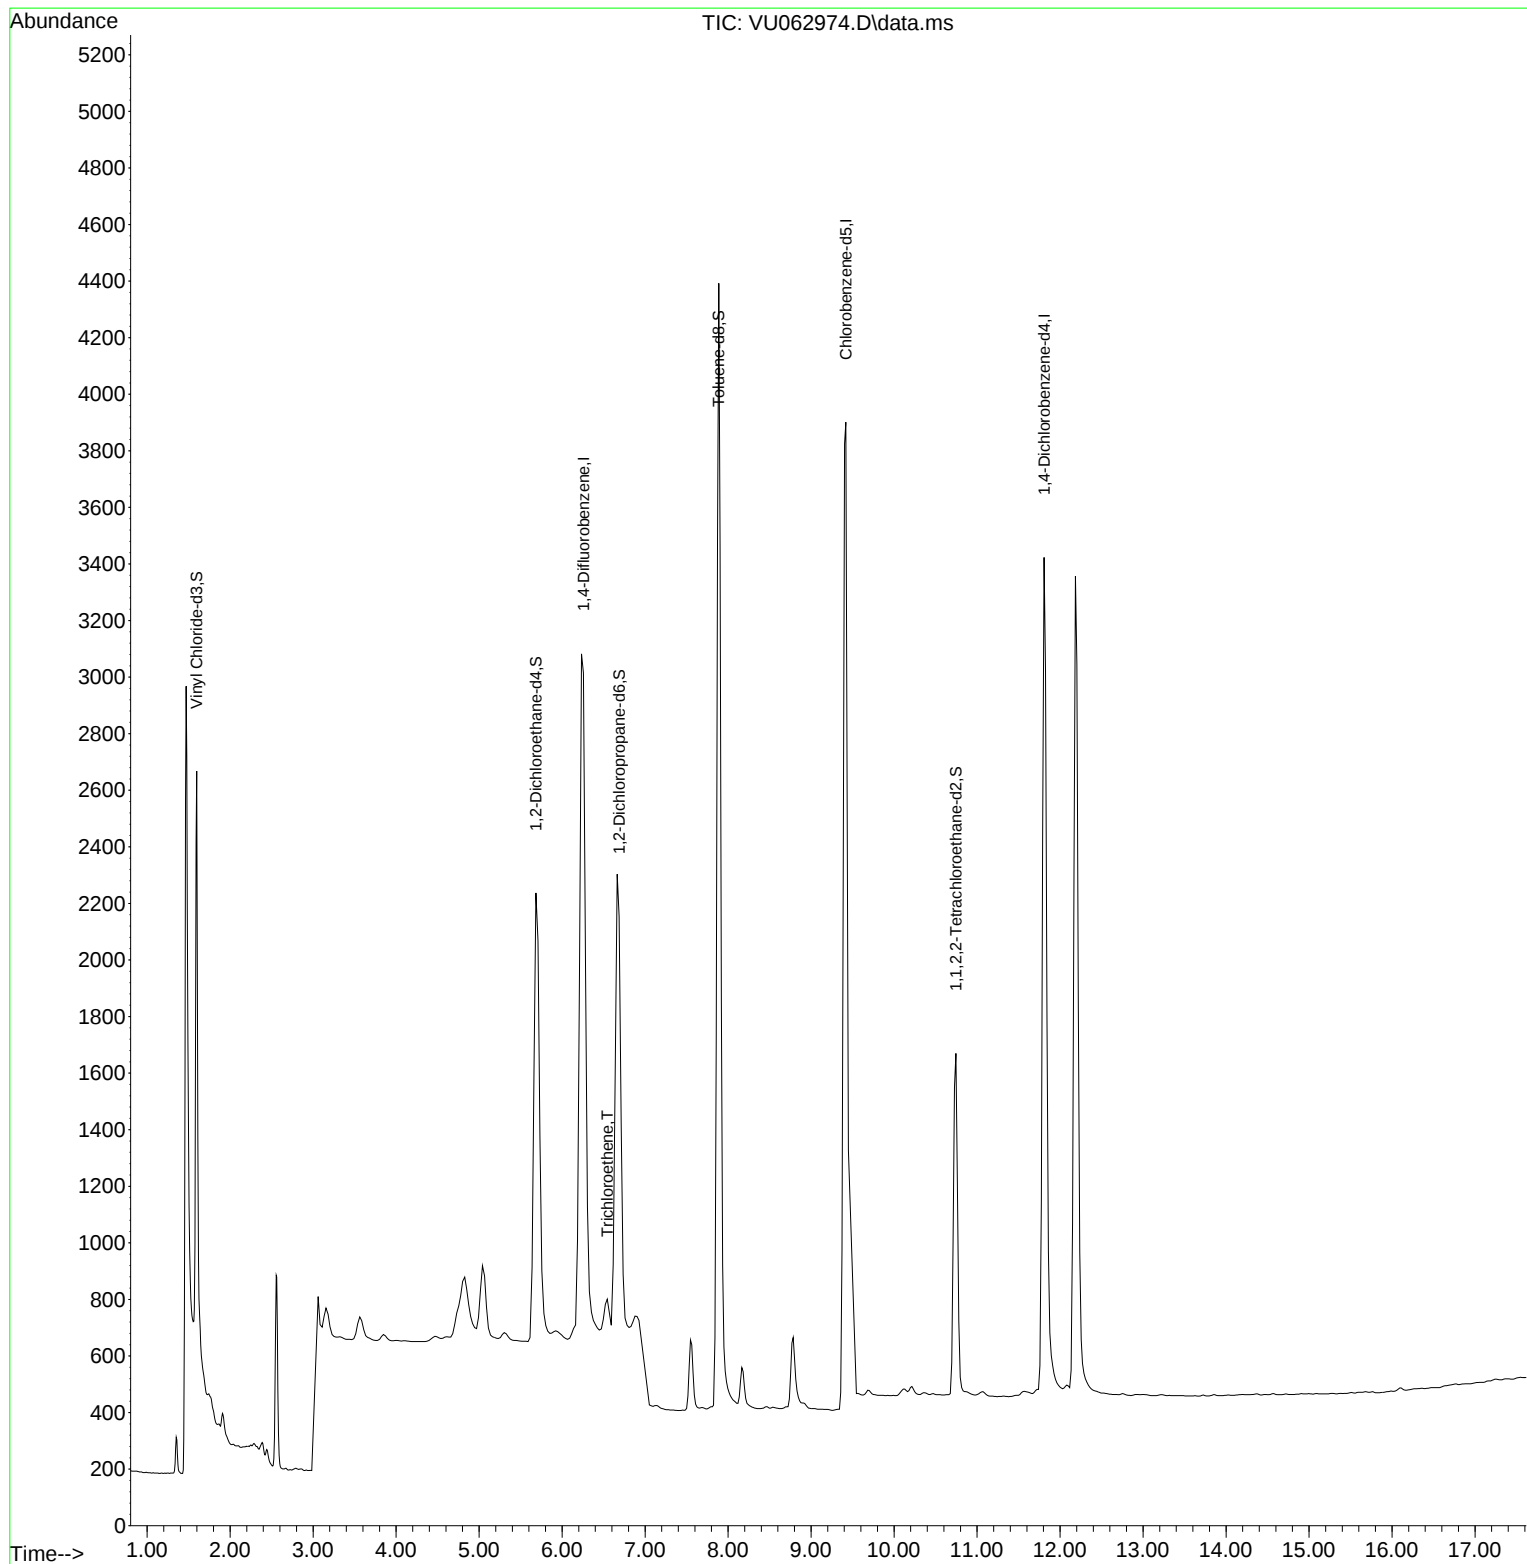

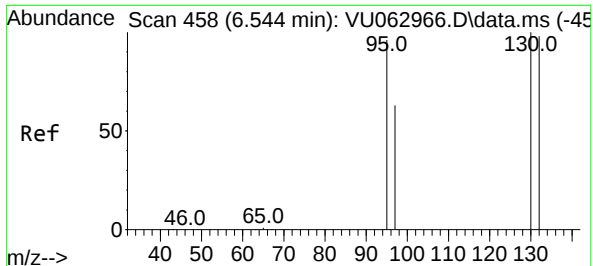

#6
 Trichloroethene
 Concen: 0.021 ug/L
 RT: 6.544 min Scan# 4
 Delta R.T. -0.000 min
 Lab File: VU062974.D
 Acq: 23 Jan 2025 18:28

Instrument :
 MSVOA_U
 ClientSampleId :

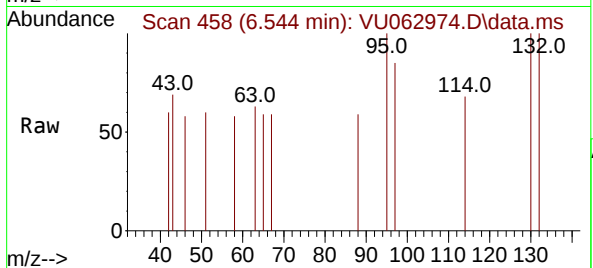

Tgt Ion: 95	Resp: 173
Ion Ratio	Lower Upper
95 100	
97 85.0	47.0 87.4
132 100.0	71.5 132.9
130 100.0	72.7 135.1

