

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
 Data File : VU062975.D
 Acq On : 23 Jan 2025 18:52
 Operator : MD/SY
 Sample : Q1137-05
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 24 02:22:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 24 00:16:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	8740	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	10181	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3488	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	1994	0.428	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	86.000%		
4) 1,2-Dichloroethane-d4	5.685	65	3622	0.474	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
7) 1,2-Dichloropropane-d6	6.687	67	3004	0.547	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	110.000%		
8) Toluene-d8	7.887	98	7185	0.474	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1724	0.382	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	76.000%		
Target Compounds						
6) Trichloroethene	6.544	95	183	0.023	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
Data File : VU062975.D
Acq On : 23 Jan 2025 18:52
Operator : MD/SY
Sample : Q1137-05
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jan 24 02:22:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 24 00:16:16 2025
Response via : Initial Calibration

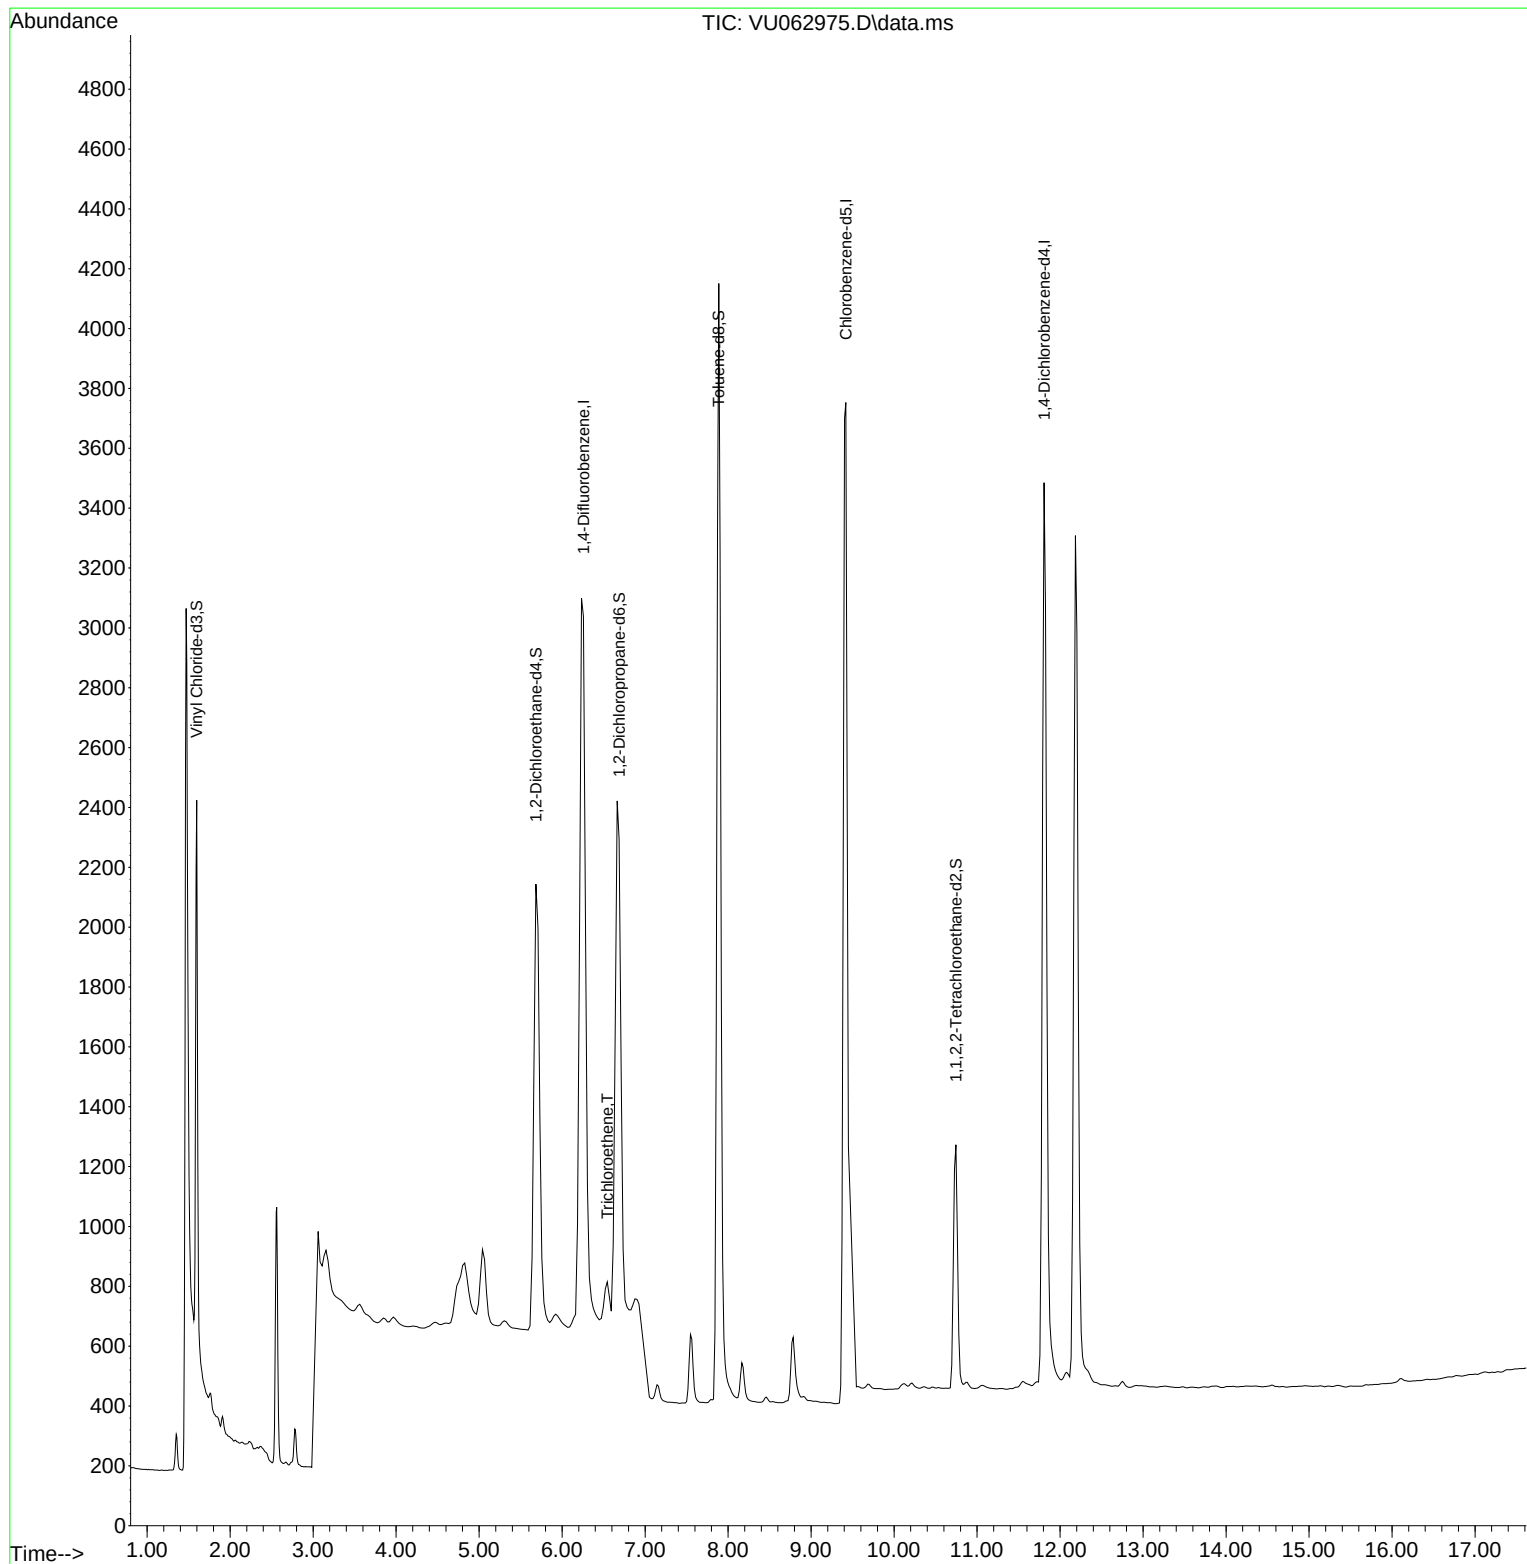

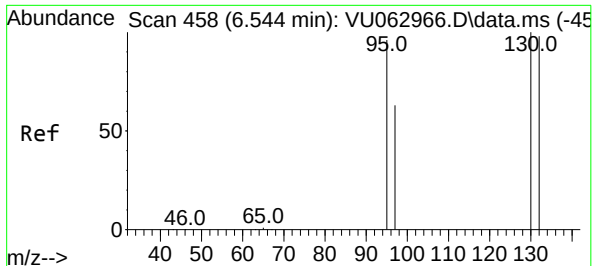

#6
 Trichloroethene
 Concen: 0.023 ug/L
 RT: 6.544 min Scan# 4
 Delta R.T. -0.000 min
 Lab File: VU062975.D
 Acq: 23 Jan 2025 18:52

Instrument :
 MSVOA_U
 ClientSampleId :

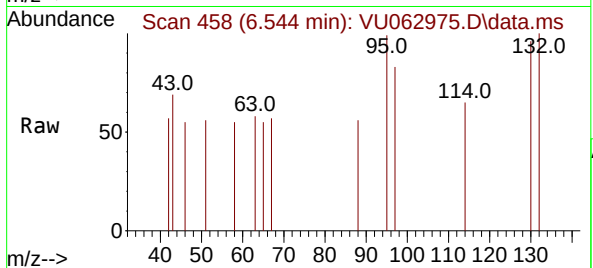

Tgt Ion	Ratio	Lower	Upper
95	100		
97	84.3	47.0	87.4
132	101.2	71.5	132.9
130	97.6	72.7	135.1

