
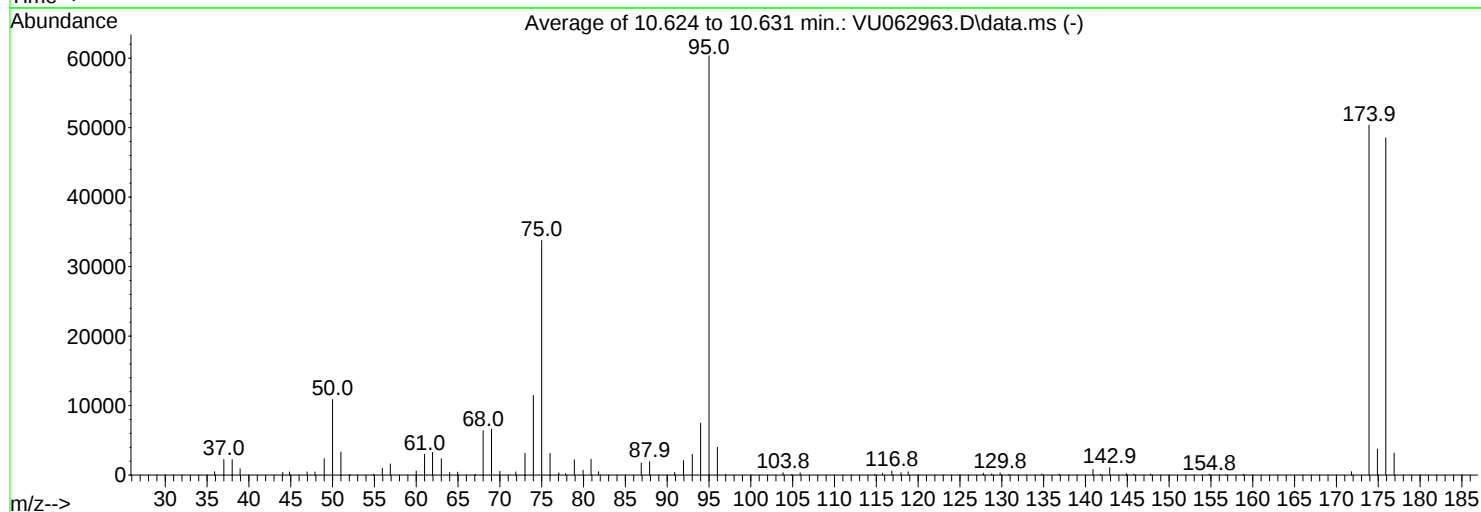


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012325\
Data File : VU062963.D
Acq On : 23 Jan 2025 10:43
Operator : MD/SY
Sample : BFB020
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM012325.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jan 24 00:16:16 2025

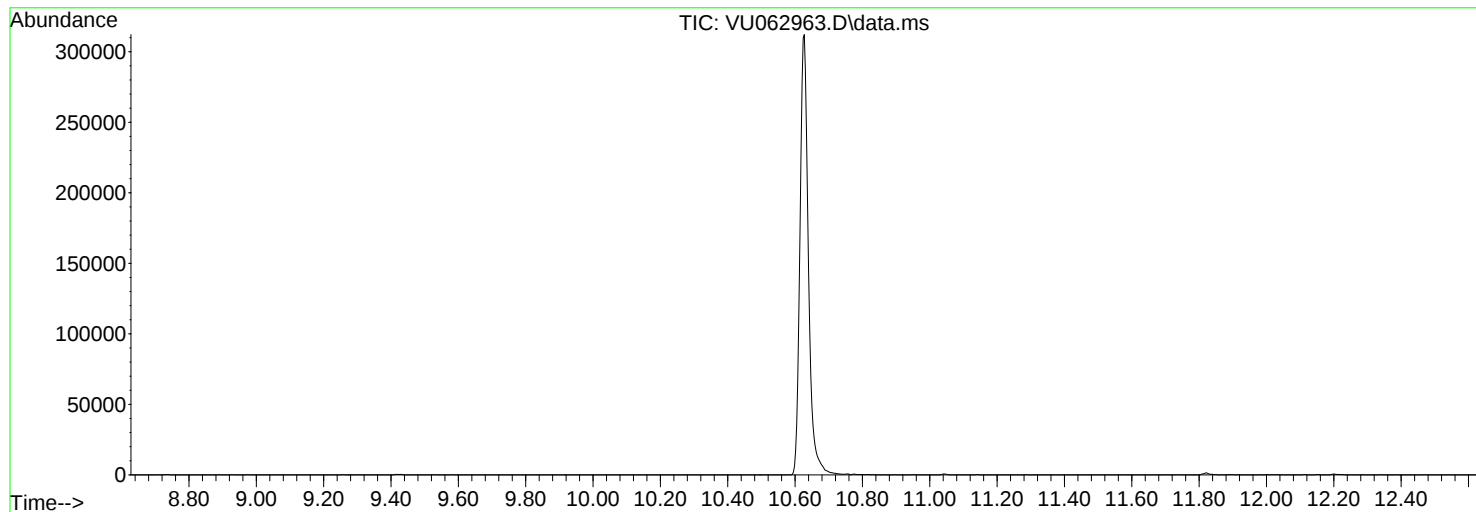

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10874	PASS
75	95	30	80	56.0	33771	PASS
95	95	100	100	100.0	60347	PASS
96	95	5	9	6.6	4003	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	50368	PASS
175	174	5	9	7.5	3756	PASS
176	174	95	101	96.3	48507	PASS
177	176	5	9	6.5	3174	PASS

m/z	Abundance
39.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	470.0
37.00	2388.0
38.00	2317.0
39.00	940.0
44.10	342.0
44.80	455.0
47.00	466.0
47.80	522.0
49.00	2572.0
50.00	11363.0
51.00	3527.0
54.90	137.0
56.00	1019.0
56.90	1744.0
60.00	595.0
61.00	3122.0
61.90	3283.0
63.00	2415.0
64.00	398.0
65.00	397.0
68.00	6538.0
69.00	7223.0
70.00	566.0
71.90	405.0
73.00	3218.0
74.00	12014.0
75.00	34744.0
76.00	3325.0
77.10	359.0
77.90	210.0
78.90	2228.0
79.90	751.0
80.90	2395.0
81.80	502.0
86.90	1765.0
87.90	1938.0
90.90	390.0
92.00	2141.0
93.00	3122.0
94.00	7839.0
95.00	61888.0
96.00	4272.0
96.90	143.0
103.80	332.0
105.90	309.0
114.80	165.0
115.70	244.0
116.80	615.0
118.00	361.0
118.80	525.0
127.80	266.0
128.80	183.0
129.80	308.0
130.90	109.0
134.80	124.0
136.80	175.0
140.90	855.0
141.80	129.0
142.90	1055.0
144.90	241.0
145.80	171.0
147.90	187.0
154.80	117.0
156.80	158.0
158.90	138.0
171.80	529.0
173.90	50896.0
174.90	3759.0
175.90	47848.0
176.90	3165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	504.0
37.00	2308.0
38.00	2305.0
39.00	951.0
44.10	429.0
44.90	483.0
47.00	497.0
47.90	472.0
49.00	2411.0
50.00	11124.0
51.00	3458.0
52.10	128.0
54.90	128.0
55.90	1018.0
56.90	1646.0
60.00	602.0
61.00	3062.0
61.90	3380.0
63.00	2372.0
64.00	374.0
64.90	435.0
67.10	192.0
68.00	6575.0
69.00	6817.0
70.00	567.0
71.90	465.0
73.00	3276.0
74.00	11859.0
75.00	34544.0
76.00	3213.0
77.10	340.0
77.80	257.0
78.90	2286.0
79.90	734.0
80.90	2330.0
81.80	500.0
86.90	1768.0
87.90	2041.0
90.90	402.0
91.90	2158.0
93.00	3013.0
94.00	7652.0
95.00	62040.0
96.00	4132.0
96.90	127.0
103.80	352.0
104.90	114.0
105.90	317.0
114.80	150.0
115.80	272.0
116.90	611.0
117.90	380.0
118.80	517.0
127.80	273.0
128.80	209.0
129.80	334.0
130.80	107.0
134.80	189.0
136.80	173.0
140.90	840.0
141.80	145.0
142.90	1086.0
144.90	218.0
145.80	174.0
147.80	158.0
154.80	148.0
156.80	120.0
158.90	146.0
171.80	483.0
173.90	51832.0
174.90	3879.0
175.90	50184.0
176.90	3330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	461.0
37.00	2008.0
38.00	2005.0
38.90	834.0
44.00	432.0
44.90	424.0
46.90	441.0
48.00	351.0
49.00	2135.0
50.00	10135.0
51.00	2973.0
52.10	143.0
54.90	140.0
56.00	927.0
56.90	1415.0
60.00	568.0
61.00	2829.0
62.00	3095.0
63.00	2285.0
64.00	334.0
64.90	454.0
67.00	180.0
68.00	6035.0
69.00	5811.0
70.00	528.0
71.90	480.0
73.00	2895.0
74.00	10504.0
75.00	32024.0
76.00	2823.0
77.00	264.0
77.80	223.0
78.90	2053.0
80.00	633.0
80.90	2125.0
81.80	452.0
86.90	1726.0
87.90	1776.0
90.90	340.0
91.90	1982.0
93.00	2787.0
94.00	6918.0
95.00	57112.0
96.00	3605.0
97.00	106.0
103.90	363.0
104.80	114.0
105.90	332.0
115.80	289.0
116.90	537.0
117.90	333.0
118.80	443.0
127.80	272.0
128.80	176.0
129.80	296.0
130.80	111.0
134.80	234.0
136.90	131.0
140.90	748.0
141.80	132.0
142.90	1068.0
144.90	169.0
145.80	116.0
147.70	157.0
154.80	159.0
158.90	102.0
171.80	453.0
173.90	48376.0
174.90	3630.0
175.90	47488.0
176.90	3026.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020