
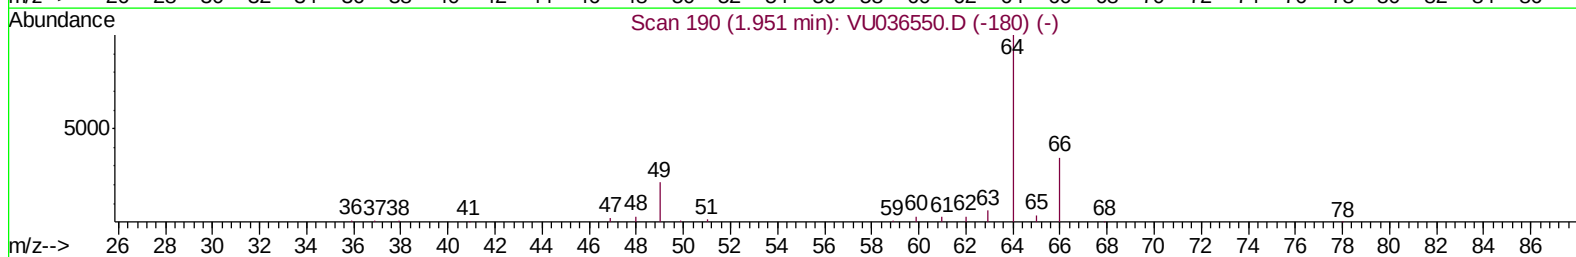
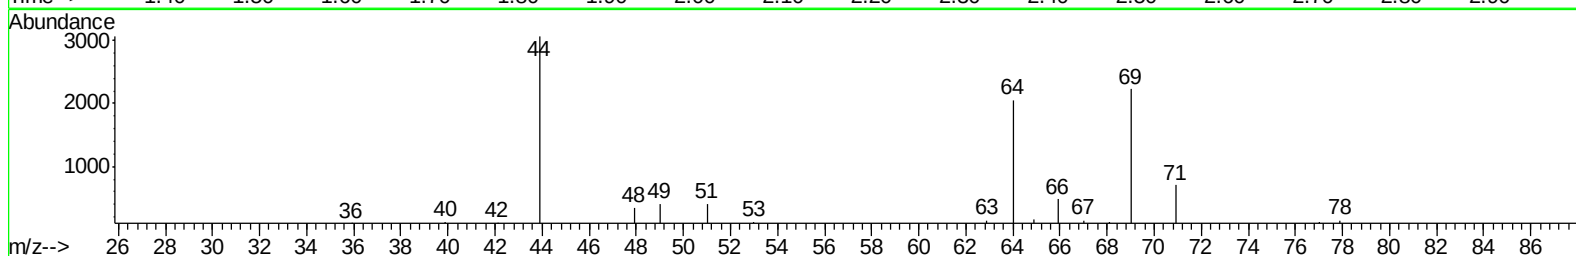


Data File : VU036557.D
Acq On : 24 Jan 2020 16:06
Operator : JC/MD
Sample : MDL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Jan 24 23:23:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012420WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 24 23:19:07 2020
Response via : Initial Calibration

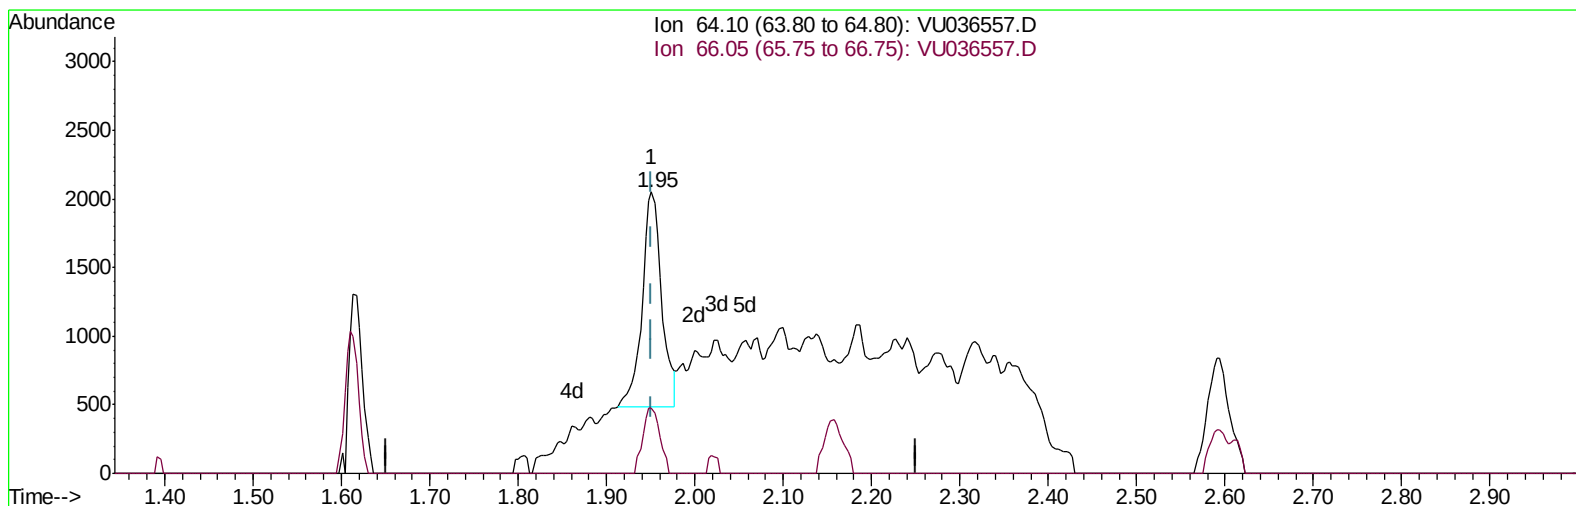

TIC: VU036557.D

(8) Chloroethane (T)

1.951min (+0.000) 0.32ug/L m

response 2418

Ion	Exp%	Act%
64.10	100	100
66.05	34.50	23.34#
0.00	0.00	0.00
0.00	0.00	0.00