


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU012420\
 Data File : VU036547.D
 Acq On : 24 Jan 2020 10:36
 Operator : JC/MD
 Sample : BFB29
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB601

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012420WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 29 06:28:33 2020

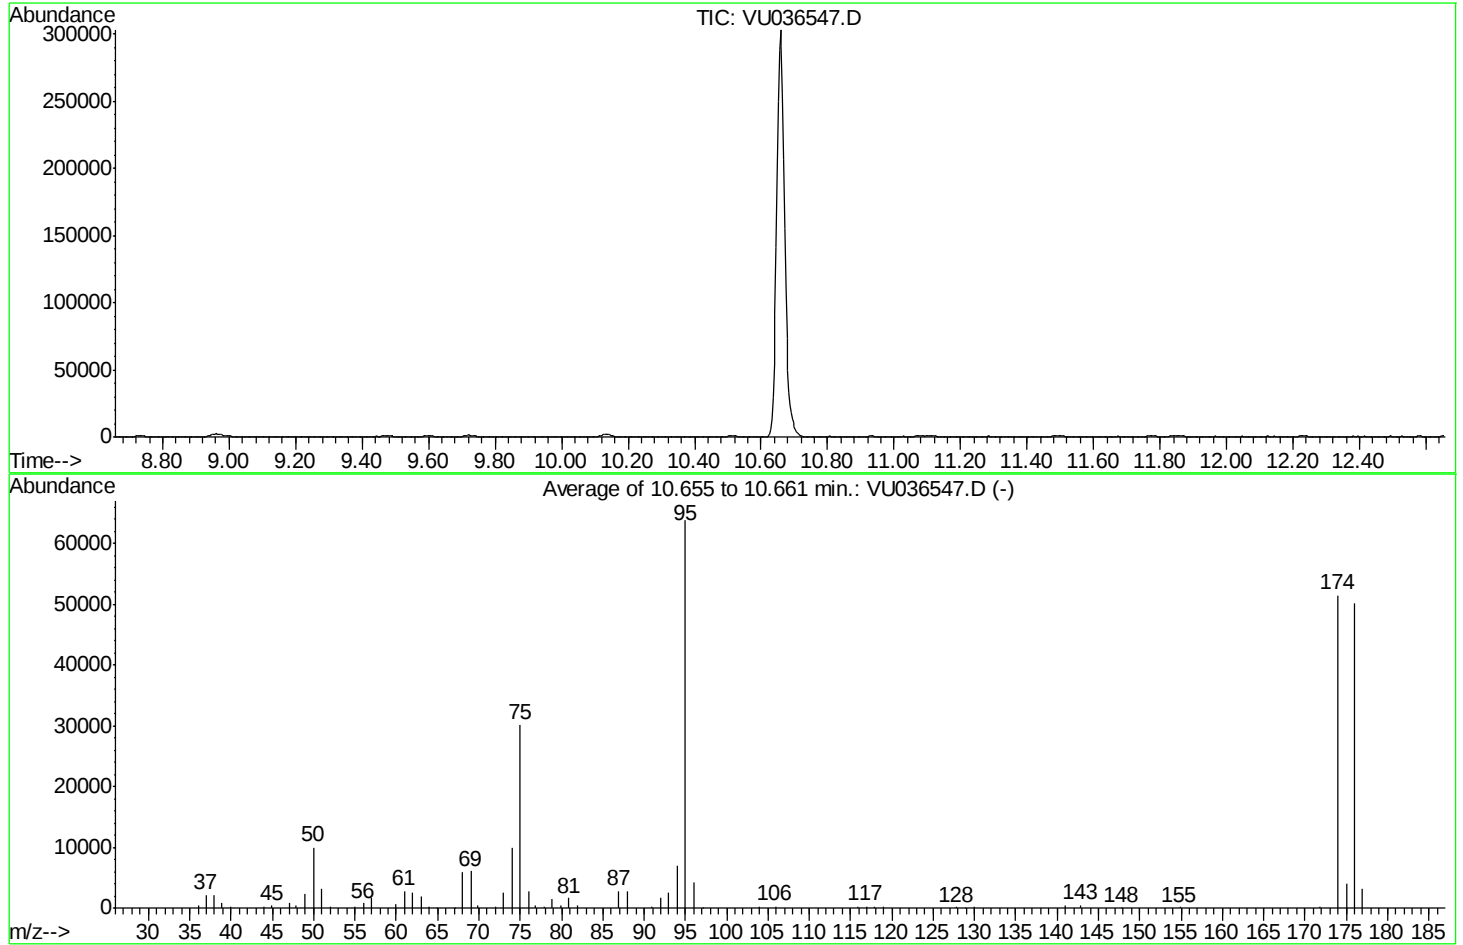

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9974	PASS
75	95	30	80	47.4	30213	PASS
95	95	100	100	100.0	63797	PASS
96	95	5	9	6.6	4197	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.6	51432	PASS
175	174	5	9	7.9	4053	PASS
176	174	95	101	97.6	50200	PASS
177	176	5	9	6.5	3246	PASS

m/z	Abundance
43.90	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB601

m/z	Abundance
36.00	437.0
37.00	2156.0
38.00	1967.0
38.90	824.0
39.90	110.0
43.90	542.0
45.00	405.0
47.00	728.0
47.80	392.0
49.00	2338.0
50.00	9872.0
51.00	3243.0
52.00	122.0
54.90	132.0
56.00	777.0
57.00	1704.0
60.00	664.0
61.00	2885.0
62.00	2603.0
63.00	1859.0
63.90	161.0
65.00	106.0
68.00	5854.0
69.00	6005.0
69.90	492.0
72.00	336.0
73.00	2549.0
74.00	9530.0
75.00	30296.0
76.00	2765.0
76.80	361.0
77.90	224.0
78.90	1408.0
79.90	389.0
80.90	1644.0
81.90	337.0
86.90	2852.0
87.90	2621.0
90.90	236.0
92.00	1599.0
93.00	2419.0
94.00	6984.0
95.00	63024.0
96.00	4054.0
97.00	107.0
103.90	205.0
105.90	217.0
115.90	169.0
116.90	276.0
117.80	197.0
118.90	241.0
127.90	196.0
129.90	171.0
140.90	410.0
142.90	495.0
147.80	116.0
154.90	120.0
171.80	186.0
174.00	49536.0
175.00	3933.0
176.00	48392.0
177.00	3191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB601

m/z	Abundance
36.00	484.0
37.00	2235.0
38.00	2057.0
38.90	873.0
39.90	127.0
43.90	604.0
44.90	425.0
47.00	783.0
47.80	384.0
49.00	2424.0
50.00	10246.0
51.00	3241.0
52.00	116.0
54.90	157.0
56.00	806.0
57.00	1766.0
60.00	753.0
61.00	2907.0
62.00	2651.0
63.00	1925.0
64.00	191.0
64.90	119.0
68.00	5974.0
69.00	6233.0
69.90	571.0
72.00	323.0
73.00	2703.0
74.00	10253.0
75.00	31120.0
76.00	2859.0
76.90	431.0
77.90	223.0
78.90	1417.0
79.90	405.0
80.90	1693.0
81.90	342.0
86.90	2898.0
87.90	2828.0
90.90	232.0
92.00	1646.0
93.00	2605.0
94.00	7251.0
95.00	65728.0
96.00	4348.0
97.10	111.0
103.90	224.0
105.90	256.0
115.90	180.0
116.90	270.0
117.80	202.0
118.90	269.0
127.80	195.0
128.80	112.0
129.90	155.0
140.90	437.0
142.90	546.0
154.90	144.0
171.90	175.0
174.00	53064.0
175.00	4167.0
176.00	51728.0
177.00	3365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB601

m/z	Abundance
36.00	461.0
37.00	2178.0
38.00	2041.0
38.90	815.0
39.90	145.0
43.90	622.0
44.90	417.0
47.00	799.0
47.80	342.0
49.00	2236.0
50.00	9805.0
51.00	2972.0
52.00	103.0
54.90	171.0
56.00	756.0
57.00	1614.0
60.00	681.0
61.00	2658.0
62.00	2548.0
63.00	1803.0
63.90	218.0
64.90	110.0
67.10	145.0
68.00	5656.0
69.00	5879.0
69.90	536.0
72.00	253.0
73.00	2599.0
74.00	10025.0
75.00	29224.0
76.00	2678.0
76.90	466.0
77.90	234.0
78.90	1323.0
79.80	409.0
80.90	1561.0
81.90	319.0
86.90	2730.0
88.00	2627.0
90.90	224.0
92.00	1563.0
93.00	2620.0
94.00	6837.0
95.00	62640.0
96.00	4191.0
103.90	235.0
105.90	280.0
115.90	170.0
116.90	268.0
117.90	184.0
118.90	275.0
127.90	179.0
128.90	105.0
129.90	160.0
140.90	430.0
142.90	524.0
154.80	145.0
171.90	134.0
174.00	51696.0
175.00	4060.0
176.00	50480.0
177.00	3183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB601