

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
 Data File : VU052792.D
 Acq On : 24 Jan 2023 15:27
 Operator : JC/MD
 Sample : 01245-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jan 25 01:38:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.112	96	35971	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.629	95	11670	0.975	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	12779	1.038	ug/l	0.00
Spiked Amount 1.000			Recovery	=	104.000%	
Target Compounds						
						Qvalue
4) Vinyl Chloride	1.604	62	461630	41.382	ug/l	99
9) 1,1-Dichloroethene	2.578	96	129668	15.448	ug/l	97
11) Allyl Chloride	3.041	41	4296	0.428	ug/l #	12
15) Methylene Chloride	3.044	84	145143	14.317	ug/l	98
16) trans-1,2-Dichloroethene	3.350	96	158155	16.936	ug/l	98
22) cis-1,2-Dichloroethene	4.662	96	164518	16.856	ug/l	89
23) Diethyl Ether	2.581	59	6378	1.075	ug/l #	14
24) tert-Butyl Alcohol	3.350	59	6652	9.310	ug/l #	22
27) Chloroform	5.086	83	3460	0.205	ug/l	89
28) 1,1,1-Trichloroethane	5.314	97	295225	18.913	ug/l	98
29) 1,1-Dichloropropene	5.768	75	10057	0.764	ug/l #	1
30) Carbon Tetrachloride	5.520	117	211734	14.949	ug/l	99
32) Ethyl-t-butyl ether	4.665	59	4570	0.216	ug/l #	31
35) Benzene	5.771	78	586872	15.369	ug/l	100
36) 1,2-Dichloroethane	5.790	62	173953	15.167	ug/l	100
37) Trichloroethene	6.539	130	161783	15.541	ug/l	100
38) 1,2-Dichloropropane	6.787	63	174820	18.045	ug/l	99
45) 4-Methyl-2-Pentanone	7.964	43	4433	0.860	ug/l #	1
46) t-1,4-Dichloro-2-butene	10.632	75	6299	2.331	ug/l #	25
49) Toluene	7.967	92	435832	18.798	ug/l	98
50) t-1,3-Dichloropropene	7.967	75	4975	0.429	ug/l #	1
52) 1,1,2-Trichloroethane	8.395	97	90087	12.919	ug/l	98
58) Tetrachloroethene	8.549	164	51125	5.442	ug/l	97
59) Chlorobenzene	9.443	112	370280	14.674	ug/l	98
63) Ethyl Benzene	9.568	91	469786	11.494	ug/l	100
64) m/p-Xylenes	9.690	106	230267	14.130	ug/l	99
65) o-Xylene	10.095	106	223568	14.218	ug/l	100
66) Styrene	10.112	104	388764	12.705	ug/l	100
73) n-propylbenzene	10.909	120	45	0.444	ug/l #	1
78) 1,2,4-Trimethylbenzene	11.465	105	226	0.460	ug/l #	30
79) sec-Butylbenzene	11.636	105	73	0.430	ug/l #	56
81) p-Isopropyltoluene	11.793	119	80	0.486	ug/l #	51
82) 1,3-Dichlorobenzene	11.832	146	272765	13.146	ug/l	98
83) 1,4-Dichlorobenzene	11.832	146	272765	13.094	ug/l	99
84) n-Butylbenzene	12.208	91	429	0.564	ug/l #	74
85) 1,2-Dichlorobenzene	12.208	146	391505	19.994	ug/l	99
87) 1,2,4-Trichlorobenzene	13.835	180	222287	18.927	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052792.D
Acq On : 24 Jan 2023 15:27
Operator : JC/MD
Sample : 01245-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jan 25 01:38:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




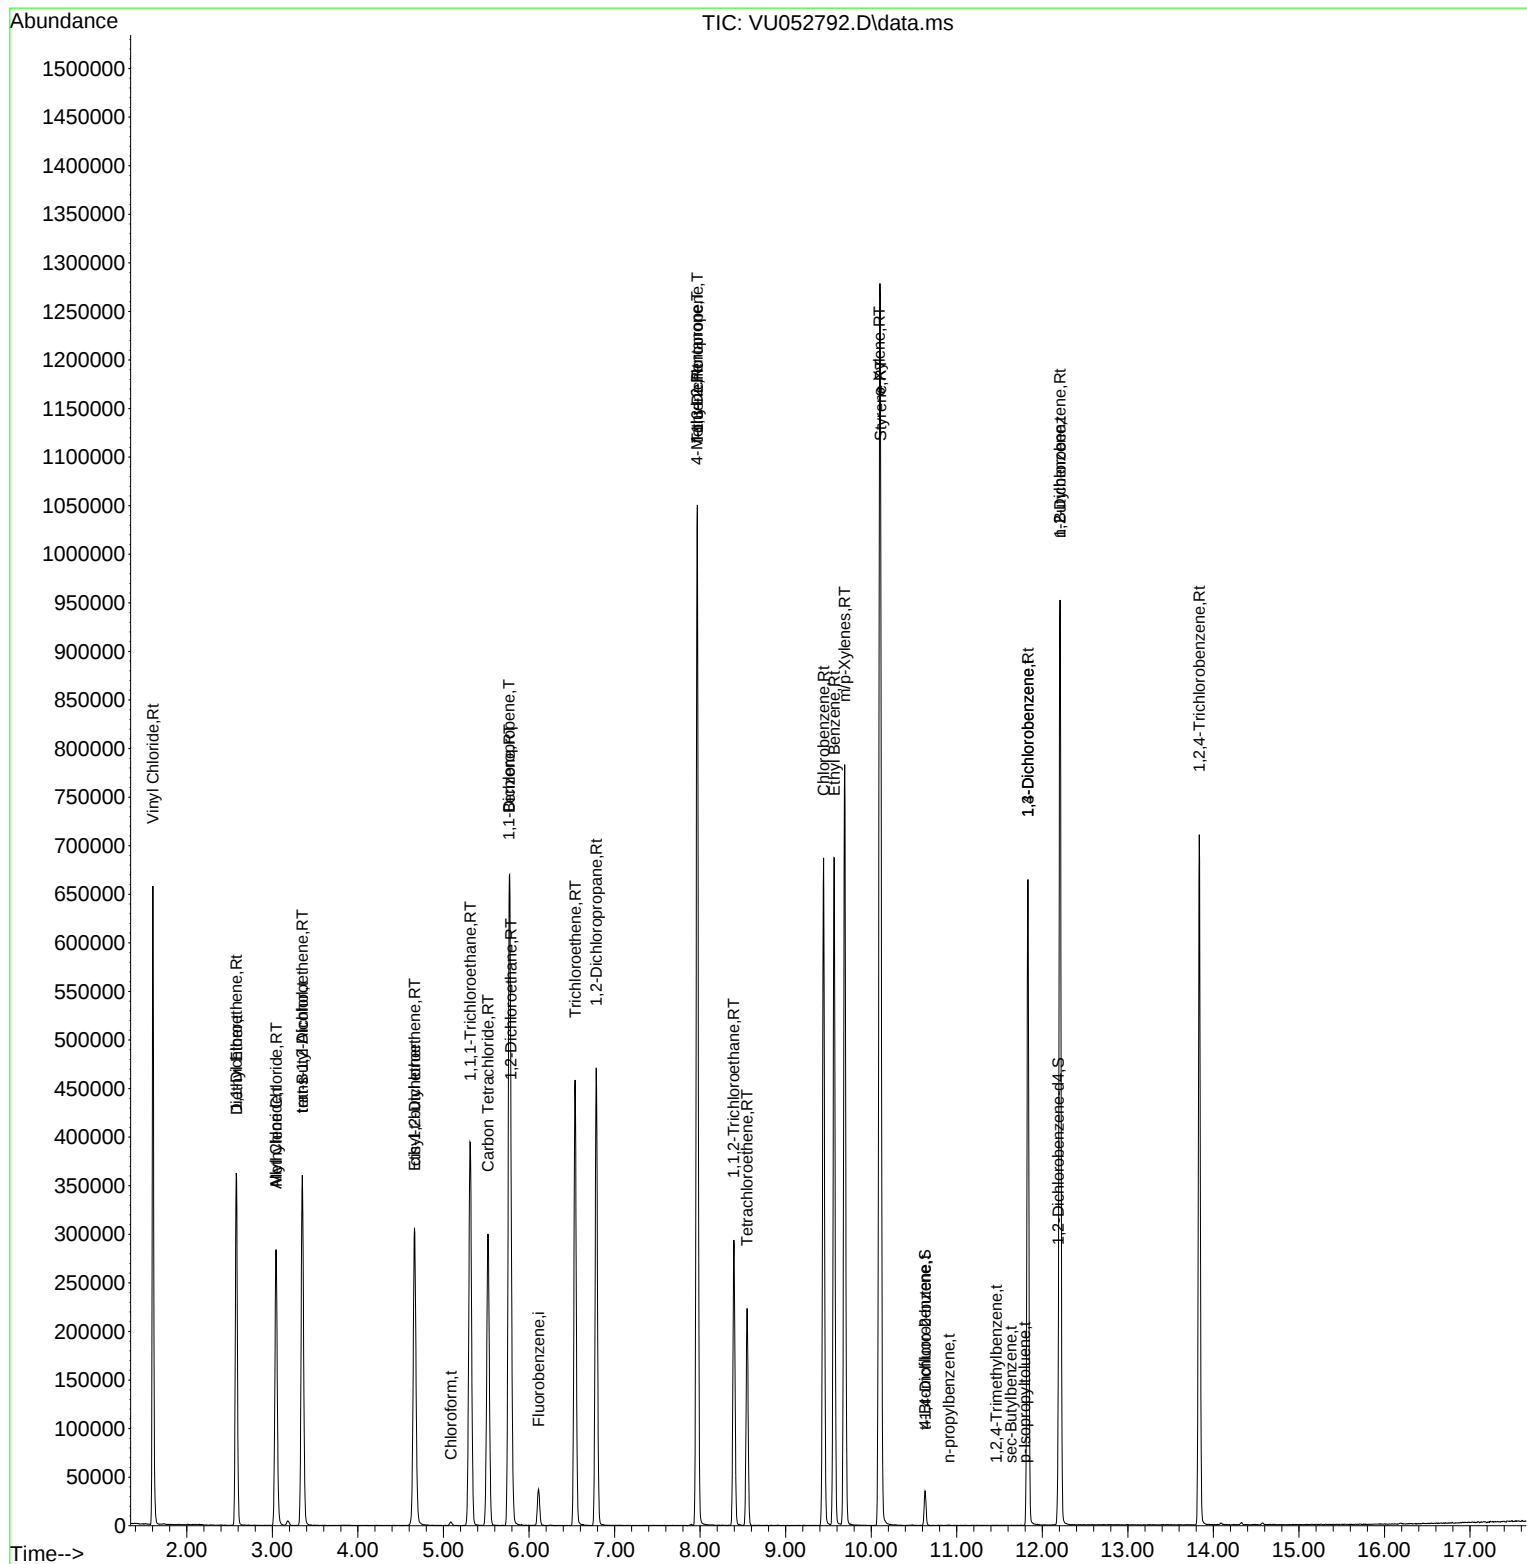


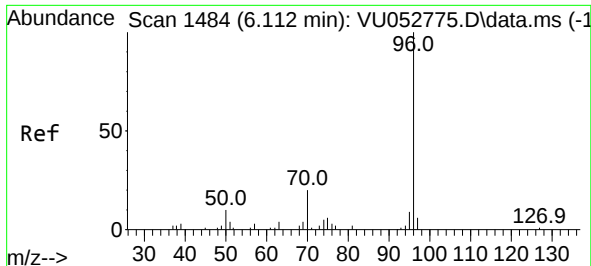

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1484
Delta R.T. -0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 96	Resp: 35971
Ion Ratio	Lower Upper
96 100	
70 18.2	16.2 24.4
95 9.4	7.4 11.0
97 0.0	0.0 0.0

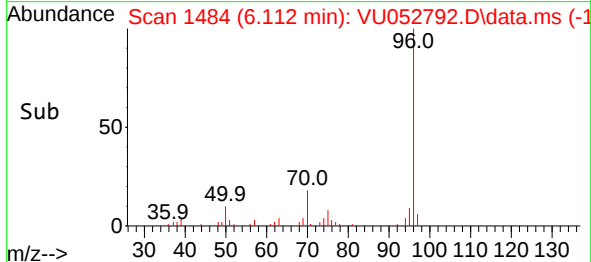

#4
Vinyl Chloride
Concen: 41.382 ug/l
RT: 1.604 min Scan# 82
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion: 62	Resp: 461630
Ion Ratio	Lower Upper
62 100	
64 32.8	26.0 39.0


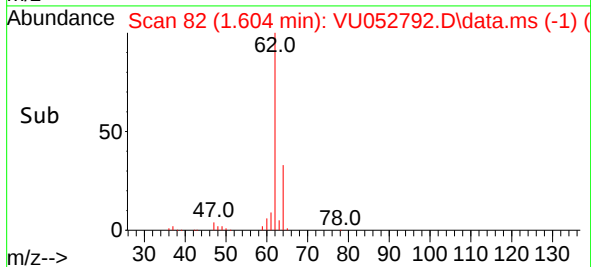

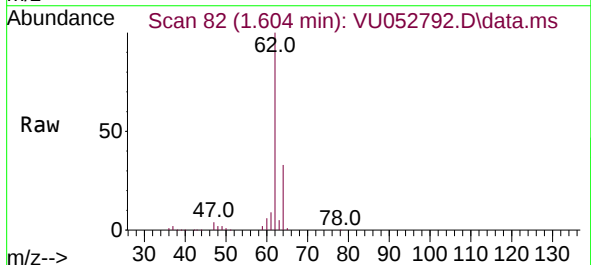


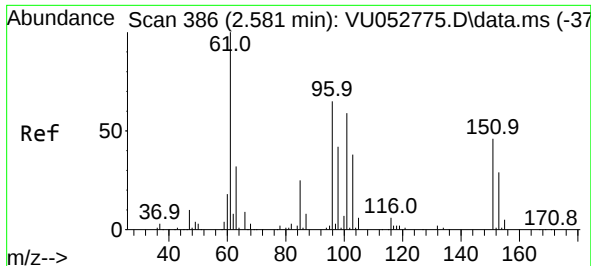

#9
1,1-Dichloroethene
Concen: 15.448 ug/l
RT: 2.578 min Scan# 31
Delta R.T. -0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 96 Resp: 129668
Ion Ratio Lower Upper
96 100
61 158.2 0.0 460.5
98 64.1 0.0 128.0

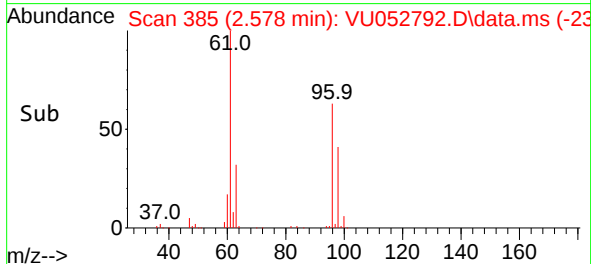

#11
Allyl Chloride
Concen: 0.428 ug/l
RT: 3.041 min Scan# 529
Delta R.T. 0.119 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27


Tgt Ion: 41 Resp: 4296
Ion Ratio Lower Upper
41 100
39 0.0 59.3 88.9#

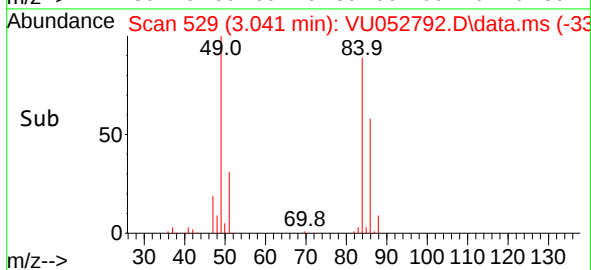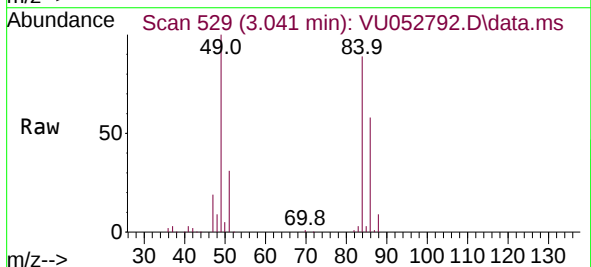

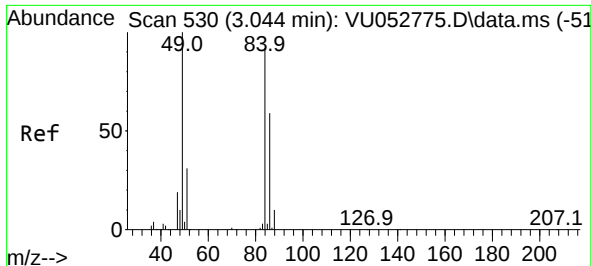




#15
Methylene Chloride
Concen: 14.317 ug/l
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Instrument :
MSVOA_U
ClientSampleId :



Tgt Ion: 84 Resp: 145143




Ion	Ratio	Lower	Upper
84	100		
49	110.9	86.7	130.1
51	34.7	0.0	66.8
86	65.2	51.5	77.3

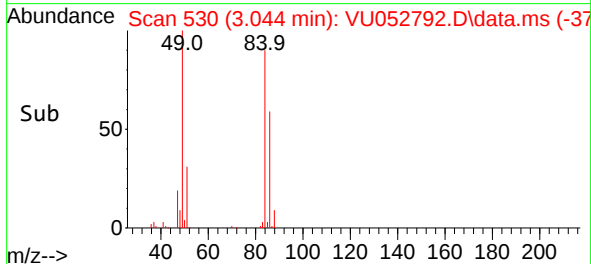


#16
trans-1,2-Dichloroethene
Concen: 16.936 ug/l
RT: 3.350 min Scan# 625
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion: 96 Resp: 158155


Ion	Ratio	Lower	Upper
96	100		
61	135.2	105.7	158.5
98	64.3	51.4	77.2

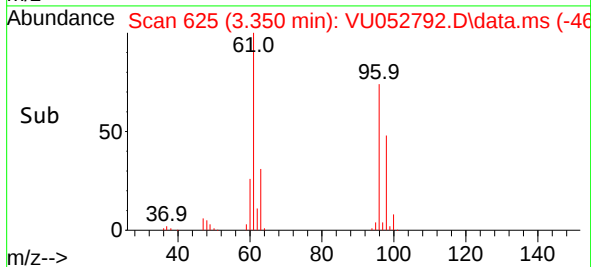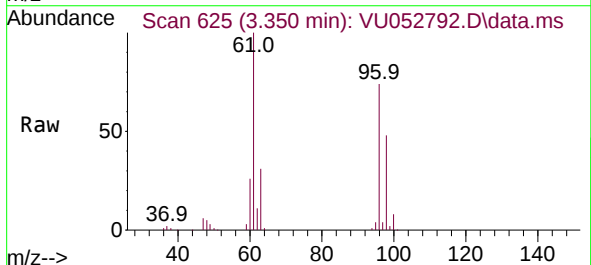






#22
 cis-1,2-Dichloroethene
 Concen: 16.856 ug/l
 RT: 4.662 min Scan# 1033
 Delta R.T. -0.000 min
 Lab File: VU052792.D
 Acq: 24 Jan 2023 15:27

Instrument :
 MSVOA_U
 ClientSampleId :



Tgt Ion: 96 Resp: 164518




Ion	Ratio	Lower	Upper
96	100		
61	122.5	0.0	353.3
98	63.9	32.6	97.7

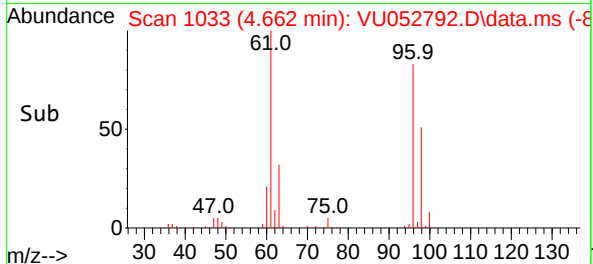


#23
 Diethyl Ether
 Concen: 1.075 ug/l
 RT: 2.581 min Scan# 386
 Delta R.T. 0.206 min
 Lab File: VU052792.D
 Acq: 24 Jan 2023 15:27

Tgt Ion: 59 Resp: 6378


Ion	Ratio	Lower	Upper
59	100		
45	0.0	52.1	78.1#
74	0.0	61.6	92.4#

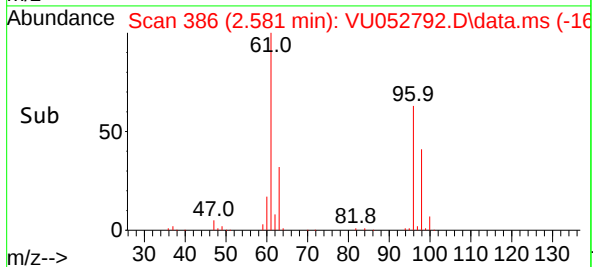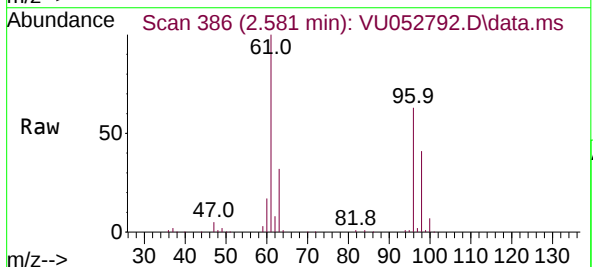



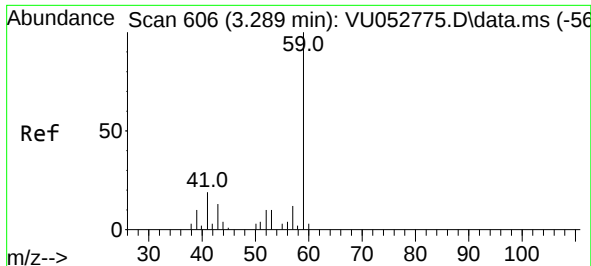


#24
tert-Butyl Alcohol
Concen: 9.310 ug/l
RT: 3.350 min Scan# 61
Delta R.T. 0.061 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27


Instrument :
MSVOA_U
ClientSampleId :





Tgt Ion: 59 Resp: 6652
Ion Ratio Lower Upper
59 100
57 0.0 45.8 68.8#

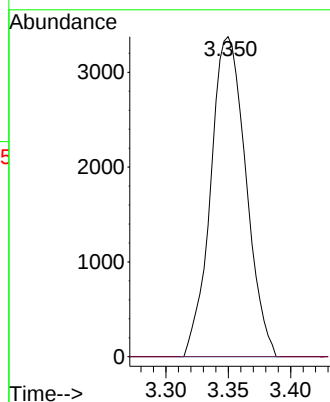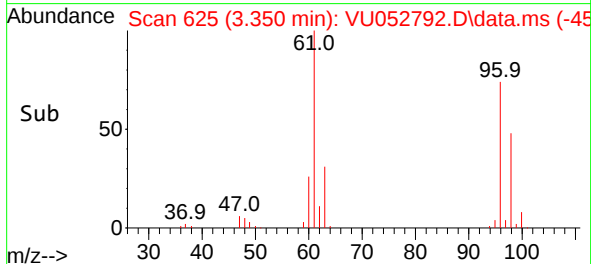


#27
Chloroform
Concen: 0.205 ug/l
RT: 5.086 min Scan# 1165
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

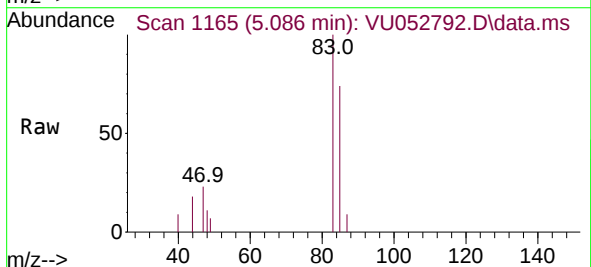

Tgt Ion: 83 Resp: 3460
Ion Ratio Lower Upper
83 100
85 73.9 0.0 130.6

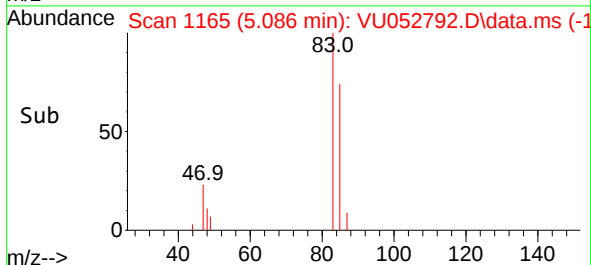



#28

1,1,1-Trichloroethane

Concen: 18.913 ug/l

RT: 5.314 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion: 97 Resp: 295225

Ion Ratio Lower Upper

97 100

99 65.1 31.9 95.5

61 43.0 20.8 62.2

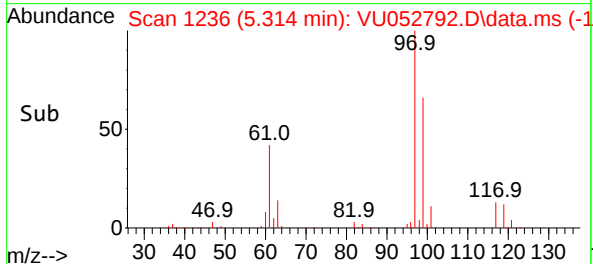

#29

1,1-Dichloropropene

Concen: 0.764 ug/l

RT: 5.768 min Scan# 1377

Delta R.T. 0.248 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27




Tgt Ion: 75 Resp: 10057


Ion Ratio Lower Upper

75 100

110 0.0 17.4 52.2#

77 1387.6 24.8 37.2#


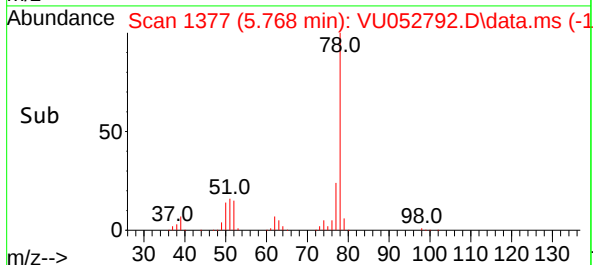
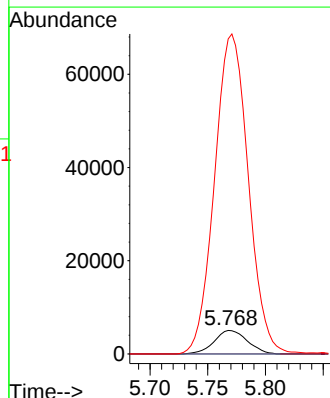
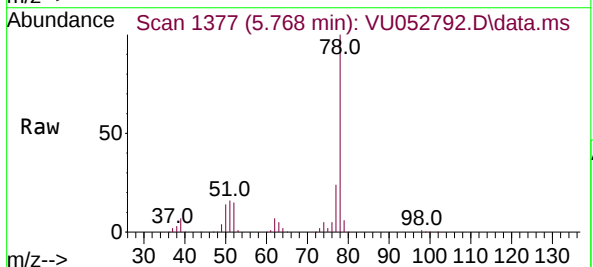




#30
Carbon Tetrachloride
Concen: 14.949 ug/l
RT: 5.520 min Scan# 1117
Delta R.T. 0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:117 Resp: 211734
Ion Ratio Lower Upper
117 100
119 93.9 76.4 114.6
121 31.0 25.0 37.6

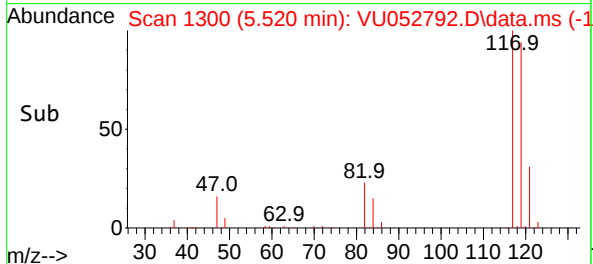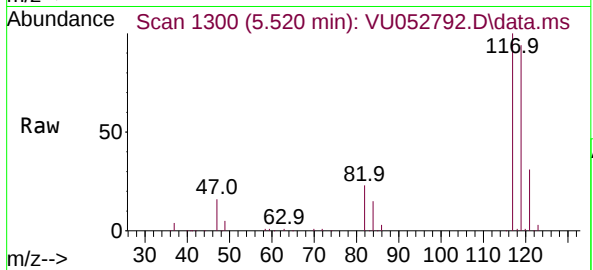

#32
Ethyl-t-butyl ether
Concen: 0.216 ug/l
RT: 4.665 min Scan# 1034
Delta R.T. 0.161 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion: 59 Resp: 4570
Ion Ratio Lower Upper
59 100
87 0.0 36.2 54.2#




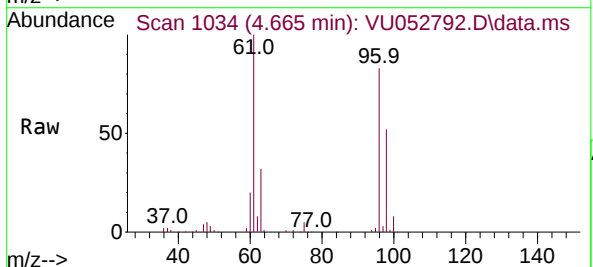




#35
Benzene
Concen: 15.369 ug/l
RT: 5.771 min Scan# 1378
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 78 Resp: 586872
Ion Ratio Lower Upper
78 100
77 23.6 19.0 28.4

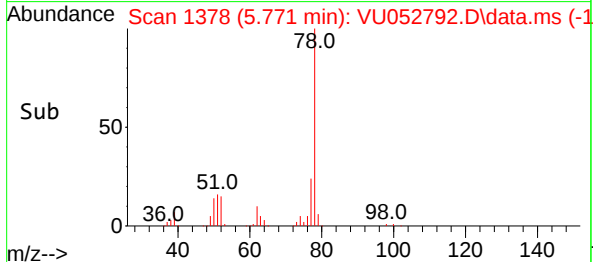

#36
1,2-Dichloroethane
Concen: 15.167 ug/l
RT: 5.790 min Scan# 1384
Delta R.T. -0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion: 62 Resp: 173953
Ion Ratio Lower Upper
62 100
98 9.5 7.5 11.3

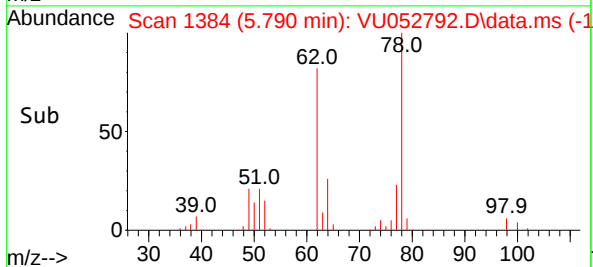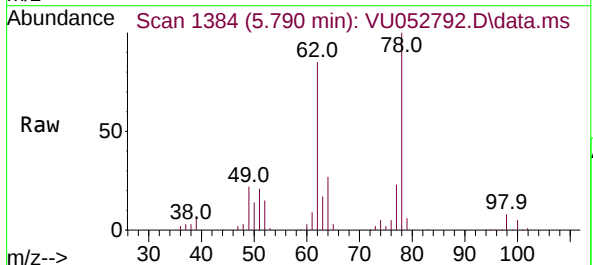



#37

Trichloroethene

Concen: 15.541 ug/l

RT: 6.539 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:130 Resp: 161783

Ion Ratio Lower Upper

130 100

95 95.9 76.6 114.8

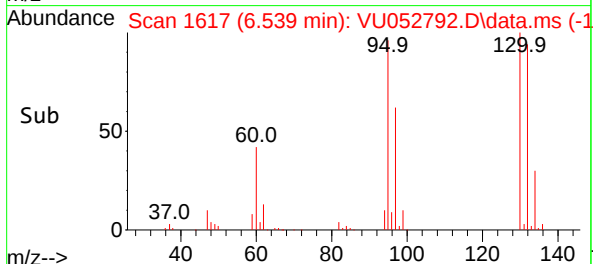

#38

1,2-Dichloropropane

Concen: 18.045 ug/l

RT: 6.787 min Scan# 1694

Delta R.T. -0.003 min

Lab File: VU052792.D




Acq: 24 Jan 2023 15:27


Tgt Ion: 63 Resp: 174820

Ion Ratio Lower Upper

63 100

65 31.4 24.6 36.8

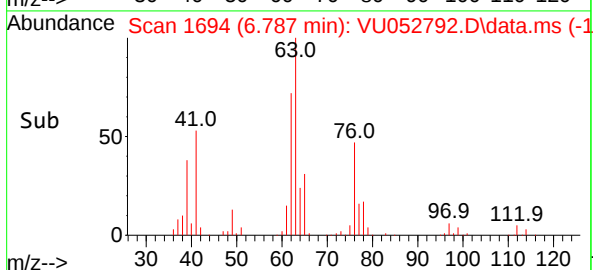



#45

4-Methyl-2-Pentanone

Concen: 0.860 ug/l

RT: 7.964 min Scan# 2008

Delta R.T. 0.167 min


Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U

ClientSampleId :






Tgt Ion: 43 Resp: 4433

Ion Ratio Lower Upper

43 100

58 0.0 21.7 65.1#

85 101.5 16.2 24.4#

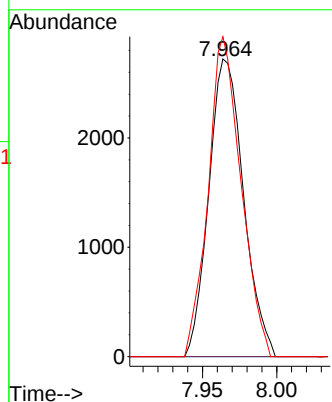

#46

t-1,4-Dichloro-2-butene

Concen: 2.331 ug/l

RT: 10.632 min Scan# 2890

Delta R.T. -0.196 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Tgt Ion: 75 Resp: 6299




Ion Ratio Lower Upper


75 100

53 0.0 57.0 85.4#

89 0.0 41.1 61.7#

88 5.5 32.3 48.5#

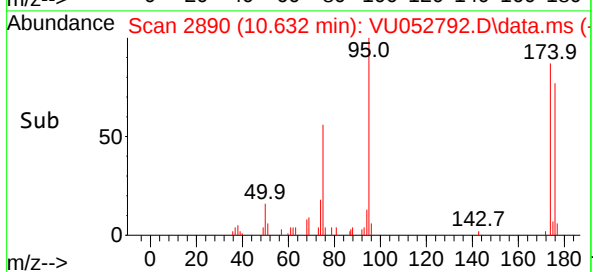



#49

Toluene

Concen: 18.798 ug/l

RT: 7.967 min Scan# 2061

Delta R.T. -0.000 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion: 92 Resp: 435832

Ion Ratio Lower Upper

92 100

91 169.6 133.8 200.8

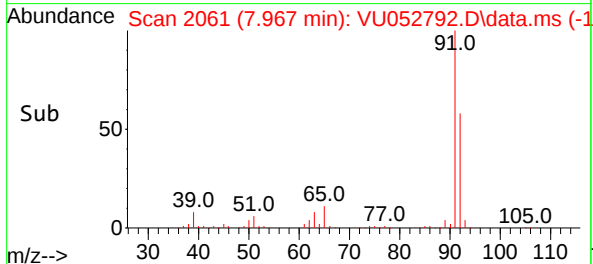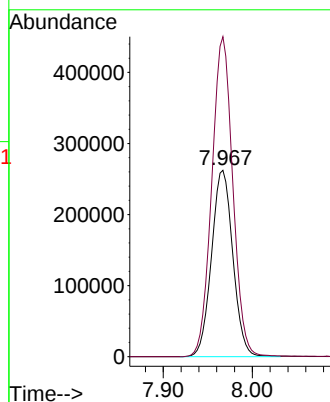

#50

t-1,3-Dichloropropene

Concen: 0.429 ug/l

RT: 7.967 min Scan# 2061

Delta R.T. -0.241 min

Lab File: VU052792.D




Acq: 24 Jan 2023 15:27


Tgt Ion: 75 Resp: 4975

Ion Ratio Lower Upper

75 100

77 163.4 24.4 36.6#


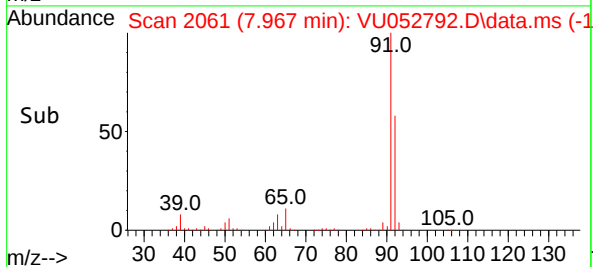
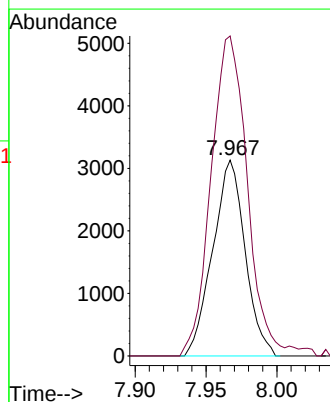
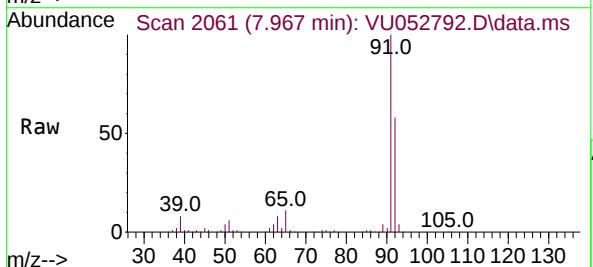




#52
1,1,2-Trichloroethane
Concen: 12.919 ug/l
RT: 8.395 min Scan# 2195
Delta R.T. -0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 97	Resp: 90087
Ion Ratio	Lower Upper
97 100	
83 84.8	68.2 102.2
85 54.5	44.5 66.7
99 61.3	51.0 76.4

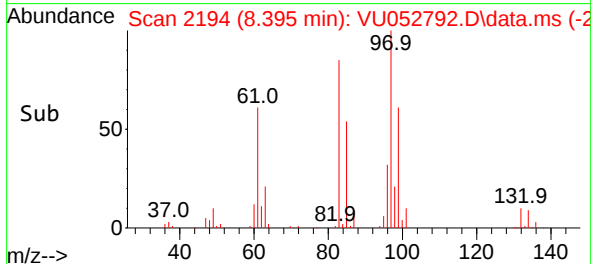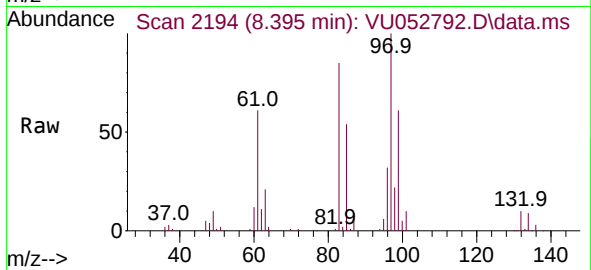

#57
4-Bromofluorobenzene
Concen: 0.975 ug/l
RT: 10.629 min Scan# 2889
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27


Tgt Ion: 95	Resp: 11670
Ion Ratio	Lower Upper
95 100	
174 91.6	66.9 100.3
176 82.3	61.9 92.9

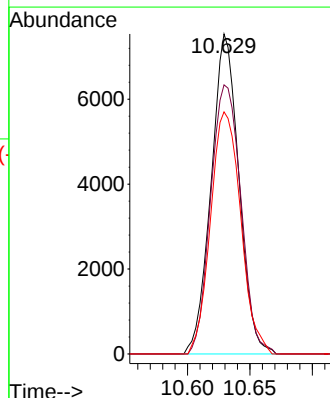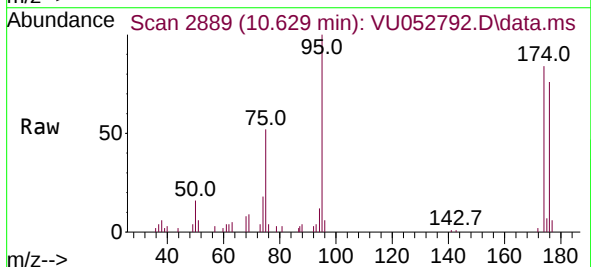



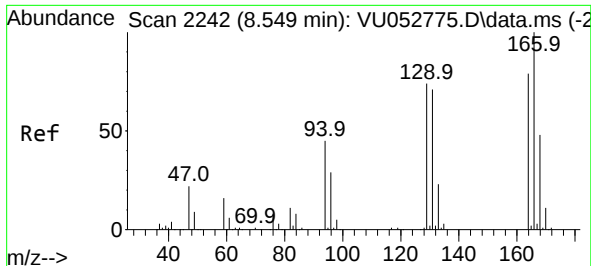


#58
Tetrachloroethene
Concen: 5.442 ug/l
RT: 8.549 min Scan# 211
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Instrument :
MSVOA_U
ClientSampleId :







Tgt Ion:164 Resp: 51125
Ion Ratio Lower Upper
164 100
166 129.9 101.5 152.3
129 90.0 75.2 112.8
131 87.1 72.2 108.2

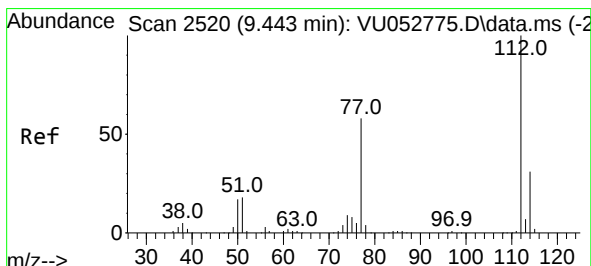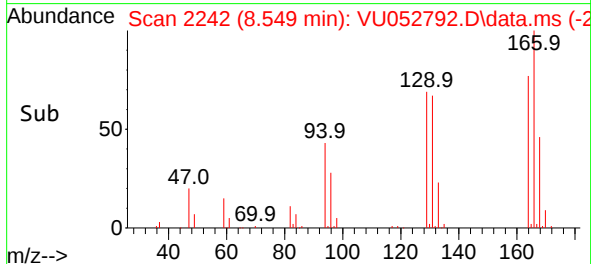

#59
Chlorobenzene
Concen: 14.674 ug/l
RT: 9.443 min Scan# 2520
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion:112 Resp: 370280
Ion Ratio Lower Upper
112 100
114 32.6 25.2 37.8


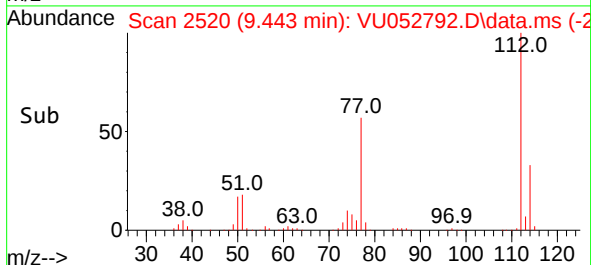
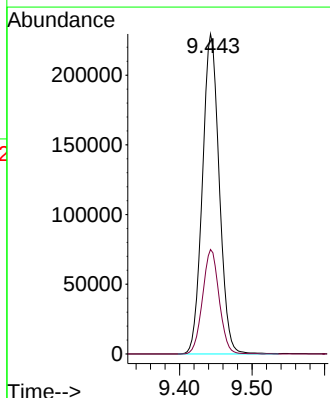
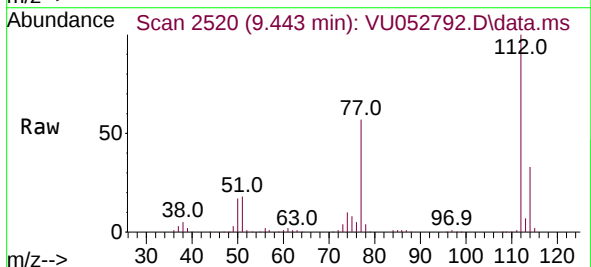




#63
Ethyl Benzene
Concen: 11.494 ug/l
RT: 9.568 min Scan# 2559
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 91 Resp: 469786
Ion Ratio Lower Upper
91 100
106 31.2 25.1 37.7

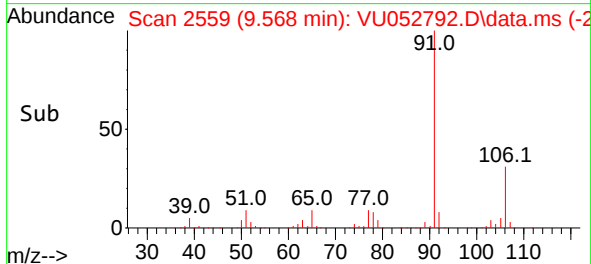

#64
m/p-Xylenes
Concen: 14.130 ug/l
RT: 9.690 min Scan# 2597
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion:106 Resp: 230267
Ion Ratio Lower Upper
106 100
91 197.0 158.7 238.1




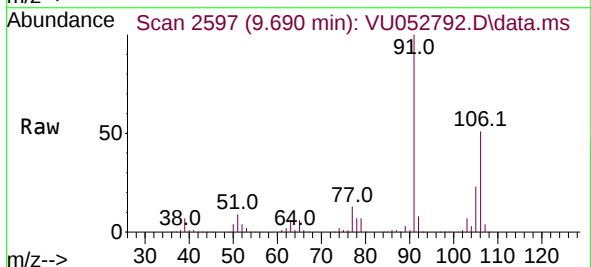


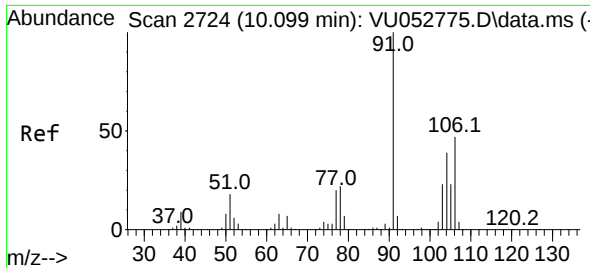

#65
o-Xylene
Concen: 14.218 ug/l
RT: 10.095 min Scan# 2723
Delta R.T. -0.004 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:106 Resp: 223568
Ion Ratio Lower Upper
106 100
91 211.0 105.6 316.8

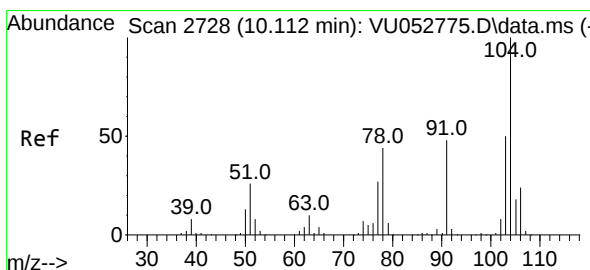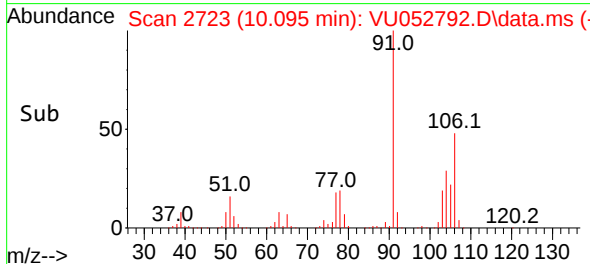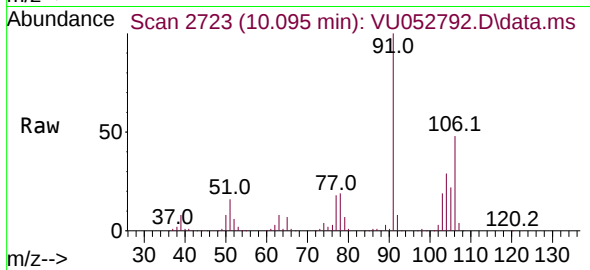

#66
Styrene
Concen: 12.705 ug/l
RT: 10.112 min Scan# 2728
Delta R.T. -0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27


Tgt Ion:104 Resp: 388764
Ion Ratio Lower Upper
104 100
78 49.5 39.6 59.4
103 53.7 42.9 64.3

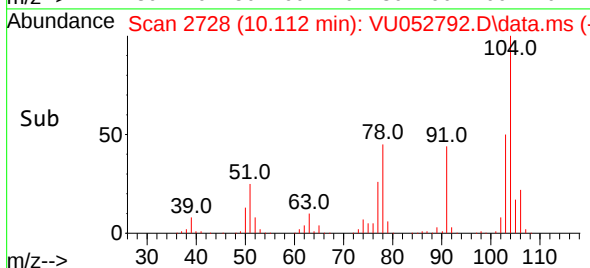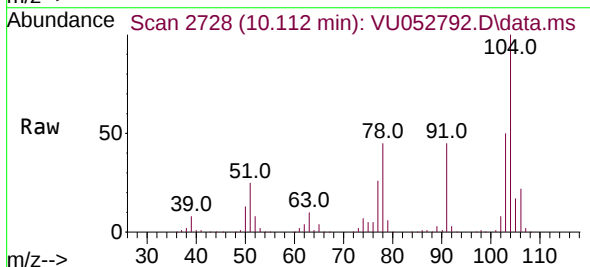



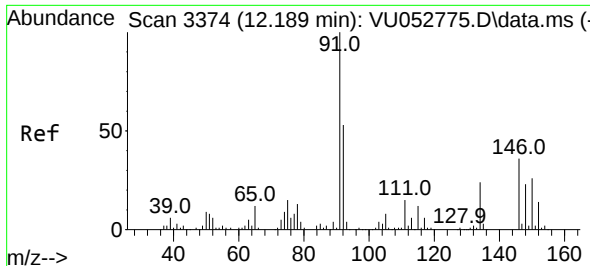


#68
1,2-Dichlorobenzene-d4
Concen: 1.038 ug/l
RT: 12.189 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27


Instrument :
MSVOA_U
ClientSampleId :

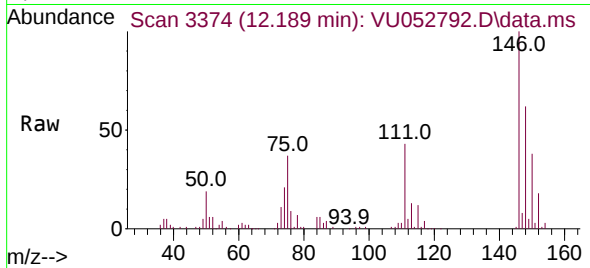



Tgt Ion:152 Resp: 12779
Ion Ratio Lower Upper
152 100
115 67.6 0.0 262.6
150 472.6 0.0 638.0

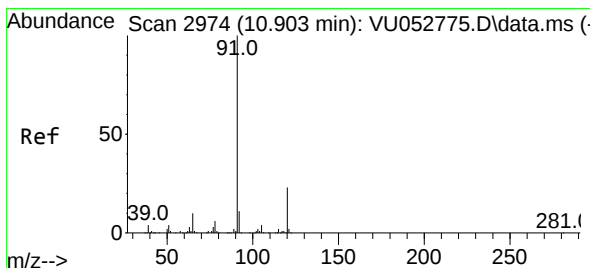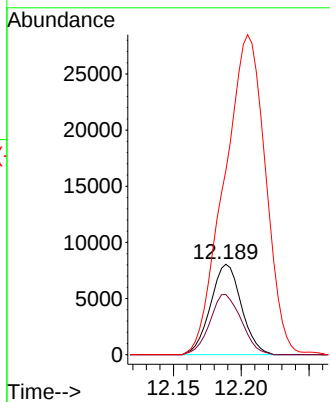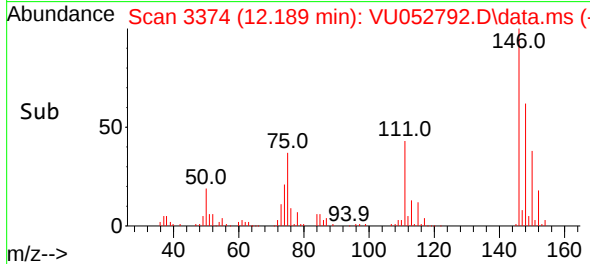


#73
n-propylbenzene
Concen: 0.444 ug/l
RT: 10.909 min Scan# 2976
Delta R.T. 0.006 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

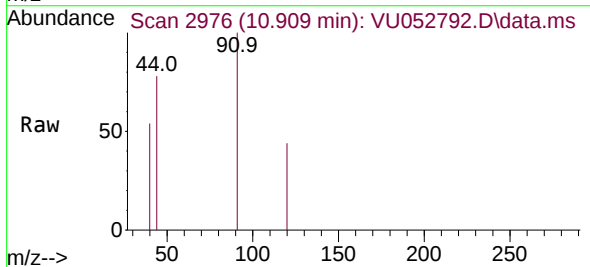

Tgt Ion:120 Resp: 45
Ion Ratio Lower Upper
120 100
91 1120.0 348.0 522.0#

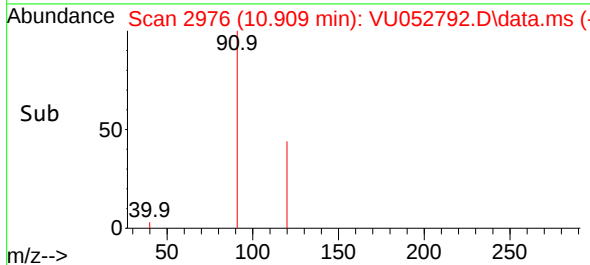



#78

1,2,4-Trimethylbenzene

Concen: 0.460 ug/l

RT: 11.465 min Scan# 3149

Delta R.T. 0.000 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U





ClientSampleId :

Tgt Ion:105 Resp: 226

Ion Ratio Lower Upper

105 100

120 0.0 23.4 70.3#

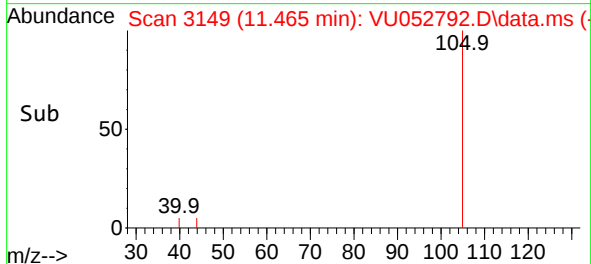

#79

sec-Butylbenzene

Concen: 0.430 ug/l

RT: 11.636 min Scan# 3202

Delta R.T. -0.003 min

Lab File: VU052792.D




Acq: 24 Jan 2023 15:27


Tgt Ion:105 Resp: 73

Ion Ratio Lower Upper

105 100

134 0.0 16.5 24.7#




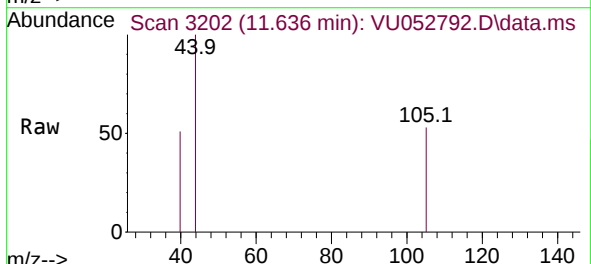


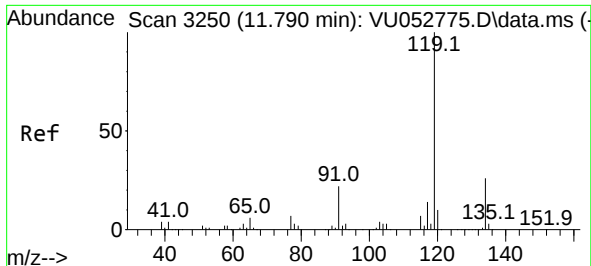

#81
p-Isopropyltoluene
Concen: 0.486 ug/l
RT: 11.793 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:119 Resp: 80
Ion Ratio Lower Upper
119 100
134 0.0 20.7 31.1#
91 0.0 17.6 26.4#

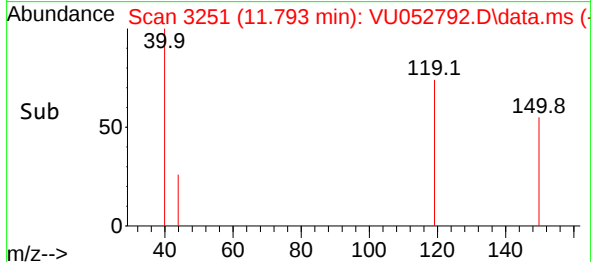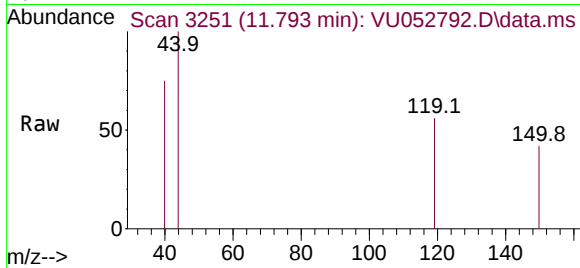

#82
1,3-Dichlorobenzene
Concen: 13.146 ug/l
RT: 11.832 min Scan# 3263
Delta R.T. 0.090 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion:146 Resp: 272765
Ion Ratio Lower Upper
146 100
111 38.5 32.6 48.8
148 64.4 51.9 77.9


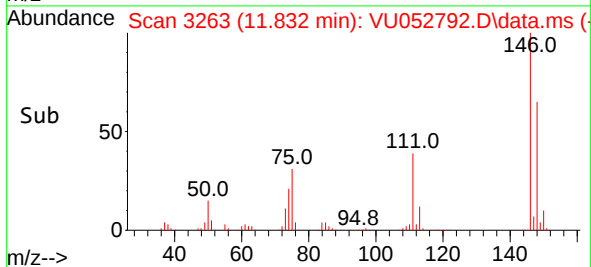

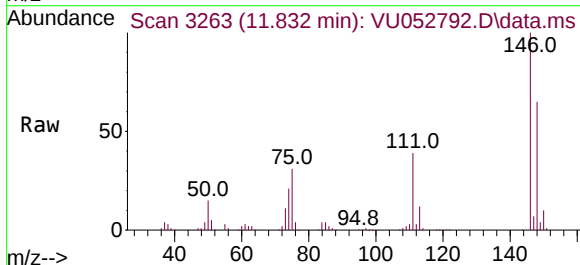


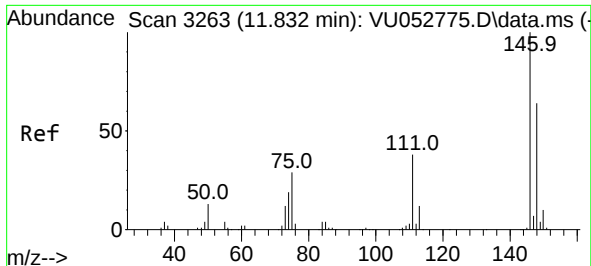

#83
1,4-Dichlorobenzene
Concen: 13.094 ug/l
RT: 11.832 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion:146 Resp: 272765
Ion Ratio Lower Upper
146 100
111 38.5 29.5 44.3
148 64.4 51.4 77.0

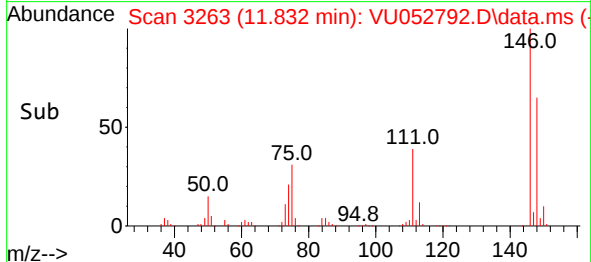

#84
n-Butylbenzene
Concen: 0.564 ug/l
RT: 12.208 min Scan# 3380
Delta R.T. 0.003 min
Lab File: VU052792.D
Acq: 24 Jan 2023 15:27

Tgt Ion: 91 Resp: 429
Ion Ratio Lower Upper
91 100
92 45.0 43.4 65.0
134 0.0 21.2 31.8#

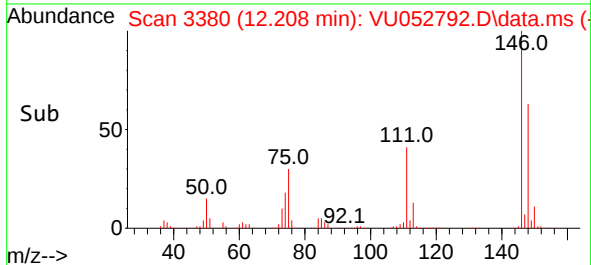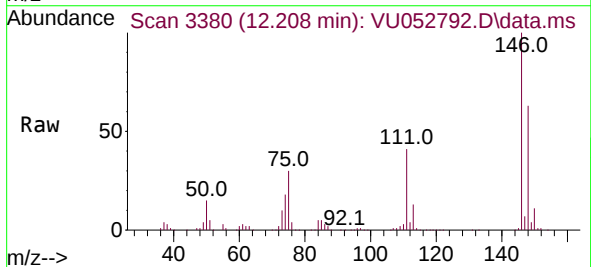

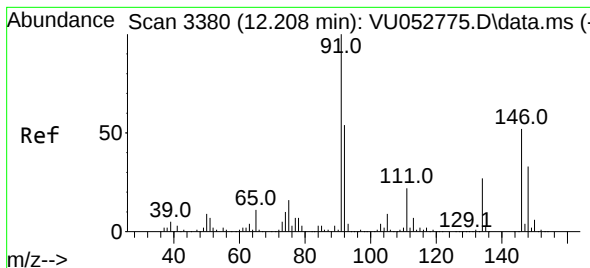

#85

1,2-Dichlorobenzene

Concen: 19.994 ug/l

RT: 12.208 min Scan# 3380

Delta R.T. 0.000 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Instrument :

MSVOA_U

ClientSampleId :





Tgt Ion:146 Resp: 391505

Ion Ratio Lower Upper

146 100

111 41.1 20.8 62.5

148 63.0 31.4 94.2

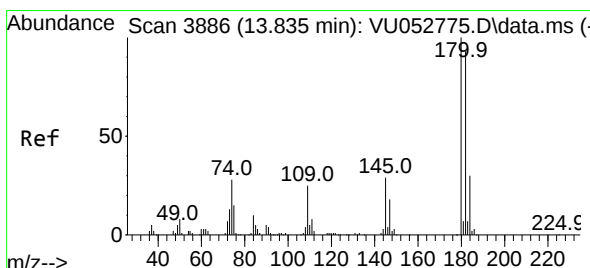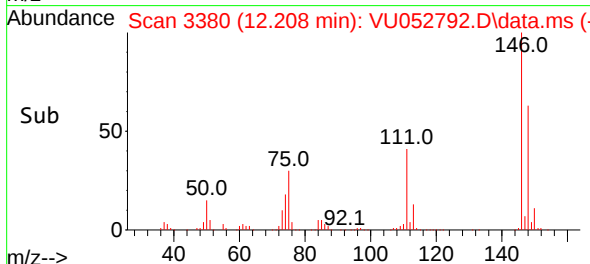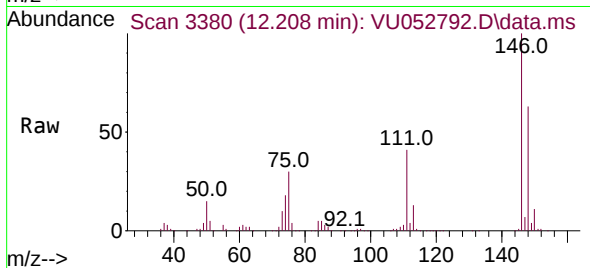

#87

1,2,4-Trichlorobenzene

Concen: 18.927 ug/l

RT: 13.835 min Scan# 3886

Delta R.T. 0.000 min

Lab File: VU052792.D

Acq: 24 Jan 2023 15:27

Tgt Ion:180 Resp: 222287

Ion Ratio Lower Upper

180 100

182 95.3 74.6 112.0

145 29.8 23.4 35.0

