

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
 Data File : VU052782.D
 Acq On : 24 Jan 2023 11:03
 Operator : JC/MD
 Sample : VU0124WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0124WBL01

Quant Time: Jan 25 01:34:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jan 24 05:16:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.112	96	33882	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.629	95	8789	0.780	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	
68) 1,2-Dichlorobenzene-d4	12.189	152	9208	0.794	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052782.D
Acq On : 24 Jan 2023 11:03
Operator : JC/MD
Sample : VU0124WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0124WBL01

Quant Time: Jan 25 01:34:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jan 24 05:16:59 2023
Response via : Initial Calibration




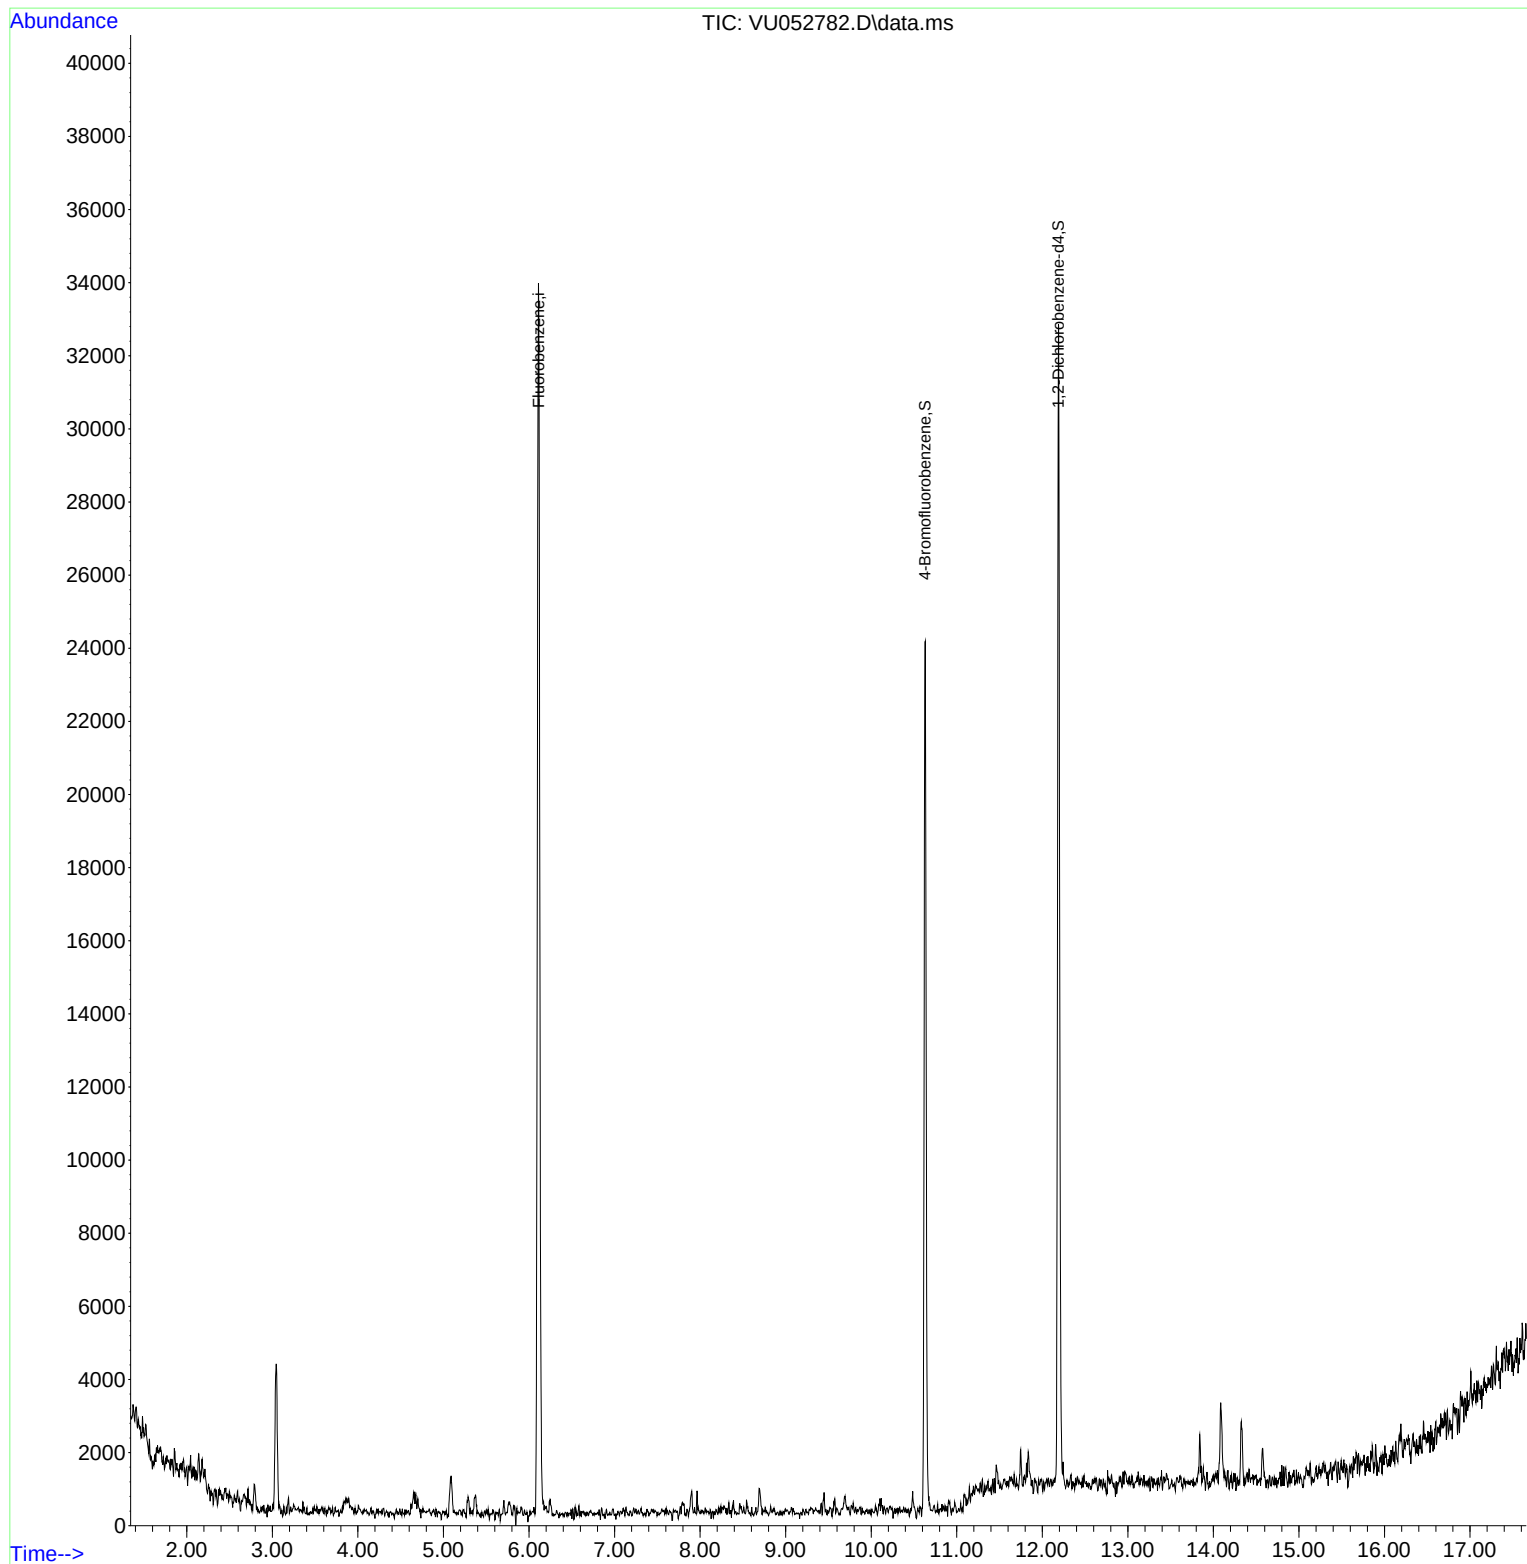


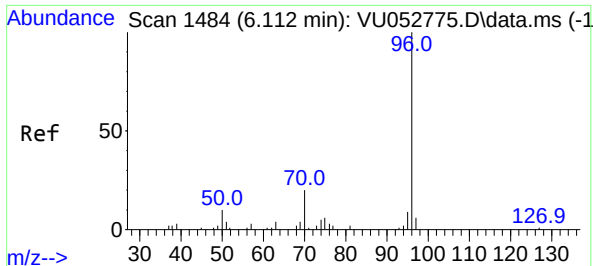

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.112 min Scan# 1484
Delta R.T. -0.000 min
Lab File: VU052782.D
Acq: 24 Jan 2023 11:03




Instrument :
MSVOA_U
ClientSampleId :
VU0124WBL01


Tgt Ion:	96	Resp:	33882
Ion	Ratio	Lower	Upper
96	100		
70	18.8	16.2	24.4
95	9.7	7.4	11.0
97	6.2	0.0	0.0

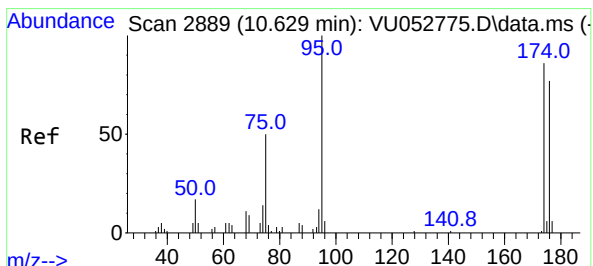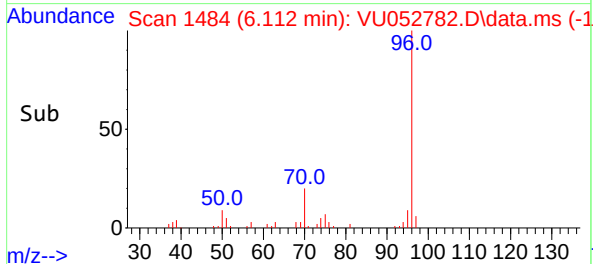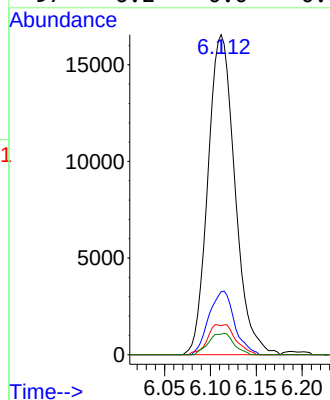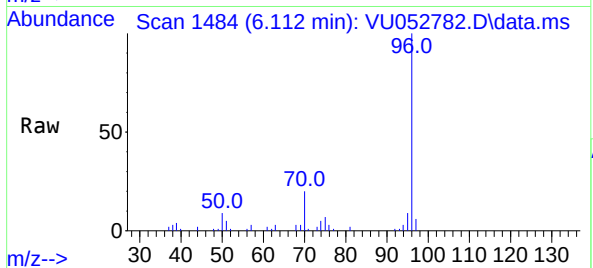

#57
4-Bromofluorobenzene
Concen: 0.780 ug/l
RT: 10.629 min Scan# 2889
Delta R.T. 0.000 min
Lab File: VU052782.D
Acq: 24 Jan 2023 11:03


Tgt Ion:	95	Resp:	8789
Ion	Ratio	Lower	Upper
95	100		
174	86.5	66.9	100.3
176	81.3	61.9	92.9

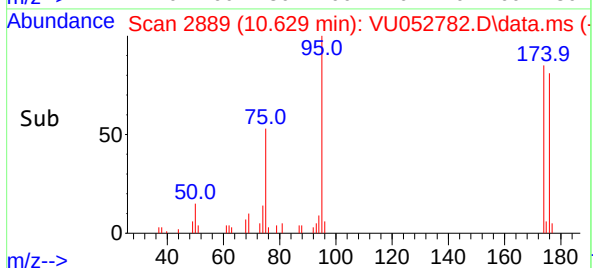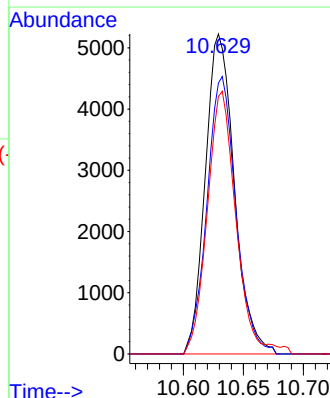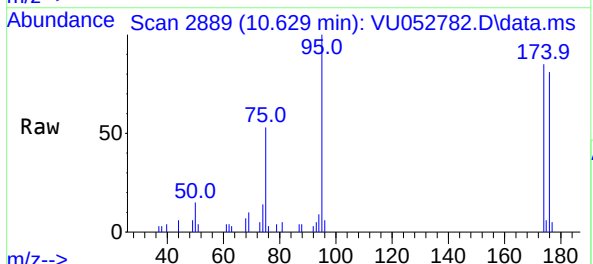

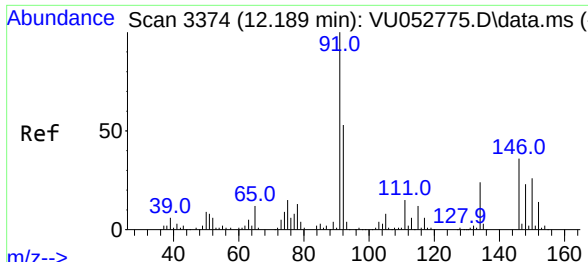

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.794 ug/l
 RT: 12.189 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU052782.D
 Acq: 24 Jan 2023 11:03

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0124WBL01

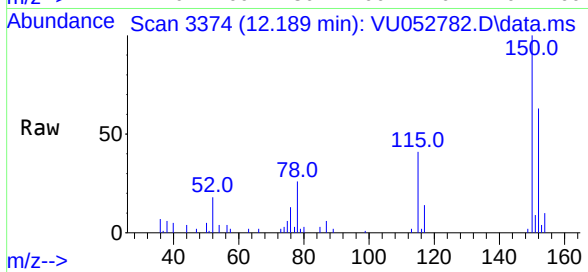

Tgt Ion:	152	Resp:	9208
Ion	Ratio	Lower	Upper
152	100		
115	62.4	0.0	262.6
150	159.1	0.0	638.0

