

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
 Data File : VU052782.D
 Acq On : 24 Jan 2023 11:03
 Operator : JC/MD
 Sample : VU0124WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0124WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU052782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.855	157	160	166	rBV3	769	818	1.23%	0.434%
2	2.138	244	248	254	rVB5	755	859	1.29%	0.456%
3	2.787	445	450	458	rBV2	724	1064	1.60%	0.564%
4	3.048	521	531	541	rBV3	3936	7174	10.79%	3.805%
5	5.089	1157	1166	1175	rBV3	1116	2245	3.38%	1.191%
6	6.112	1471	1484	1500	rBV2	33668	66465	100.00%	35.250%
7	7.903	2029	2041	2046	rBV4	688	1146	1.72%	0.608%
8	8.690	2276	2286	2294	rBV3	716	1216	1.83%	0.645%
9	10.632	2880	2890	2902	rBV	23742	38267	57.57%	20.295%
10	11.462	3144	3148	3152	rBV2	779	903	1.36%	0.479%
11	11.748	3229	3237	3244	rBV4	1084	1346	2.03%	0.714%
12	11.835	3261	3264	3275	rVB5	925	1300	1.96%	0.689%
13	12.189	3365	3374	3389	rBV2	31528	52270	78.64%	27.722%
14	13.841	3884	3888	3892	rVB4	1045	887	1.33%	0.470%
15	13.883	3898	3901	3908	rVB4	643	692	1.04%	0.367%
16	14.086	3955	3964	3976	rBV2	2202	4077	6.13%	2.162%
17	14.327	4033	4039	4040	rBV4	1661	1455	2.19%	0.772%
18	14.574	4111	4116	4122	rBV4	836	1027	1.55%	0.545%
19	14.841	4195	4199	4208	rVB5	518	718	1.08%	0.381%
20	15.896	4524	4527	4532	rVB3	867	762	1.15%	0.404%
21	16.172	4608	4613	4616	rBV4	735	866	1.30%	0.459%
22	16.735	4784	4788	4792	rBV4	815	740	1.11%	0.392%
23	16.806	4806	4810	4812	rBV3	986	850	1.28%	0.451%
24	16.889	4832	4836	4841	rBV5	1148	1407	2.12%	0.746%




Sum of corrected areas: 188554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052782.D
Acq On : 24 Jan 2023 11:03
Operator : JC/MD
Sample : VU0124WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0124WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

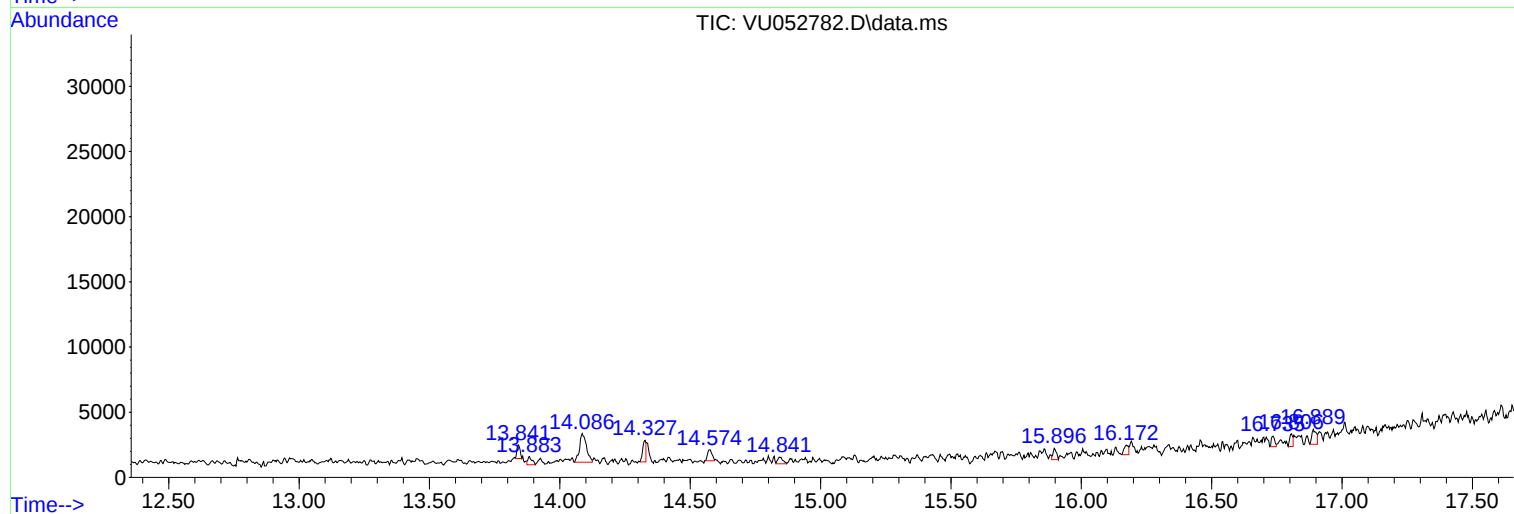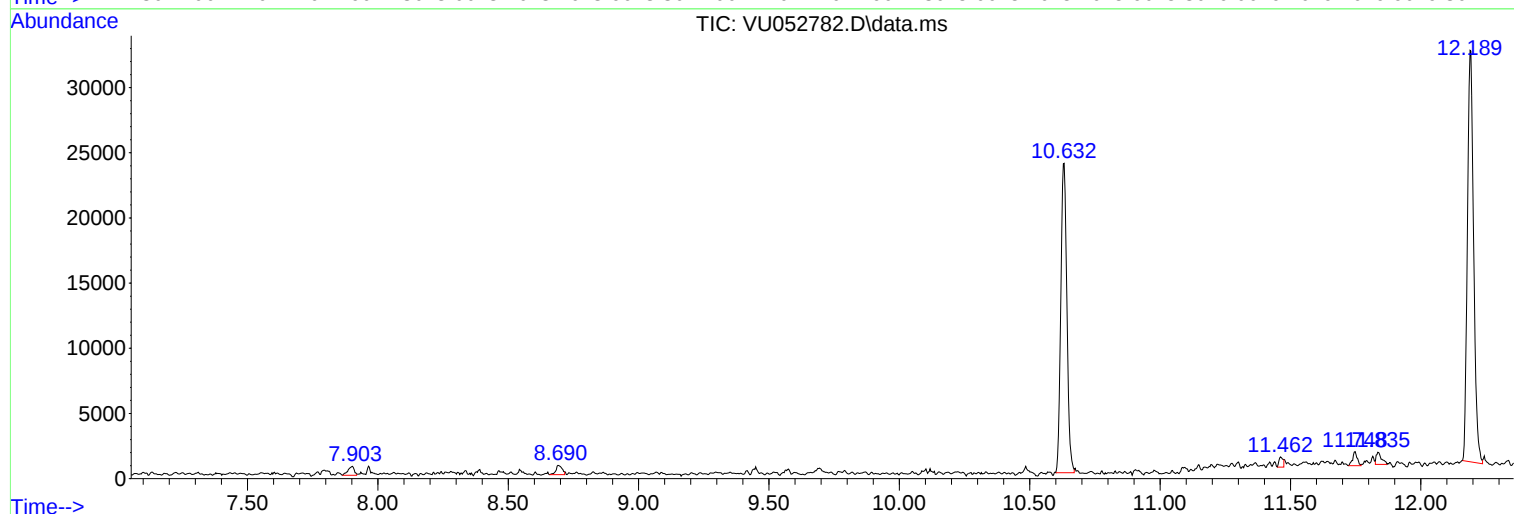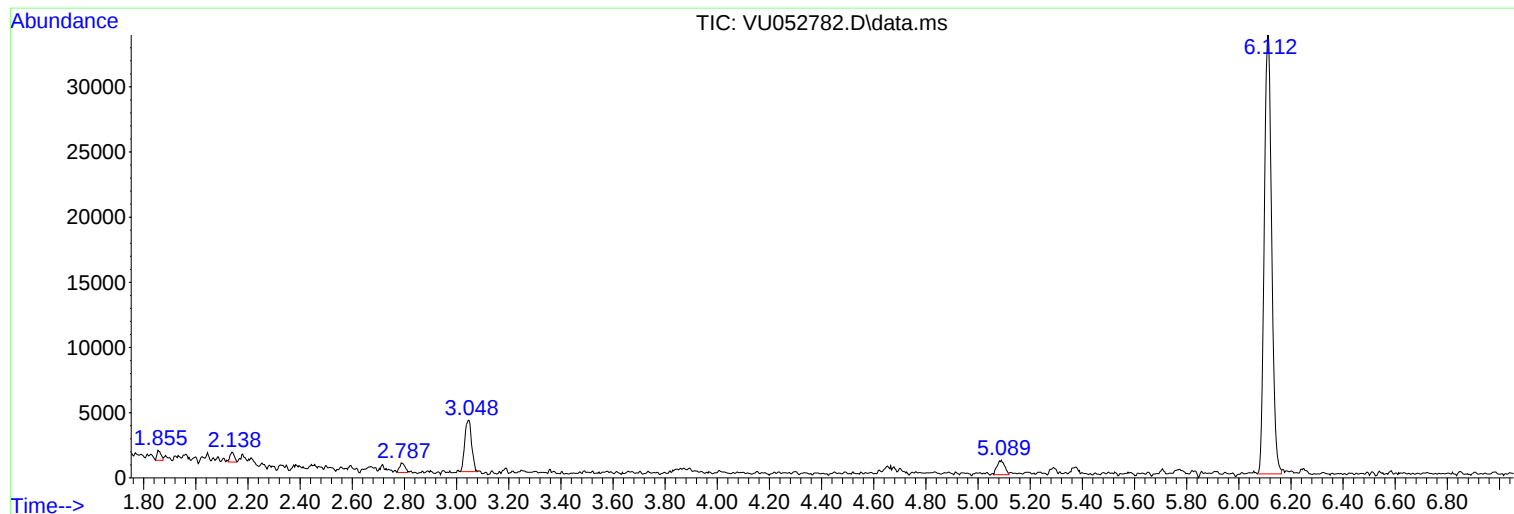

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052782.D
Acq On : 24 Jan 2023 11:03
Operator : JC/MD
Sample : VU0124WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0124WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052782.D
Acq On : 24 Jan 2023 11:03
Operator : JC/MD
Sample : VU0124WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0124WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------