

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
 Data File : VU052791.D
 Acq On : 24 Jan 2023 15:00
 Operator : JC/MD
 Sample : IBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0125

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU052791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.041	520	529	542	rBV2	10512	19575	29.57%	7.779%
2	3.186	561	574	585	rVB2	4452	10765	16.26%	4.278%
3	4.636	1008	1025	1026	rBV2	6316	9582	14.47%	3.808%
4	5.089	1153	1166	1175	rBV2	1718	3145	4.75%	1.250%
5	5.292	1222	1229	1233	rBV2	667	751	1.13%	0.298%
6	5.369	1249	1253	1266	rVB4	744	1270	1.92%	0.505%
7	6.112	1471	1484	1498	rBV	33944	66199	100.00%	26.307%
8	6.259	1520	1530	1534	rVB3	650	943	1.42%	0.375%
9	7.896	2031	2039	2047	rVB3	959	1709	2.58%	0.679%
10	8.922	2348	2358	2368	rVB3	3852	7196	10.87%	2.860%
11	10.629	2877	2889	2906	rBV2	24185	38837	58.67%	15.434%
12	10.819	2938	2948	2959	rBV2	21585	33705	50.91%	13.394%
13	12.188	3364	3374	3389	rBV2	31828	52531	79.35%	20.876%
14	12.996	3618	3625	3631	rVB5	1492	2154	3.25%	0.856%
15	14.571	4107	4115	4116	rBV3	1096	1189	1.80%	0.473%
16	16.526	4720	4723	4730	rVB4	1207	1114	1.68%	0.443%
17	16.571	4730	4737	4739	rBV6	886	973	1.47%	0.387%




Sum of corrected areas: 251638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052791.D
Acq On : 24 Jan 2023 15:00
Operator : JC/MD
Sample : IBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

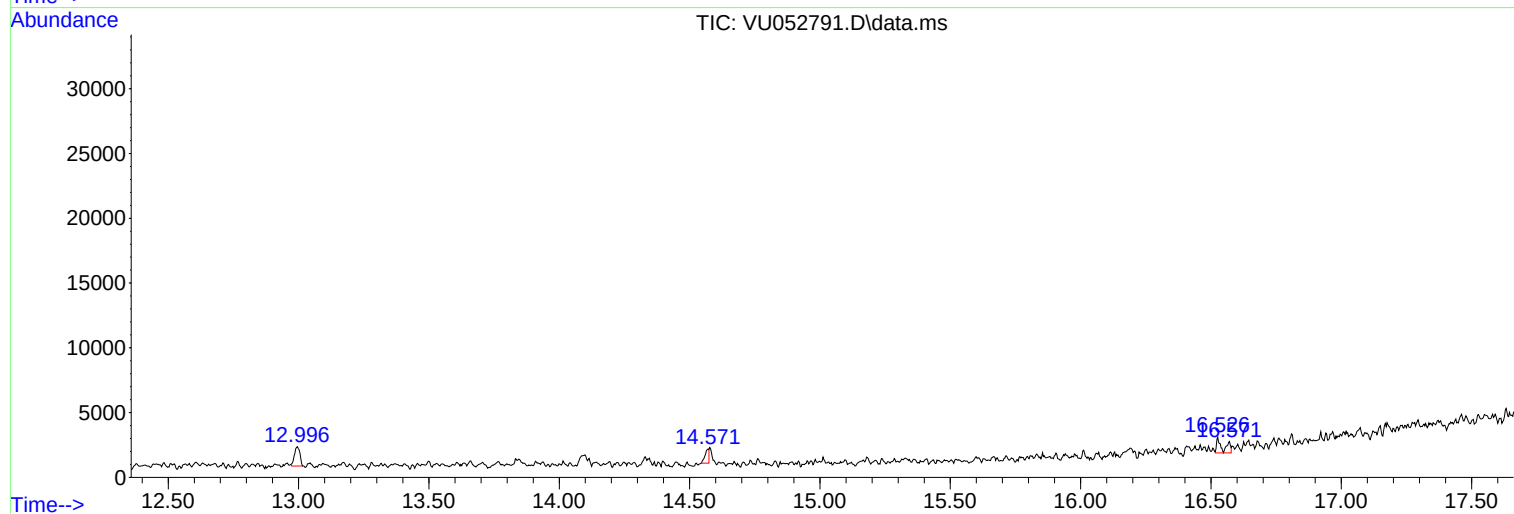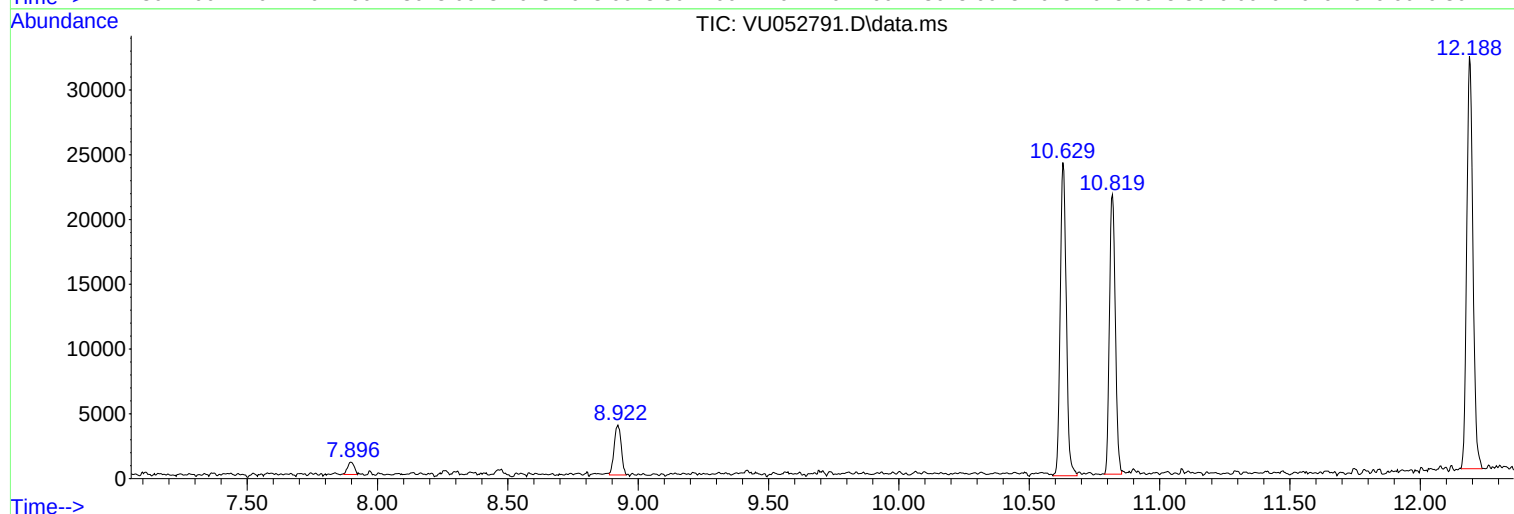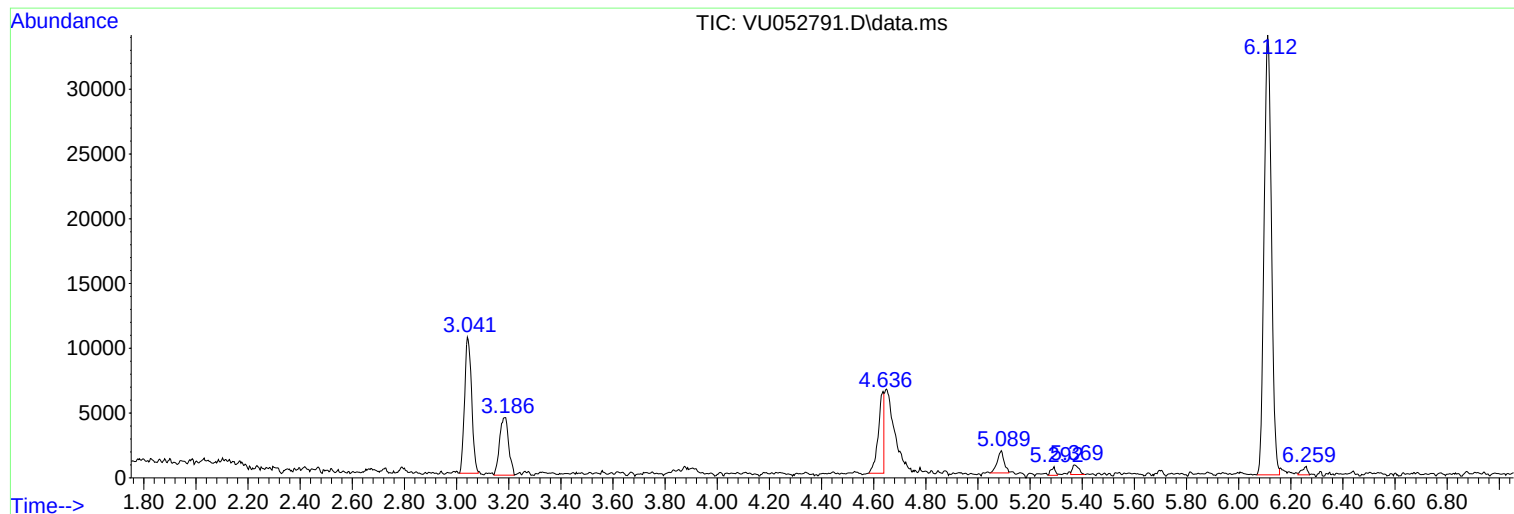

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052791.D
Acq On : 24 Jan 2023 15:00
Operator : JC/MD
Sample : IBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052791.D
Acq On : 24 Jan 2023 15:00
Operator : JC/MD
Sample : IBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0125

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------