

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
 Data File : VU052792.D
 Acq On : 24 Jan 2023 15:27
 Operator : JC/MD
 Sample : 01245-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU052792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.578	371	385	405	rBV	362425	596425	23.94%	3.009%
2	3.044	514	530	558	rBV	283918	548982	22.03%	2.769%
3	3.350	610	625	652	rBV	360542	709827	28.49%	3.581%
4	4.662	998	1033	1066	rBV	306493	706473	28.35%	3.564%
5	5.311	1216	1235	1263	rBV	394738	896882	35.99%	4.524%
6	5.520	1282	1300	1319	rBV	300190	649392	26.06%	3.276%
7	5.774	1362	1379	1413	rBV2	669826	1609876	64.61%	8.121%
8	6.112	1471	1484	1499	rBV	37231	71387	2.86%	0.360%
9	6.539	1603	1617	1638	rBV	458605	854730	34.30%	4.312%
10	6.787	1675	1694	1717	rBV	471241	876986	35.20%	4.424%
11	7.967	2046	2061	2085	rBV	1050500	1732217	69.52%	8.738%
12	8.395	2180	2194	2210	rBV	293868	494742	19.86%	2.496%
13	8.549	2230	2242	2261	rVB	223686	373998	15.01%	1.887%
14	9.443	2505	2520	2543	rBV	687353	1104766	44.34%	5.573%
15	9.565	2545	2558	2578	rBV	686686	1070499	42.96%	5.400%
16	9.690	2584	2597	2615	rBV	782121	1284683	51.56%	6.481%
17	10.102	2710	2725	2760	rBV4	1278420	2491701	100.00%	12.570%
18	10.629	2878	2889	2903	rBV2	35587	56185	2.25%	0.283%
19	11.832	3249	3263	3287	rBV	664925	1033998	41.50%	5.216%
20	12.208	3363	3380	3401	rBV	952012	1567212	62.90%	7.906%
21	13.835	3873	3886	3914	rBV	710345	1092414	43.84%	5.511%




Sum of corrected areas: 19823375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052792.D
Acq On : 24 Jan 2023 15:27
Operator : JC/MD
Sample : 01245-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

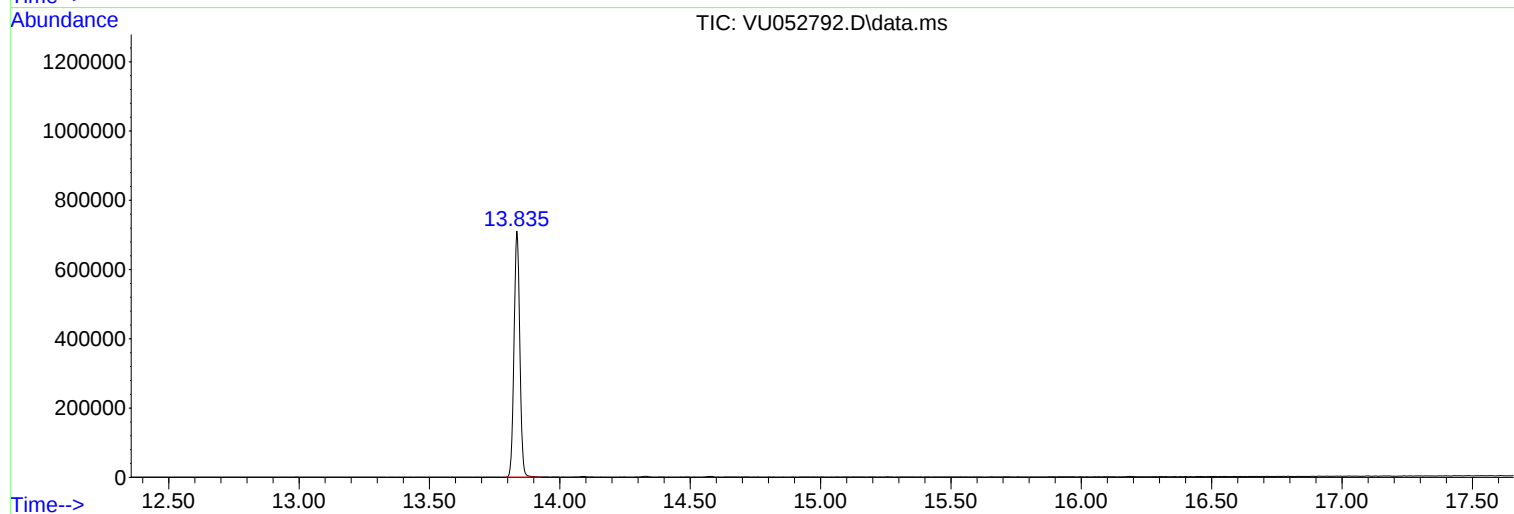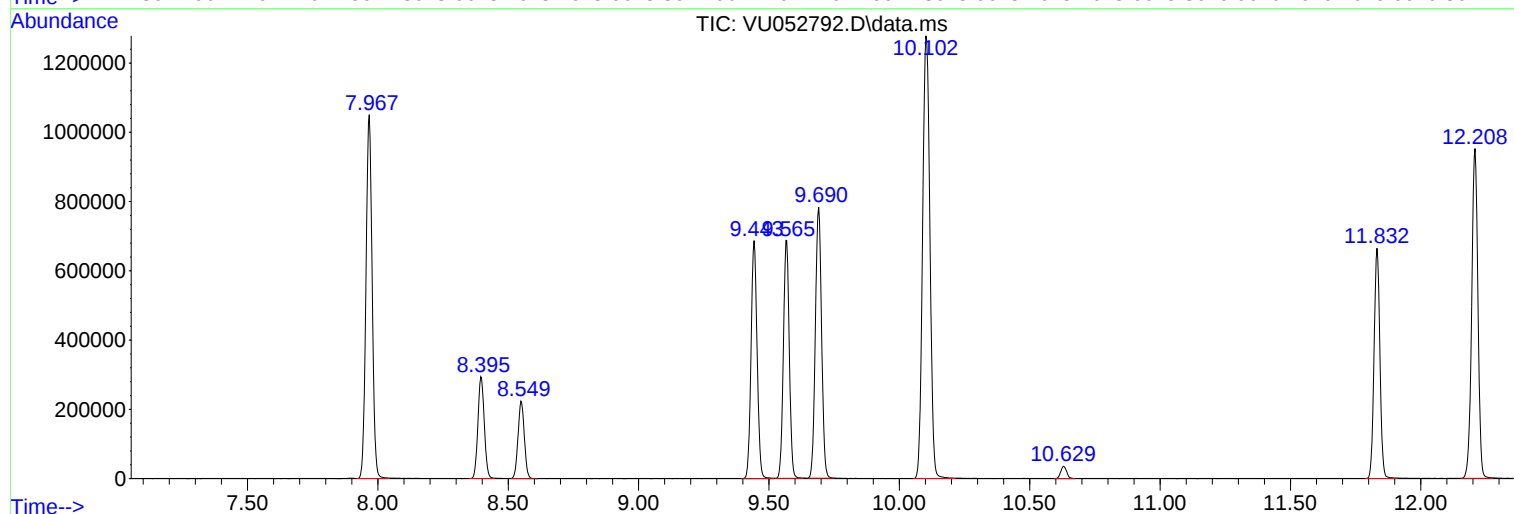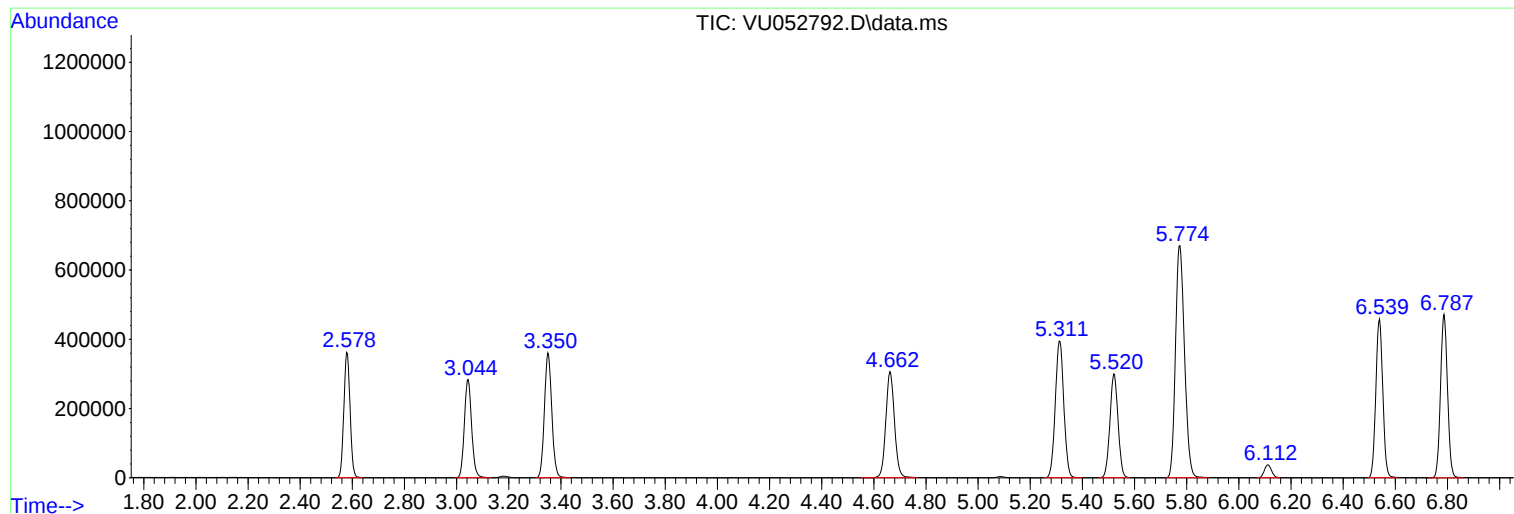

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052792.D
Acq On : 24 Jan 2023 15:27
Operator : JC/MD
Sample : 01245-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052792.D
Acq On : 24 Jan 2023 15:27
Operator : JC/MD
Sample : 01245-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------