


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012423\
Data File : VU052780.D
Acq On : 24 Jan 2023 09:42
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U012323DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jan 24 05:16:59 2023

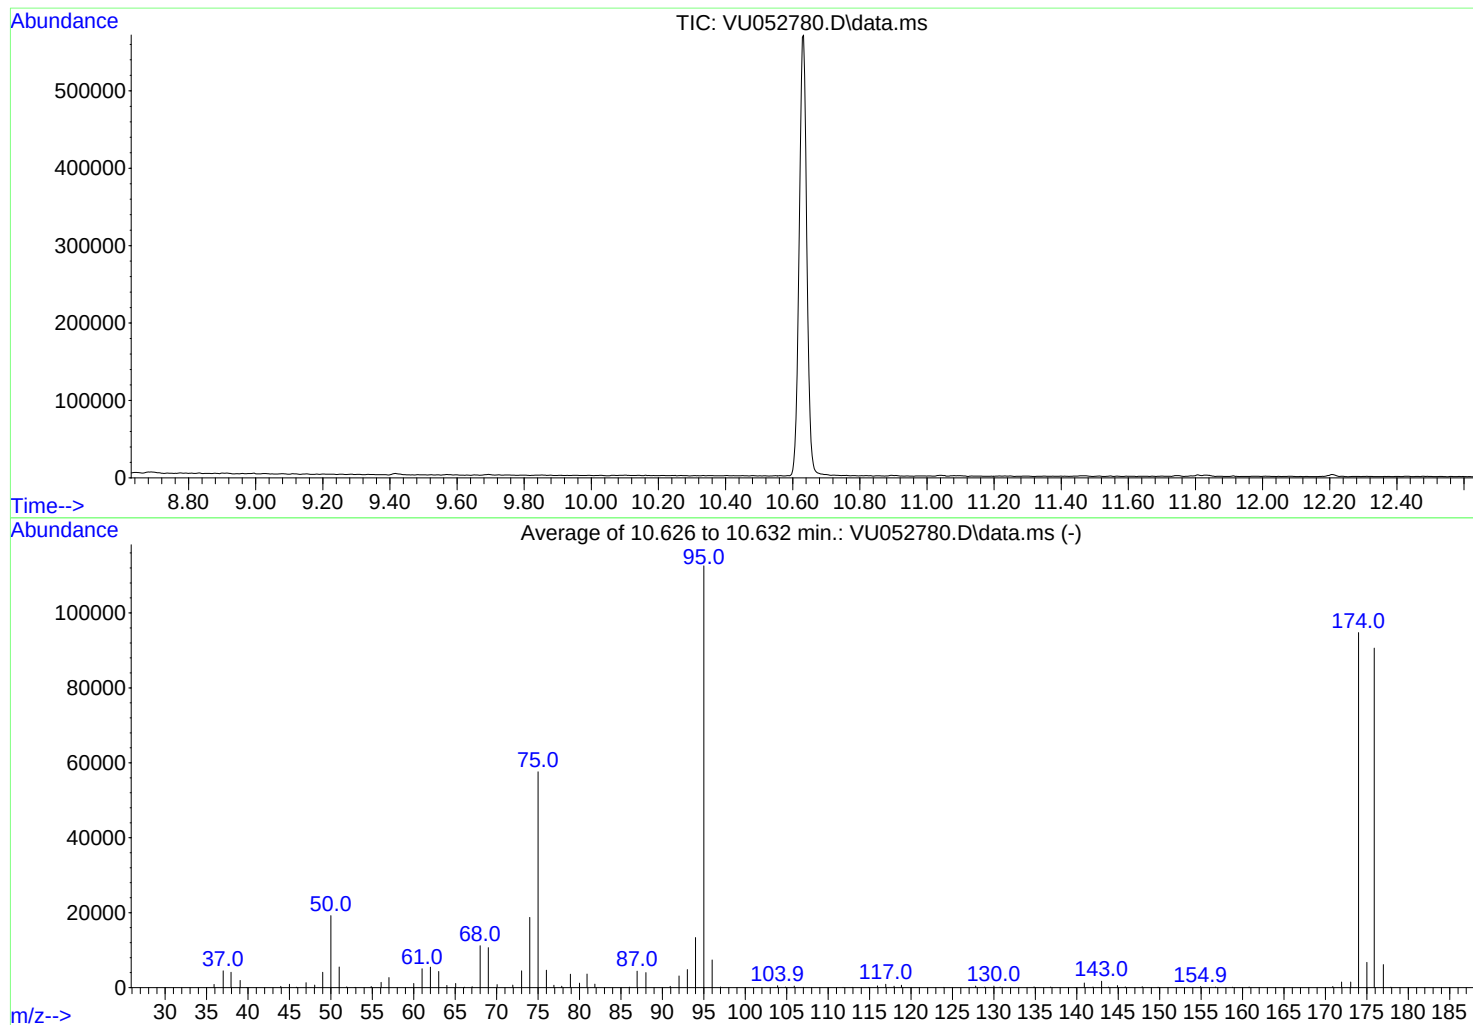

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	19200	PASS
75	95	30	60	51.2	57589	PASS
95	95	100	100	100.0	112568	PASS
96	95	5	9	6.6	7388	PASS
173	174	0.00	2	1.6	1490	PASS
174	95	50	100	84.2	94747	PASS
175	174	5	9	7.1	6766	PASS
176	174	95	101	95.6	90616	PASS
177	176	5	9	6.8	6164	PASS