




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012425\
Data File : VU062998.D
Acq On : 24 Jan 2025 17:17
Operator : MD/SY
Sample : Q1174-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2940

Manual IntegrationsAPPROVED

Quant Time: Jan 24 19:08:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 24 19:02:27 2025
Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2025
Supervised By :Mahesh Dadoda 01/27/2025

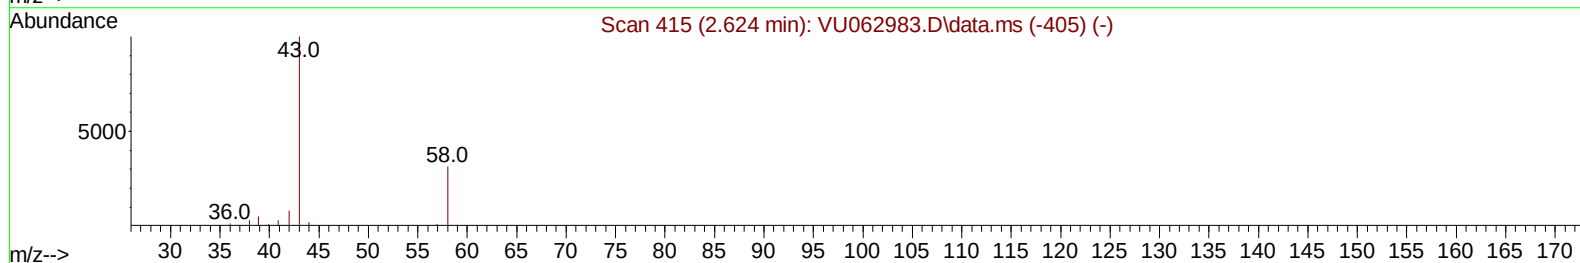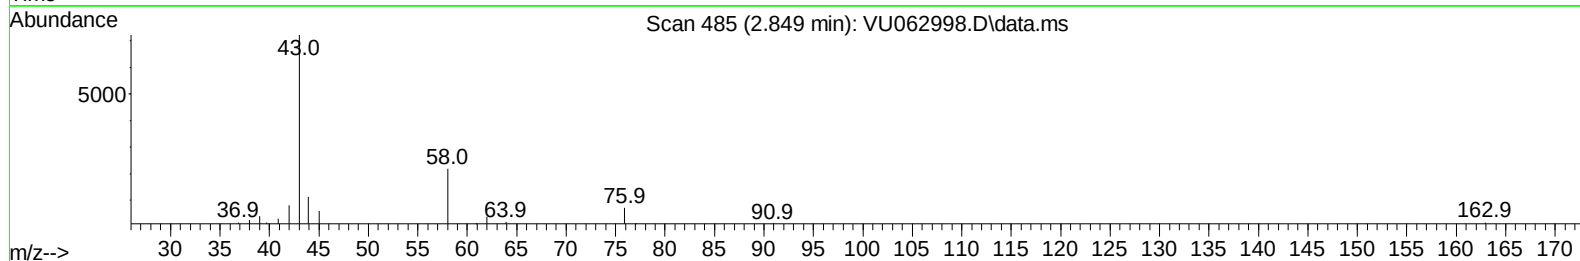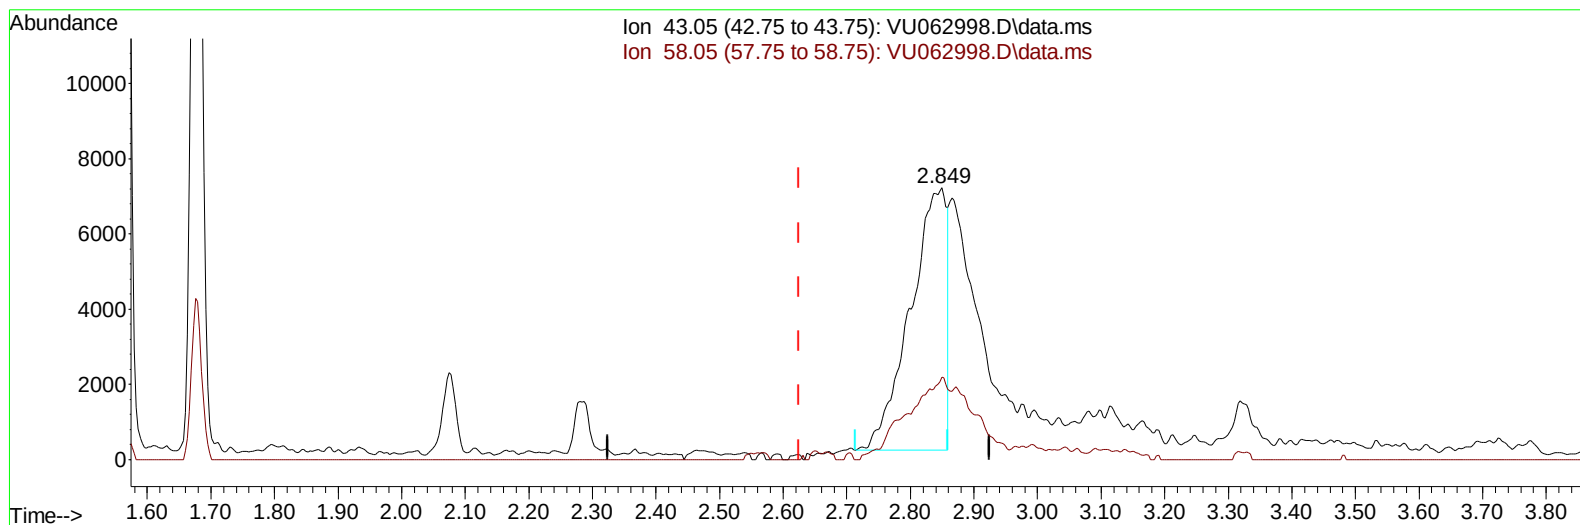

TIC: VU062998.D\data.ms

(13) Acetone (T)

2.849min (+ 0.225) 31.37 ug/L

response 27689

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	36.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012425\
Data File : VU062998.D
Acq On : 24 Jan 2025 17:17
Operator : MD/SY
Sample : Q1174-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2940

Manual IntegrationsAPPROVED

Quant Time: Jan 24 19:08:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 24 19:02:27 2025
Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2025
Supervised By :Mahesh Dadoda 01/27/2025

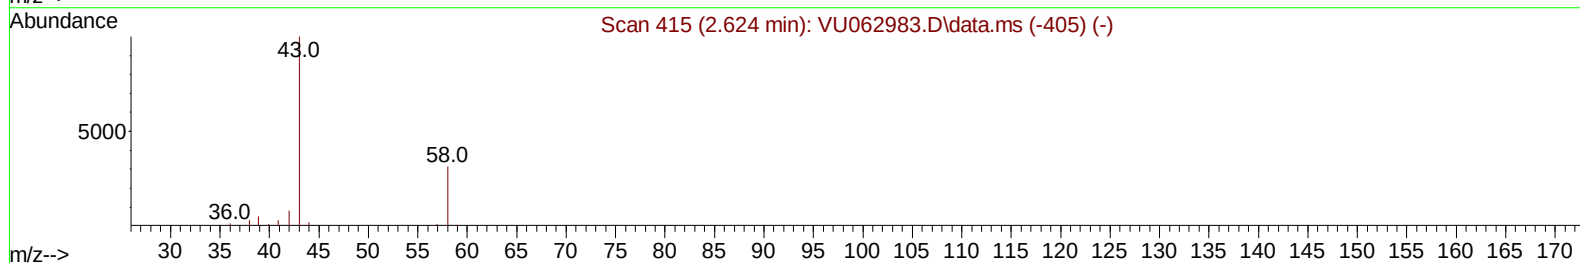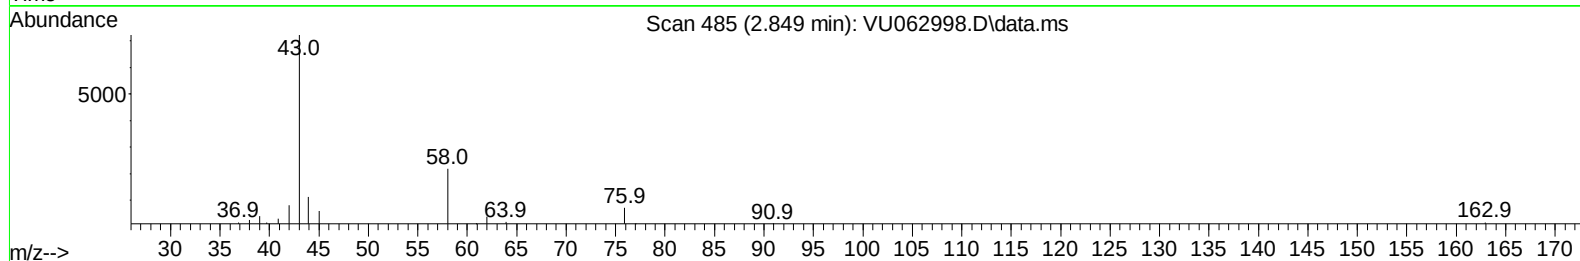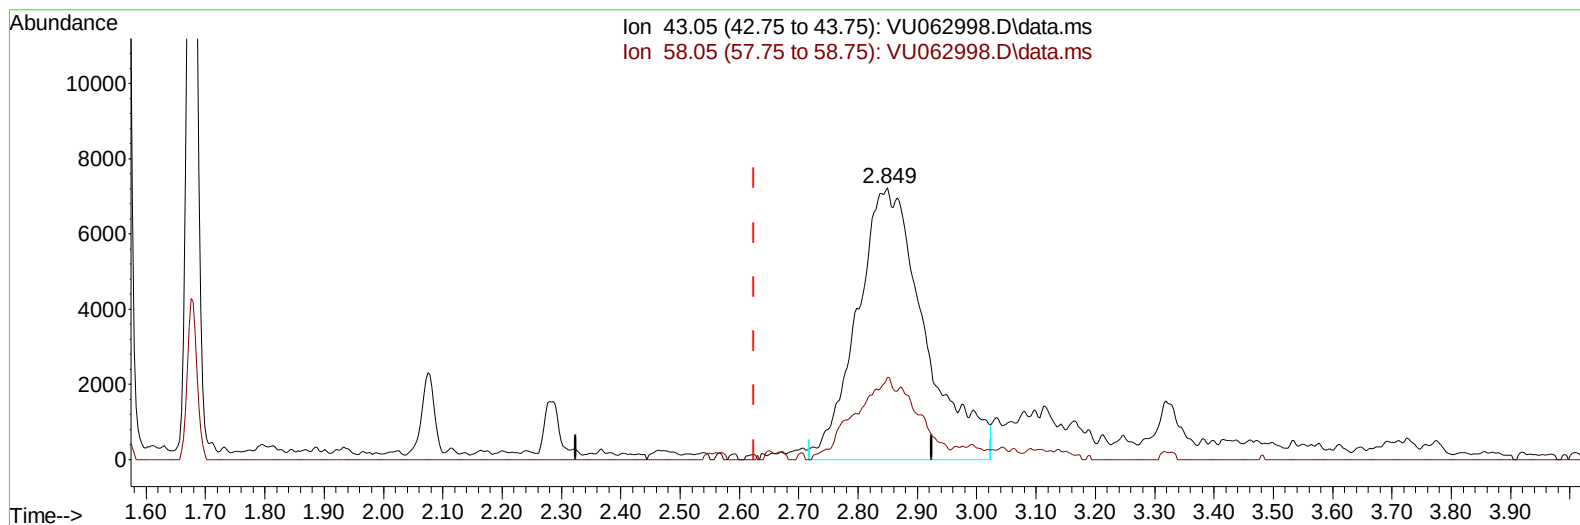

TIC: VU062998.D\data.ms

(13) Acetone (T)

2.849min (+ 0.225) 64.51 ug/L m

response 56945

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	17.75
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012425\
 Data File : VU062998.D
 Acq On : 24 Jan 2025 17:17
 Operator : MD/SY
 Sample : Q1174-10
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2940

Manual IntegrationsAPPROVED

Quant Time: Jan 24 19:08:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jan 24 19:02:27 2025
 Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2025
 Supervised By :Mahesh Dadoda 01/27/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.335	114	98448	5.000	ug/L	0.10
28) Chlorobenzene-d5	9.428	117	91230	5.000	ug/L	0.02
58) 1,4-Dichlorobenzene-d4	11.807	152	45942	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.676	65	28412	5.211	ug/L	0.08
Spiked Amount 5.000	Range 40	- 130	Recovery	=	104.200%	
7) Chloroethane-d5	1.994	69	17953	4.093	ug/L	0.09
Spiked Amount 5.000	Range 65	- 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.653	65	10001	3.541	ug/L	0.10
Spiked Amount 5.000	Range 60	- 125	Recovery	=	70.800%	
20) 2-Butanone-d5	4.782	46	33176	29.771	ug/L	0.17
Spiked Amount 50.000	Range 40	- 130	Recovery	=	59.540%	
24) Chloroform-d	5.113	84	44374	3.308	ug/L	0.06
Spiked Amount 5.000	Range 70	- 125	Recovery	=	66.200%#	
26) 1,2-Dichloroethane-d4	5.788	65	30509	4.193	ug/L	0.10
Spiked Amount 5.000	Range 70	- 130	Recovery	=	83.800%	
32) Benzene-d6	5.808	84	96500	4.327	ug/L	0.09
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.600%	
36) 1,2-Dichloropropane-d6	6.762	67	29470	4.766	ug/L	0.08
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.400%	
41) Toluene-d8	7.933	98	92388	4.252	ug/L	0.05
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	8.209	79	12624	4.096	ug/L	0.04
Spiked Amount 5.000	Range 55	- 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.659	63	40812	42.102	ug/L	0.04
Spiked Amount 50.000	Range 45	- 130	Recovery	=	84.200%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	22864	4.415	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	88.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152	33517	4.385	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	87.800%	
Target Compounds					Qvalue	
13) Acetone	2.849	43	56945m	64.506	ug/L	
14) Carbon disulfide	2.875	76	18537	0.950	ug/L	97
16) Methylene chloride	3.139	84	51019	7.621	ug/L	93
19) 1,1-Dichloroethane	3.962	63	87975	7.515	ug/L	96
21) 2-Butanone	4.853	43	26869	22.854	ug/L	94
33) Benzene	5.859	78	71241	2.718	ug/L	100
40) 4-Methyl-2-pentanone	7.840	43	27915	9.665	ug/L	94
42) Toluene	8.004	91	203731	7.093	ug/L	100
52) Ethylbenzene	9.579	91	80510	2.470	ug/L	100
53) m,p-Xylene	9.701	106	50343	4.130	ug/L	95
54) o-Xylene	10.103	106	28652	2.454	ug/L	90
55) Styrene	10.119	104	59348	3.039	ug/L	95
62) 1,3,5-Trimethylbenzene	11.087	105	9394	0.349	ug/L	95
63) 1,2,4-Trimethylbenzene	11.463	105	25035	0.962	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012425\
Data File : VU062998.D
Acq On : 24 Jan 2025 17:17
Operator : MD/SY
Sample : Q1174-10
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2940

Manual IntegrationsAPPROVED

Quant Time: Jan 24 19:08:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jan 24 19:02:27 2025
Response via : Initial Calibration

Reviewed By :John Carlone 01/27/2025
Supervised By :Mahesh Dadoda 01/27/2025

