
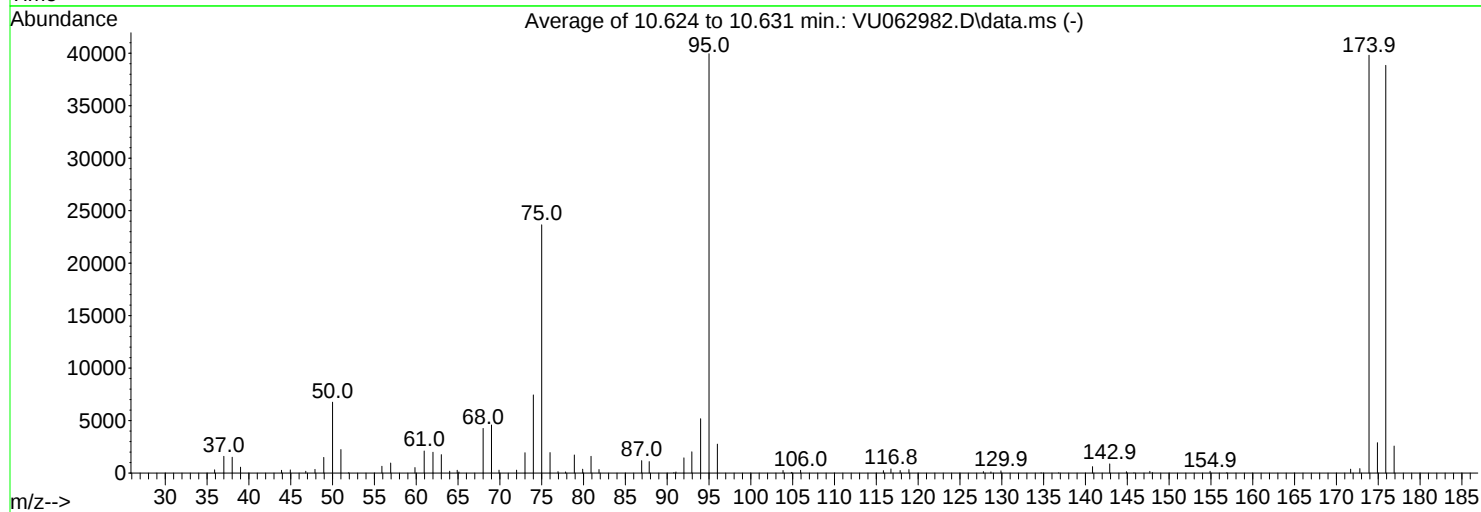


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012425\
Data File : VU062982.D
Acq On : 24 Jan 2025 08:31
Operator : MD/SY
Sample : BFB067
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB067

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR010225WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jan 24 19:02:27 2025

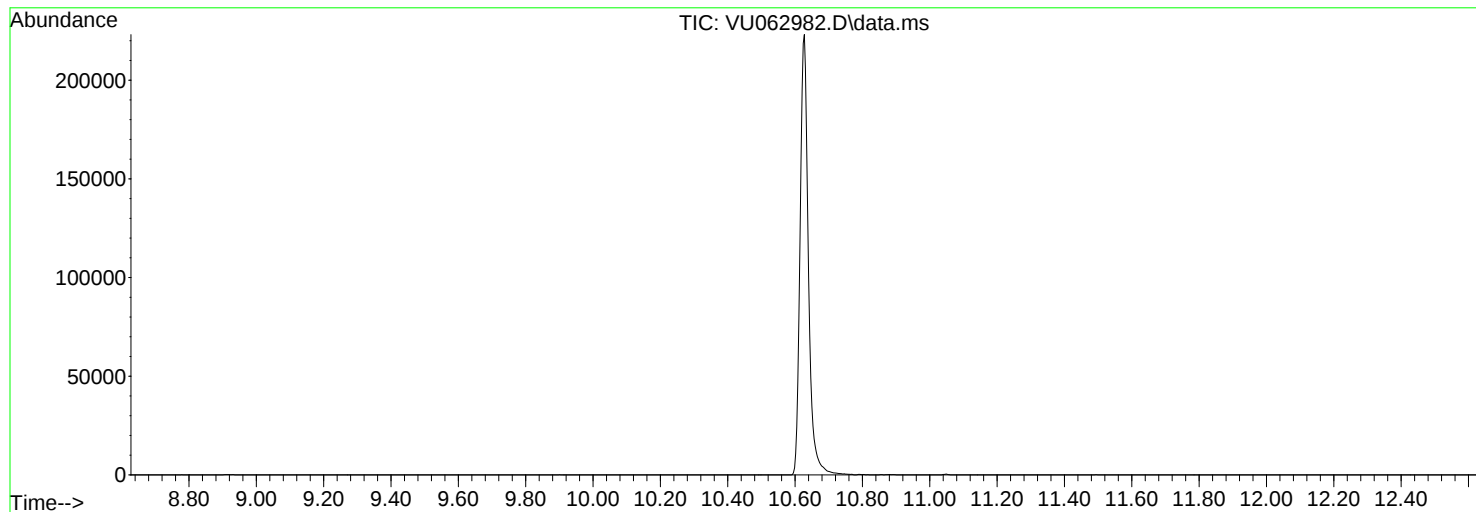

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	6754	PASS
75	95	30	80	59.2	23653	PASS
95	95	100	100	100.0	39952	PASS
96	95	5	9	6.9	2756	PASS
173	174	0.00	2	1.1	425	PASS
174	95	50	120	99.6	39811	PASS
175	174	5	9	7.3	2895	PASS
176	174	95	101	97.6	38845	PASS
177	176	5	9	6.6	2575	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB067

m/z	Abundance
35.90	340.0
37.00	1600.0
38.00	1522.0
39.00	602.0
43.90	292.0
44.90	279.0
46.80	193.0
47.90	392.0
49.00	1435.0
50.00	6897.0
51.00	2323.0
51.90	105.0
55.90	670.0
57.00	987.0
59.90	553.0
61.00	2241.0
62.00	2120.0
63.00	1696.0
63.90	181.0
64.90	272.0
68.00	4392.0
69.00	4662.0
69.90	298.0
72.00	242.0
73.00	2008.0
74.00	7627.0
75.00	24296.0
76.00	2066.0
77.00	152.0
78.00	110.0
78.90	1688.0
79.90	378.0
80.90	1648.0
81.80	342.0
86.90	1265.0
87.90	1185.0
90.80	160.0
92.00	1441.0
92.90	2046.0
94.00	5198.0
95.00	41016.0
96.00	2773.0
103.80	263.0
104.80	101.0
106.00	282.0
115.90	273.0
116.70	376.0
117.90	280.0
118.90	295.0
127.80	145.0
128.70	120.0
129.90	228.0
136.80	105.0
140.90	592.0
142.90	858.0
144.80	165.0
145.80	101.0
147.70	141.0
148.00	142.0
154.90	153.0
156.90	127.0
171.70	343.0
172.80	456.0
173.90	39832.0
174.90	2875.0
175.90	38120.0
176.90	2550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	324.0
37.00	1645.0
38.00	1602.0
39.00	578.0
43.90	291.0
44.90	323.0
46.80	196.0
47.90	356.0
48.90	1583.0
50.00	6877.0
51.00	2302.0
55.90	646.0
57.00	996.0
59.80	559.0
60.90	2167.0
62.00	2039.0
63.00	1826.0
64.00	156.0
64.80	267.0
65.00	268.0
68.00	4386.0
69.00	4702.0
69.90	295.0
72.00	289.0
73.00	1988.0
74.00	7671.0
75.00	24384.0
76.00	2019.0
77.00	136.0
77.80	115.0
78.90	1806.0
79.90	373.0
80.90	1643.0
81.90	334.0
87.00	1214.0
87.90	1134.0
91.00	152.0
92.00	1516.0
92.90	2078.0
94.00	5398.0
95.00	41144.0
96.00	2866.0
103.80	269.0
104.90	104.0
105.90	270.0
115.80	237.0
116.80	407.0
117.90	252.0
118.90	349.0
127.80	134.0
128.70	121.0
129.90	220.0
134.70	105.0
140.80	639.0
142.90	914.0
144.90	139.0
147.70	189.0
154.90	189.0
171.70	394.0
172.80	424.0
173.90	41208.0
174.90	3018.0
175.90	40168.0
176.90	2672.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	271.0
37.00	1537.0
38.00	1406.0
39.00	513.0
43.90	217.0
45.00	302.0
46.80	143.0
47.90	305.0
48.90	1456.0
50.00	6488.0
51.00	2099.0
55.90	631.0
56.90	881.0
59.80	472.0
60.90	1899.0
62.00	1801.0
63.00	1739.0
64.10	196.0
65.10	312.0
68.00	3980.0
69.00	4386.0
69.90	249.0
72.00	310.0
73.00	1826.0
74.00	7035.0
75.00	22280.0
76.00	1781.0
76.90	130.0
77.80	115.0
78.90	1675.0
79.90	364.0
80.90	1499.0
81.90	340.0
87.00	1077.0
87.80	965.0
91.10	164.0
92.00	1397.0
93.00	1964.0
94.00	4940.0
95.00	37696.0
96.00	2629.0
103.90	212.0
105.90	249.0
115.80	191.0
116.80	401.0
117.80	208.0
118.90	352.0
127.80	147.0
128.70	101.0
129.90	190.0
140.90	609.0
142.90	848.0
145.00	101.0
147.70	172.0
154.90	190.0
171.70	373.0
172.80	394.0
173.90	38392.0
174.90	2793.0
175.90	38248.0
176.90	2504.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067