


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU012519\
Data File : VU029277.D
Acq On : 25 Jan 2019 09:37
Operator : JC/SP
Sample : BFB42
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012519WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jan 28 02:17:15 2019

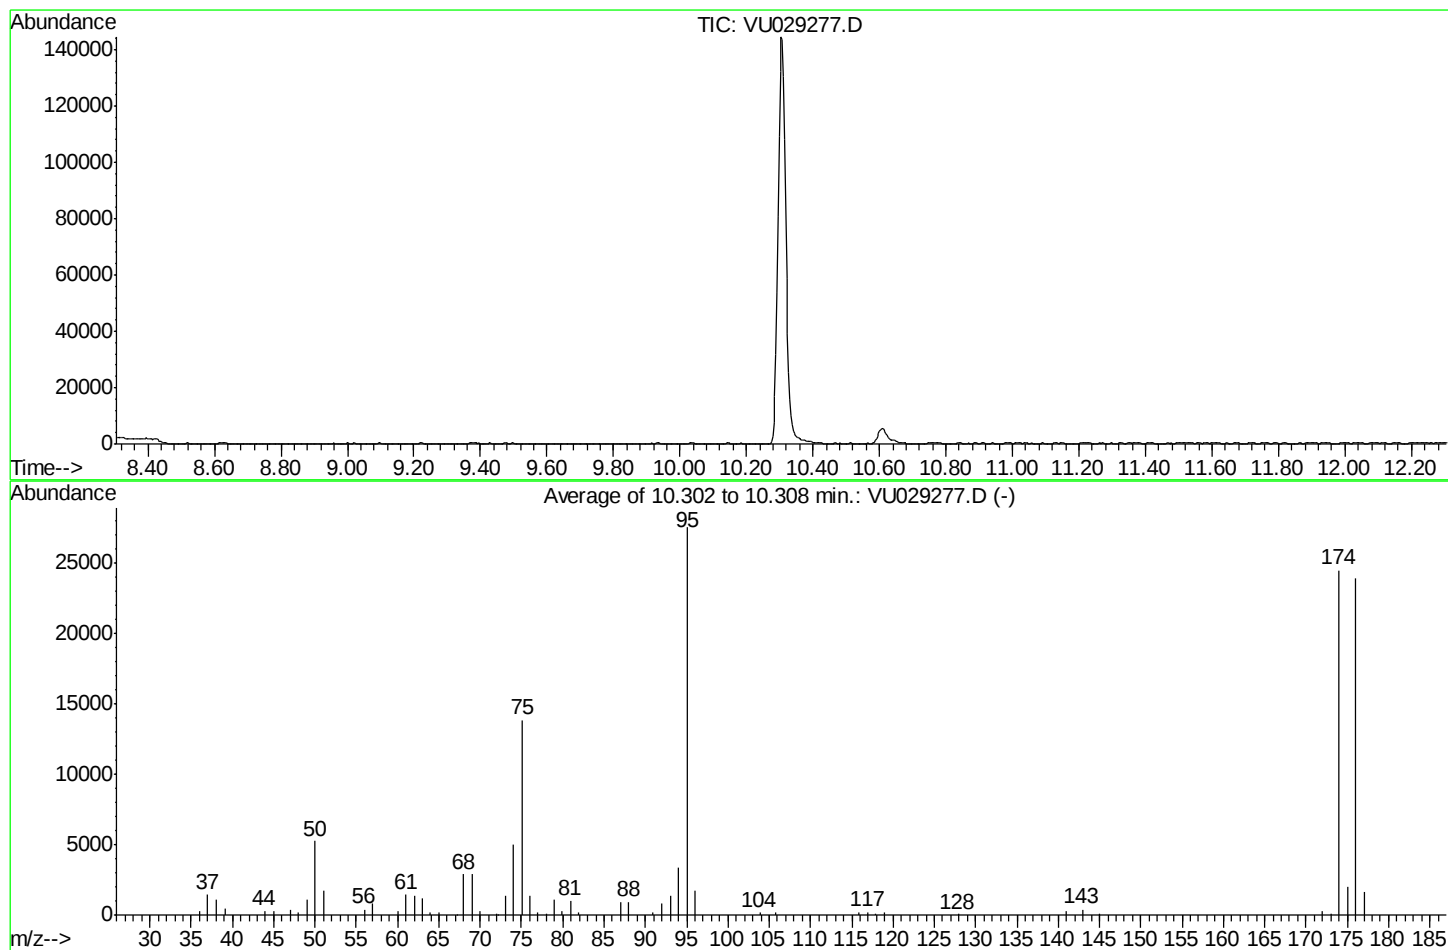

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	5259	PASS
75	95	30	80	50.4	13846	PASS
95	95	100	100	100.0	27498	PASS
96	95	5	9	6.3	1743	PASS
173	174	0.00	2	0.5	133	PASS
174	95	50	120	88.9	24445	PASS
175	174	5	9	8.1	1989	PASS
176	174	95	101	97.6	23853	PASS
177	176	5	9	6.8	1631	PASS

m/z	Abundance
43.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	245.0
37.00	1305.0
38.00	1050.0
39.10	419.0
43.90	451.0
45.10	217.0
47.10	335.0
48.00	176.0
49.00	1095.0
50.00	5093.0
51.00	1637.0
55.90	319.0
57.00	764.0
60.00	322.0
61.00	1420.0
62.00	1296.0
63.00	1099.0
64.00	208.0
65.00	188.0
68.00	2671.0
69.00	2781.0
69.90	221.0
72.00	165.0
73.00	1413.0
74.00	4826.0
75.10	13151.0
76.00	1377.0
76.90	166.0
78.00	126.0
78.90	1029.0
80.00	245.0
80.90	1032.0
81.90	227.0
87.10	889.0
88.00	940.0
90.90	144.0
92.00	751.0
93.00	1284.0
94.00	3197.0
95.10	26016.0
96.00	1621.0
103.90	162.0
105.80	135.0
115.90	136.0
117.00	191.0
117.80	105.0
118.90	153.0
140.90	267.0
142.90	306.0
144.90	131.0
172.00	259.0
173.00	400.0
174.00	22520.0
175.00	1891.0
176.00	22088.0
177.00	1579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	275.0
37.00	1485.0
38.00	1091.0
39.10	466.0
43.90	484.0
45.00	254.0
47.10	373.0
48.00	207.0
49.00	1096.0
50.00	5423.0
51.00	1759.0
56.00	402.0
57.00	797.0
60.00	329.0
61.00	1447.0
62.00	1450.0
63.00	1202.0
64.00	202.0
65.00	230.0
67.10	106.0
68.00	2963.0
69.10	2948.0
70.00	249.0
72.00	143.0
73.10	1457.0
74.00	5145.0
75.10	14244.0
76.00	1428.0
76.90	205.0
77.90	108.0
78.90	1133.0
79.90	265.0
80.90	1069.0
81.90	219.0
87.00	922.0
88.00	973.0
90.90	167.0
92.00	813.0
93.00	1446.0
94.00	3445.0
95.10	28392.0
96.10	1791.0
103.90	184.0
105.80	162.0
115.90	155.0
117.00	217.0
117.80	125.0
118.90	151.0
127.90	103.0
140.90	292.0
142.90	411.0
145.00	124.0
172.00	305.0
174.00	25216.0
175.00	2046.0
176.00	24736.0
177.00	1654.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
35.90	271.0
37.00	1483.0
38.00	1098.0
39.00	501.0
43.90	415.0
45.00	260.0
47.00	336.0
48.00	192.0
49.00	1073.0
50.00	5262.0
51.00	1754.0
56.00	461.0
57.00	774.0
60.00	297.0
61.00	1414.0
62.00	1436.0
63.00	1260.0
63.90	153.0
65.10	271.0
68.00	3067.0
69.10	2869.0
70.10	232.0
72.20	137.0
73.10	1343.0
74.00	4967.0
75.10	14145.0
76.00	1302.0
77.00	203.0
79.00	1187.0
79.90	272.0
80.90	1032.0
81.90	212.0
86.90	976.0
88.00	940.0
90.90	178.0
92.00	795.0
93.00	1445.0
94.00	3355.0
95.10	28088.0
96.10	1818.0
103.90	178.0
105.80	163.0
115.90	170.0
117.00	199.0
117.80	127.0
118.90	137.0
127.90	121.0
140.90	282.0
143.00	463.0
172.00	347.0
174.00	25600.0
175.00	2032.0
176.00	24736.0
177.00	1662.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42