

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012521\
 Data File : VU042192.D
 Acq On : 25 Jan 2021 13:28
 Operator : SY/MD
 Sample : VU0125WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK125

Quant Time: Jan 25 17:13:16 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jan 25 17:02:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	104617	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	98761	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.822	152	50280	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	25813	4.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.20%
7) Chloroethane-d5	1.919	69	22650	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.572	65	14656	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.20%
20) 2-Butanone-d5	4.645	46	103888	42.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.34%
24) Chloroform-d	5.073	84	65179	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
26) 1,2-Dichloroethane-d4	5.710	65	40571	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	5.735	84	120640	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	6.700	67	40008	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.906	98	114136	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
43) trans-1,3-Dichloroprop...	8.189	79	19310	4.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.00%
46) 2-Hexanone-d5	8.645	63	89684	51.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.96%
56) 1,1,2,2-Tetrachloroeth...	10.767	84	34806	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.20%
66) 1,2-Dichlorobenzene-d4	12.201	152	44964	5.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.60%
Target Compounds						Qvalue
16) Methylene chloride	3.057	84	1146	0.14	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012521\
Data File : VU042192.D
Acq On : 25 Jan 2021 13:28
Operator : SY/MD
Sample : VU0125WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK125


Quant Time: Jan 25 17:13:16 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jan 25 17:02:55 2021
Response via : Initial Calibration

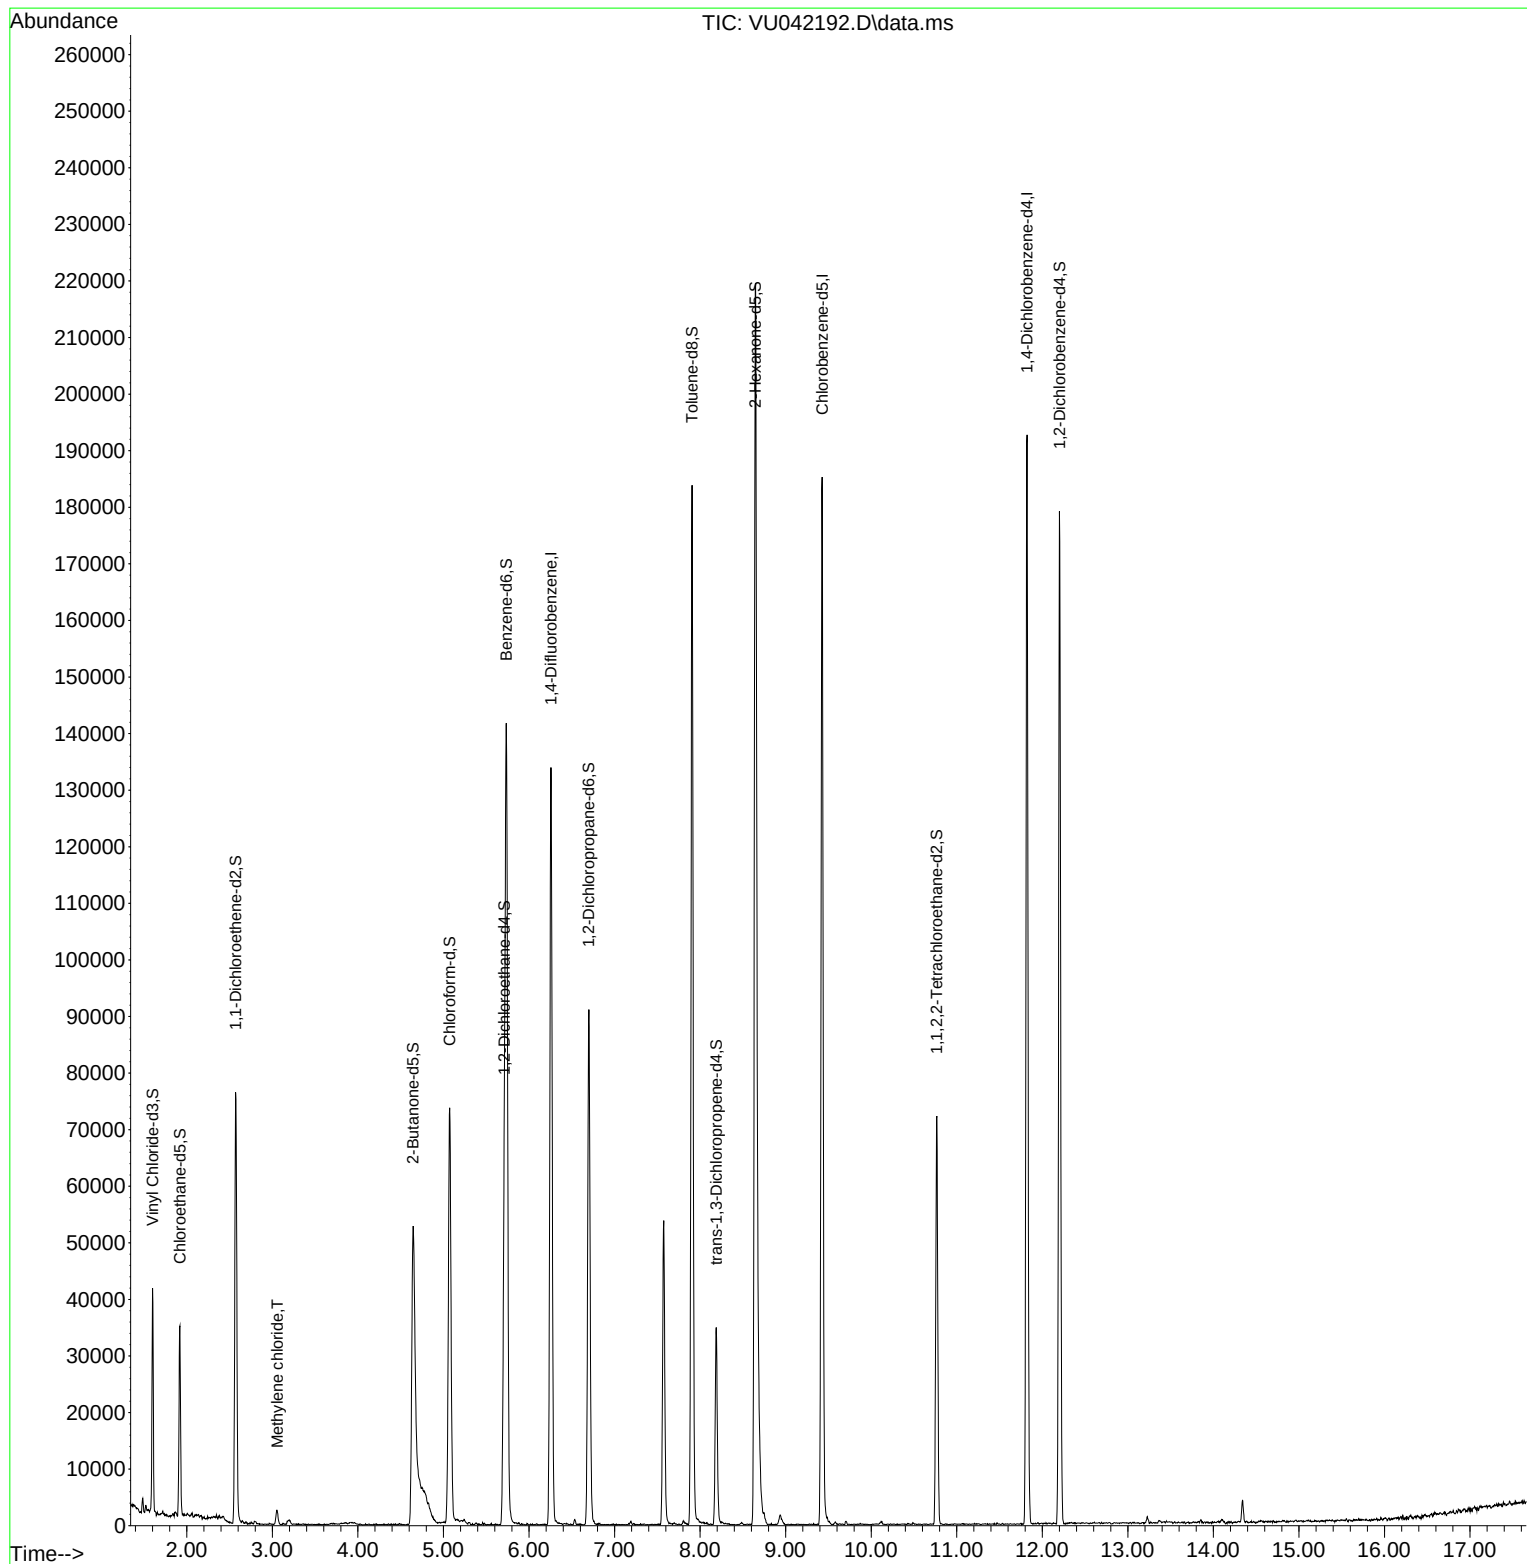

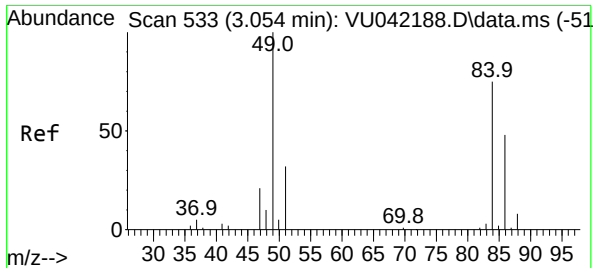

#16
Methylene chloride
Concen: 0.14 ug/L
RT: 3.057 min Scan# 534
Delta R.T. 0.003 min
Lab File: VU042192.D
Acq: 25 Jan 2021 13:28

Instrument :
MSVOA_U
ClientSampleId :
VBLK125

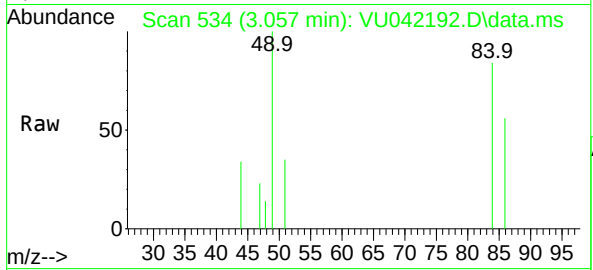

Tgt Ion:	84	Resp:	1146
Ion	Ratio	Lower	Upper
84	100		
86	67.2	44.9	83.5
49	119.4	79.0	146.8

