
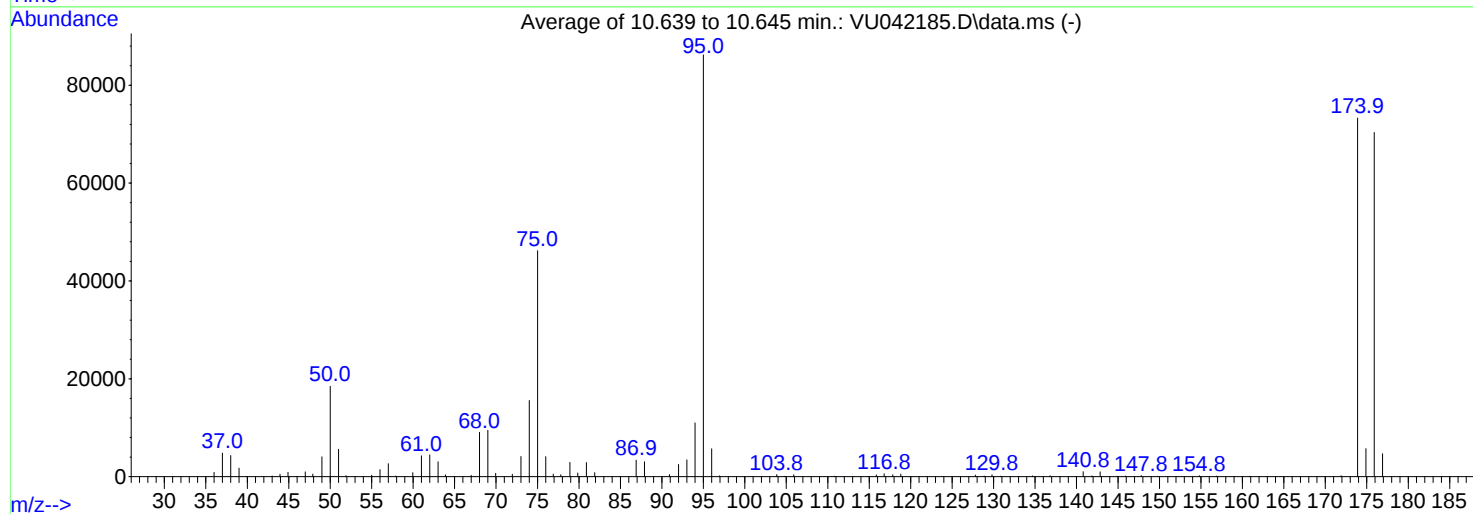


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012521\
 Data File : VU042185.D
 Acq On : 25 Jan 2021 09:08
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB382

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jan 25 17:02:55 2021

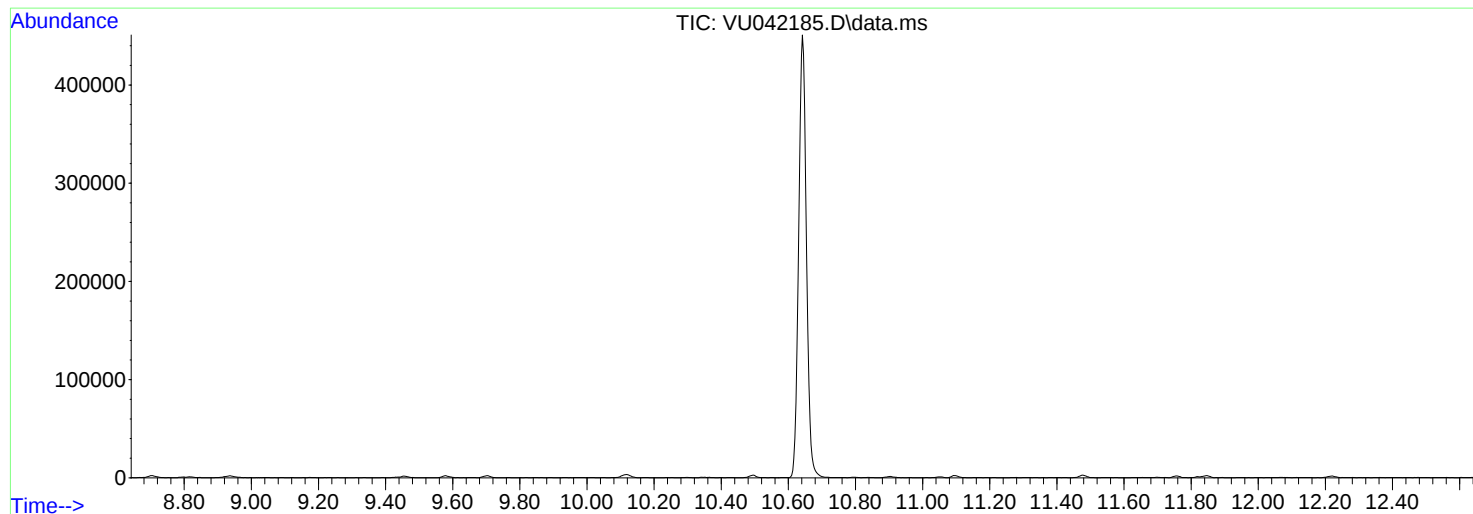

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	18493	PASS
75	95	30	80	53.6	46192	PASS
95	95	100	100	100.0	86219	PASS
96	95	5	9	6.6	5703	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.0	73291	PASS
175	174	5	9	7.8	5712	PASS
176	174	95	101	96.0	70360	PASS
177	176	5	9	6.7	4683	PASS

m/z	Abundance
36.00	968.0
37.00	4916.0
38.00	4252.0
39.00	1726.0
39.90	161.0
43.00	122.0
44.00	725.0
44.90	901.0
45.90	111.0
47.00	977.0
47.90	605.0
49.00	4053.0
50.00	18680.0
51.00	5718.0
51.90	215.0
55.00	295.0
56.00	1370.0
57.00	2696.0
57.90	104.0
59.90	813.0
61.00	4375.0
62.00	4431.0
63.00	3031.0
63.90	364.0
67.00	307.0
68.00	9330.0
69.00	9310.0
70.00	754.0
71.90	504.0
73.00	4109.0
74.00	15360.0
75.00	45936.0
76.00	4007.0
76.90	554.0
77.80	344.0
78.90	2879.0
79.90	731.0
80.90	2984.0
81.90	787.0
86.90	3374.0
87.90	3117.0
90.90	399.0
92.00	2457.0
93.00	3477.0
94.00	11145.0
95.00	84744.0
96.00	5870.0
96.90	174.0
103.80	405.0
105.90	398.0
110.80	113.0
115.90	393.0
116.80	556.0
117.80	384.0
118.80	512.0
127.80	311.0
128.90	130.0
129.80	373.0
130.90	109.0
134.70	162.0
136.80	156.0
140.80	938.0
141.80	176.0
142.90	992.0
144.90	108.0
145.90	131.0
147.80	222.0
149.80	102.0
154.80	188.0
156.80	119.0
172.00	181.0
173.90	70360.0
174.90	5497.0
175.90	66576.0
176.90	4553.0

Instrument :
MSVOA_U
ClientSampleId :
BFB382

m/z	Abundance
36.00	941.0
37.00	4947.0
38.00	4500.0
39.00	1802.0
39.90	183.0
43.00	132.0
43.90	757.0
44.90	943.0
45.90	124.0
47.00	1027.0
47.90	540.0
49.00	4243.0
50.00	19112.0
51.00	5783.0
51.90	188.0
55.00	324.0
56.00	1507.0
57.00	2747.0
57.90	139.0
60.00	842.0
61.00	4399.0
62.00	4627.0
63.00	3164.0
63.90	362.0
67.00	290.0
68.00	9362.0
69.00	9791.0
70.00	702.0
71.90	510.0
73.00	4254.0
74.00	16025.0
75.00	47608.0
76.00	4292.0
76.90	558.0
77.80	440.0
78.90	2993.0
79.80	772.0
80.90	2946.0
81.90	864.0
86.90	3485.0
87.90	3091.0
90.90	446.0
92.00	2590.0
93.00	3470.0
94.00	11321.0
95.00	88832.0
96.00	5898.0
97.00	178.0
103.90	442.0
104.80	106.0
105.90	425.0
110.80	119.0
114.80	103.0
115.90	379.0
116.80	616.0
117.80	388.0
118.80	535.0
127.80	326.0
128.80	150.0
129.80	409.0
130.90	107.0
134.70	163.0
136.80	202.0
140.80	1049.0
141.90	178.0
142.90	1035.0
144.90	120.0
145.90	150.0
147.80	230.0
149.80	100.0
154.80	212.0
156.90	124.0
160.90	111.0
171.80	204.0
173.90	75568.0
174.90	5903.0
175.90	72528.0
176.90	4852.0

Instrument :
MSVOA_U
ClientSampleId :
BFB382

m/z	Abundance
36.00	785.0
37.00	4526.0
38.00	4187.0
39.00	1707.0
39.90	184.0
43.00	106.0
43.90	766.0
44.90	837.0
47.00	979.0
47.90	484.0
49.00	3917.0
50.00	17688.0
51.00	5294.0
51.90	168.0
55.00	307.0
56.00	1437.0
57.00	2489.0
57.90	148.0
60.00	810.0
61.00	4038.0
62.00	4312.0
63.00	2976.0
63.90	354.0
67.00	219.0
68.00	8482.0
69.00	9319.0
69.90	635.0
72.00	501.0
73.00	3961.0
74.00	15331.0
75.00	45032.0
76.00	4012.0
76.90	507.0
77.80	445.0
78.90	2920.0
79.90	741.0
80.90	2718.0
81.90	802.0
86.90	3213.0
87.90	2886.0
90.90	434.0
92.00	2445.0
93.00	3324.0
94.00	10526.0
95.00	85080.0
96.00	5342.0
96.90	179.0
103.90	478.0
104.80	113.0
105.90	410.0
110.80	104.0
115.80	358.0
116.80	572.0
117.90	370.0
118.80	482.0
127.80	333.0
128.80	154.0
129.80	399.0
130.80	102.0
134.70	132.0
136.80	223.0
140.80	1018.0
141.90	162.0
142.80	935.0
144.90	107.0
145.90	138.0
147.80	228.0
154.80	211.0
156.80	128.0
160.80	103.0
171.90	227.0
173.90	73944.0
174.90	5735.0
175.90	71976.0
176.90	4644.0
177.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB382

m/z	Abundance
39.90	102.0
44.00	258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB382