
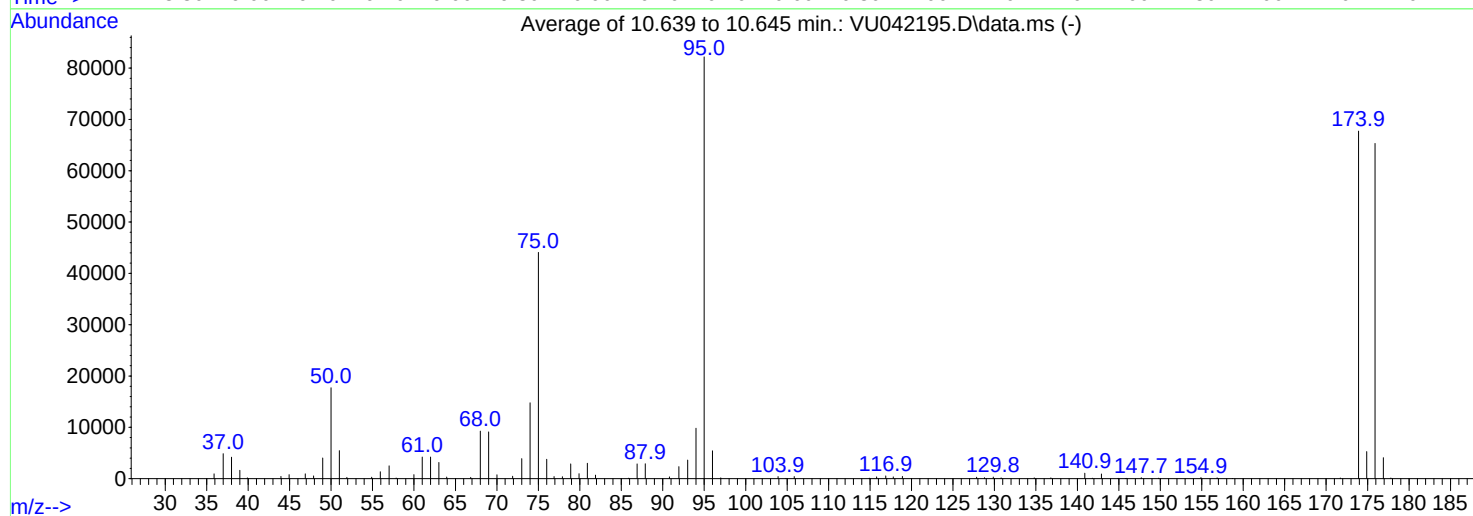


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012621\
 Data File : VU042195.D
 Acq On : 26 Jan 2021 09:22
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR012021WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 23 06:18:59 2021

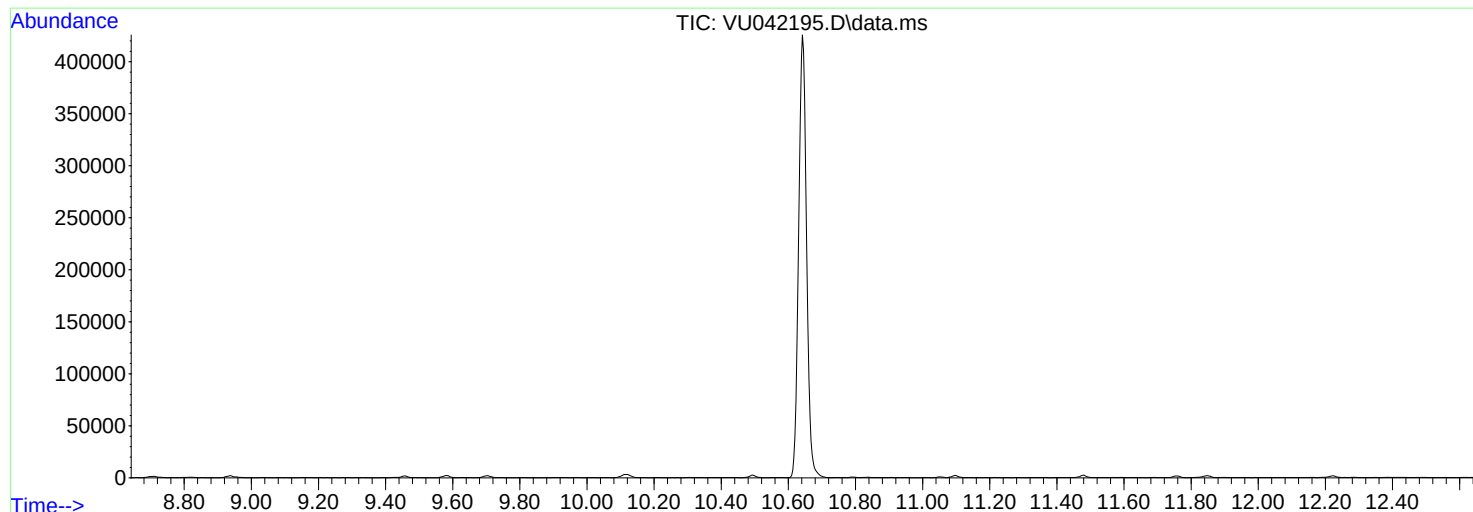

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	17717	PASS
75	95	30	80	53.6	44075	PASS
95	95	100	100	100.0	82192	PASS
96	95	5	9	6.6	5416	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.4	67733	PASS
175	174	5	9	7.8	5273	PASS
176	174	95	101	96.5	65333	PASS
177	176	5	9	6.2	4080	PASS

m/z	Abundance
35.90	855.0
37.00	4993.0
38.00	4083.0
39.00	1658.0
39.90	146.0
44.00	707.0
45.00	844.0
46.90	977.0
47.90	545.0
49.00	4043.0
50.00	17560.0
51.00	5333.0
51.90	237.0
54.90	267.0
55.90	1343.0
57.00	2572.0
57.90	130.0
60.00	795.0
61.00	4269.0
62.00	4346.0
63.00	3275.0
64.00	325.0
66.90	233.0
68.00	9020.0
69.00	8872.0
70.00	770.0
71.90	527.0
73.00	3850.0
74.00	14551.0
75.00	43232.0
76.00	3638.0
76.90	407.0
77.90	308.0
78.90	2776.0
79.90	972.0
80.90	2977.0
81.90	692.0
86.90	2805.0
87.90	2944.0
90.80	338.0
91.90	2198.0
93.00	3538.0
94.00	9938.0
95.00	80008.0
96.00	5447.0
97.00	169.0
103.90	406.0
104.90	103.0
105.80	376.0
114.90	105.0
115.80	350.0
116.90	544.0
117.80	333.0
118.90	425.0
127.90	264.0
128.80	167.0
129.80	322.0
130.80	158.0
134.80	154.0
136.80	165.0
140.90	1042.0
141.80	117.0
142.90	843.0
144.90	128.0
145.80	104.0
147.70	183.0
149.80	100.0
154.90	200.0
156.90	160.0
171.70	174.0
173.90	64376.0
174.90	5133.0
175.90	62408.0
176.90	3864.0
177.80	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	953.0
37.00	4987.0
38.00	4321.0
39.00	1668.0
39.90	143.0
44.00	687.0
45.00	815.0
46.90	967.0
47.90	550.0
49.00	4195.0
50.00	18224.0
51.00	5636.0
51.90	253.0
54.90	282.0
55.90	1381.0
57.00	2578.0
57.80	120.0
60.00	788.0
61.00	4314.0
62.00	4364.0
63.00	3204.0
64.00	326.0
66.80	264.0
68.00	9581.0
69.00	9430.0
70.00	763.0
71.90	482.0
73.00	3993.0
74.00	15128.0
75.00	45456.0
76.00	3921.0
76.90	424.0
77.90	384.0
78.90	2967.0
79.90	979.0
80.90	3096.0
81.90	694.0
85.90	127.0
86.90	2914.0
87.90	2967.0
90.80	362.0
92.00	2398.0
93.00	3731.0
94.00	10043.0
95.00	84880.0
96.00	5612.0
97.00	166.0
103.90	424.0
104.80	110.0
105.90	427.0
114.90	109.0
115.80	352.0
116.90	571.0
117.80	350.0
118.90	440.0
127.90	303.0
128.80	183.0
129.80	330.0
130.80	146.0
134.80	147.0
136.80	175.0
140.90	1105.0
141.80	112.0
142.90	957.0
144.90	108.0
146.00	112.0
147.70	186.0
149.80	103.0
154.90	229.0
156.90	140.0
171.70	196.0
173.90	69744.0
174.90	5400.0
175.90	67280.0
176.90	4196.0
177.80	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	965.0
37.00	4603.0
38.00	4110.0
39.00	1528.0
39.90	143.0
44.00	680.0
44.90	739.0
46.90	889.0
47.90	542.0
49.00	3853.0
50.00	17368.0
51.00	5367.0
51.90	230.0
54.90	258.0
56.00	1351.0
57.00	2371.0
57.80	107.0
60.00	744.0
61.00	4095.0
62.00	3966.0
63.00	2974.0
63.90	286.0
66.90	240.0
68.00	9170.0
69.00	8986.0
70.00	684.0
71.90	439.0
73.00	3852.0
74.00	14638.0
75.00	43536.0
76.00	3730.0
76.90	405.0
77.90	423.0
78.90	2910.0
79.90	910.0
80.90	2906.0
81.90	653.0
85.90	115.0
86.90	2848.0
87.90	2776.0
90.80	341.0
91.90	2393.0
93.00	3612.0
94.00	9476.0
95.00	81688.0
96.00	5189.0
97.00	162.0
103.90	407.0
105.90	431.0
114.90	105.0
115.80	297.0
116.90	510.0
117.80	314.0
118.90	409.0
127.80	315.0
128.80	197.0
129.90	298.0
130.80	128.0
134.80	146.0
136.80	177.0
140.90	1021.0
141.80	104.0
142.90	945.0
145.90	109.0
147.70	203.0
149.80	103.0
154.90	228.0
156.80	131.0
158.70	123.0
173.90	69080.0
174.90	5285.0
175.90	66312.0
176.90	4179.0
177.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
43.90	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41