

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052818.D
 Acq On : 26 Jan 2023 16:08
 Operator : JC/MD
 Sample : 01316-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H5

Quant Time: Jan 27 04:33:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 27 04:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	230898	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	222169	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	119488	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	120887	72.740	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	145.480%#
7) Chloroethane-d5	1.912	69	103457	75.551	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	151.100%#
11) 1,1-Dichloroethene-d2	2.559	63	221345	66.963	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	133.920%#
21) 2-Butanone-d5	4.629	46	155319	151.288	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	151.290%#
24) Chloroform-d	5.057	84	252782	71.271	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	142.540%#
26) 1,2-Dichloroethane-d4	5.697	65	170459	75.268	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	150.540%#
32) Benzene-d6	5.719	84	520929	76.747	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	153.500%#
36) 1,2-Dichloropropane-d6	6.684	67	154674	77.698	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	155.400%#
41) Toluene-d8	7.893	98	482253	78.025	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	156.060%#
43) trans-1,3-Dichloroprop...	8.176	79	77863	78.037	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	156.080%#
47) 2-Hexanone-d5	8.652	63	120901	172.845	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	172.850%#
56) 1,1,2,2-Tetrachloroeth...	10.761	84	220063	74.820	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	149.640%#
66) 1,2-Dichlorobenzene-d4	12.192	152	188092	81.070	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	162.140%#
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.604	62	87398	44.303	ug/L	97
8) Chloroethane	1.932	64	73263	59.127	ug/L	96
12) 1,1-Dichloroethene	2.572	96	63324	37.073	ug/L	# 77
14) Carbon disulfide	2.784	76	294197	57.027	ug/L	100
15) Methyl Acetate	2.948	43	114206	67.600	ug/L	98
16) Methylene chloride	3.041	84	70281	34.589	ug/L	95
18) Methyl tert-butyl Ether	3.359	73	254631	46.913	ug/L	99
19) 1,1-Dichloroethane	3.861	63	77025	23.793	ug/L	100
20) cis-1,2-Dichloroethene	4.661	96	45131	22.900	ug/L	94
27) 1,2-Dichloroethane	5.787	62	183927	63.929	ug/L	99
30) 1,1,1-Trichloroethane	5.308	97	143828	44.012	ug/L	99
34) Trichloroethene	6.536	95	146612	76.273	ug/L	96
37) 1,2-Dichloropropane	6.787	63	50729	27.284	ug/L	100
40) 4-Methyl-2-pentanone	7.809	43	120473	54.998	ug/L	100
42) Toluene	7.967	91	266444	34.376	ug/L	99
44) trans-1,3-Dichloropropene	8.208	75	48063	16.792	ug/L	99
45) 1,1,2-Trichloroethane	8.398	97	86498	45.493	ug/L	98
46) Tetrachloroethene	8.549	164	66380	40.104	ug/L	97
48) 2-Hexanone	8.703	43	114132	61.589	ug/L	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052818.D
 Acq On : 26 Jan 2023 16:08
 Operator : JC/MD
 Sample : 01316-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H5

Quant Time: Jan 27 04:33:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 27 04:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


50) 1,2-Dibromoethane	8.922	107	90123	44.040	ug/L	97
51) Chlorobenzene	9.446	112	300250	56.306	ug/L	98
52) Ethylbenzene	9.568	91	587284	70.902	ug/L	100
53) m,p-Xylene	9.687	106	162494	48.459	ug/L	96
54) o-xylene	10.099	106	76824	23.999	ug/L	99
55) Styrene	10.115	104	211440	38.491	ug/L	96
57) 1,1,2,2-Tetrachloroethane	10.783	83	230532	74.920	ug/L	99
59) Bromoform	10.295	173	38174	23.314	ug/L	99
61) Isopropylbenzene	10.481	105	396265	51.349	ug/L	99
64) 1,3-Dichlorobenzene	11.745	146	89450	22.974	ug/L	95
65) 1,4-Dichlorobenzene	11.835	146	184307	45.726	ug/L	97
67) 1,2-Dichlorobenzene	12.211	146	279411	70.950	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.996	75	53780	80.949	ug/L	96
72) 1,2,3-Trichlorobenzene	14.327	180	103096	40.368	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052818.D
Acq On : 26 Jan 2023 16:08
Operator : JC/MD
Sample : 01316-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H5

Quant Time: Jan 27 04:33:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 27 04:23:26 2023
Response via : Initial Calibration




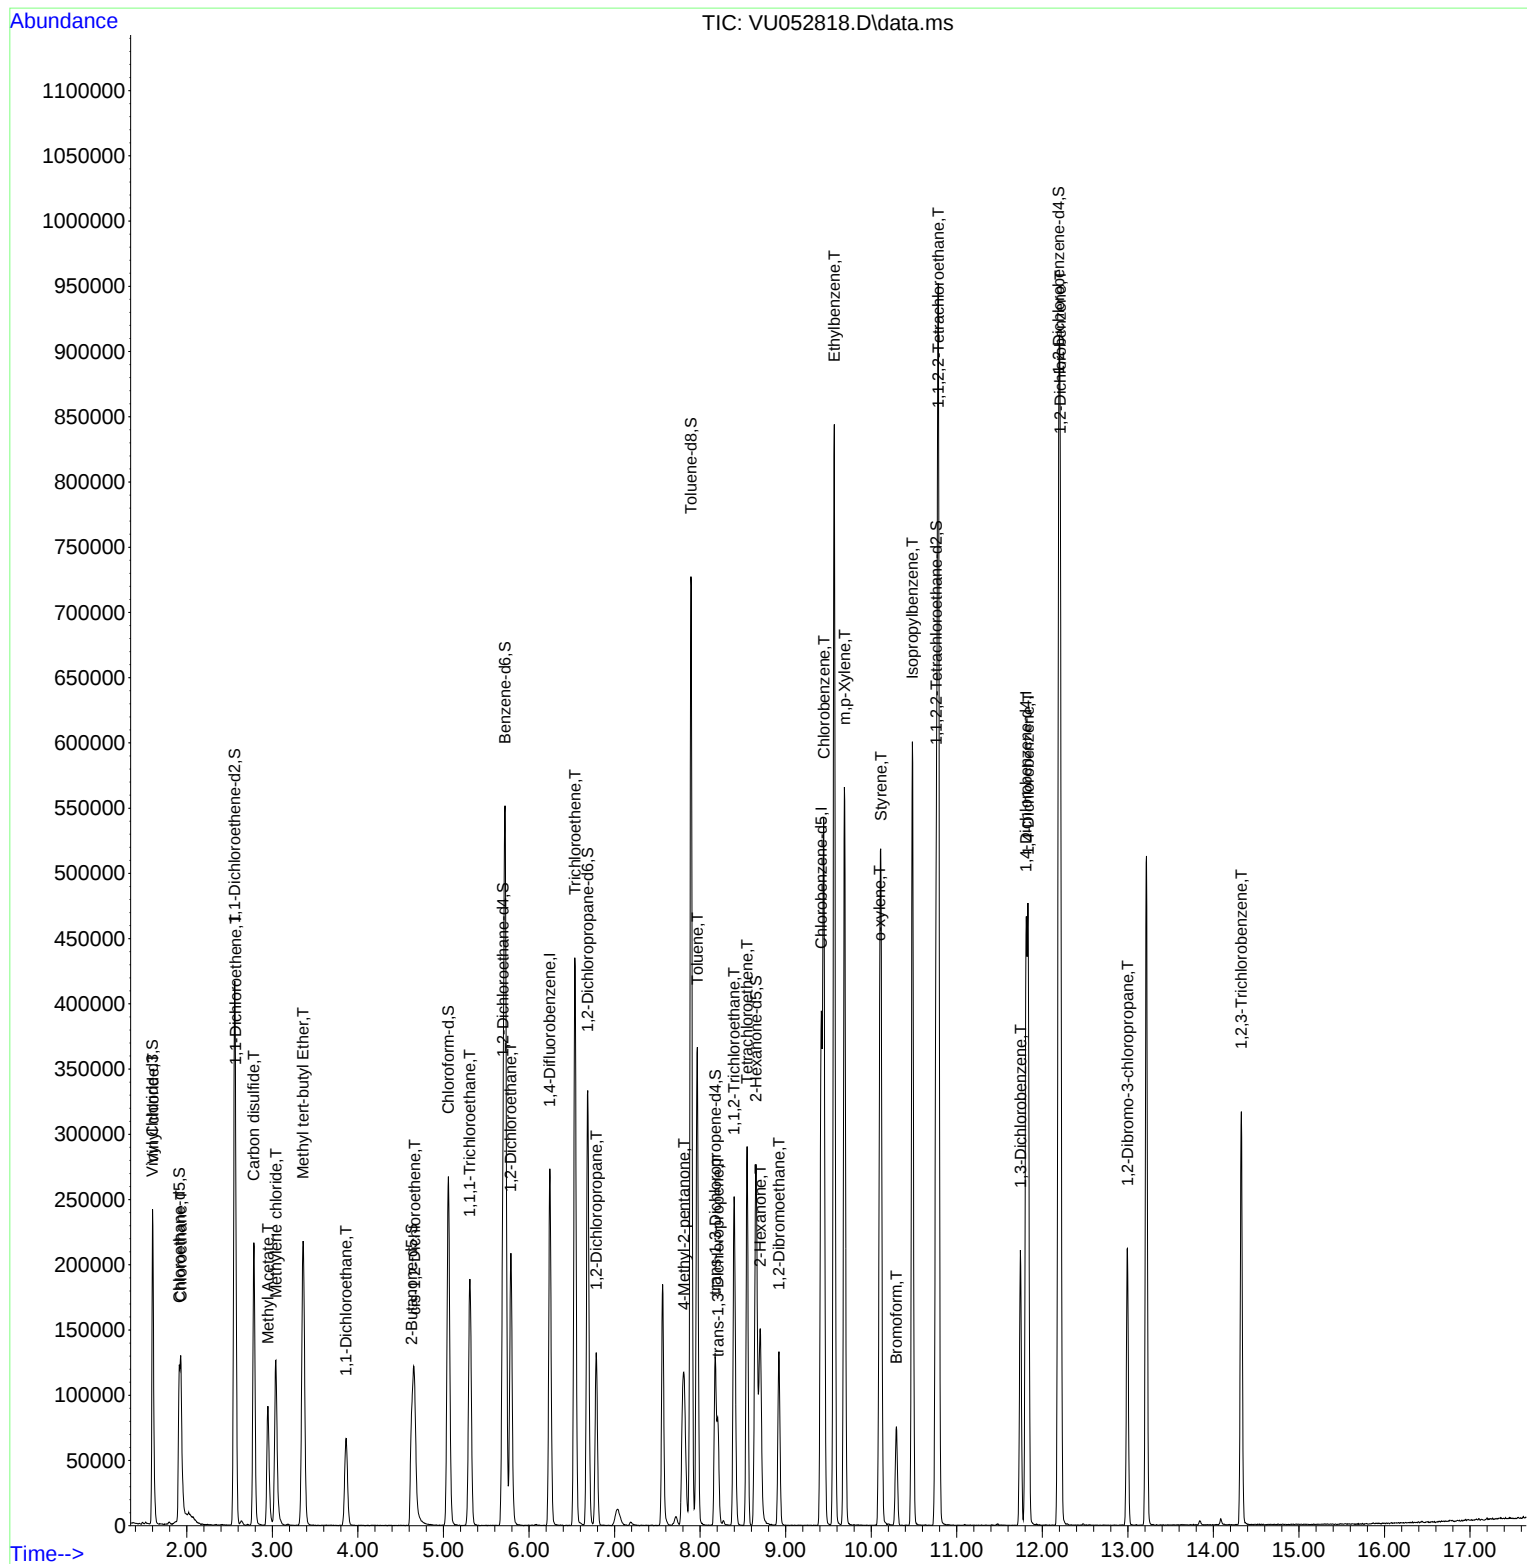




#5
 Vinyl chloride
 Concen: 44.303 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU052818.D
 Acq: 26 Jan 2023 16:08




Instrument :
 MSVOA_U
 ClientSampleId :
 A44H5


Tgt Ion: 62 Resp: 87398
 Ion Ratio Lower Upper
 62 100
 64 33.8 22.4 41.6

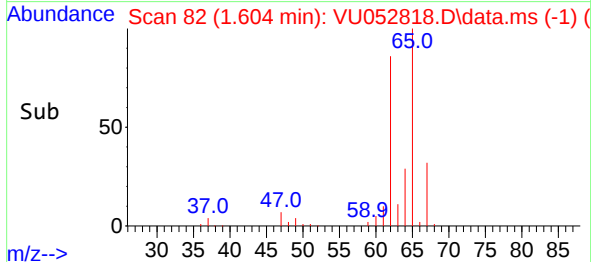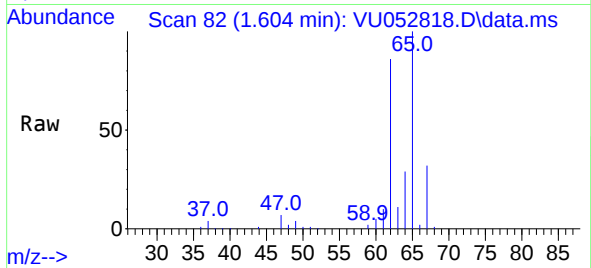

#8
 Chloroethane
 Concen: 59.127 ug/L
 RT: 1.932 min Scan# 184
 Delta R.T. -0.000 min
 Lab File: VU052818.D
 Acq: 26 Jan 2023 16:08

Tgt Ion: 64 Resp: 73263
 Ion Ratio Lower Upper
 64 100
 66 32.0 24.1 44.7

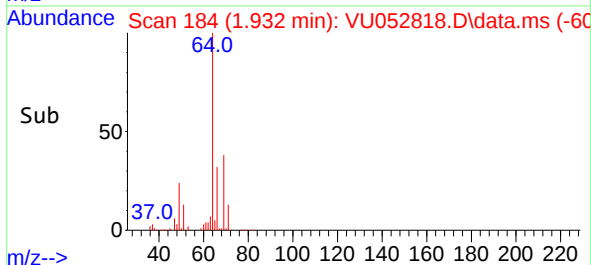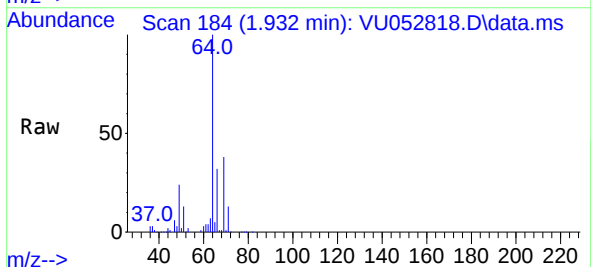



#12

1,1-Dichloroethene

Concen: 37.073 ug/L

RT: 2.572 min Scan# 3

Delta R.T. -0.006 min

Lab File: VU052818.D

Acq: 26 Jan 2023 16:08

Instrument :

MSVOA_U

ClientSampleId :

A44H5





Tgt Ion: 96 Resp: 63324

Ion Ratio Lower Upper

96 100

61 167.8 114.3 212.3

63 169.3 80.6 149.6#

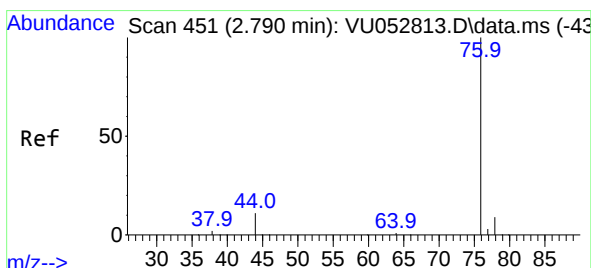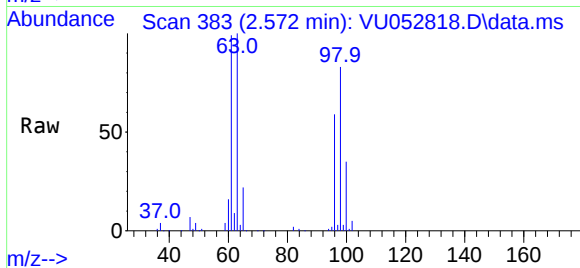

#14

Carbon disulfide

Concen: 57.027 ug/L

RT: 2.784 min Scan# 449

Delta R.T. -0.007 min

Lab File: VU052818.D




Acq: 26 Jan 2023 16:08


Tgt Ion: 76 Resp: 294197

Ion Ratio Lower Upper

76 100

78 8.9 7.1 10.7


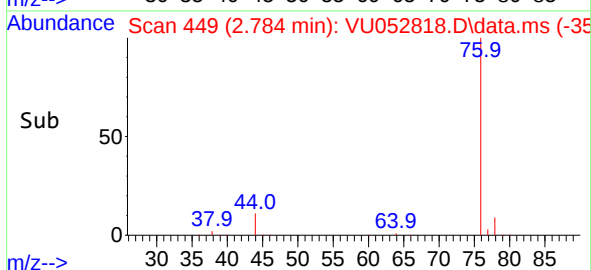

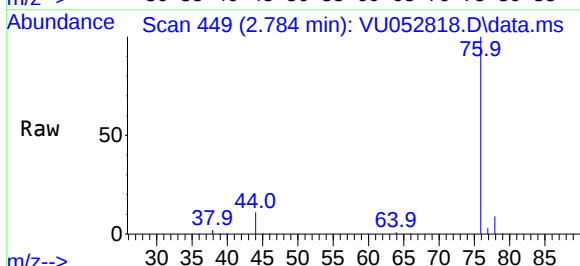




#15
Methyl Acetate
Concen: 67.600 ug/L
RT: 2.948 min Scan# 500
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion: 43 Resp: 114206
Ion Ratio Lower Upper
43 100
74 28.5 22.0 33.0



#16
Methylene chloride
Concen: 34.589 ug/L
RT: 3.041 min Scan# 529
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 84 Resp: 70281
Ion Ratio Lower Upper
84 100
86 65.5 43.4 80.6
49 108.6 72.4 134.5


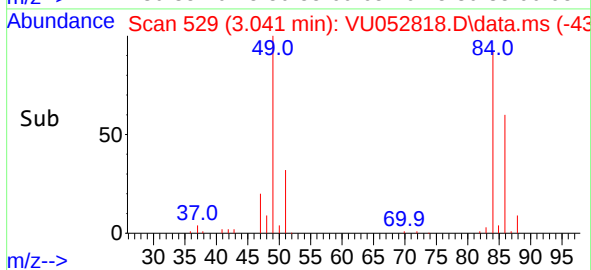




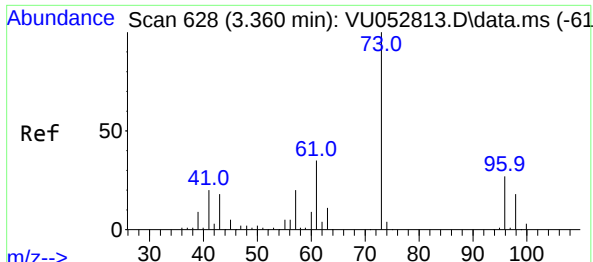

#18
Methyl tert-butyl Ether
Concen: 46.913 ug/L
RT: 3.359 min Scan# 61
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion: 73 Resp: 254631
Ion Ratio Lower Upper
73 100
43 18.4 14.2 21.2
57 20.3 16.3 24.5

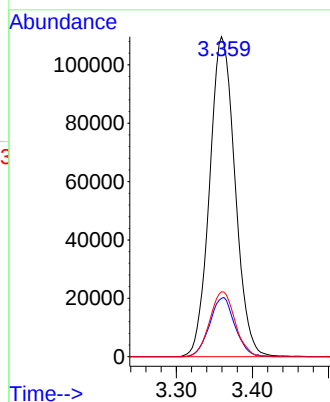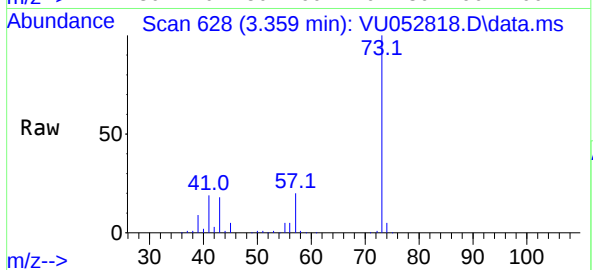

#19
1,1-Dichloroethane
Concen: 23.793 ug/L
RT: 3.861 min Scan# 784
Delta R.T. -0.004 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 63 Resp: 77025
Ion Ratio Lower Upper
63 100
65 32.0 22.4 41.6
83 13.5 9.2 17.2


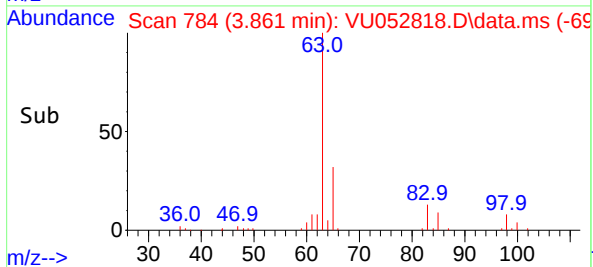
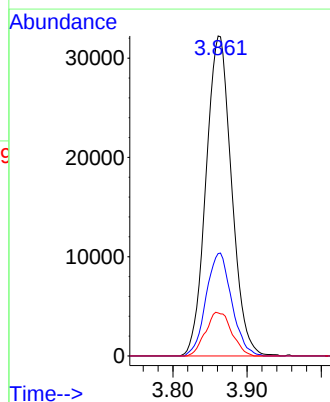
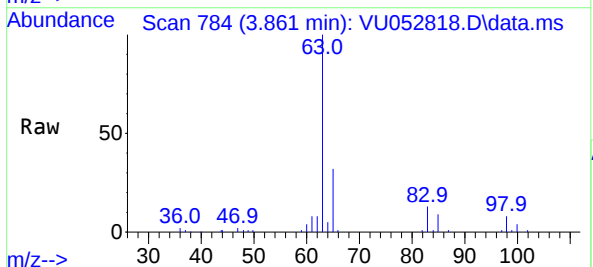




#20
cis-1,2-Dichloroethene
Concen: 22.900 ug/L
RT: 4.661 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion: 96 Resp: 45131
Ion Ratio Lower Upper
96 100
61 113.4 84.1 156.1
68 0.0 0.0 0.0



#27
1,2-Dichloroethane
Concen: 63.929 ug/L
RT: 5.787 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 62 Resp: 183927
Ion Ratio Lower Upper
62 100
98 9.9 7.6 11.4


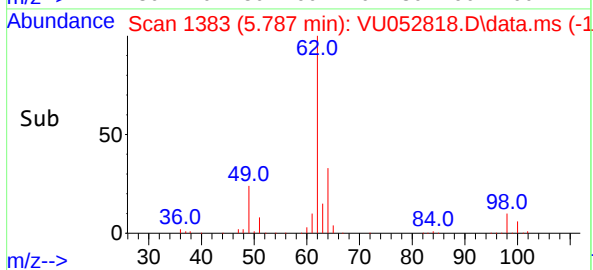






#30
1,1,1-Trichloroethane
Concen: 44.012 ug/L
RT: 5.308 min Scan# 11
Delta R.T. -0.004 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion: 97 Resp: 143828
Ion Ratio Lower Upper
97 100
99 64.9 51.4 77.0
61 40.8 33.0 49.6

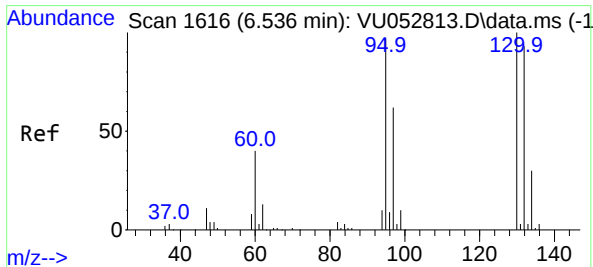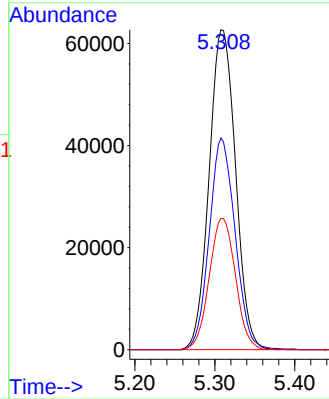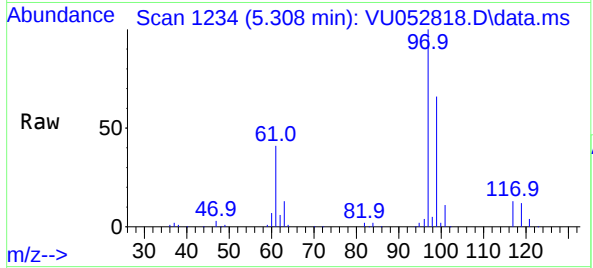

#34
Trichloroethene
Concen: 76.273 ug/L
RT: 6.536 min Scan# 1616
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 95 Resp: 146612
Ion Ratio Lower Upper
95 100
97 64.3 44.5 82.7
132 100.8 66.8 124.0
130 106.9 71.9 133.5


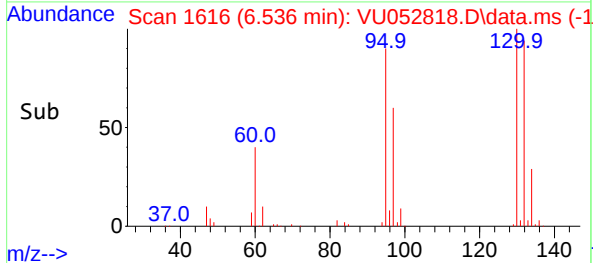
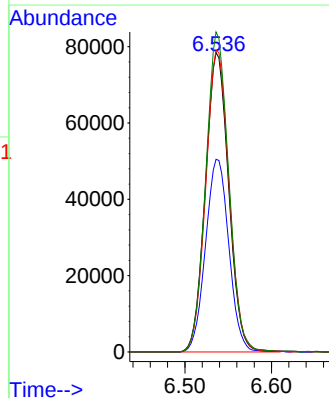
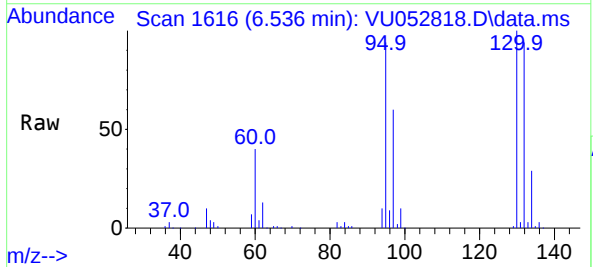




#37
1,2-Dichloropropane
Concen: 27.284 ug/L
RT: 6.787 min Scan# 10
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion: 63 Resp: 50729
Ion Ratio Lower Upper
63 100
112 4.9 3.8 5.8

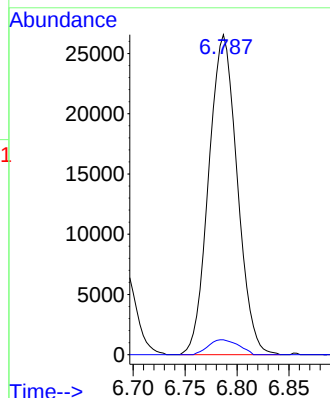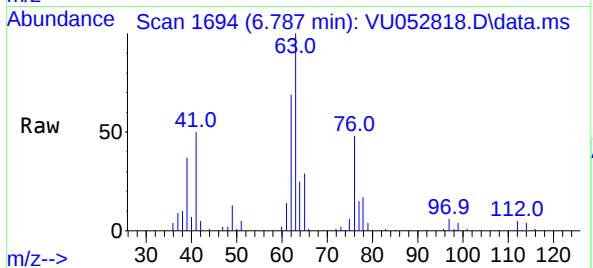

#40
4-Methyl-2-pentanone
Concen: 54.998 ug/L
RT: 7.809 min Scan# 2012
Delta R.T. 0.019 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 43 Resp: 120473
Ion Ratio Lower Upper
43 100
58 44.0 35.4 53.2
100 19.9 16.0 24.0

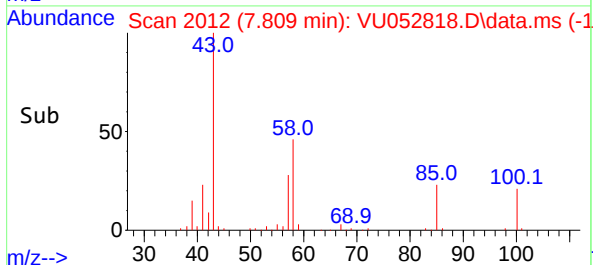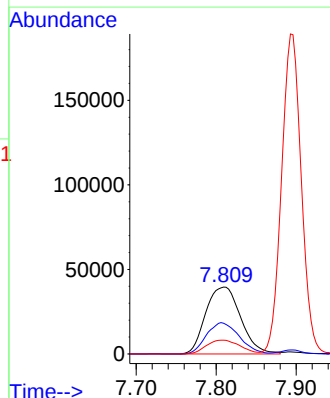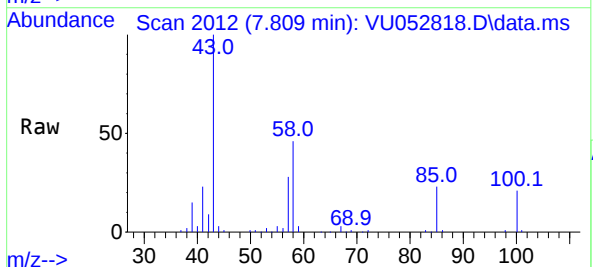



#42

Toluene

Concen: 34.376 ug/L

RT: 7.967 min Scan# 2060

Delta R.T. 0.003 min

Lab File: VU052818.D

Acq: 26 Jan 2023 16:08

Instrument :

MSVOA_U

ClientSampleId :





A44H5

Tgt Ion: 91 Resp: 266444

Ion Ratio Lower Upper

91 100

92 61.2 42.6 79.0

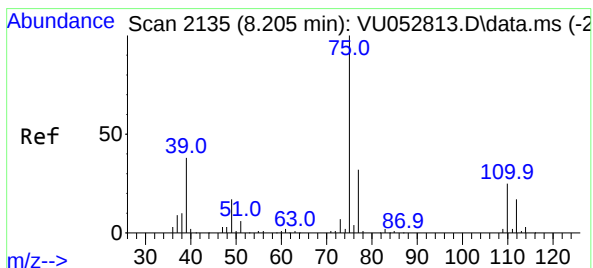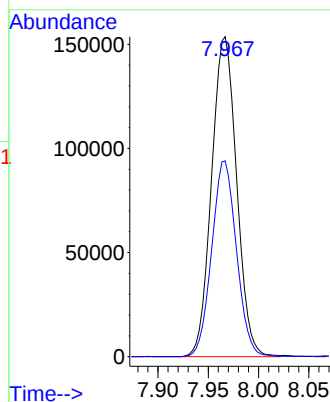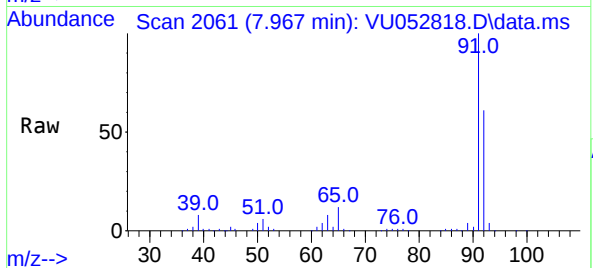

#44

trans-1,3-Dichloropropene

Concen: 16.792 ug/L

RT: 8.208 min Scan# 2136

Delta R.T. 0.003 min

Lab File: VU052818.D




Acq: 26 Jan 2023 16:08


Tgt Ion: 75 Resp: 48063

Ion Ratio Lower Upper

75 100

77 32.2 22.3 41.3

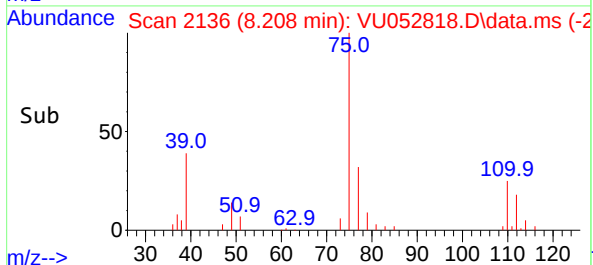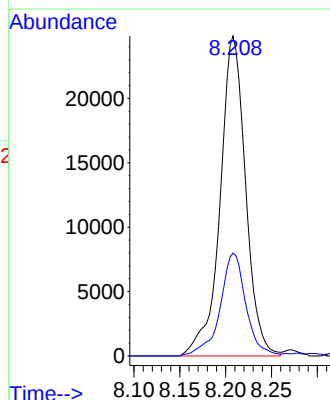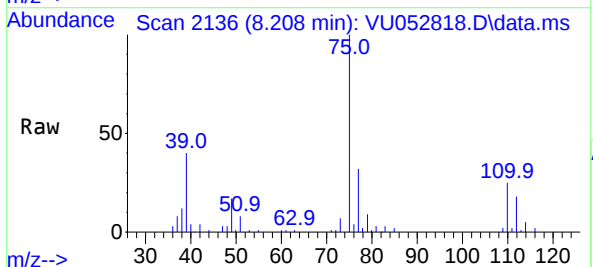







#45
1,1,2-Trichloroethane
Concen: 45.493 ug/L
RT: 8.398 min Scan# 2195
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Instrument :
MSVOA_U
ClientSampleId :
A44H5

Tgt Ion: 97 Resp: 86498




Ion	Ratio	Lower	Upper
97	100		
99	62.0	44.7	83.1
83	85.1	60.3	112.1
85	53.9	38.3	71.1

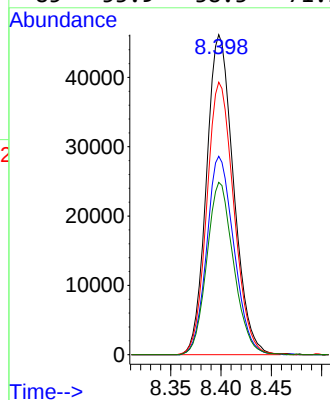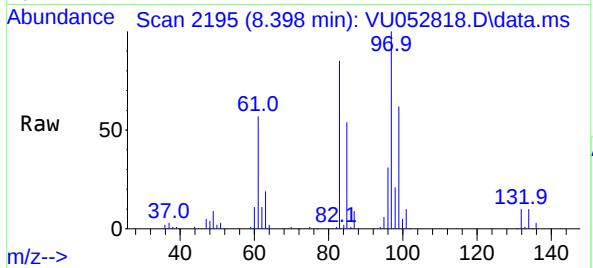


#46
Tetrachloroethene
Concen: 40.104 ug/L
RT: 8.549 min Scan# 2242
Delta R.T. -0.000 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 164 Resp: 66380

Ion	Ratio	Lower	Upper
164	100		
129	91.2	64.8	120.3
131	91.7	61.2	113.6
166	124.4	89.2	165.8

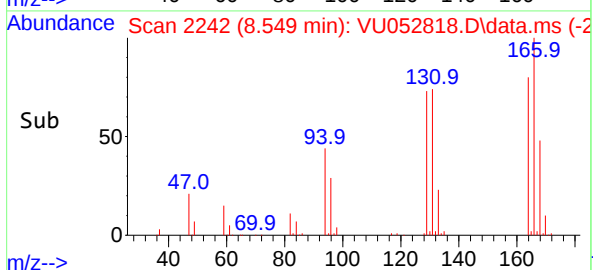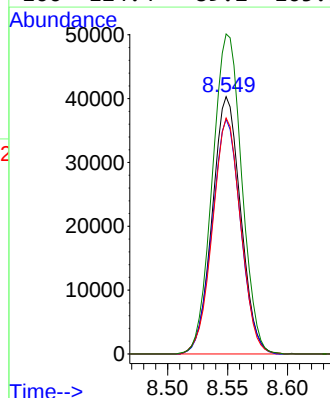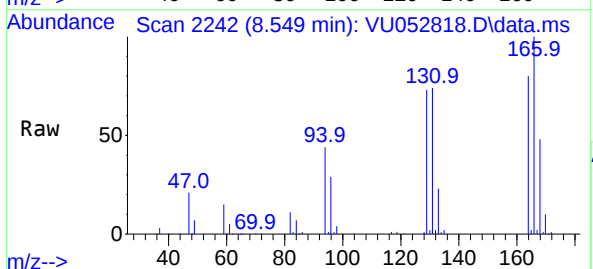



#48

2-Hexanone

Concen: 61.589 ug/L

RT: 8.703 min Scan# 21

Delta R.T. 0.019 min

Lab File: VU052818.D

Acq: 26 Jan 2023 16:08

Instrument :

MSVOA_U

ClientSampleId :

A44H5

Tgt Ion: 43 Resp: 114132





Ion Ratio Lower Upper

43 100

58 65.7 48.0 72.0

57 21.6 16.8 25.2

100 15.4 12.7 19.1

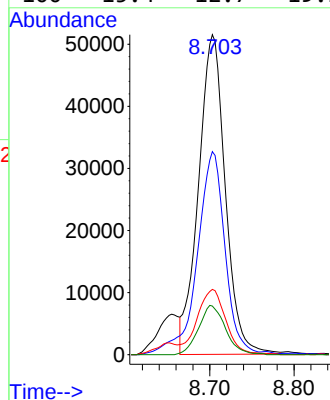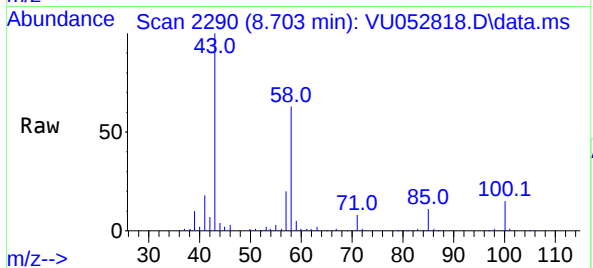

#50

1,2-Dibromoethane

Concen: 44.040 ug/L

RT: 8.922 min Scan# 2358

Delta R.T. 0.003 min

Lab File: VU052818.D

Acq: 26 Jan 2023 16:08




Tgt Ion:107 Resp: 90123


Ion Ratio Lower Upper

107 100

109 96.7 65.5 121.6

188 4.4 3.2 4.8


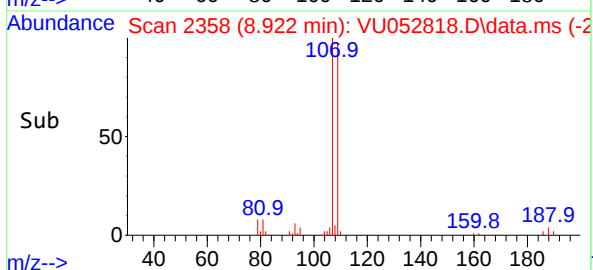
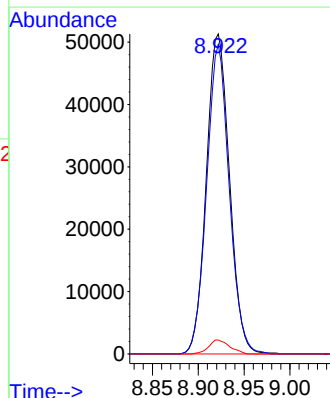





#51
Chlorobenzene
Concen: 56.306 ug/L
RT: 9.446 min Scan# 21
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:112 Resp: 300250
Ion Ratio Lower Upper
112 100
114 31.9 22.8 42.4
77 56.0 45.9 68.9



#52
Ethylbenzene
Concen: 70.902 ug/L
RT: 9.568 min Scan# 2559
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 91 Resp: 587284
Ion Ratio Lower Upper
91 100
106 31.5 22.0 40.8


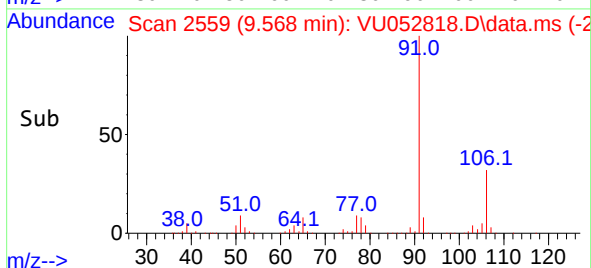
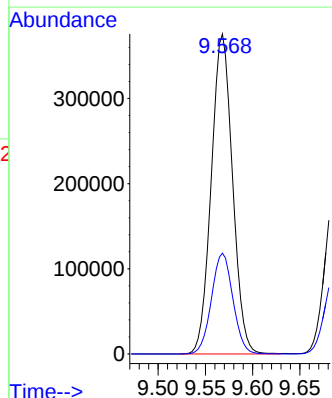





#53
m,p-Xylene
Concen: 48.459 ug/L
RT: 9.687 min Scan# 21
Delta R.T. -0.004 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:106 Resp: 162494
Ion Ratio Lower Upper
106 100
91 202.9 137.4 255.2

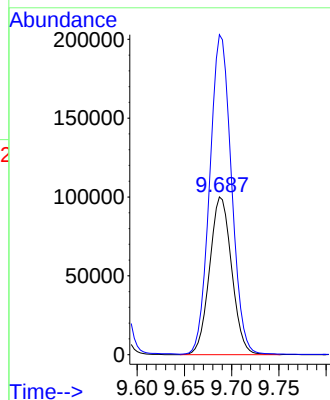

#54
o-xylene
Concen: 23.999 ug/L
RT: 10.099 min Scan# 2724
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion:106 Resp: 76824
Ion Ratio Lower Upper
106 100
91 206.0 143.4 266.2


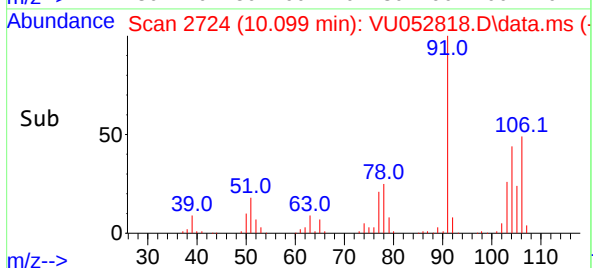
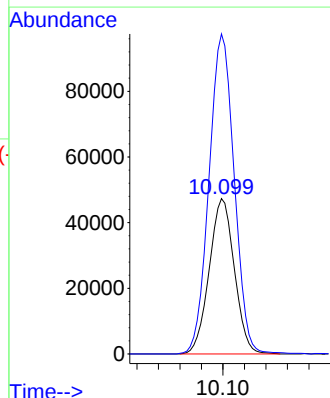





#55
Styrene
Concen: 38.491 ug/L
RT: 10.115 min Scan# 21
Delta R.T. 0.006 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:104 Resp: 211440
Ion Ratio Lower Upper
104 100
78 43.2 31.9 59.2

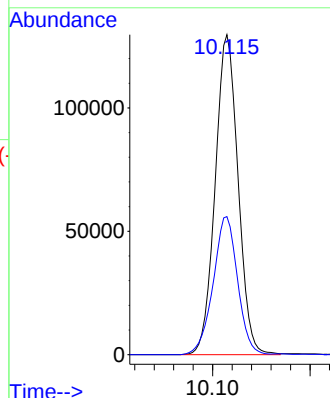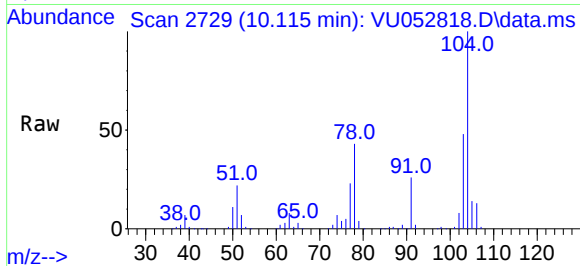

#57
1,1,2,2-Tetrachloroethane
Concen: 74.920 ug/L
RT: 10.783 min Scan# 2937
Delta R.T. 0.006 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 83 Resp: 230532
Ion Ratio Lower Upper
83 100
85 65.5 45.0 83.6
131 11.1 8.6 12.8


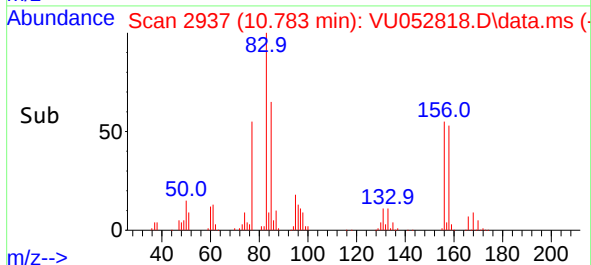
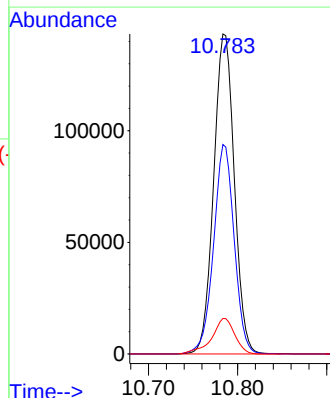
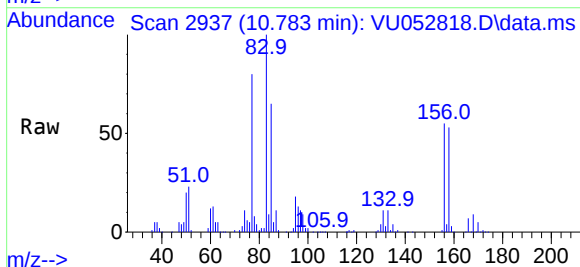




#59
Bromoform
Concen: 23.314 ug/L
RT: 10.295 min Scan# 21
Delta R.T. 0.009 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:173 Resp: 38174
Ion Ratio Lower Upper
173 100
175 48.0 37.7 56.5
254 10.3 8.3 12.5

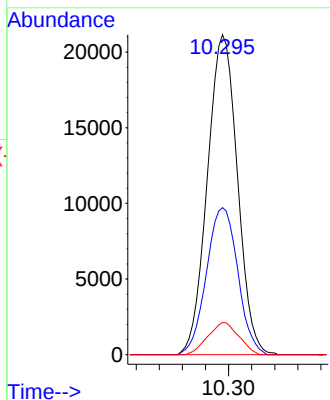

#61
Isopropylbenzene
Concen: 51.349 ug/L
RT: 10.481 min Scan# 2843
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion:105 Resp: 396265
Ion Ratio Lower Upper
105 100
120 26.0 21.4 32.2
77 15.2 12.2 18.2


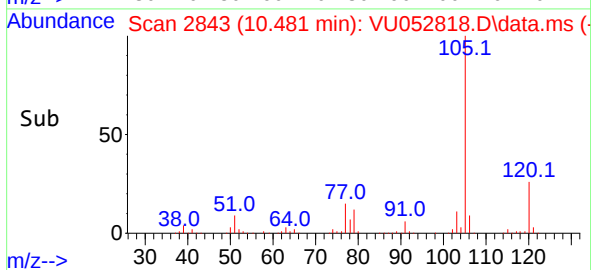
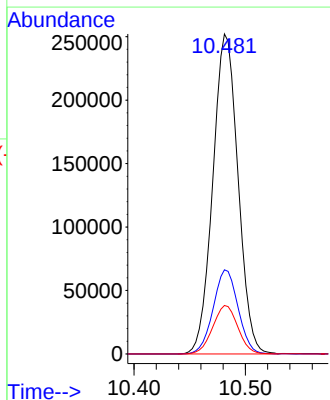



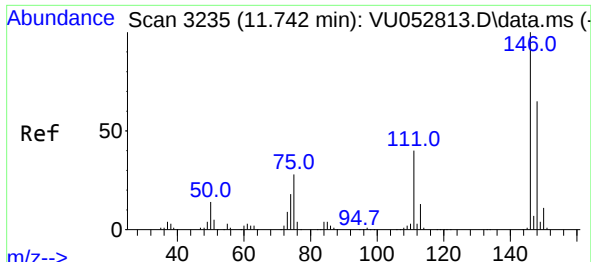

#64
1,3-Dichlorobenzene
Concen: 22.974 ug/L
RT: 11.745 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:146 Resp: 89450
Ion Ratio Lower Upper
146 100
111 36.9 27.8 51.6
148 61.2 45.5 84.5

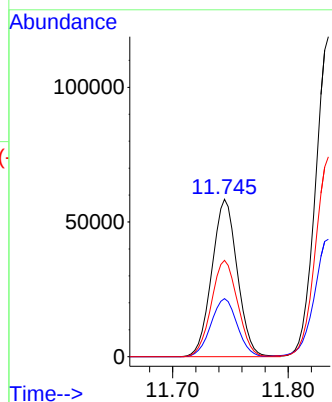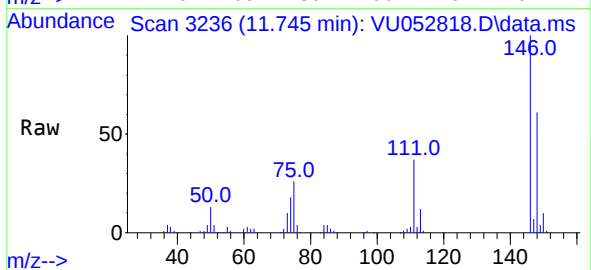

#65
1,4-Dichlorobenzene
Concen: 45.726 ug/L
RT: 11.835 min Scan# 3264
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion:146 Resp: 184307
Ion Ratio Lower Upper
146 100
111 36.7 26.7 49.7
148 62.5 45.6 84.6


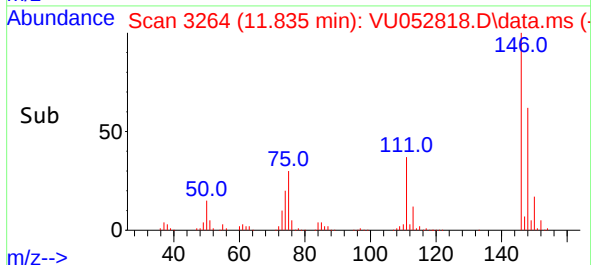

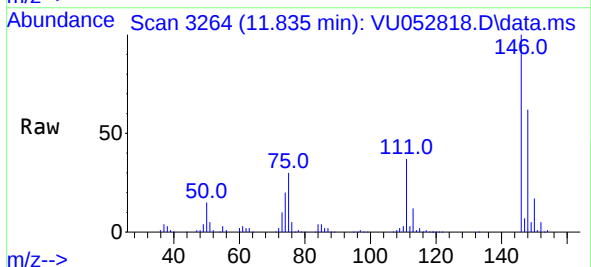




#67
1,2-Dichlorobenzene
Concen: 70.950 ug/L
RT: 12.211 min Scan# 311
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08




Instrument :
MSVOA_U
ClientSampleId :
A44H5


Tgt Ion:146 Resp: 279411
Ion Ratio Lower Upper
146 100
111 42.1 33.2 49.8
148 64.8 50.2 75.4

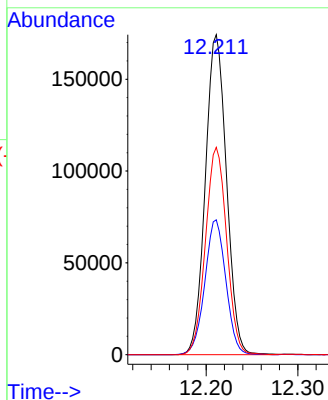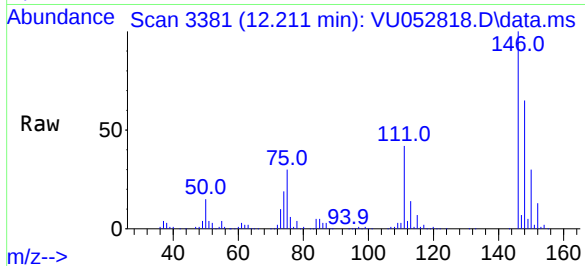

#68
1,2-Dibromo-3-chloropropane
Concen: 80.949 ug/L
RT: 12.996 min Scan# 3625
Delta R.T. 0.003 min
Lab File: VU052818.D
Acq: 26 Jan 2023 16:08

Tgt Ion: 75 Resp: 53780
Ion Ratio Lower Upper
75 100
155 91.5 69.2 103.8
157 116.5 91.2 136.8

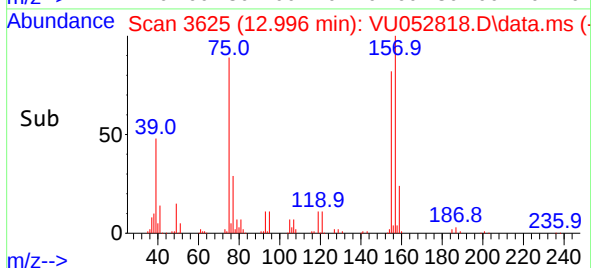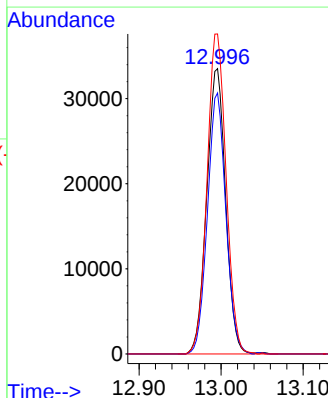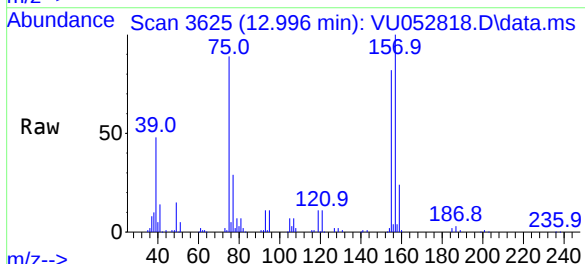

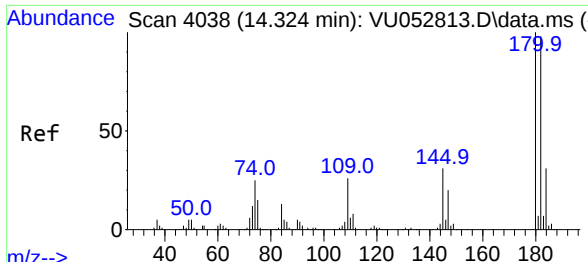

#72
 1,2,3-Trichlorobenzene
 Concen: 40.368 ug/L
 RT: 14.327 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU052818.D
 Acq: 26 Jan 2023 16:08

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H5

Tgt Ion:180 Resp: 103096

Ion	Ratio	Lower	Upper
180	100		
182	95.4	77.5	116.3
145	30.7	24.2	36.4

