

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052829.D
 Acq On : 26 Jan 2023 20:22
 Operator : JC/MD
 Sample : 01316-02MS
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7MS

Quant Time: Jan 27 04:36:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 27 04:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	272032	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	258817	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	150878	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	82604	42.189	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.380%
7) Chloroethane-d5	1.906	69	72272	44.797	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.600%
11) 1,1-Dichloroethene-d2	2.565	63	174120	44.711	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.420%
21) 2-Butanone-d5	4.620	46	114338	94.530	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.530%
24) Chloroform-d	5.057	84	194920	46.647	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.300%
26) 1,2-Dichloroethane-d4	5.694	65	123919	46.444	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.880%
32) Benzene-d6	5.723	84	370400	46.843	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.680%
36) 1,2-Dichloropropane-d6	6.684	67	108879	46.949	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.900%
41) Toluene-d8	7.893	98	340347	47.268	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.540%
43) trans-1,3-Dichloroprop...	8.176	79	55626	47.856	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.720%
47) 2-Hexanone-d5	8.629	63	83985	103.067	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.070%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	162422	47.403	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	12.189	152	138564	47.297	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.600%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.385	85	114174	44.822	ug/L	98
3) Chloromethane	1.520	50	95501	45.457	ug/L	99
5) Vinyl chloride	1.604	62	103609	44.579	ug/L	100
6) Bromomethane	1.855	94	66199	45.163	ug/L	99
8) Chloroethane	1.929	64	66565	45.598	ug/L	96
9) Trichlorofluoromethane	2.134	101	174263	44.765	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.578	101	95584	43.561	ug/L	99
12) 1,1-Dichloroethene	2.578	96	91027	45.233	ug/L	99
13) Acetone	2.626	43	83607	56.597	ug/L	98
14) Carbon disulfide	2.790	76	261333	42.997	ug/L	100
15) Methyl Acetate	2.945	43	87400	43.911	ug/L	97
16) Methylene chloride	3.041	84	104773	43.767	ug/L	99
17) trans-1,2-Dichloroethene	3.350	96	96812	44.517	ug/L	99
18) Methyl tert-butyl Ether	3.359	73	302359	47.283	ug/L	98
19) 1,1-Dichloroethane	3.864	63	174291	45.697	ug/L	98
20) cis-1,2-Dichloroethene	4.662	96	107770	46.414	ug/L	100
22) 2-Butanone	4.697	43	129065	81.739	ug/L	98
23) Bromochloromethane	4.970	128	57955	44.448	ug/L	98
25) Chloroform	5.083	83	201024	46.950	ug/L	99


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052829.D
 Acq On : 26 Jan 2023 20:22
 Operator : JC/MD
 Sample : 01316-02MS
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7MS

Quant Time: Jan 27 04:36:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 27 04:23:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	5.787	62	157723	46.531	ug/L	100
29) Cyclohexane	5.385	56	145444	47.422	ug/L	98
30) 1,1,1-Trichloroethane	5.311	97	174493	45.835	ug/L	98
31) Carbon tetrachloride	5.520	117	157634	47.766	ug/L	100
33) Benzene	5.768	78	415777	47.193	ug/L	100
34) Trichloroethene	6.536	95	101076	45.137	ug/L	96
35) Methylcyclohexane	6.758	83	162999	45.990	ug/L	99
37) 1,2-Dichloropropane	6.787	63	101730	46.967	ug/L	99
38) Bromodichloromethane	7.099	83	147681	46.462	ug/L	99
39) cis-1,3-Dichloropropene	7.604	75	155202	45.742	ug/L	97
40) 4-Methyl-2-pentanone	7.787	43	253046	99.162	ug/L	100
42) Toluene	7.964	91	433157	47.972	ug/L	100
44) trans-1,3-Dichloropropene	8.205	75	158880	47.648	ug/L	98
45) 1,1,2-Trichloroethane	8.395	97	105319	47.548	ug/L	99
46) Tetrachloroethene	8.549	164	87222	45.235	ug/L	99
48) 2-Hexanone	8.681	43	200730	92.982	ug/L	98
49) Dibromochloromethane	8.803	129	123153	46.493	ug/L	100
50) 1,2-Dibromoethane	8.919	107	114976	48.230	ug/L	99
51) Chlorobenzene	9.443	112	286750	46.160	ug/L	99
52) Ethylbenzene	9.565	91	463415	48.025	ug/L	100
53) m,p-Xylene	9.690	106	189573	48.529	ug/L	99
54) o-xylene	10.095	106	184727	49.535	ug/L	96
55) Styrene	10.108	104	311991	48.754	ug/L	98
57) 1,1,2,2-Tetrachloroethane	10.777	83	168146	46.907	ug/L	100
59) Bromoform	10.285	173	95782	46.327	ug/L	98
60) 1,2,3-Trichloropropane	10.819	75	132738	45.355	ug/L	99
61) Isopropylbenzene	10.481	105	467653	47.992	ug/L	100
62) 1,3,5-Trimethylbenzene	11.082	105	395417	48.735	ug/L	99
63) 1,2,4-Trimethylbenzene	11.462	105	389401	49.597	ug/L	99
64) 1,3-Dichlorobenzene	11.742	146	221424	45.038	ug/L	100
65) 1,4-Dichlorobenzene	11.832	146	223101	43.835	ug/L	98
67) 1,2-Dichlorobenzene	12.208	146	228693	45.989	ug/L	100
68) 1,2-Dibromo-3-chloropr...	12.989	75	37402	44.584	ug/L	98
69) 1,3,5-Trichlorobenzene	13.214	180	157228	43.199	ug/L	99
70) 1,2,4-trichlorobenzene	13.835	180	129223	42.348	ug/L	99
71) Naphthalene	14.082	128	394671	45.007	ug/L	100
72) 1,2,3-Trichlorobenzene	14.324	180	140891	43.689	ug/L	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
Dichlorodifluoromethane
Concen: 44.822 ug/L
RT: 1.385 min Scan# 14
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 85 Resp: 114174
Ion Ratio Lower Upper
85 100
87 31.9 26.4 39.6

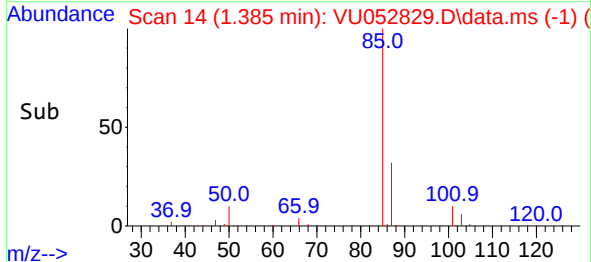

#3
Chloromethane
Concen: 45.457 ug/L
RT: 1.520 min Scan# 56
Delta R.T. 0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 50 Resp: 95501
Ion Ratio Lower Upper
50 100
52 32.6 23.4 43.4


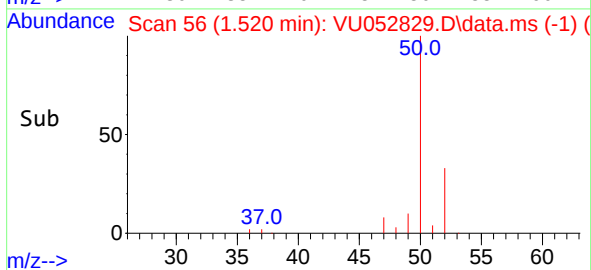




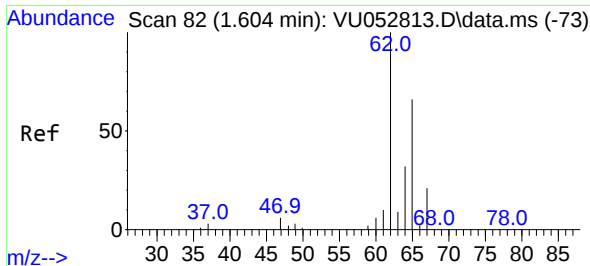

#5
 Vinyl chloride
 Concen: 44.579 ug/L
 RT: 1.604 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU052829.D
 Acq: 26 Jan 2023 20:22




Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7MS


Tgt Ion: 62 Resp: 103609
 Ion Ratio Lower Upper
 62 100
 64 32.0 22.4 41.6

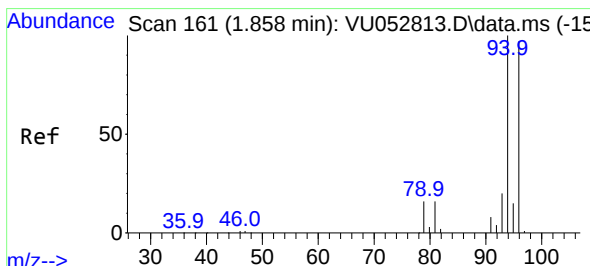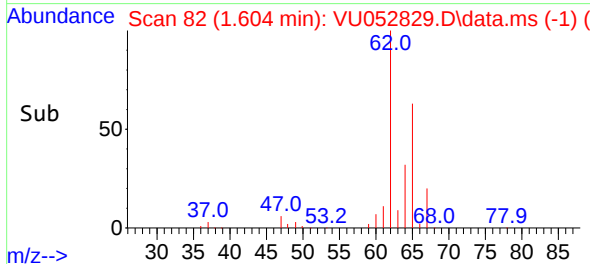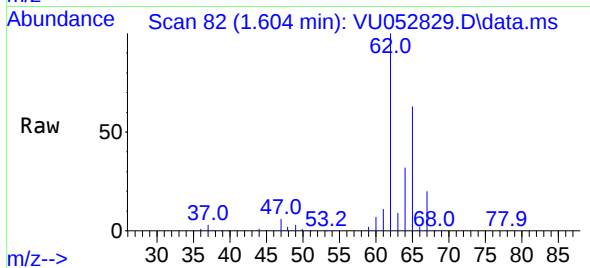

#6
 Bromomethane
 Concen: 45.163 ug/L
 RT: 1.855 min Scan# 160
 Delta R.T. -0.003 min
 Lab File: VU052829.D
 Acq: 26 Jan 2023 20:22

Tgt Ion: 94 Resp: 66199
 Ion Ratio Lower Upper
 94 100
 96 95.9 67.8 125.8


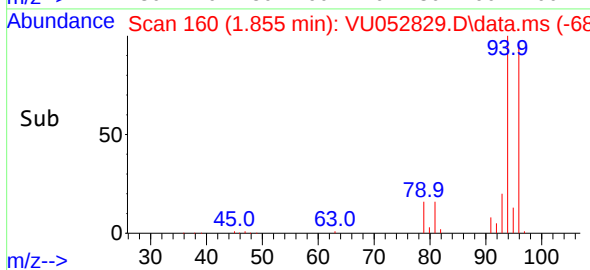

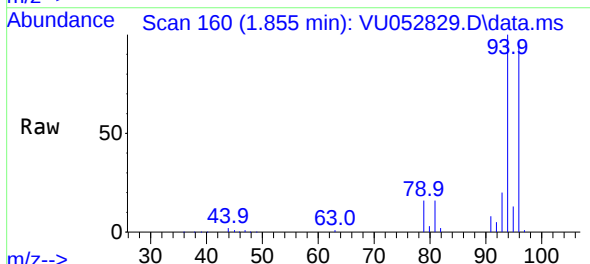




#8
Chloroethane
Concen: 45.598 ug/L
RT: 1.929 min Scan# 184
Delta R.T. -0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 64 Resp: 66565
Ion Ratio Lower Upper
64 100
66 32.1 24.1 44.7

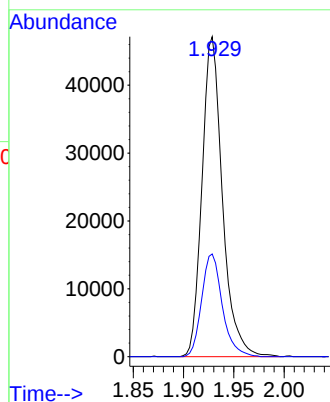

#9
Trichlorofluoromethane
Concen: 44.765 ug/L
RT: 2.134 min Scan# 247
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 101 Resp: 174263
Ion Ratio Lower Upper
101 100
103 64.9 52.0 78.0


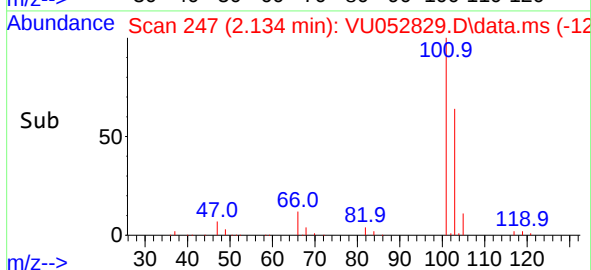






#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 43.561 ug/L
RT: 2.578 min Scan# 385
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:101 Resp: 95584
Ion Ratio Lower Upper
101 100
85 41.6 32.9 49.3
151 79.0 62.6 94.0

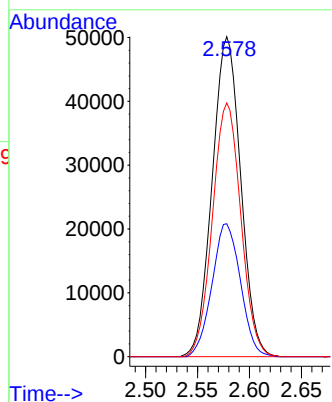

#12
1,1-Dichloroethene
Concen: 45.233 ug/L
RT: 2.578 min Scan# 385
Delta R.T. 0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 96 Resp: 91027
Ion Ratio Lower Upper
96 100
61 163.5 114.3 212.3
63 112.1 80.6 149.6

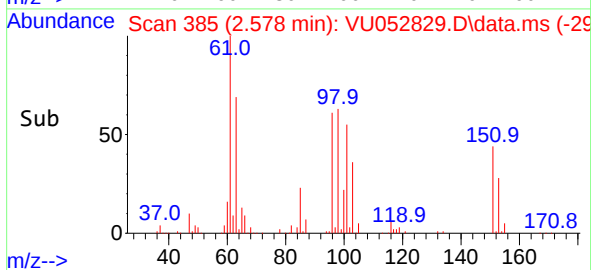



#13

Acetone

Concen: 56.597 ug/L

RT: 2.626 min Scan# 404

Delta R.T. -0.013 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :





A44G7MS

Tgt Ion: 43 Resp: 83607

Ion Ratio Lower Upper

43 100

58 33.8 0.0 70.2



#14

Carbon disulfide

Concen: 42.997 ug/L

RT: 2.790 min Scan# 451

Delta R.T. -0.000 min

Lab File: VU052829.D




Acq: 26 Jan 2023 20:22


Tgt Ion: 76 Resp: 261333

Ion Ratio Lower Upper

76 100

78 9.0 7.1 10.7


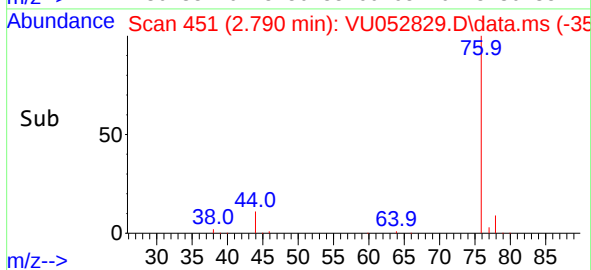






#15
Methyl Acetate
Concen: 43.911 ug/L
RT: 2.945 min Scan# 499
Delta R.T. -0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 43 Resp: 87400
Ion Ratio Lower Upper
43 100
74 29.3 22.0 33.0

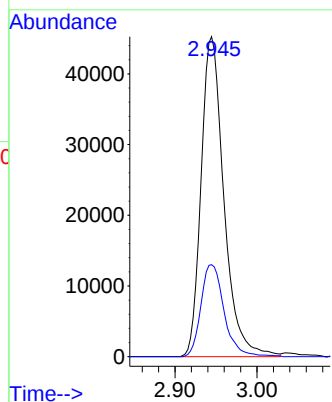

#16
Methylene chloride
Concen: 43.767 ug/L
RT: 3.041 min Scan# 529
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 84 Resp: 104773
Ion Ratio Lower Upper
84 100
86 64.1 43.4 80.6
49 103.9 72.4 134.5









#17
trans-1,2-Dichloroethene
Concen: 44.517 ug/L
RT: 3.350 min Scan# 61
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 96 Resp: 96812
Ion Ratio Lower Upper
96 100
61 132.0 92.7 172.3
98 65.5 44.7 82.9

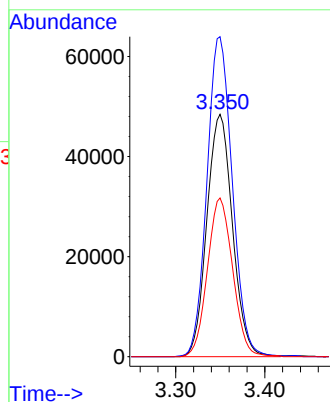

#18
Methyl tert-butyl Ether
Concen: 47.283 ug/L
RT: 3.359 min Scan# 628
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 73 Resp: 302359
Ion Ratio Lower Upper
73 100
43 18.6 14.2 21.2
57 20.9 16.3 24.5









#19
1,1-Dichloroethane
Concen: 45.697 ug/L
RT: 3.864 min Scan# 785
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 63 Resp: 174291
Ion Ratio Lower Upper
63 100
65 32.9 22.4 41.6
83 14.2 9.2 17.2



#20
cis-1,2-Dichloroethene
Concen: 46.414 ug/L
RT: 4.662 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 96 Resp: 107770
Ion Ratio Lower Upper
96 100
61 119.7 84.1 156.1
68 0.0 0.0 0.0


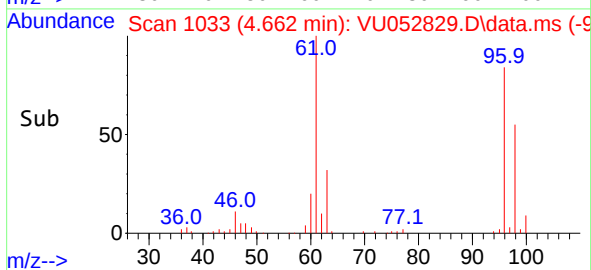






#22
2-Butanone
Concen: 81.739 ug/L
RT: 4.697 min Scan# 1104
Delta R.T. -0.007 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 43 Resp: 129065
Ion Ratio Lower Upper
43 100
72 32.1 15.5 46.5

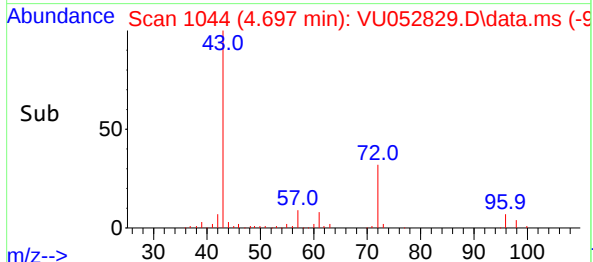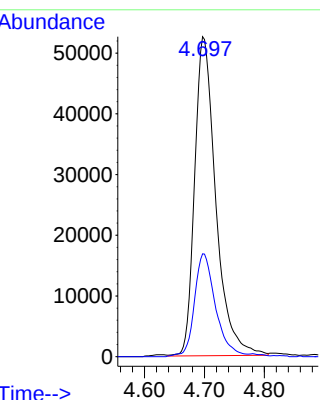

#23
Bromochloromethane
Concen: 44.448 ug/L
RT: 4.970 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:128 Resp: 57955
Ion Ratio Lower Upper
128 100
49 131.7 90.1 167.3
130 130.7 90.1 167.3
51 42.6 35.0 52.6



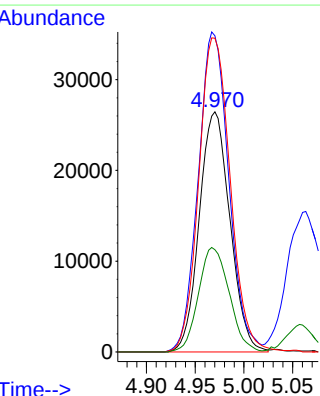





#25
Chloroform
Concen: 46.950 ug/L
RT: 5.083 min Scan# 1164
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 83 Resp: 201024
Ion Ratio Lower Upper
83 100
85 66.4 45.8 85.0

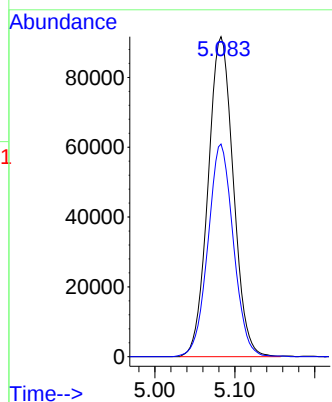

#27
1,2-Dichloroethane
Concen: 46.531 ug/L
RT: 5.787 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 62 Resp: 157723
Ion Ratio Lower Upper
62 100
98 9.6 7.6 11.4

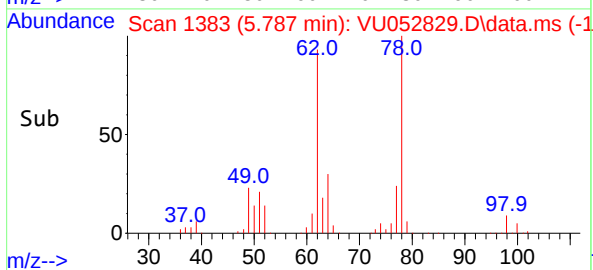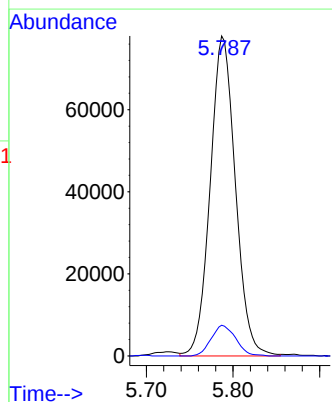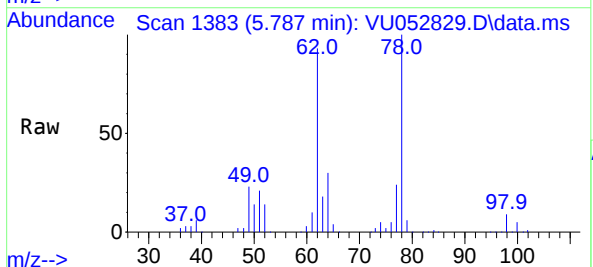



#29

Cyclohexane

Concen: 47.422 ug/L

RT: 5.385 min Scan# 11

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :

A44G7MS





Tgt Ion: 56 Resp: 145444

Ion Ratio Lower Upper

56 100

69 33.2 26.6 40.0

84 99.0 77.0 115.4

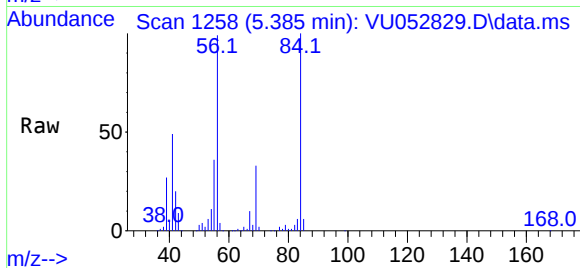

#30

1,1,1-Trichloroethane

Concen: 45.835 ug/L

RT: 5.311 min Scan# 1235

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22




Tgt Ion: 97 Resp: 174493


Ion Ratio Lower Upper

97 100

99 66.1 51.4 77.0

61 41.8 33.0 49.6


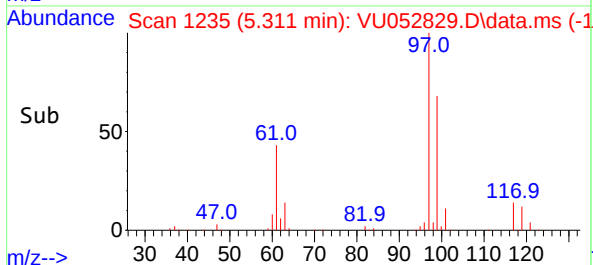
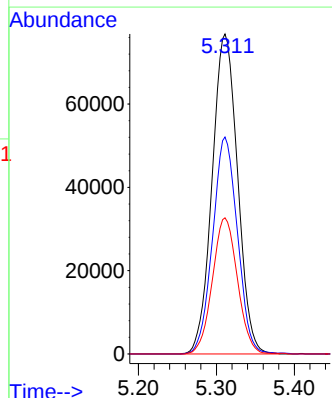
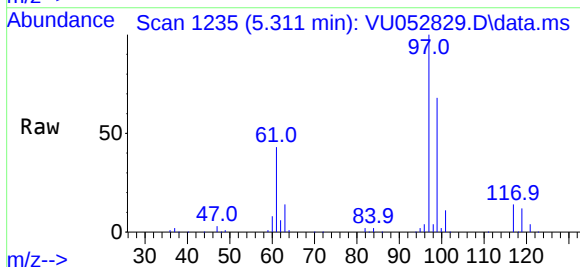




#31
Carbon tetrachloride
Concen: 47.766 ug/L
RT: 5.520 min Scan# 111
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:117 Resp: 157634
Ion Ratio Lower Upper
117 100
119 95.0 76.2 114.4



#33
Benzene
Concen: 47.193 ug/L
RT: 5.768 min Scan# 1377
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 78 Resp: 415777

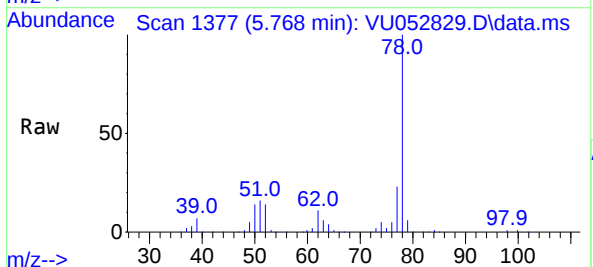







#34
Trichloroethene
Concen: 45.137 ug/L
RT: 6.536 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Instrument :
MSVOA_U
ClientSampleId :
A44G7MS

Tgt Ion: 95 Resp: 101076




Ion	Ratio	Lower	Upper
95	100		
97	65.5	44.5	82.7
132	100.5	66.8	124.0
130	105.3	71.9	133.5




#35
Methylcyclohexane
Concen: 45.990 ug/L
RT: 6.758 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 83 Resp: 162999

Ion	Ratio	Lower	Upper
83	100		
55	71.7	57.1	85.7
98	50.5	38.9	58.3

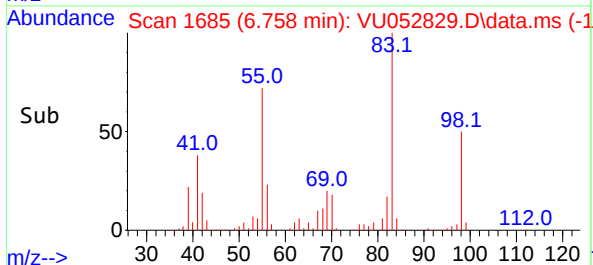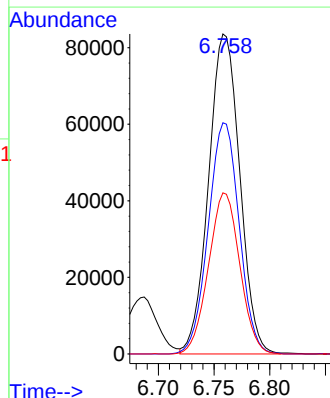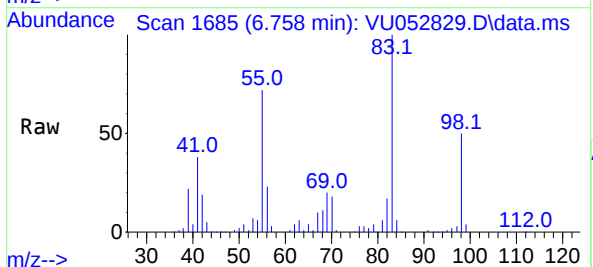



#37

1,2-Dichloropropane

Concen: 46.967 ug/L

RT: 6.787 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :





A44G7MS

Tgt Ion: 63 Resp: 101730

Ion Ratio Lower Upper

63 100

112 5.1 3.8 5.8



#38

Bromodichloromethane

Concen: 46.462 ug/L

RT: 7.099 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22




Tgt Ion: 83 Resp: 147681


Ion Ratio Lower Upper

83 100

85 63.5 45.2 84.0

127 9.2 7.4 11.0


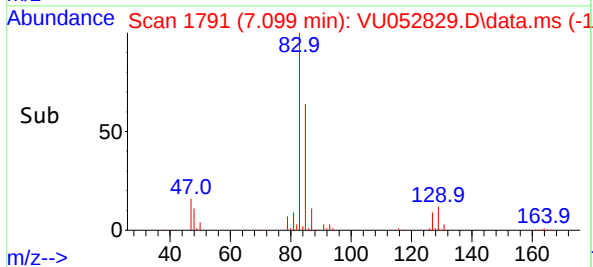

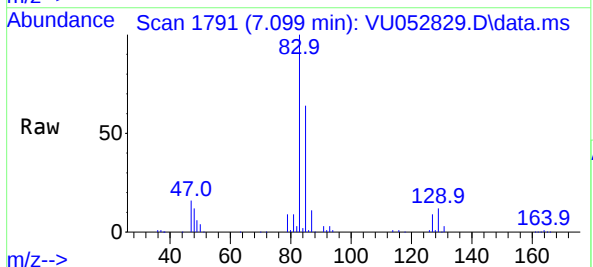




#39
 cis-1,3-Dichloropropene
 Concen: 45.742 ug/L
 RT: 7.604 min Scan# 1948
 Delta R.T. -0.000 min
 Lab File: VU052829.D
 Acq: 26 Jan 2023 20:22




Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7MS


Tgt Ion: 75 Resp: 155202
 Ion Ratio Lower Upper
 75 100
 77 32.3 21.6 40.0



#40
 4-Methyl-2-pentanone
 Concen: 99.162 ug/L
 RT: 7.787 min Scan# 2005
 Delta R.T. -0.003 min
 Lab File: VU052829.D
 Acq: 26 Jan 2023 20:22

Tgt Ion: 43 Resp: 253046
 Ion Ratio Lower Upper
 43 100
 58 44.2 35.4 53.2
 100 20.2 16.0 24.0


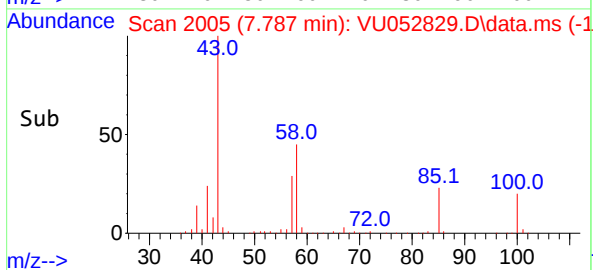






#42
Toluene
Concen: 47.972 ug/L
RT: 7.964 min Scan# 2060
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 91 Resp: 433157
Ion Ratio Lower Upper
91 100
92 60.5 42.6 79.0

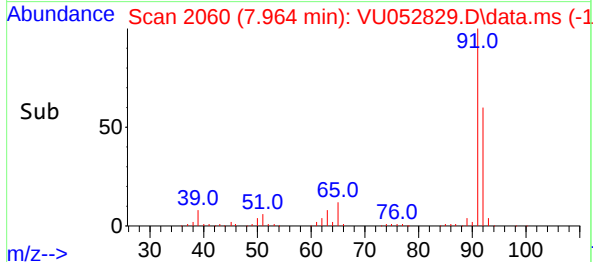

#44
trans-1,3-Dichloropropene
Concen: 47.648 ug/L
RT: 8.205 min Scan# 2135
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 75 Resp: 158880
Ion Ratio Lower Upper
75 100
77 30.9 22.3 41.3

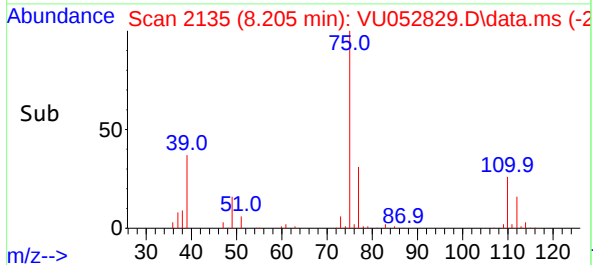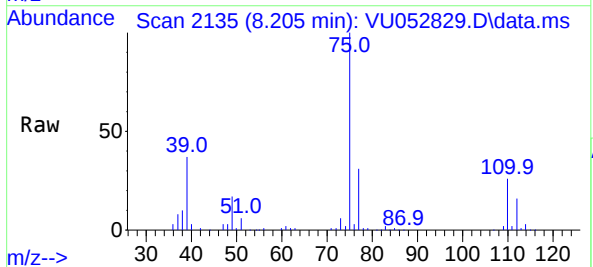







#45
1,1,2-Trichloroethane
Concen: 47.548 ug/L
RT: 8.395 min Scan# 2194
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Instrument :
MSVOA_U
ClientSampleId :
A44G7MS

Tgt Ion: 97 Resp: 105319




Ion	Ratio	Lower	Upper
97	100		
99	63.1	44.7	83.1
83	85.2	60.3	112.1
85	54.6	38.3	71.1

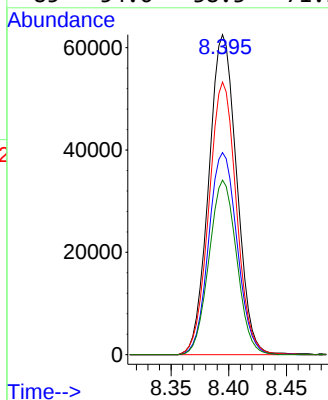


#46
Tetrachloroethene
Concen: 45.235 ug/L
RT: 8.549 min Scan# 2242
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:164 Resp: 87222

Ion	Ratio	Lower	Upper
164	100		
129	92.6	64.8	120.3
131	85.6	61.2	113.6
166	125.4	89.2	165.8



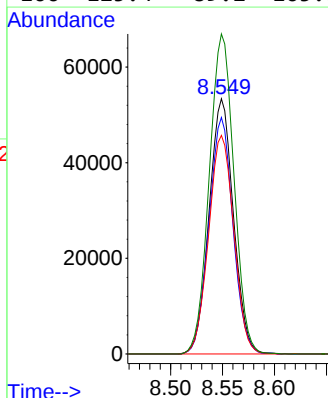





#48
2-Hexanone
Concen: 92.982 ug/L
RT: 8.681 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 43 Resp: 200730
Ion Ratio Lower Upper
43 100
58 61.4 48.0 72.0
57 22.5 16.8 25.2
100 15.9 12.7 19.1

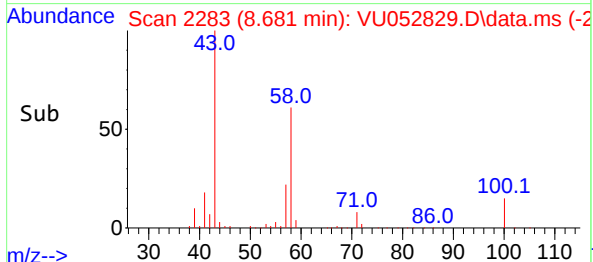

#49
Dibromochloromethane
Concen: 46.493 ug/L
RT: 8.803 min Scan# 2321
Delta R.T. -0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 129 Resp: 123153
Ion Ratio Lower Upper
129 100
127 76.3 53.2 98.8


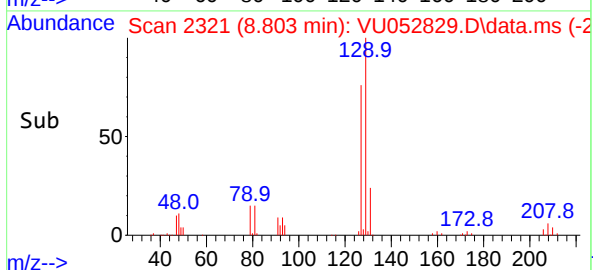






#50
1,2-Dibromoethane
Concen: 48.230 ug/L
RT: 8.919 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:107 Resp: 114976
Ion Ratio Lower Upper
107 100
109 94.6 65.5 121.6
188 4.2 3.2 4.8

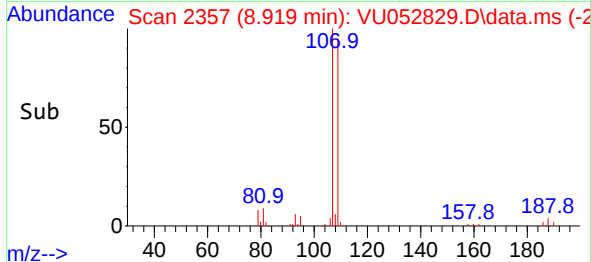

#51
Chlorobenzene
Concen: 46.160 ug/L
RT: 9.443 min Scan# 2520
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:112 Resp: 286750
Ion Ratio Lower Upper
112 100
114 31.5 22.8 42.4
77 57.8 45.9 68.9


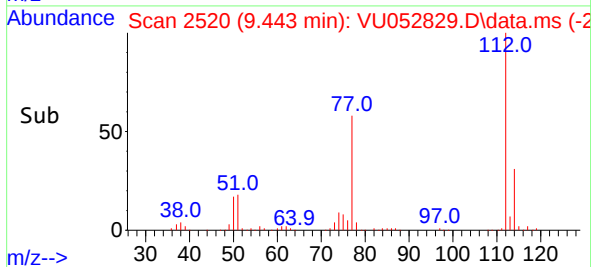

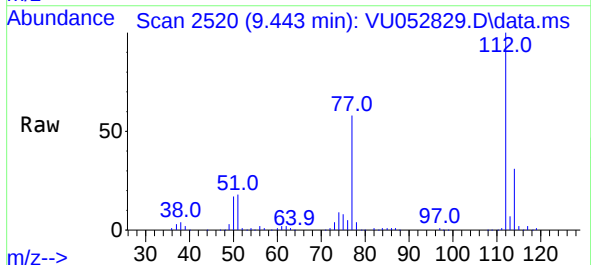




#52
Ethylbenzene
Concen: 48.025 ug/L
RT: 9.565 min Scan# 2558
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 91 Resp: 463415
Ion Ratio Lower Upper
91 100
106 31.6 22.0 40.8



#53
m,p-Xylene
Concen: 48.529 ug/L
RT: 9.690 min Scan# 2597
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 106 Resp: 189573
Ion Ratio Lower Upper
106 100
91 197.7 137.4 255.2


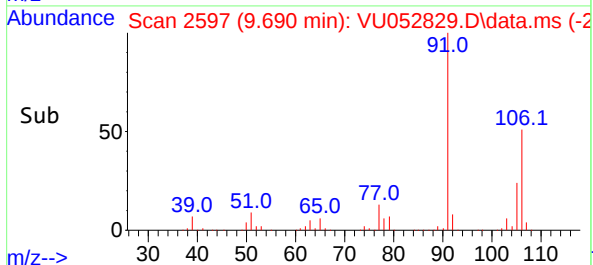

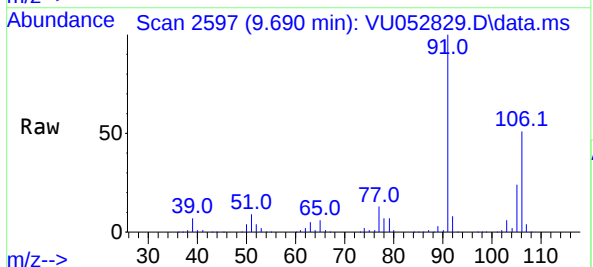




#54
o-xylene
Concen: 49.535 ug/L
RT: 10.095 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:106 Resp: 184727
Ion Ratio Lower Upper
106 100
91 210.4 143.4 266.2

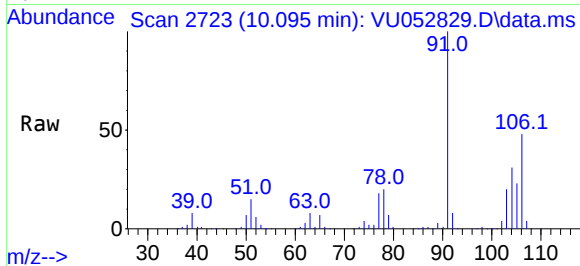

#55
Styrene
Concen: 48.754 ug/L
RT: 10.108 min Scan# 2727
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:104 Resp: 311991
Ion Ratio Lower Upper
104 100
78 46.9 31.9 59.2

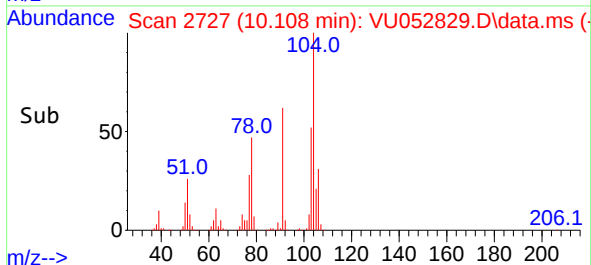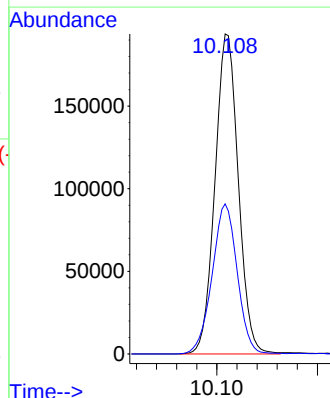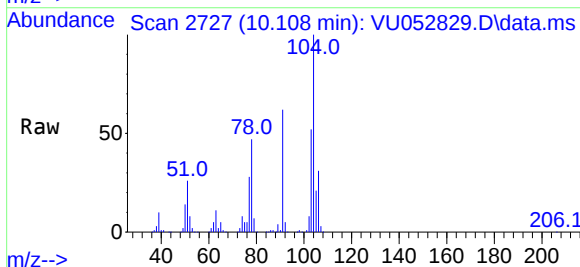



#57

1,1,2,2-Tetrachloroethane

Concen: 46.907 ug/L

RT: 10.777 min Scan# 2935

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :

A44G7MS





Tgt Ion: 83 Resp: 168146

Ion Ratio Lower Upper

83 100

85 64.0 45.0 83.6

131 10.6 8.6 12.8



#59

Bromoform

Concen: 46.327 ug/L

RT: 10.285 min Scan# 2782

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22




Tgt Ion:173 Resp: 95782


Ion Ratio Lower Upper

173 100

175 48.4 37.7 56.5

254 9.9 8.3 12.5


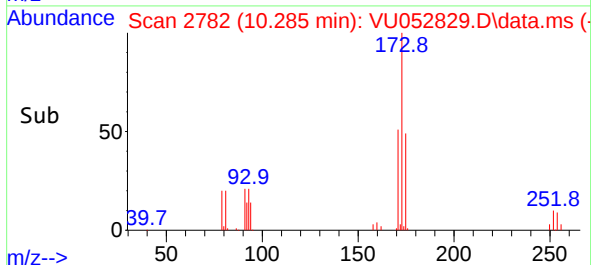

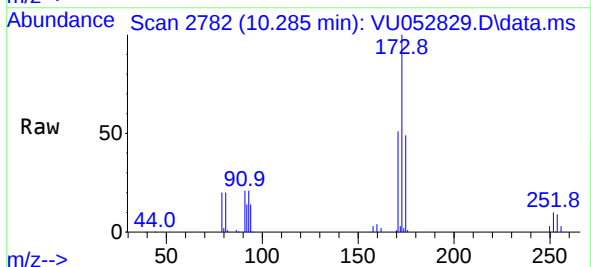




#60
1,2,3-Trichloropropane
Concen: 45.355 ug/L
RT: 10.819 min Scan# 2948
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion: 75 Resp: 132738
Ion Ratio Lower Upper
75 100
77 31.9 25.8 38.8
110 41.7 32.4 48.6

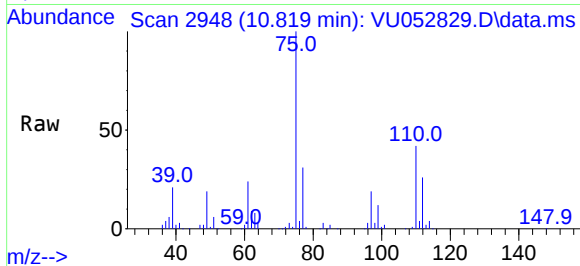

#61
Isopropylbenzene
Concen: 47.992 ug/L
RT: 10.481 min Scan# 2843
Delta R.T. 0.003 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion: 105 Resp: 467653
Ion Ratio Lower Upper
105 100
120 26.6 21.4 32.2
77 15.1 12.2 18.2


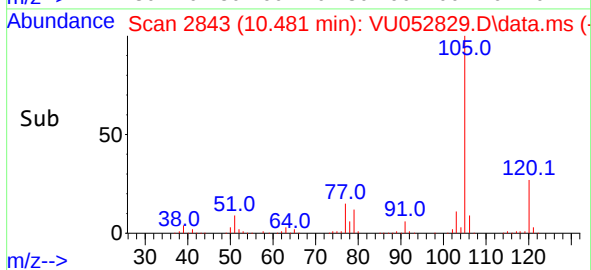

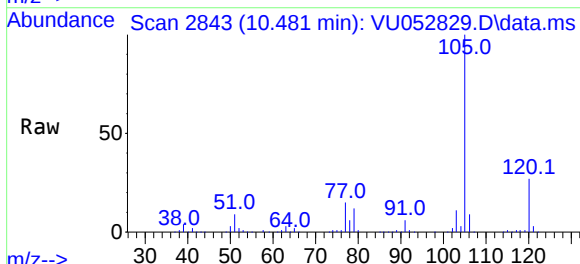




#62
1,3,5-Trimethylbenzene
Concen: 48.735 ug/L
RT: 11.082 min Scan# 3030
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:105 Resp: 395417
Ion Ratio Lower Upper
105 100
120 51.3 40.4 60.6

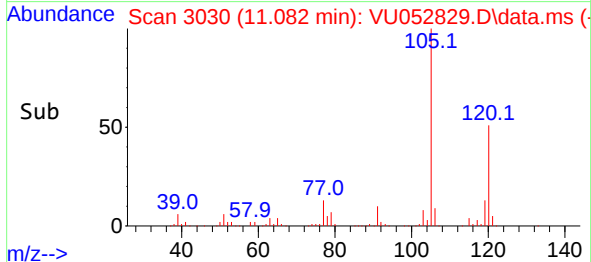

#63
1,2,4-Trimethylbenzene
Concen: 49.597 ug/L
RT: 11.462 min Scan# 3148
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:105 Resp: 389401
Ion Ratio Lower Upper
105 100
120 47.0 38.1 57.1


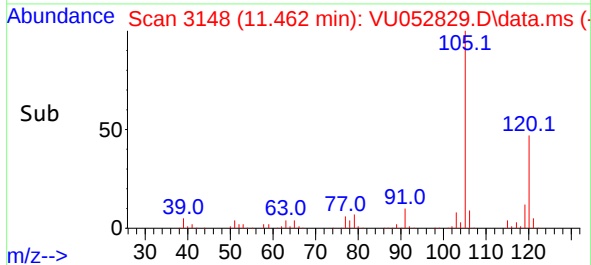

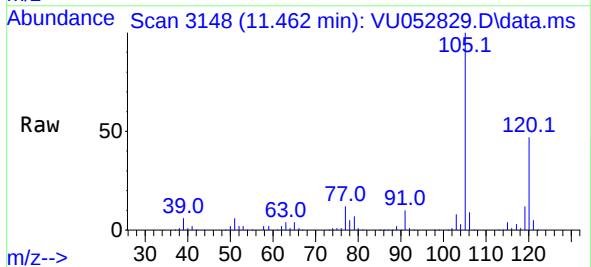


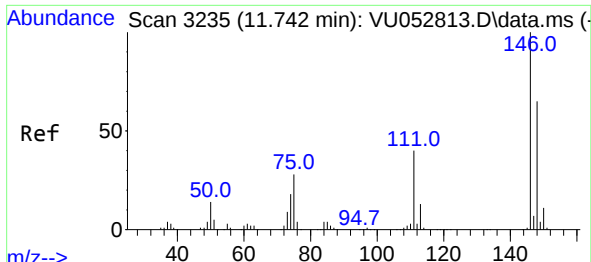

#64
1,3-Dichlorobenzene
Concen: 45.038 ug/L
RT: 11.742 min Scan# 3235
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22




Instrument :
MSVOA_U
ClientSampleId :
A44G7MS


Tgt Ion:146 Resp: 221424
Ion Ratio Lower Upper
146 100
111 39.3 27.8 51.6
148 64.9 45.5 84.5

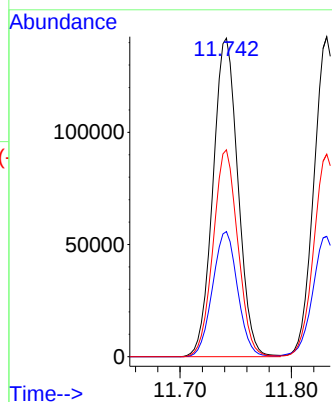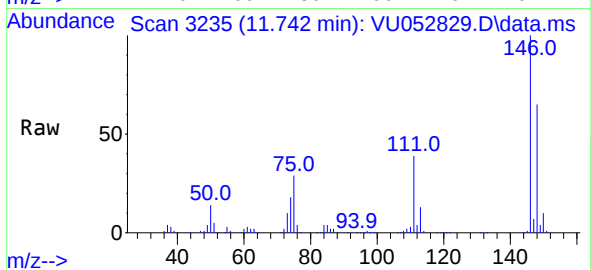

#65
1,4-Dichlorobenzene
Concen: 43.835 ug/L
RT: 11.832 min Scan# 3263
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:146 Resp: 223101
Ion Ratio Lower Upper
146 100
111 37.6 26.7 49.7
148 63.3 45.6 84.6

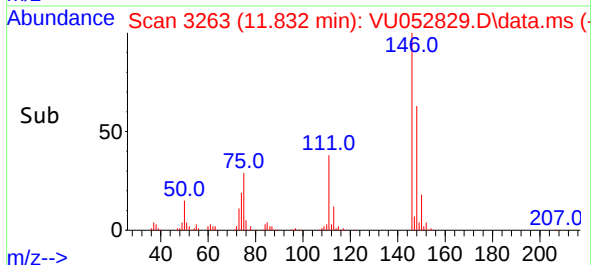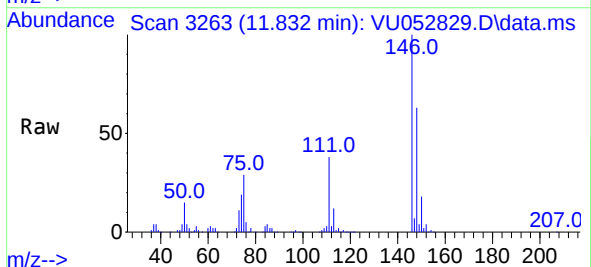



#67

1,2-Dichlorobenzene

Concen: 45.989 ug/L

RT: 12.208 min Scan# 31

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :

A44G7MS





Tgt Ion:146 Resp: 228693

Ion Ratio Lower Upper

146 100

111 41.4 33.2 49.8

148 63.3 50.2 75.4

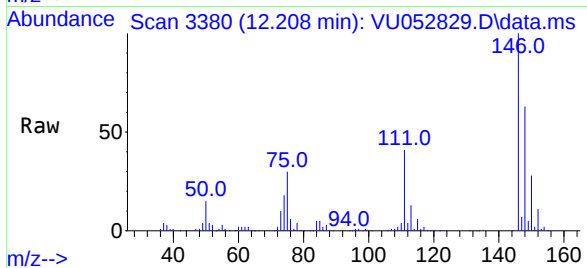

#68

1,2-Dibromo-3-chloropropane

Concen: 44.584 ug/L

RT: 12.989 min Scan# 3623

Delta R.T. -0.003 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22




Tgt Ion: 75 Resp: 37402


Ion Ratio Lower Upper

75 100

155 89.6 69.2 103.8

157 113.5 91.2 136.8

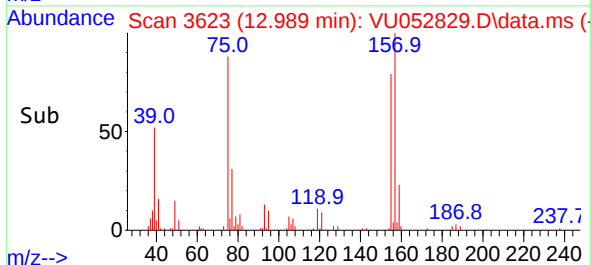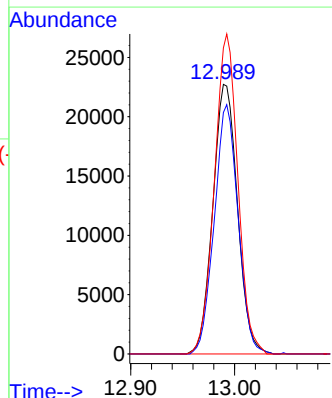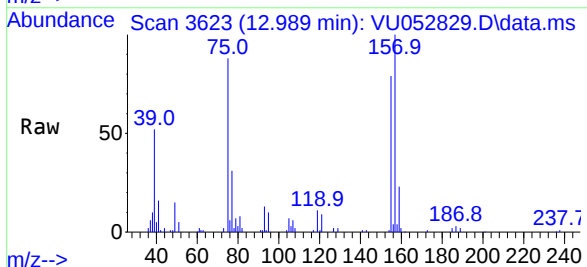



#69

1,3,5-Trichlorobenzene

Concen: 43.199 ug/L

RT: 13.214 min Scan# 3693

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22

Instrument :

MSVOA_U

ClientSampleId :

A44G7MS

Tgt Ion:180 Resp: 157228





Ion Ratio Lower Upper

180 100

182 94.9 77.0 115.6

184 30.4 24.4 36.6

145 28.5 23.3 34.9

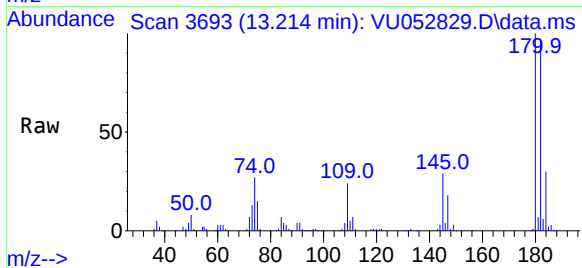

#70

1,2,4-trichlorobenzene

Concen: 42.348 ug/L

RT: 13.835 min Scan# 3886

Delta R.T. -0.000 min

Lab File: VU052829.D

Acq: 26 Jan 2023 20:22




Tgt Ion:180 Resp: 129223


Ion Ratio Lower Upper

180 100

182 97.3 78.2 117.2

145 28.5 23.4 35.2


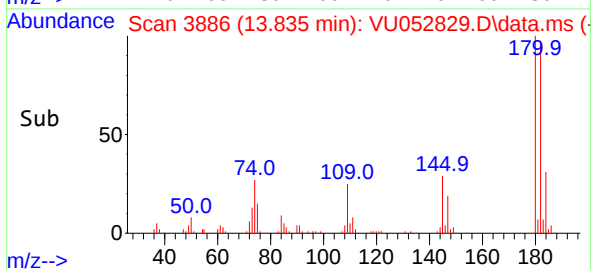

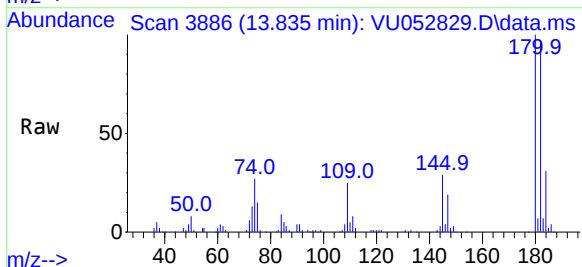


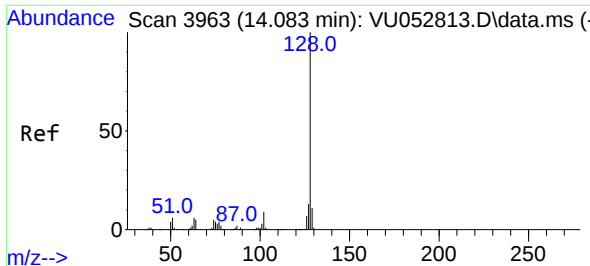

#71
Naphthalene
Concen: 45.007 ug/L
RT: 14.082 min Scan# 3963
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Instrument :
MSVOA_U
ClientSampleId :
A44G7MS

Tgt Ion:	128	Resp:	394671
Ion	Ratio	Lower	Upper
128	100		
127	12.8	10.3	15.5
129	10.8	8.8	13.2

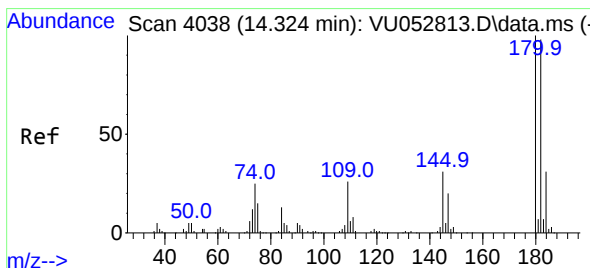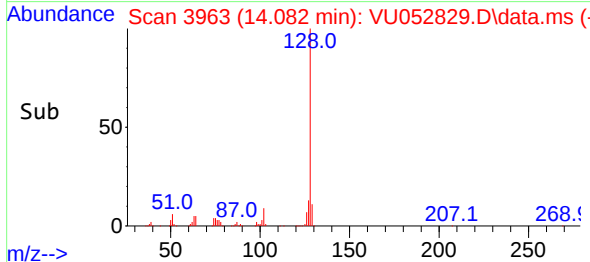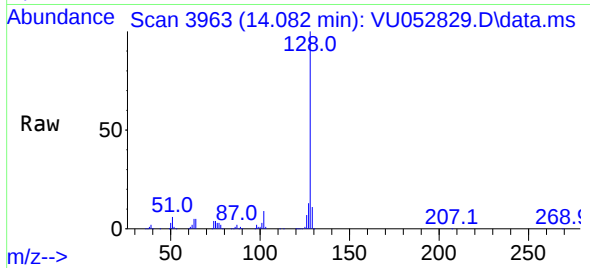

#72
1,2,3-Trichlorobenzene
Concen: 43.689 ug/L
RT: 14.324 min Scan# 4038
Delta R.T. -0.000 min
Lab File: VU052829.D
Acq: 26 Jan 2023 20:22

Tgt Ion:	180	Resp:	140891
Ion	Ratio	Lower	Upper
180	100		
182	95.6	77.5	116.3
145	30.5	24.2	36.4

