

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052817.D
 Acq On : 26 Jan 2023 15:15
 Operator : JC/MD
 Sample : VU0126WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	94	rVB	128320	149186	13.54%	1.872%
2	1.912	169	178	202	rVB	105234	141811	12.87%	1.780%
3	2.224	272	275	280	rBV3	365	311	0.03%	0.004%
4	2.314	300	303	308	rVB3	437	303	0.03%	0.004%
5	2.565	369	381	398	rVV	241685	391710	35.56%	4.916%
6	2.636	398	403	408	rVB2	364	373	0.03%	0.005%
7	2.703	421	424	426	rBV	374	246	0.02%	0.003%
8	2.793	444	452	461	rVB2	1888	3081	0.28%	0.039%
9	2.838	462	466	470	rBV2	324	280	0.03%	0.004%
10	3.047	523	531	539	rVB	1615	2599	0.24%	0.033%
11	3.118	547	553	556	rBV2	321	396	0.04%	0.005%
12	3.176	567	571	572	rBV	345	242	0.02%	0.003%
13	3.276	597	602	605	rBV2	223	281	0.03%	0.004%
14	3.314	609	614	617	rBV2	208	246	0.02%	0.003%
15	3.353	624	626	631	rVB2	355	246	0.02%	0.003%
16	3.555	684	689	691	rBV2	282	313	0.03%	0.004%
17	3.899	792	796	799	rBV2	251	264	0.02%	0.003%
18	4.079	846	852	857	rBV2	360	339	0.03%	0.004%
19	4.118	857	864	868	rBV2	281	418	0.04%	0.005%
20	4.186	882	885	888	rVB2	308	244	0.02%	0.003%
21	4.221	890	896	899	rBV2	258	328	0.03%	0.004%
22	4.301	918	921	927	rBV2	355	350	0.03%	0.004%
23	4.337	927	932	935	rVV	292	264	0.02%	0.003%
24	4.462	967	971	979	rBV2	213	339	0.03%	0.004%
25	4.626	1008	1022	1058	rBV	74548	201800	18.32%	2.533%
26	4.764	1062	1065	1066	rBV	398	244	0.02%	0.003%
27	4.874	1096	1099	1102	rBV2	405	311	0.03%	0.004%
28	4.909	1107	1110	1114	rVB3	390	374	0.03%	0.005%
29	4.931	1115	1117	1121	rBV2	314	276	0.03%	0.003%
30	5.057	1139	1156	1179	rBV	208356	450127	40.86%	5.649%
31	5.288	1222	1228	1232	rBV2	496	665	0.06%	0.008%
32	5.620	1326	1331	1333	rBV2	398	383	0.03%	0.005%
33	5.722	1338	1363	1388	rBV2	407226	1101619	100.00%	13.825%
34	6.047	1462	1464	1467	rVB2	372	251	0.02%	0.003%
35	6.111	1478	1484	1488	rBV3	481	507	0.05%	0.006%
36	6.169	1498	1502	1507	rBV2	284	316	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052817.D
 Acq On : 26 Jan 2023 15:15
 Operator : JC/MD
 Sample : VU0126WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.247	1512	1526	1548	rBV	311868	587997	53.38%	7.379%
38	6.349	1556	1558	1564	rVB3	337	324	0.03%	0.004%
39	6.436	1583	1585	1592	rVB2	462	497	0.05%	0.006%
40	6.481	1594	1599	1606	rVB3	240	293	0.03%	0.004%
41	6.526	1606	1613	1621	rBV6	1795	2749	0.25%	0.034%
42	6.632	1638	1646	1649	rBV2	336	508	0.05%	0.006%
43	6.687	1649	1663	1686	rVV	253429	487411	44.24%	6.117%
44	6.767	1686	1688	1693	rVV2	562	374	0.03%	0.005%
45	6.809	1697	1701	1706	rVB2	561	505	0.05%	0.006%
46	7.015	1760	1765	1771	rBV2	245	403	0.04%	0.005%
47	7.060	1774	1779	1784	rVB2	396	555	0.05%	0.007%
48	7.179	1808	1816	1826	rBV2	1601	2576	0.23%	0.032%
49	7.311	1851	1857	1860	rBV	320	302	0.03%	0.004%
50	7.562	1918	1935	1950	rBV	133904	235200	21.35%	2.952%
51	7.693	1968	1976	1983	rBV5	1240	2144	0.19%	0.027%
52	7.761	1995	1997	2002	rVB2	477	378	0.03%	0.005%
53	7.790	2002	2006	2007	rBV2	563	444	0.04%	0.006%
54	7.896	2024	2039	2059	rBV	512128	878091	79.71%	11.020%
55	8.176	2114	2126	2146	rBV	95276	161246	14.64%	2.024%
56	8.311	2165	2168	2172	rVB3	559	428	0.04%	0.005%
57	8.632	2255	2268	2302	rVV2	230131	444621	40.36%	5.580%
58	8.761	2305	2308	2312	rVB2	618	488	0.04%	0.006%
59	8.861	2336	2339	2345	rVB	340	286	0.03%	0.004%
60	8.922	2353	2358	2362	rBV3	471	451	0.04%	0.006%
61	9.414	2499	2511	2541	rBV	441682	720271	65.38%	9.039%
62	9.565	2554	2558	2571	rVB4	762	1240	0.11%	0.016%
63	10.034	2699	2704	2707	rBV2	355	386	0.04%	0.005%
64	10.095	2719	2723	2726	rBV2	480	419	0.04%	0.005%
65	10.295	2782	2785	2790	rVB	337	284	0.03%	0.004%
66	10.324	2790	2794	2796	rBV2	264	242	0.02%	0.003%
67	10.478	2837	2842	2844	rBV2	581	459	0.04%	0.006%
68	10.584	2869	2875	2878	rBV2	362	435	0.04%	0.005%
69	10.626	2881	2888	2891	rBV2	252	370	0.03%	0.005%
70	10.751	2915	2927	2944	rBV	325873	529949	48.11%	6.651%
71	10.812	2944	2946	2950	rVB2	681	425	0.04%	0.005%
72	10.944	2983	2987	2992	rBV2	353	414	0.04%	0.005%
73	11.092	3027	3033	3040	rBV4	671	981	0.09%	0.012%
74	11.127	3040	3044	3047	rBV3	331	326	0.03%	0.004%
75	11.272	3084	3089	3091	rBV2	275	270	0.02%	0.003%
76	11.468	3144	3150	3158	rVB2	827	1134	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052817.D
 Acq On : 26 Jan 2023 15:15
 Operator : JC/MD
 Sample : VU0126WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.745	3229	3236	3243	rVB4	1966	2472	0.22%	0.031%
78	11.809	3243	3256	3279	rBV	416903	663296	60.21%	8.324%
79	11.944	3295	3298	3301	rBV2	310	274	0.02%	0.003%
80	11.976	3305	3308	3312	rBV3	316	262	0.02%	0.003%
81	12.188	3361	3374	3399	rBV	463435	750135	68.09%	9.414%
82	12.532	3475	3481	3487	rBV2	355	396	0.04%	0.005%
83	12.565	3487	3491	3497	rBV	342	405	0.04%	0.005%
84	12.902	3592	3596	3600	rBV	426	381	0.03%	0.005%
85	12.992	3618	3624	3628	rBV	304	319	0.03%	0.004%
86	13.079	3647	3651	3653	rBV	406	364	0.03%	0.005%
87	13.114	3656	3662	3663	rBV2	276	271	0.02%	0.003%
88	13.221	3687	3695	3704	rBV5	2651	3796	0.34%	0.048%
89	13.333	3727	3730	3733	rBV	360	291	0.03%	0.004%
90	13.462	3766	3770	3773	rBV3	333	319	0.03%	0.004%
91	13.841	3880	3888	3897	rBV2	4774	6643	0.60%	0.083%
92	13.986	3931	3933	3940	rBV2	397	496	0.05%	0.006%
93	14.089	3954	3965	3984	rVB2	6485	11632	1.06%	0.146%
94	14.327	4031	4039	4050	rBV4	4699	7246	0.66%	0.091%
95	14.671	4142	4146	4153	rVB2	535	496	0.05%	0.006%
96	14.716	4156	4160	4163	rBV2	375	380	0.03%	0.005%
97	14.761	4172	4174	4177	rBV3	421	303	0.03%	0.004%
98	14.886	4210	4213	4215	rBV	397	268	0.02%	0.003%
99	15.002	4246	4249	4252	rBV3	554	439	0.04%	0.006%
100	16.056	4575	4577	4579	rBV	698	439	0.04%	0.006%




Sum of corrected areas: 7968242

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052817.D
Acq On : 26 Jan 2023 15:15
Operator : JC/MD
Sample : VU0126WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

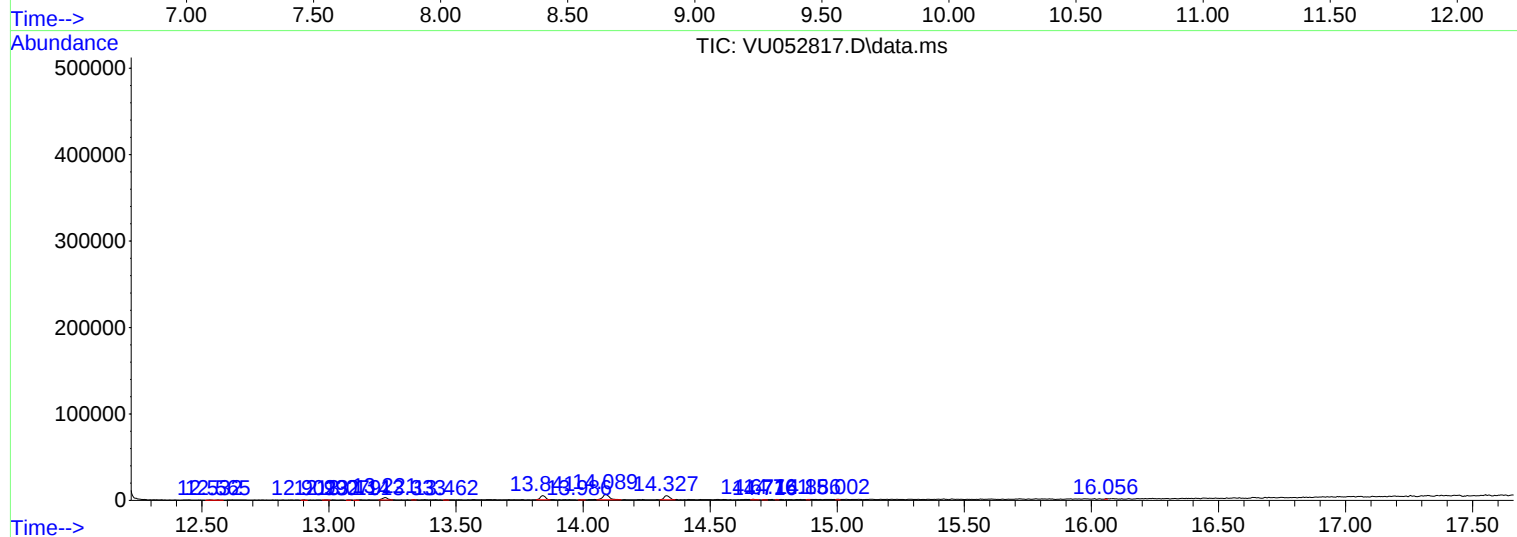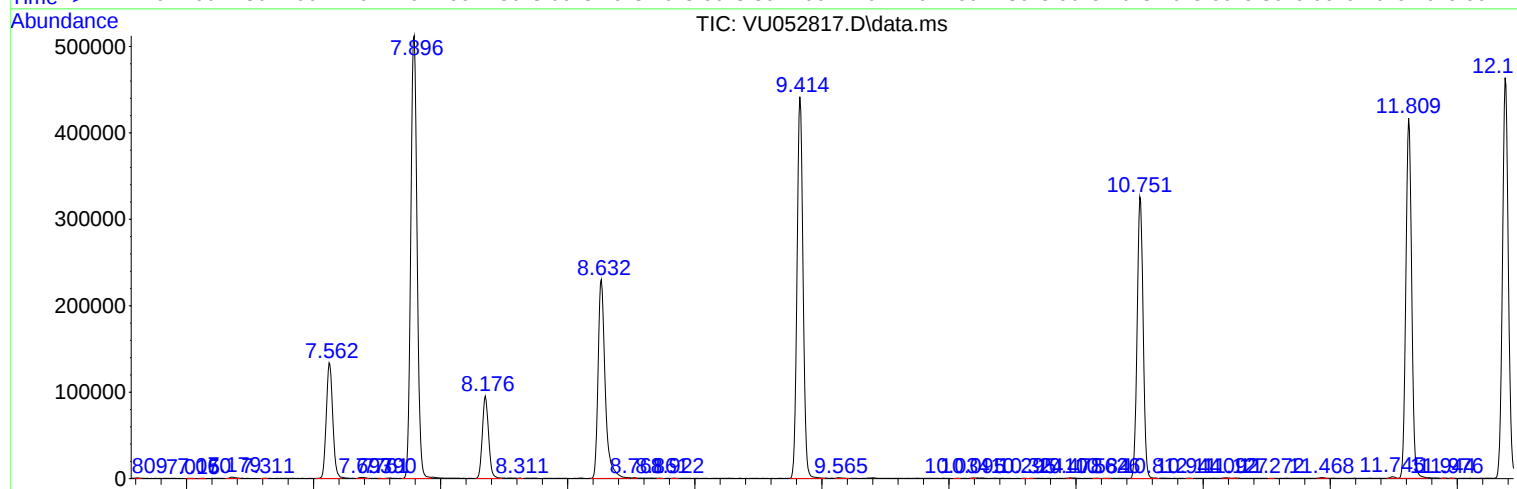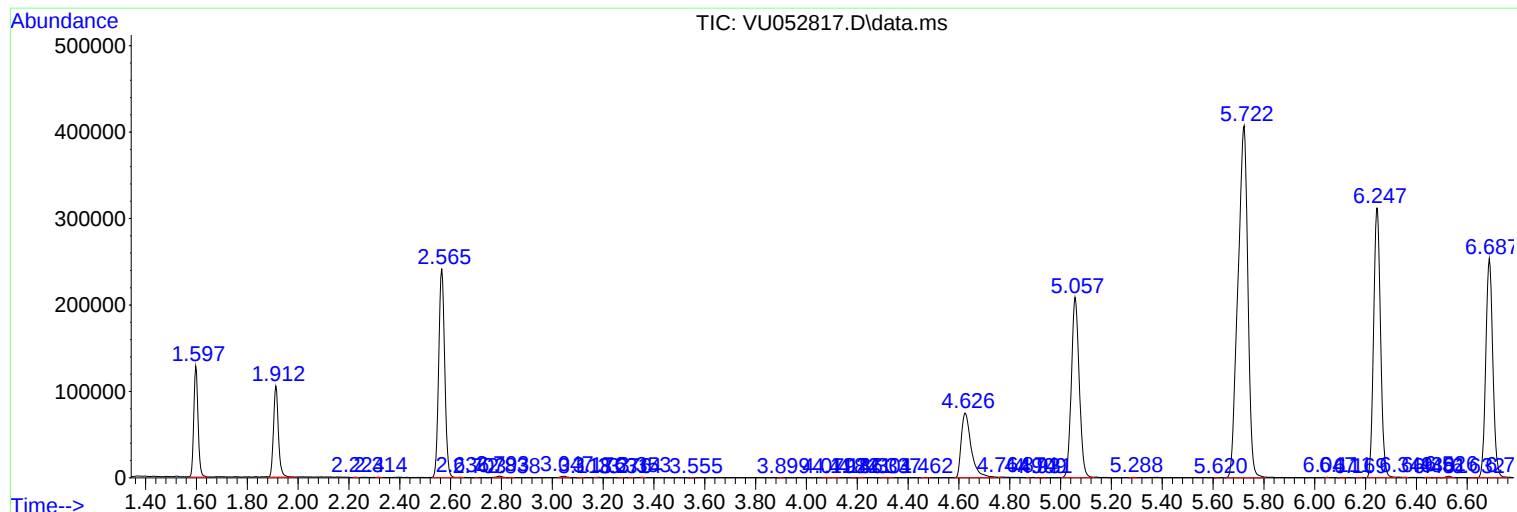

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052817.D
Acq On : 26 Jan 2023 15:15
Operator : JC/MD
Sample : VU0126WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052817.D
Acq On : 26 Jan 2023 15:15
Operator : JC/MD
Sample : VU0126WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------