

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052821.D
 Acq On : 26 Jan 2023 17:15
 Operator : JC/MD
 Sample : 01316-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	51	57	64	rVB4	1503	2129	0.19%	0.025%
2	1.597	72	80	94	rBV	119161	146754	13.09%	1.755%
3	1.909	169	177	192	rBV	101763	143909	12.84%	1.721%
4	2.324	301	306	309	rBV3	577	529	0.05%	0.006%
5	2.562	367	380	394	rBV	239961	390763	34.86%	4.672%
6	2.633	394	402	425	rVB	17465	36803	3.28%	0.440%
7	2.787	442	450	461	rVB	3218	5458	0.49%	0.065%
8	3.041	522	529	536	rVV4	1623	2690	0.24%	0.032%
9	3.179	556	572	590	rBV2	5055	11587	1.03%	0.139%
10	3.253	591	595	600	rBV3	372	400	0.04%	0.005%
11	3.388	631	637	639	rBV2	219	264	0.02%	0.003%
12	3.719	736	740	748	rBV2	315	567	0.05%	0.007%
13	3.832	771	775	779	rBV2	285	271	0.02%	0.003%
14	3.916	797	801	804	rBV2	299	271	0.02%	0.003%
15	4.623	1005	1021	1060	rBV2	78427	214274	19.12%	2.562%
16	4.973	1127	1130	1132	rBV	365	316	0.03%	0.004%
17	5.057	1140	1156	1176	rBV	208800	452672	40.39%	5.413%
18	5.173	1190	1192	1196	rVB3	441	282	0.03%	0.003%
19	5.199	1196	1200	1205	rVB2	363	298	0.03%	0.004%
20	5.234	1208	1211	1216	rBV2	247	272	0.02%	0.003%
21	5.282	1216	1226	1229	rBV3	729	1007	0.09%	0.012%
22	5.362	1248	1251	1262	rBV4	514	627	0.06%	0.007%
23	5.424	1266	1270	1276	rBV	296	357	0.03%	0.004%
24	5.719	1341	1362	1381	rBV2	418351	1120876	100.00%	13.402%
25	5.874	1407	1410	1413	rBV2	331	246	0.02%	0.003%
26	6.118	1481	1486	1490	rVB3	349	402	0.04%	0.005%
27	6.160	1496	1499	1503	rBV	221	231	0.02%	0.003%
28	6.243	1511	1525	1542	rBV	335252	631885	56.37%	7.555%
29	6.523	1606	1612	1613	rBV2	1629	1175	0.10%	0.014%
30	6.588	1627	1632	1633	rBV	328	231	0.02%	0.003%
31	6.684	1646	1662	1690	rBV	256027	491818	43.88%	5.881%
32	6.797	1694	1697	1698	rBV2	579	358	0.03%	0.004%
33	6.806	1698	1700	1707	rVB3	662	415	0.04%	0.005%
34	6.932	1735	1739	1742	rBV	282	240	0.02%	0.003%
35	7.067	1776	1781	1784	rVB2	467	388	0.03%	0.005%
36	7.089	1784	1788	1790	rBV2	355	278	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052821.D
 Acq On : 26 Jan 2023 17:15
 Operator : JC/MD
 Sample : 01316-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	7.157	1803	1809	1811	rBV2	290	334	0.03%	0.004%
38	7.186	1811	1818	1826	rBV3	1979	3070	0.27%	0.037%
39	7.269	1837	1844	1847	rVB2	227	297	0.03%	0.004%
40	7.562	1921	1935	1954	rBV	138867	241943	21.59%	2.893%
41	7.684	1968	1973	1977	rBV4	884	1096	0.10%	0.013%
42	7.748	1989	1993	1999	rBV2	273	363	0.03%	0.004%
43	7.796	1999	2008	2021	rVB3	3713	6727	0.60%	0.080%
44	7.893	2025	2038	2055	rBV	521152	889460	79.35%	10.635%
45	8.079	2091	2096	2098	rBV	371	240	0.02%	0.003%
46	8.176	2114	2126	2141	rBV	97259	163025	14.54%	1.949%
47	8.317	2166	2170	2174	rVB3	386	393	0.04%	0.005%
48	8.350	2174	2180	2185	rVB3	560	851	0.08%	0.010%
49	8.378	2185	2189	2192	rBV	547	512	0.05%	0.006%
50	8.398	2192	2195	2198	rVB	447	315	0.03%	0.004%
51	8.468	2204	2217	2227	rBV3	7207	12615	1.13%	0.151%
52	8.552	2237	2243	2249	rVB3	1279	1236	0.11%	0.015%
53	8.636	2255	2269	2296	rBV2	233467	473232	42.22%	5.658%
54	8.777	2311	2313	2315	rBV2	460	298	0.03%	0.004%
55	8.925	2352	2359	2362	rBV2	425	474	0.04%	0.006%
56	9.317	2478	2481	2483	rBV	316	252	0.02%	0.003%
57	9.333	2483	2486	2489	rVV2	285	260	0.02%	0.003%
58	9.414	2497	2511	2533	rBV	453205	753483	67.22%	9.009%
59	9.568	2551	2559	2568	rBV2	2232	3373	0.30%	0.040%
60	9.690	2589	2597	2607	rBV2	1489	2451	0.22%	0.029%
61	10.102	2719	2725	2727	rBV3	1241	1201	0.11%	0.014%
62	10.247	2766	2770	2772	rBV2	319	241	0.02%	0.003%
63	10.414	2818	2822	2827	rBV2	227	251	0.02%	0.003%
64	10.481	2836	2843	2852	rBV4	1575	2227	0.20%	0.027%
65	10.578	2860	2873	2877	rBV3	729	1090	0.10%	0.013%
66	10.642	2889	2893	2896	rBV2	280	266	0.02%	0.003%
67	10.755	2914	2928	2945	rBV	345154	559286	49.90%	6.687%
68	10.890	2959	2970	2980	rVB3	5904	9657	0.86%	0.115%
69	10.986	2995	3000	3002	rBV2	214	234	0.02%	0.003%
70	11.095	3031	3034	3041	rVB3	432	432	0.04%	0.005%
71	11.131	3041	3045	3054	rBV2	280	518	0.05%	0.006%
72	11.234	3075	3077	3081	rBV	250	234	0.02%	0.003%
73	11.472	3147	3151	3153	rBV	354	325	0.03%	0.004%
74	11.610	3190	3194	3196	rBV2	279	230	0.02%	0.003%
75	11.742	3228	3235	3243	rBV3	2593	3121	0.28%	0.037%
76	11.809	3243	3256	3282	rBV	450952	723090	64.51%	8.646%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052821.D
 Acq On : 26 Jan 2023 17:15
 Operator : JC/MD
 Sample : 01316-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	12.057	3324	3333	3348	rVB4	6592	11476	1.02%	0.137%
78	12.189	3361	3374	3396	rBV	485823	782842	69.84%	9.360%
79	12.423	3442	3447	3452	rBV	370	496	0.04%	0.006%
80	12.497	3467	3470	3478	rBV	379	447	0.04%	0.005%
81	12.706	3529	3535	3538	rBV2	307	370	0.03%	0.004%
82	12.767	3544	3554	3562	rBV	2130	3353	0.30%	0.040%
83	12.886	3587	3591	3596	rVV4	624	669	0.06%	0.008%
84	12.996	3619	3625	3635	rVB5	2008	2843	0.25%	0.034%
85	13.217	3684	3694	3704	rVB4	8695	13237	1.18%	0.158%
86	13.443	3761	3764	3769	rVB2	399	333	0.03%	0.004%
87	13.632	3819	3823	3828	rBV2	333	328	0.03%	0.004%
88	13.722	3845	3851	3857	rVB3	386	534	0.05%	0.006%
89	13.844	3882	3889	3896	rBV4	928	1354	0.12%	0.016%
90	13.996	3932	3936	3940	rBV2	424	458	0.04%	0.005%
91	14.086	3961	3964	3970	rBV3	789	788	0.07%	0.009%
92	14.327	4029	4039	4052	rBV3	13053	20740	1.85%	0.248%
93	14.632	4130	4134	4137	rVB4	399	350	0.03%	0.004%
94	14.841	4195	4199	4204	rBV2	456	578	0.05%	0.007%
95	15.250	4324	4326	4330	rBV3	386	352	0.03%	0.004%
96	15.500	4401	4404	4406	rBV	443	276	0.02%	0.003%
97	15.574	4424	4427	4434	rBV3	567	519	0.05%	0.006%
98	15.603	4434	4436	4441	rBV4	562	516	0.05%	0.006%
99	15.735	4474	4477	4479	rBV3	638	411	0.04%	0.005%
100	15.986	4552	4555	4557	rBV2	619	392	0.03%	0.005%




Sum of corrected areas: 8363408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052821.D
Acq On : 26 Jan 2023 17:15
Operator : JC/MD
Sample : 01316-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

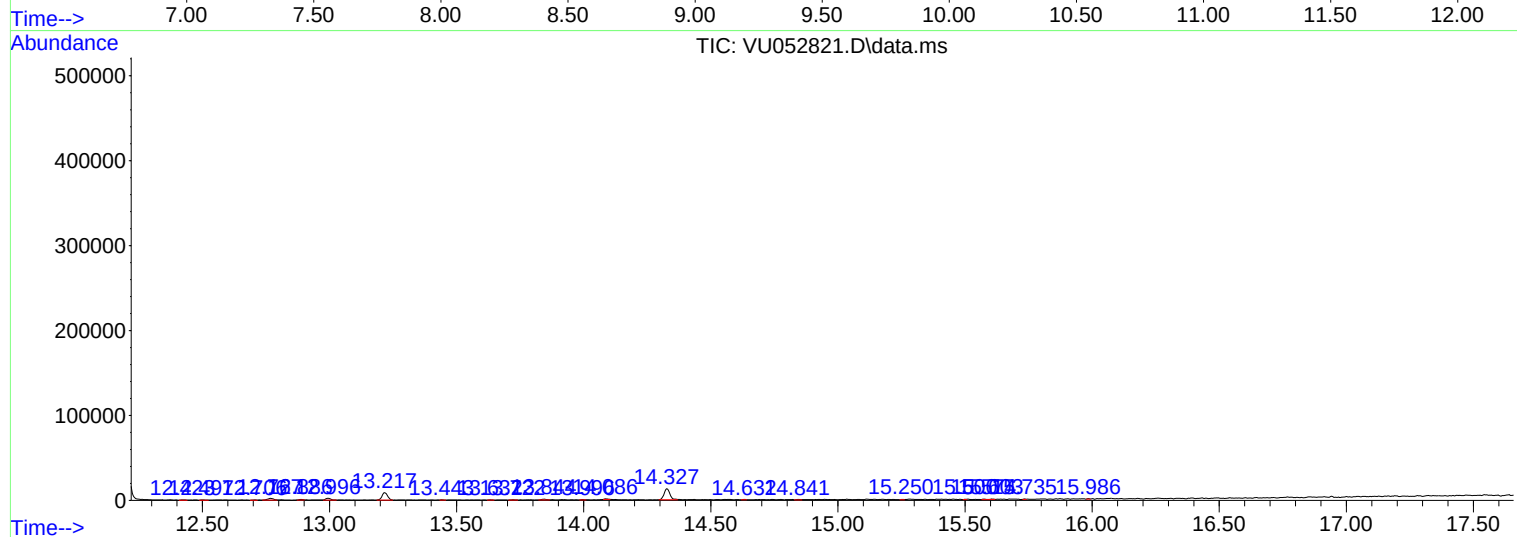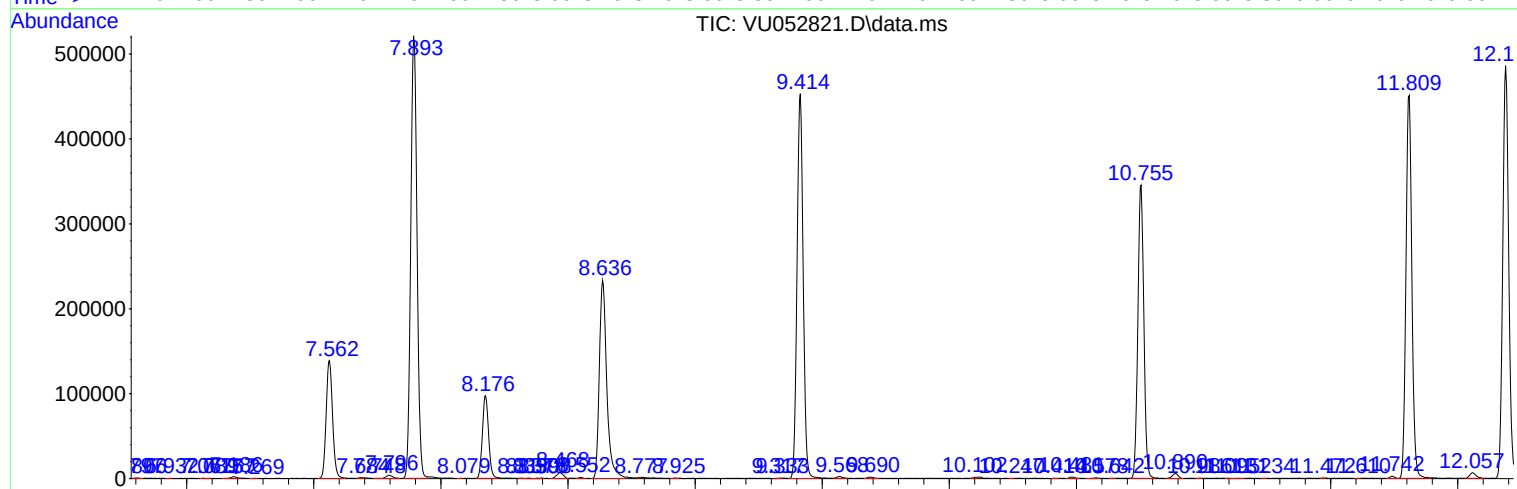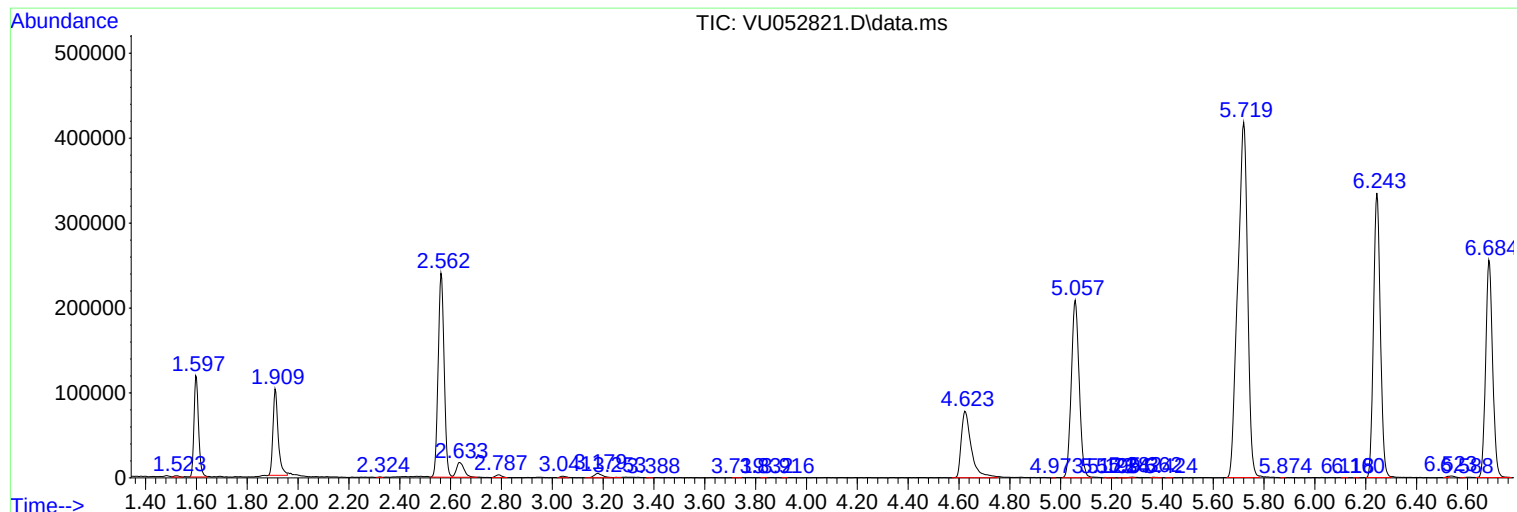

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052821.D
Acq On : 26 Jan 2023 17:15
Operator : JC/MD
Sample : 01316-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052821.D
Acq On : 26 Jan 2023 17:15
Operator : JC/MD
Sample : 01316-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc