

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052822.D
 Acq On : 26 Jan 2023 17:39
 Operator : JC/MD
 Sample : 01316-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	117241	142896	12.88%	1.741%
2	1.912	169	178	197	rBV	95048	138549	12.49%	1.688%
3	2.028	211	214	219	rBV3	901	878	0.08%	0.011%
4	2.282	291	293	299	rVB	513	235	0.02%	0.003%
5	2.350	311	314	318	rVB2	440	303	0.03%	0.004%
6	2.469	349	351	354	rVB3	488	298	0.03%	0.004%
7	2.562	368	380	396	rBV	236766	385449	34.74%	4.696%
8	2.649	397	407	427	rVB	13362	33498	3.02%	0.408%
9	2.793	442	452	461	rBV	1657	2751	0.25%	0.034%
10	2.954	499	502	505	rBV	301	227	0.02%	0.003%
11	3.044	523	530	537	rVV3	1155	1595	0.14%	0.019%
12	3.179	559	572	587	rVB2	3226	7254	0.65%	0.088%
13	3.244	587	592	596	rBV2	328	285	0.03%	0.003%
14	3.404	634	642	645	rBV2	296	369	0.03%	0.004%
15	3.623	705	710	714	rBV2	279	235	0.02%	0.003%
16	3.726	737	742	746	rVB2	274	293	0.03%	0.004%
17	3.752	746	750	753	rVB2	326	260	0.02%	0.003%
18	3.784	756	760	763	rBV2	371	400	0.04%	0.005%
19	3.951	807	812	817	rVB2	442	584	0.05%	0.007%
20	3.977	817	820	822	rBV	400	280	0.03%	0.003%
21	4.346	932	935	941	rVB	297	264	0.02%	0.003%
22	4.633	1010	1024	1047	rBV	69644	198521	17.89%	2.418%
23	4.925	1110	1115	1117	rBV2	263	252	0.02%	0.003%
24	4.948	1119	1122	1126	rVB2	357	272	0.02%	0.003%
25	4.993	1132	1136	1140	rBV	423	363	0.03%	0.004%
26	5.057	1140	1156	1175	rBV	203697	445983	40.20%	5.433%
27	5.179	1190	1194	1197	rVB3	481	374	0.03%	0.005%
28	5.276	1218	1224	1226	rBV2	566	594	0.05%	0.007%
29	5.369	1247	1253	1254	rBV2	515	412	0.04%	0.005%
30	5.616	1324	1330	1332	rBV2	238	270	0.02%	0.003%
31	5.719	1340	1362	1382	rBV2	413581	1109404	100.00%	13.515%
32	5.915	1419	1423	1426	rBV2	294	226	0.02%	0.003%
33	5.967	1438	1439	1446	rVB2	290	248	0.02%	0.003%
34	5.999	1446	1449	1452	rVB2	418	247	0.02%	0.003%
35	6.173	1500	1503	1505	rBV	356	274	0.02%	0.003%
36	6.243	1510	1525	1544	rBV	331476	616745	55.59%	7.513%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052822.D
 Acq On : 26 Jan 2023 17:39
 Operator : JC/MD
 Sample : 01316-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.398	1569	1573	1576	rVB2	479	397	0.04%	0.005%
38	6.530	1604	1614	1615	rBV4	1031	1137	0.10%	0.014%
39	6.581	1625	1630	1633	rBV2	340	435	0.04%	0.005%
40	6.600	1633	1636	1639	rVV3	298	231	0.02%	0.003%
41	6.687	1648	1663	1684	rBV	254640	489356	44.11%	5.962%
42	7.092	1785	1789	1792	rVB	342	317	0.03%	0.004%
43	7.118	1792	1797	1798	rBV	355	360	0.03%	0.004%
44	7.182	1810	1817	1834	rVB5	2020	3866	0.35%	0.047%
45	7.346	1861	1868	1873	rVB2	245	319	0.03%	0.004%
46	7.401	1876	1885	1888	rBV2	306	447	0.04%	0.005%
47	7.562	1922	1935	1956	rBV	132898	235832	21.26%	2.873%
48	7.636	1956	1958	1963	rVB2	733	375	0.03%	0.005%
49	7.693	1969	1976	1981	rBV4	1398	1912	0.17%	0.023%
50	7.800	2000	2009	2020	rBV7	2586	5056	0.46%	0.062%
51	7.893	2024	2038	2056	rBV	509053	876265	78.99%	10.675%
52	8.176	2114	2126	2149	rVV	95725	161976	14.60%	1.973%
53	8.468	2208	2217	2231	rVB	10562	18144	1.64%	0.221%
54	8.574	2246	2250	2253	rBV	398	280	0.03%	0.003%
55	8.639	2257	2270	2298	rBV2	225605	468644	42.24%	5.709%
56	8.922	2355	2358	2363	rVB3	298	265	0.02%	0.003%
57	8.964	2363	2371	2374	rBV2	249	389	0.04%	0.005%
58	9.414	2497	2511	2535	rBV	453109	745999	67.24%	9.088%
59	9.565	2552	2558	2560	rBV3	716	787	0.07%	0.010%
60	9.684	2591	2595	2597	rVV	445	397	0.04%	0.005%
61	9.700	2597	2600	2604	rVB2	714	537	0.05%	0.007%
62	9.754	2615	2617	2622	rVB3	370	303	0.03%	0.004%
63	9.816	2633	2636	2639	rBV2	282	235	0.02%	0.003%
64	9.909	2660	2665	2671	rBV	307	405	0.04%	0.005%
65	9.986	2683	2689	2694	rBV2	275	446	0.04%	0.005%
66	10.115	2726	2729	2734	rVB	908	801	0.07%	0.010%
67	10.246	2766	2770	2772	rBV2	314	226	0.02%	0.003%
68	10.484	2837	2844	2851	rVB2	541	755	0.07%	0.009%
69	10.571	2868	2871	2873	rBV3	394	263	0.02%	0.003%
70	10.674	2897	2903	2906	rBV2	338	464	0.04%	0.006%
71	10.754	2915	2928	2950	rBV	341406	555649	50.09%	6.769%
72	10.890	2959	2970	2981	rBV3	10451	16627	1.50%	0.203%
73	10.951	2986	2989	2995	rBV2	252	282	0.03%	0.003%
74	11.021	3006	3011	3016	rBV2	221	352	0.03%	0.004%
75	11.047	3016	3019	3023	rVB	410	288	0.03%	0.004%
76	11.221	3069	3073	3080	rBV2	400	570	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052822.D
 Acq On : 26 Jan 2023 17:39
 Operator : JC/MD
 Sample : 01316-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.291	3092	3095	3101	rVB	213	224	0.02%	0.003%
78	11.475	3147	3152	3156	rBV3	608	707	0.06%	0.009%
79	11.555	3174	3177	3180	rBV2	322	258	0.02%	0.003%
80	11.745	3232	3236	3243	rVB4	874	917	0.08%	0.011%
81	11.809	3243	3256	3273	rBV	442547	706201	63.66%	8.603%
82	11.996	3310	3314	3321	rBV2	316	303	0.03%	0.004%
83	12.057	3325	3333	3347	rVV3	9964	15135	1.36%	0.184%
84	12.134	3354	3357	3362	rVB2	426	275	0.02%	0.003%
85	12.188	3362	3374	3398	rBV	480360	781764	70.47%	9.524%
86	12.375	3428	3432	3439	rVB2	240	303	0.03%	0.004%
87	12.410	3439	3443	3447	rBV2	247	276	0.02%	0.003%
88	12.770	3546	3555	3566	rVB3	2976	4763	0.43%	0.058%
89	12.893	3589	3593	3595	rVB2	309	247	0.02%	0.003%
90	13.050	3635	3642	3645	rBV	282	316	0.03%	0.004%
91	13.221	3688	3695	3703	rVB6	2822	4481	0.40%	0.055%
92	13.278	3710	3713	3721	rBV2	388	513	0.05%	0.006%
93	13.343	3731	3733	3739	rVB2	342	239	0.02%	0.003%
94	13.690	3836	3841	3847	rBV2	378	386	0.03%	0.005%
95	13.838	3884	3887	3888	rBV2	476	242	0.02%	0.003%
96	14.028	3943	3946	3950	rBV2	305	232	0.02%	0.003%
97	14.092	3963	3966	3970	rBV3	671	613	0.06%	0.007%
98	14.327	4031	4039	4052	rBV5	4336	6979	0.63%	0.085%
99	14.561	4109	4112	4113	rBV3	455	256	0.02%	0.003%
100	15.475	4393	4396	4400	rBV3	635	463	0.04%	0.006%




Sum of corrected areas: 8208570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052822.D
Acq On : 26 Jan 2023 17:39
Operator : JC/MD
Sample : 01316-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

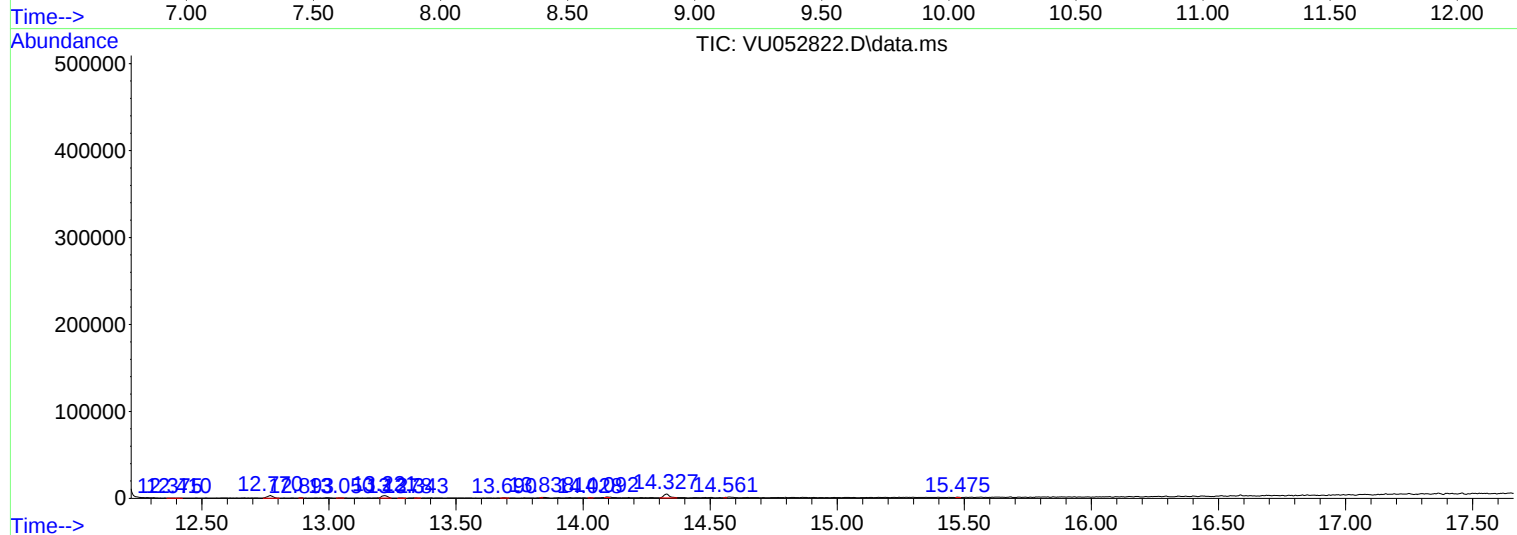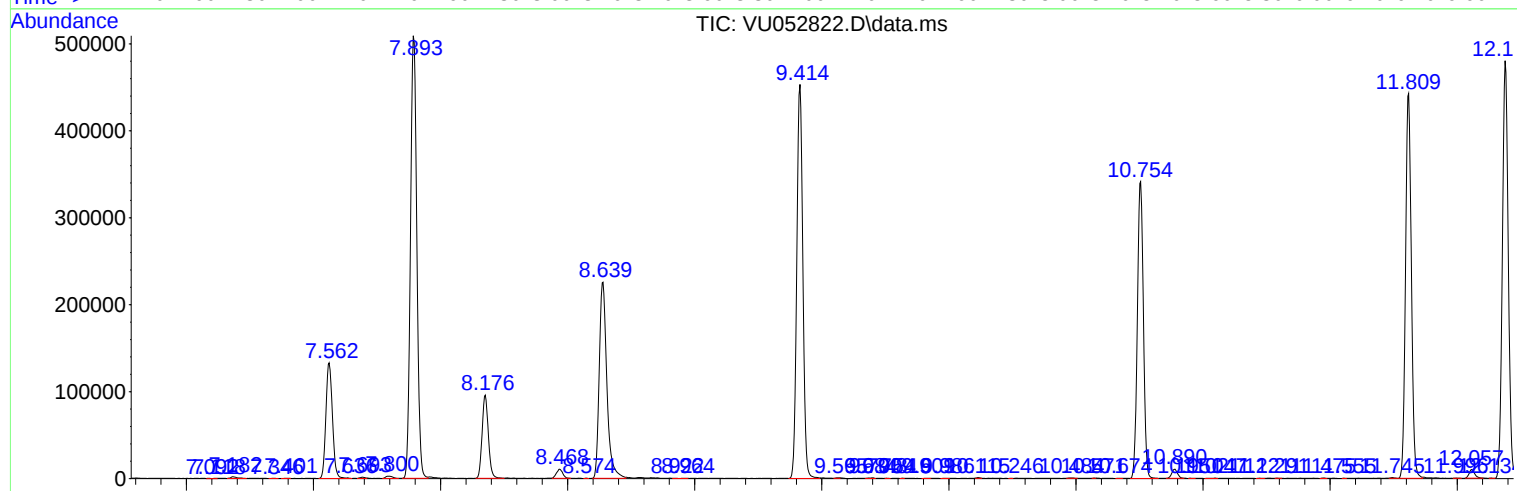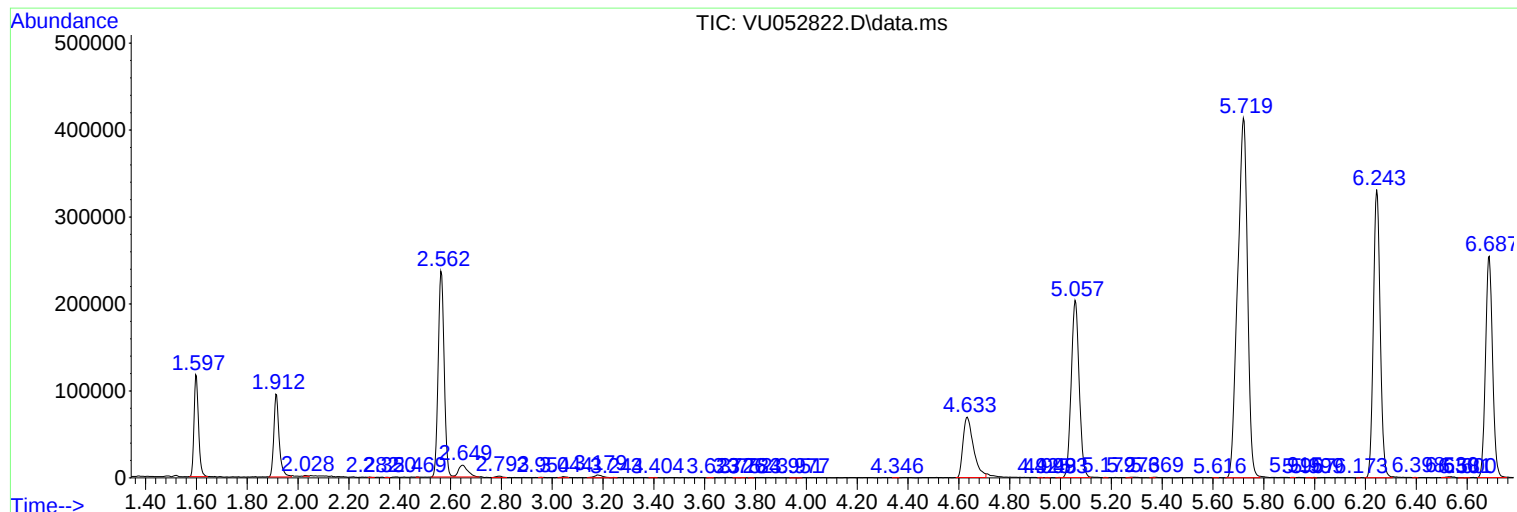

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052822.D
Acq On : 26 Jan 2023 17:39
Operator : JC/MD
Sample : 01316-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052822.D
Acq On : 26 Jan 2023 17:39
Operator : JC/MD
Sample : 01316-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------