

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052823.D
 Acq On : 26 Jan 2023 18:02
 Operator : JC/MD
 Sample : 01316-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	52	57	61	rVB3	1279	1416	0.13%	0.018%
2	1.597	72	80	96	rBV	118257	143007	13.03%	1.780%
3	1.800	138	143	145	rBV	769	699	0.06%	0.009%
4	1.861	160	162	163	rBV2	828	339	0.03%	0.004%
5	1.871	163	165	168	rVV3	1492	1185	0.11%	0.015%
6	1.909	168	177	199	rVB	103434	148796	13.55%	1.852%
7	2.253	280	284	290	rBV3	328	311	0.03%	0.004%
8	2.472	349	352	355	rBV2	486	320	0.03%	0.004%
9	2.562	364	380	396	rBV	232331	381760	34.78%	4.753%
10	2.723	426	430	433	rVB4	352	286	0.03%	0.004%
11	2.793	447	452	456	rVB3	724	751	0.07%	0.009%
12	2.858	465	472	473	rBV2	345	352	0.03%	0.004%
13	2.964	501	505	509	rBV	229	260	0.02%	0.003%
14	2.993	509	514	519	rVV2	329	368	0.03%	0.005%
15	3.044	522	530	539	rVB4	1067	1979	0.18%	0.025%
16	3.176	563	571	579	rBV4	1181	2215	0.20%	0.028%
17	3.407	639	643	646	rBV2	295	286	0.03%	0.004%
18	3.719	736	740	746	rBV	242	302	0.03%	0.004%
19	3.960	810	815	822	rBV2	297	407	0.04%	0.005%
20	4.067	845	848	854	rVB2	304	323	0.03%	0.004%
21	4.108	855	861	866	rBV2	356	460	0.04%	0.006%
22	4.305	919	922	927	rBV2	348	284	0.03%	0.004%
23	4.356	933	938	941	rBV2	229	256	0.02%	0.003%
24	4.414	951	956	960	rBV2	229	294	0.03%	0.004%
25	4.491	978	980	982	rBV	309	226	0.02%	0.003%
26	4.623	1008	1021	1057	rBV	76252	199059	18.13%	2.478%
27	4.983	1130	1133	1139	rBV	203	243	0.02%	0.003%
28	5.057	1139	1156	1178	rBV	204368	449458	40.94%	5.595%
29	5.276	1219	1224	1232	rVB3	645	741	0.07%	0.009%
30	5.372	1248	1254	1256	rBV2	529	537	0.05%	0.007%
31	5.436	1269	1274	1279	rVB2	362	380	0.03%	0.005%
32	5.501	1288	1294	1296	rBV2	259	292	0.03%	0.004%
33	5.517	1297	1299	1306	rVB2	259	272	0.02%	0.003%
34	5.719	1341	1362	1385	rBV2	405700	1097786	100.00%	13.667%
35	5.928	1425	1427	1432	rVB2	410	336	0.03%	0.004%
36	5.960	1432	1437	1440	rBV2	314	374	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052823.D
 Acq On : 26 Jan 2023 18:02
 Operator : JC/MD
 Sample : 01316-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.015	1449	1454	1456	rBV	232	233	0.02%	0.003%
38	6.243	1509	1525	1546	rBV	331446	625463	56.97%	7.787%
39	6.462	1590	1593	1599	rVB2	503	511	0.05%	0.006%
40	6.488	1599	1601	1603	rBV	390	255	0.02%	0.003%
41	6.523	1606	1612	1615	rBV2	709	814	0.07%	0.010%
42	6.607	1632	1638	1640	rBV2	311	333	0.03%	0.004%
43	6.684	1648	1662	1685	rBV	249777	484165	44.10%	6.027%
44	6.796	1693	1697	1698	rBV3	484	338	0.03%	0.004%
45	6.838	1706	1710	1716	rBV3	261	349	0.03%	0.004%
46	7.189	1811	1819	1823	rBV4	1831	2436	0.22%	0.030%
47	7.266	1839	1843	1847	rBV2	202	233	0.02%	0.003%
48	7.324	1856	1861	1864	rBV2	292	340	0.03%	0.004%
49	7.372	1871	1876	1877	rBV2	317	333	0.03%	0.004%
50	7.504	1913	1917	1922	rBV	287	326	0.03%	0.004%
51	7.562	1922	1935	1961	rVB	134823	235831	21.48%	2.936%
52	7.693	1968	1976	1984	rBV3	1010	1544	0.14%	0.019%
53	7.893	2024	2038	2059	rBV	507487	866721	78.95%	10.790%
54	8.079	2092	2096	2103	rVB3	276	314	0.03%	0.004%
55	8.176	2113	2126	2142	rBV	93358	157618	14.36%	1.962%
56	8.388	2190	2192	2196	rVB3	411	286	0.03%	0.004%
57	8.472	2208	2218	2226	rBV3	1568	2838	0.26%	0.035%
58	8.636	2256	2269	2304	rBV2	229423	460470	41.95%	5.732%
59	9.140	2420	2426	2429	rBV2	184	271	0.02%	0.003%
60	9.279	2464	2469	2473	rBV	288	273	0.02%	0.003%
61	9.414	2498	2511	2537	rBV	460581	746881	68.04%	9.298%
62	9.568	2555	2559	2567	rVB3	542	724	0.07%	0.009%
63	9.693	2592	2598	2606	rVB4	599	776	0.07%	0.010%
64	9.825	2636	2639	2644	rBV	294	360	0.03%	0.004%
65	10.115	2723	2729	2734	rBV4	651	799	0.07%	0.010%
66	10.279	2774	2780	2783	rBV2	357	369	0.03%	0.005%
67	10.340	2791	2799	2805	rVB2	367	649	0.06%	0.008%
68	10.369	2805	2808	2812	rBV	238	256	0.02%	0.003%
69	10.394	2812	2816	2819	rVB	344	303	0.03%	0.004%
70	10.414	2819	2822	2833	rBV2	267	416	0.04%	0.005%
71	10.751	2915	2927	2943	rBV	331717	539881	49.18%	6.721%
72	10.877	2961	2966	2967	rBV2	1119	655	0.06%	0.008%
73	10.947	2985	2988	2992	rBV2	266	256	0.02%	0.003%
74	10.996	2998	3003	3005	rBV	279	283	0.03%	0.004%
75	11.127	3040	3044	3048	rVB2	371	251	0.02%	0.003%
76	11.153	3048	3052	3055	rBV2	275	273	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052823.D
 Acq On : 26 Jan 2023 18:02
 Operator : JC/MD
 Sample : 01316-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.330	3104	3107	3111	rBV2	267	315	0.03%	0.004%
78	11.468	3146	3150	3154	rVB3	311	261	0.02%	0.003%
79	11.494	3154	3158	3163	rVB2	330	379	0.03%	0.005%
80	11.523	3163	3167	3170	rBV2	229	245	0.02%	0.003%
81	11.745	3230	3236	3238	rBV2	776	687	0.06%	0.009%
82	11.809	3243	3256	3273	rBV	438981	699802	63.75%	8.712%
83	11.947	3296	3299	3304	rVB2	408	366	0.03%	0.005%
84	12.188	3360	3374	3400	rBV	471634	750143	68.33%	9.339%
85	12.520	3472	3477	3483	rVB	341	409	0.04%	0.005%
86	12.561	3483	3490	3492	rBV	281	364	0.03%	0.005%
87	12.671	3519	3524	3527	rBV2	298	326	0.03%	0.004%
88	12.770	3549	3555	3565	rBV3	407	758	0.07%	0.009%
89	13.426	3755	3759	3763	rBV2	315	366	0.03%	0.005%
90	13.745	3855	3858	3862	rBV2	371	264	0.02%	0.003%
91	13.803	3873	3876	3879	rBV	430	330	0.03%	0.004%
92	13.973	3926	3929	3933	rBV	290	289	0.03%	0.004%
93	14.085	3961	3964	3965	rBV3	415	225	0.02%	0.003%
94	14.163	3985	3988	3992	rBV2	330	241	0.02%	0.003%
95	14.330	4032	4040	4049	rBV5	2221	3474	0.32%	0.043%
96	14.391	4057	4059	4063	rVB2	665	238	0.02%	0.003%
97	14.741	4166	4168	4173	rVB3	354	263	0.02%	0.003%
98	14.767	4173	4176	4180	rBV3	386	385	0.04%	0.005%
99	15.860	4514	4516	4523	rVB4	646	483	0.04%	0.006%
100	16.060	4576	4578	4579	rBV2	539	253	0.02%	0.003%




Sum of corrected areas: 8032653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052823.D
Acq On : 26 Jan 2023 18:02
Operator : JC/MD
Sample : 01316-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

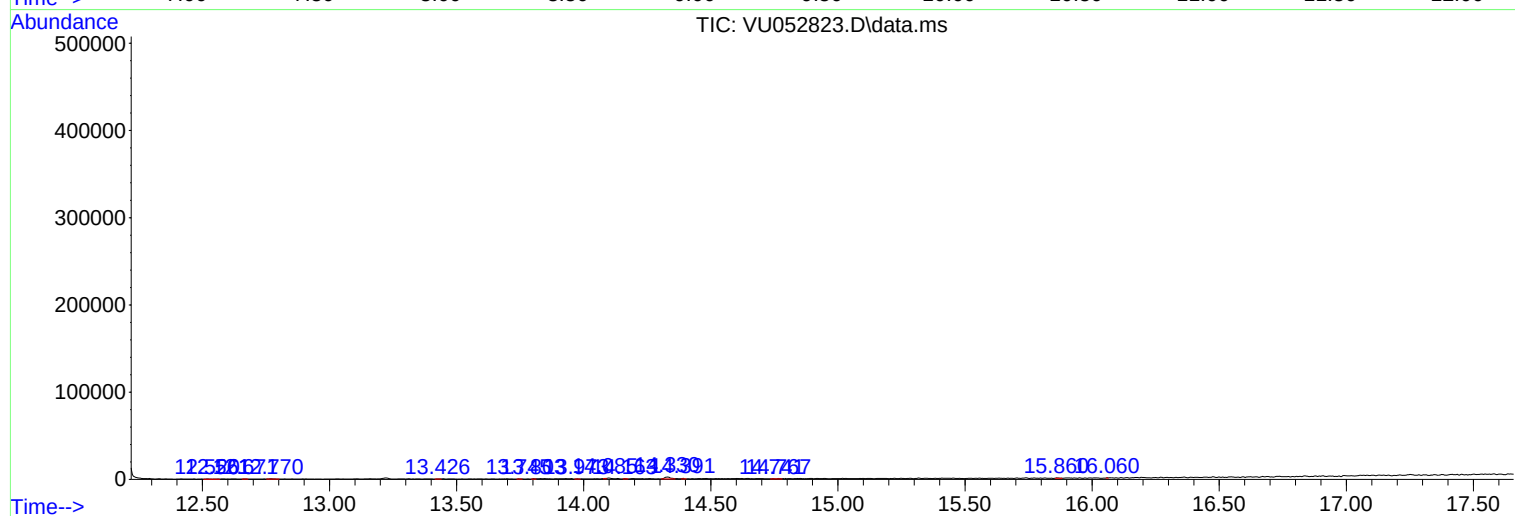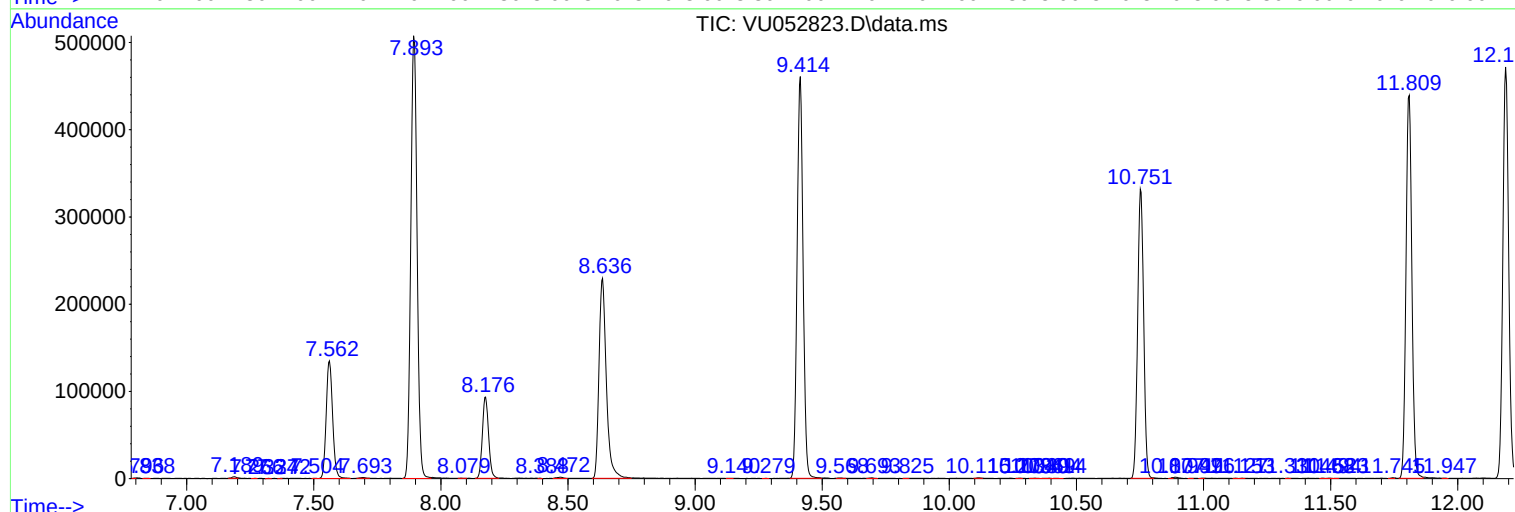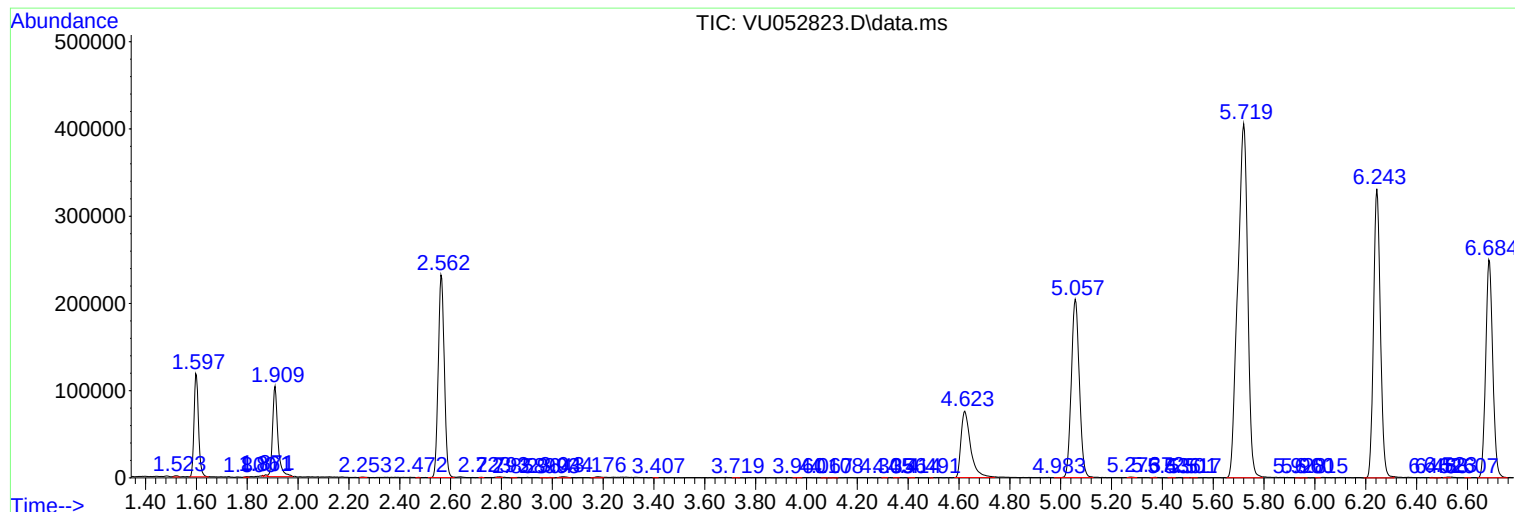

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052823.D
Acq On : 26 Jan 2023 18:02
Operator : JC/MD
Sample : 01316-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052823.D
Acq On : 26 Jan 2023 18:02
Operator : JC/MD
Sample : 01316-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------