

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052824.D
 Acq On : 26 Jan 2023 18:25
 Operator : JC/MD
 Sample : 01316-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	49	rBV3	1263	982	0.09%	0.012%
2	1.597	72	80	96	rVB	114286	138458	12.86%	1.758%
3	1.864	159	163	166	rBV5	976	809	0.08%	0.010%
4	1.909	169	177	200	rVV	97219	140656	13.07%	1.786%
5	2.205	265	269	272	rBV2	382	325	0.03%	0.004%
6	2.244	279	281	283	rBV2	409	227	0.02%	0.003%
7	2.385	320	325	326	rBV2	434	255	0.02%	0.003%
8	2.562	368	380	395	rBV	225629	369281	34.30%	4.690%
9	2.642	400	405	412	rVB5	1681	2386	0.22%	0.030%
10	2.713	423	427	429	rBV2	424	268	0.02%	0.003%
11	2.790	442	451	453	rBV2	892	1302	0.12%	0.017%
12	2.916	487	490	493	rBV3	409	307	0.03%	0.004%
13	3.048	523	531	538	rVB4	1020	1877	0.17%	0.024%
14	3.183	563	573	576	rBV3	1233	2267	0.21%	0.029%
15	3.228	583	587	589	rBV2	222	221	0.02%	0.003%
16	3.504	668	673	677	rBV	258	333	0.03%	0.004%
17	3.742	741	747	749	rVB2	355	307	0.03%	0.004%
18	3.813	766	769	773	rVB2	325	271	0.03%	0.003%
19	3.842	773	778	780	rBV	331	339	0.03%	0.004%
20	3.954	809	813	815	rBV	334	288	0.03%	0.004%
21	4.282	907	915	919	rBV2	337	474	0.04%	0.006%
22	4.334	929	931	935	rVB2	360	243	0.02%	0.003%
23	4.623	1009	1021	1049	rBV2	72388	198474	18.44%	2.521%
24	5.057	1140	1156	1183	rVV	201342	437441	40.64%	5.556%
25	5.154	1183	1186	1190	rVB4	462	468	0.04%	0.006%
26	5.231	1207	1210	1213	rVB	302	223	0.02%	0.003%
27	5.263	1216	1220	1222	rBV	315	268	0.02%	0.003%
28	5.282	1222	1226	1230	rBV2	426	441	0.04%	0.006%
29	5.334	1236	1242	1247	rBV2	276	433	0.04%	0.005%
30	5.369	1247	1253	1258	rVV3	652	852	0.08%	0.011%
31	5.546	1303	1308	1309	rBV	283	240	0.02%	0.003%
32	5.613	1326	1329	1336	rVV2	195	238	0.02%	0.003%
33	5.719	1340	1362	1393	rVV2	397523	1076509	100.00%	13.672%
34	5.826	1393	1395	1399	rBV	299	273	0.03%	0.003%
35	5.957	1429	1436	1437	rBV2	242	282	0.03%	0.004%
36	6.038	1459	1461	1466	rVB2	615	521	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052824.D
 Acq On : 26 Jan 2023 18:25
 Operator : JC/MD
 Sample : 01316-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.067	1467	1470	1474	rBV2	331	335	0.03%	0.004%
38	6.134	1488	1491	1494	rBV2	254	245	0.02%	0.003%
39	6.244	1508	1525	1545	rBV	323780	616156	57.24%	7.825%
40	6.366	1560	1563	1566	rVB	471	304	0.03%	0.004%
41	6.533	1605	1615	1616	rBV3	800	1100	0.10%	0.014%
42	6.684	1648	1662	1684	rBV2	246108	473256	43.96%	6.011%
43	6.761	1684	1686	1689	rBV2	400	240	0.02%	0.003%
44	6.797	1694	1697	1699	rBV	449	249	0.02%	0.003%
45	6.848	1710	1713	1719	rVB2	257	250	0.02%	0.003%
46	7.189	1810	1819	1822	rBV2	1794	2443	0.23%	0.031%
47	7.282	1841	1848	1850	rBV	261	284	0.03%	0.004%
48	7.562	1921	1935	1951	rBV	128531	226109	21.00%	2.872%
49	7.687	1969	1974	1975	rBV	658	537	0.05%	0.007%
50	7.893	2025	2038	2058	rBV	491514	841399	78.16%	10.686%
51	8.057	2088	2089	2094	rVB3	354	225	0.02%	0.003%
52	8.079	2094	2096	2101	rBV2	423	312	0.03%	0.004%
53	8.176	2112	2126	2142	rBV	93237	156044	14.50%	1.982%
54	8.263	2150	2153	2155	rBV2	309	234	0.02%	0.003%
55	8.388	2190	2192	2196	rBV3	301	244	0.02%	0.003%
56	8.469	2207	2217	2224	rBV3	3117	5083	0.47%	0.065%
57	8.549	2239	2242	2246	rVB	771	411	0.04%	0.005%
58	8.636	2254	2269	2298	rBV2	225764	461154	42.84%	5.857%
59	8.777	2310	2313	2315	rBV	1123	829	0.08%	0.011%
60	9.002	2378	2383	2389	rVV2	244	388	0.04%	0.005%
61	9.063	2395	2402	2404	rBV	306	434	0.04%	0.006%
62	9.414	2498	2511	2530	rBV	455794	745075	69.21%	9.463%
63	9.690	2593	2597	2603	rVV3	524	631	0.06%	0.008%
64	9.890	2656	2659	2665	rVB2	404	406	0.04%	0.005%
65	10.002	2692	2694	2701	rBV2	241	246	0.02%	0.003%
66	10.067	2707	2714	2717	rBV	292	384	0.04%	0.005%
67	10.157	2739	2742	2748	rVB	334	317	0.03%	0.004%
68	10.481	2839	2843	2847	rBV2	404	388	0.04%	0.005%
69	10.558	2863	2867	2870	rBV	337	258	0.02%	0.003%
70	10.626	2881	2888	2894	rBV2	258	447	0.04%	0.006%
71	10.665	2897	2900	2904	rVB	297	227	0.02%	0.003%
72	10.751	2914	2927	2950	rBV	328135	532349	49.45%	6.761%
73	10.890	2960	2970	2979	rVV3	2873	4171	0.39%	0.053%
74	10.976	2994	2997	3004	rBV2	261	318	0.03%	0.004%
75	11.102	3032	3036	3040	rBV2	338	340	0.03%	0.004%
76	11.462	3146	3148	3152	rVB2	479	303	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052824.D
 Acq On : 26 Jan 2023 18:25
 Operator : JC/MD
 Sample : 01316-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.491	3154	3157	3163	rBV2	197	219	0.02%	0.003%
78	11.616	3193	3196	3201	rBV	267	274	0.03%	0.003%
79	11.645	3201	3205	3211	rBV2	217	238	0.02%	0.003%
80	11.809	3243	3256	3279	rBV	433891	687404	63.85%	8.730%
81	12.060	3327	3334	3342	rBV4	2429	3701	0.34%	0.047%
82	12.189	3361	3374	3390	rBV	442625	716861	66.59%	9.104%
83	12.494	3463	3469	3472	rBV2	283	320	0.03%	0.004%
84	12.729	3537	3542	3545	rBV2	203	254	0.02%	0.003%
85	12.771	3547	3555	3562	rVV3	1193	2048	0.19%	0.026%
86	12.838	3572	3576	3579	rBV2	338	309	0.03%	0.004%
87	12.890	3587	3592	3598	rVB3	1798	1673	0.16%	0.021%
88	12.935	3602	3606	3613	rVB2	362	385	0.04%	0.005%
89	13.021	3628	3633	3635	rBV2	264	296	0.03%	0.004%
90	13.221	3688	3695	3696	rBV	913	862	0.08%	0.011%
91	13.256	3703	3706	3710	rBV2	313	266	0.02%	0.003%
92	13.590	3802	3810	3815	rBV2	317	553	0.05%	0.007%
93	13.848	3886	3890	3898	rVV6	666	804	0.07%	0.010%
94	14.144	3978	3982	3985	rBV2	410	342	0.03%	0.004%
95	14.333	4033	4041	4044	rBV3	1252	1530	0.14%	0.019%
96	14.616	4126	4129	4132	rBV	503	352	0.03%	0.004%
97	14.761	4171	4174	4177	rBV3	359	287	0.03%	0.004%
98	16.073	4578	4582	4585	rBV4	587	685	0.06%	0.009%
99	16.092	4585	4588	4590	rVV2	865	558	0.05%	0.007%
100	16.182	4613	4616	4623	rVB5	981	924	0.09%	0.012%




Sum of corrected areas: 7873809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052824.D
Acq On : 26 Jan 2023 18:25
Operator : JC/MD
Sample : 01316-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

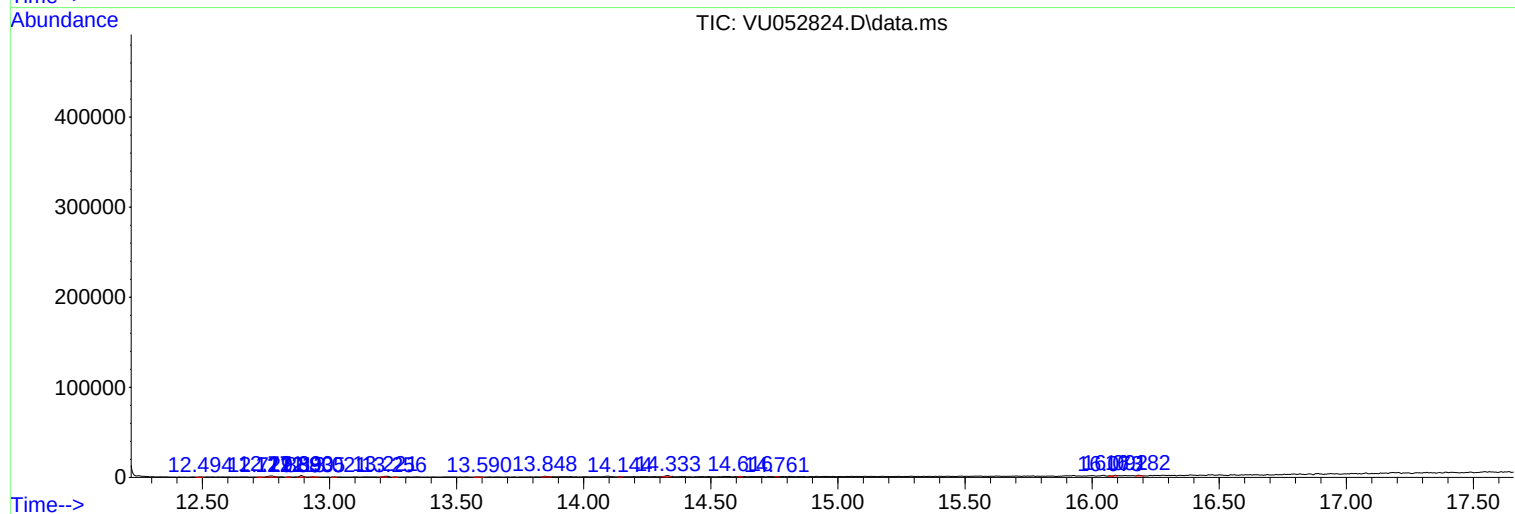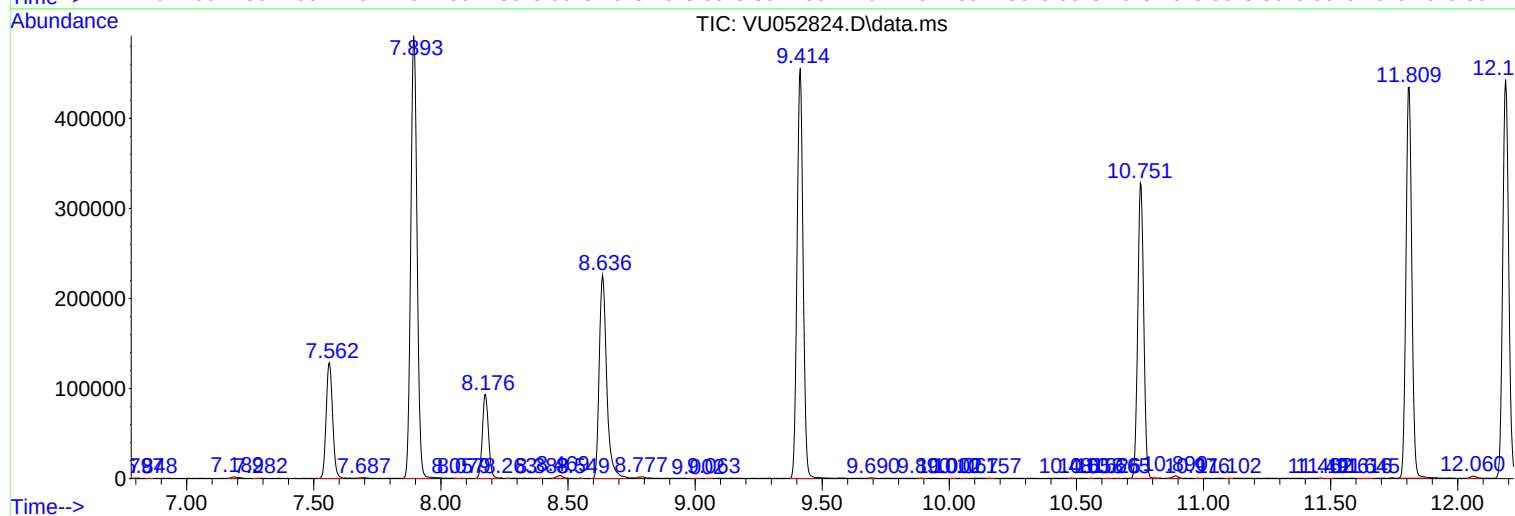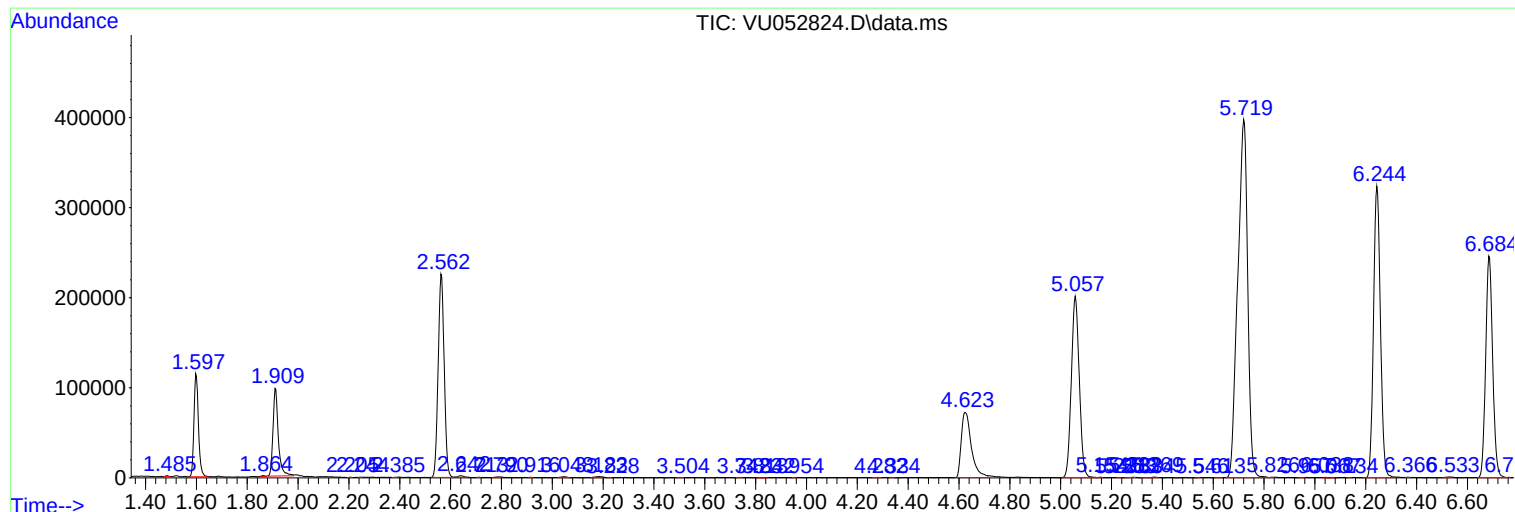

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052824.D
Acq On : 26 Jan 2023 18:25
Operator : JC/MD
Sample : 01316-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052824.D
Acq On : 26 Jan 2023 18:25
Operator : JC/MD
Sample : 01316-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------