

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052828.D
 Acq On : 26 Jan 2023 19:59
 Operator : JC/MD
 Sample : 01316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	109065	132718	12.57%	1.730%
2	1.909	169	177	195	rBV	96608	132582	12.56%	1.729%
3	2.481	352	355	362	rBV	341	371	0.04%	0.005%
4	2.565	367	381	395	rVV	223100	363459	34.43%	4.739%
5	3.038	522	528	536	rVB2	1288	2179	0.21%	0.028%
6	3.150	561	563	564	rBV	284	124	0.01%	0.002%
7	3.346	618	624	629	rBV2	363	449	0.04%	0.006%
8	3.678	724	727	730	rBV2	278	254	0.02%	0.003%
9	3.838	774	777	779	rBV	197	126	0.01%	0.002%
10	3.858	779	783	785	rBV2	319	233	0.02%	0.003%
11	3.941	804	809	811	rBV	200	216	0.02%	0.003%
12	3.954	811	813	816	rVV2	181	100	0.01%	0.001%
13	4.034	834	838	842	rBV2	192	254	0.02%	0.003%
14	4.099	855	858	860	rBV2	187	117	0.01%	0.002%
15	4.163	874	878	879	rBV	140	104	0.01%	0.001%
16	4.247	901	904	906	rBV	404	242	0.02%	0.003%
17	4.330	928	930	935	rBV2	153	113	0.01%	0.001%
18	4.401	950	952	955	rBV2	169	95	0.01%	0.001%
19	4.481	975	977	980	rBV2	190	115	0.01%	0.001%
20	4.510	984	986	989	rBV	181	125	0.01%	0.002%
21	4.562	999	1002	1004	rBV	276	180	0.02%	0.002%
22	4.578	1004	1007	1009	rVB2	203	117	0.01%	0.002%
23	4.623	1009	1021	1054	rBV	72002	191455	18.13%	2.496%
24	4.925	1112	1115	1117	rBV	352	220	0.02%	0.003%
25	4.948	1119	1122	1127	rBV2	357	352	0.03%	0.005%
26	5.057	1140	1156	1184	rBV2	200437	452793	42.89%	5.904%
27	5.224	1205	1208	1213	rBV2	176	189	0.02%	0.002%
28	5.272	1220	1223	1224	rBV2	230	151	0.01%	0.002%
29	5.475	1283	1286	1291	rBV2	215	231	0.02%	0.003%
30	5.517	1296	1299	1300	rBV	206	118	0.01%	0.002%
31	5.613	1328	1329	1330	rBV	239	73	0.01%	0.001%
32	5.719	1341	1362	1382	rBV2	384819	1055759	100.00%	13.766%
33	5.912	1418	1422	1429	rVB2	277	285	0.03%	0.004%
34	5.989	1443	1446	1451	rVB	410	282	0.03%	0.004%
35	6.034	1451	1460	1463	rBV3	375	534	0.05%	0.007%
36	6.063	1467	1469	1470	rBV	105	29	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052828.D
 Acq On : 26 Jan 2023 19:59
 Operator : JC/MD
 Sample : 01316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.086	1470	1476	1479	rBV2	178	221	0.02%	0.003%
38	6.243	1511	1525	1544	rBV	316650	592286	56.10%	7.723%
39	6.526	1604	1613	1620	rBV4	1220	1863	0.18%	0.024%
40	6.620	1639	1642	1644	rBV2	321	241	0.02%	0.003%
41	6.687	1647	1663	1683	rVV	239132	469706	44.49%	6.124%
42	6.800	1695	1698	1701	rBV2	561	400	0.04%	0.005%
43	6.851	1712	1714	1715	rBV2	137	63	0.01%	0.001%
44	6.867	1715	1719	1721	rVB2	315	188	0.02%	0.002%
45	6.880	1721	1723	1724	rBV	139	56	0.01%	0.001%
46	6.928	1734	1738	1740	rVB	321	240	0.02%	0.003%
47	6.954	1743	1746	1749	rBV2	354	305	0.03%	0.004%
48	7.099	1789	1791	1793	rBV2	233	123	0.01%	0.002%
49	7.144	1802	1805	1810	rBV2	168	194	0.02%	0.003%
50	7.189	1812	1819	1825	rVV4	1614	2510	0.24%	0.033%
51	7.218	1825	1828	1831	rVB2	511	370	0.04%	0.005%
52	7.382	1876	1879	1882	rVB	166	148	0.01%	0.002%
53	7.404	1883	1886	1890	rBV	174	166	0.02%	0.002%
54	7.446	1897	1899	1902	rBV2	144	73	0.01%	0.001%
55	7.510	1915	1919	1921	rBV2	151	136	0.01%	0.002%
56	7.562	1922	1935	1956	rVV	128517	225404	21.35%	2.939%
57	7.687	1970	1974	1983	rBV3	1086	1606	0.15%	0.021%
58	7.755	1993	1995	1998	rBV	137	71	0.01%	0.001%
59	7.806	2003	2011	2014	rBV	498	587	0.06%	0.008%
60	7.893	2024	2038	2058	rBV	486122	829356	78.56%	10.814%
61	8.176	2114	2126	2143	rBV	88314	151413	14.34%	1.974%
62	8.272	2154	2156	2157	rBV	211	85	0.01%	0.001%
63	8.285	2157	2160	2165	rVV4	468	437	0.04%	0.006%
64	8.378	2187	2189	2190	rBV	122	48	0.00%	0.001%
65	8.558	2242	2245	2249	rBV2	228	187	0.02%	0.002%
66	8.587	2252	2254	2255	rBV	108	61	0.01%	0.001%
67	8.632	2256	2268	2296	rBV3	225612	445238	42.17%	5.805%
68	8.951	2364	2367	2369	rBV2	184	118	0.01%	0.002%
69	9.266	2463	2465	2467	rBV2	157	83	0.01%	0.001%
70	9.320	2481	2482	2483	rBV	241	77	0.01%	0.001%
71	9.414	2498	2511	2532	rBV	445541	716328	67.85%	9.340%
72	9.697	2596	2599	2604	rVB	532	477	0.05%	0.006%
73	9.899	2659	2662	2667	rBV2	239	311	0.03%	0.004%
74	9.967	2681	2683	2685	rBV	181	103	0.01%	0.001%
75	10.240	2766	2768	2772	rBV2	292	196	0.02%	0.003%
76	10.262	2772	2775	2777	rBV	335	228	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
 Data File : VU052828.D
 Acq On : 26 Jan 2023 19:59
 Operator : JC/MD
 Sample : 01316-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

77	10.324	2792	2794	2796	rBV	262	146	0.01%	0.002%
78	10.385	2808	2813	2816	rBV2	260	276	0.03%	0.004%
79	10.459	2831	2836	2840	rBV	353	418	0.04%	0.005%
80	10.751	2915	2927	2945	rVB	328360	525014	49.73%	6.846%
81	10.934	2981	2984	2988	rBV	304	183	0.02%	0.002%
82	11.488	3153	3156	3159	rBV	275	223	0.02%	0.003%
83	11.809	3243	3256	3270	rBV	409175	643207	60.92%	8.387%
84	12.060	3326	3334	3341	rBV5	1958	3283	0.31%	0.043%
85	12.188	3362	3374	3394	rBV	452757	717339	67.95%	9.353%
86	13.140	3665	3670	3673	rBV2	466	480	0.05%	0.006%
87	13.606	3810	3815	3818	rBV	346	451	0.04%	0.006%


Sum of corrected areas: 7669467

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052828.D
Acq On : 26 Jan 2023 19:59
Operator : JC/MD
Sample : 01316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

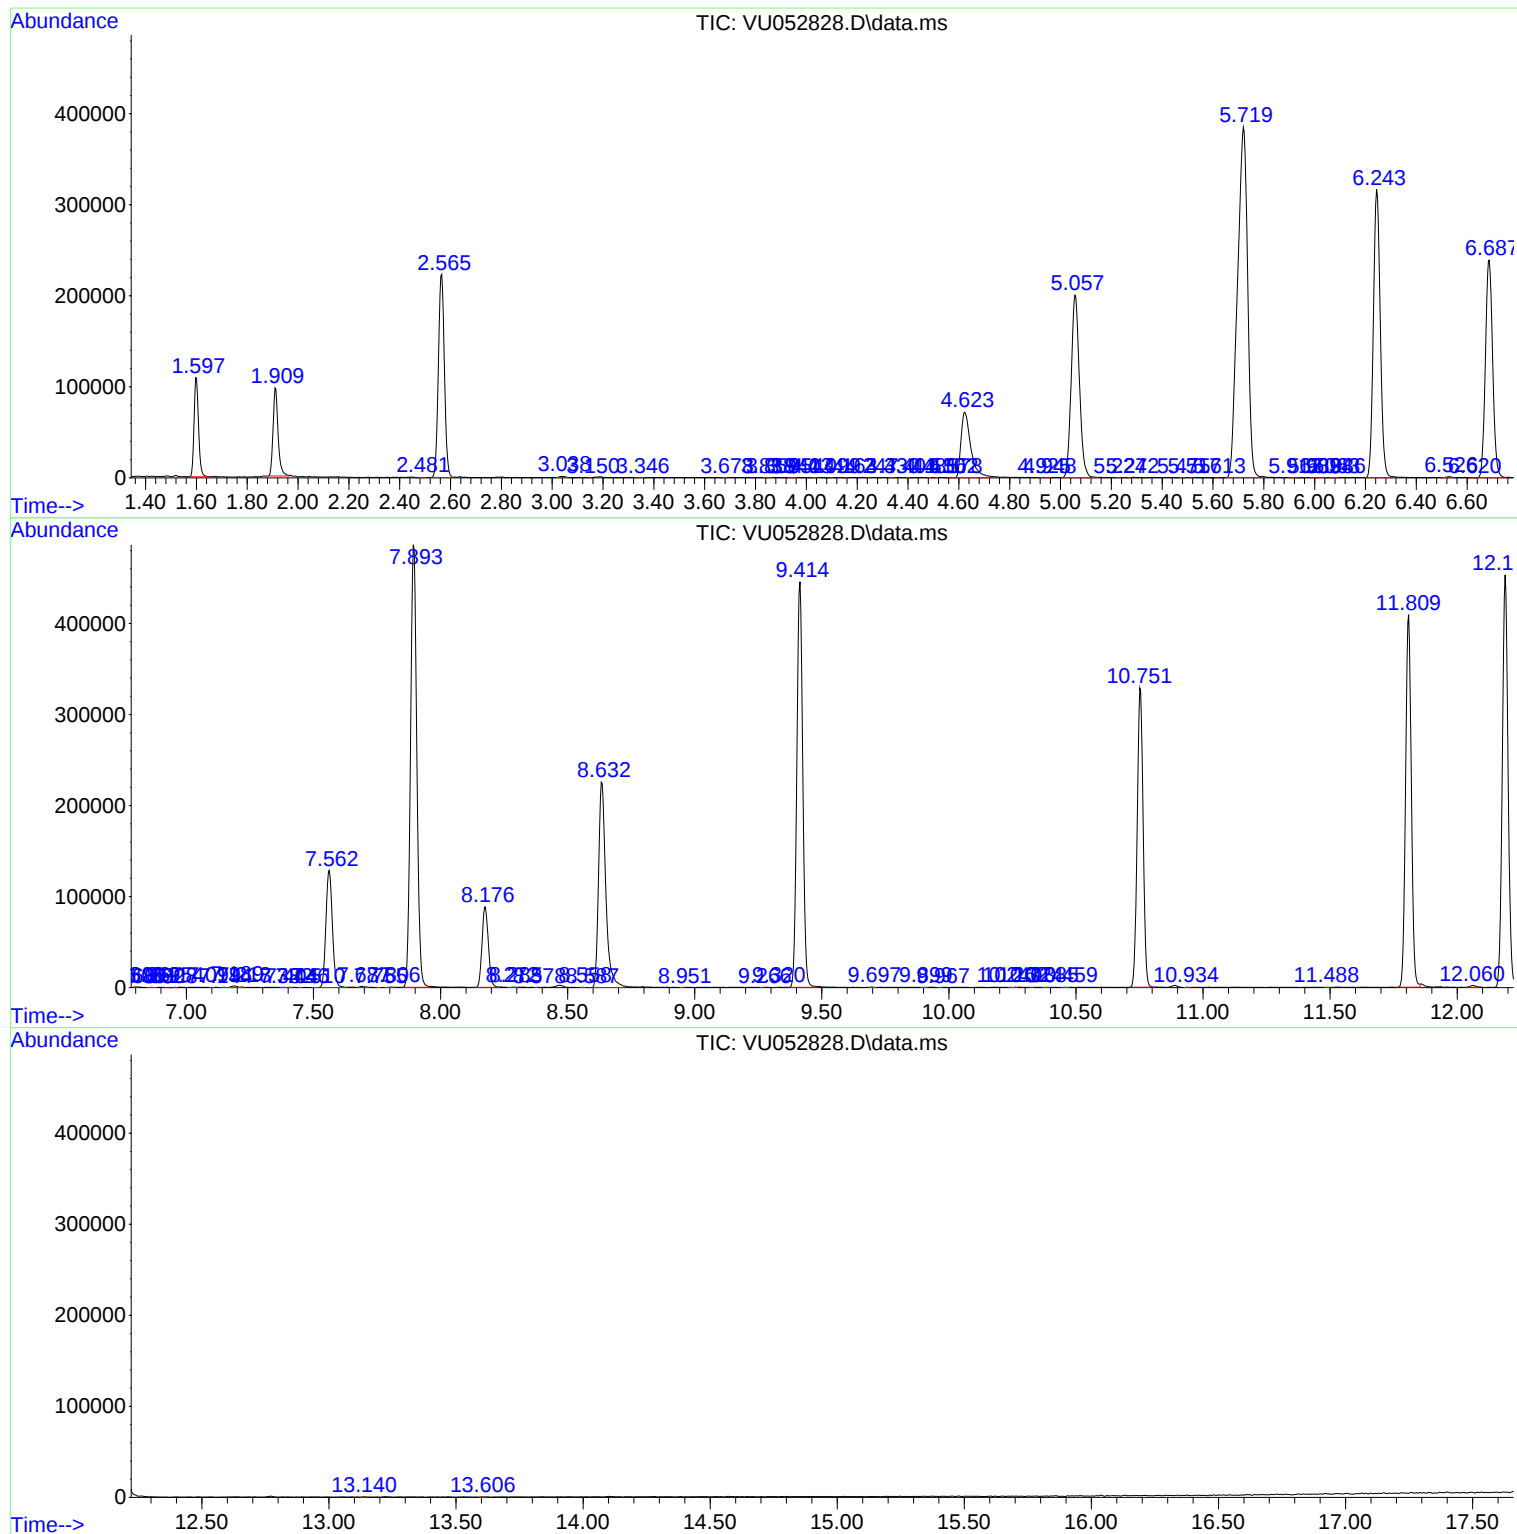

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052828.D
Acq On : 26 Jan 2023 19:59
Operator : JC/MD
Sample : 01316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052828.D
Acq On : 26 Jan 2023 19:59
Operator : JC/MD
Sample : 01316-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc