


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012623\
Data File : VU052809.D
Acq On : 26 Jan 2023 09:46
Operator : JC/MD
Sample : BFB153
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB153

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Title : VOC Analysis
Last Update : Wed Feb 01 00:53:48 2023

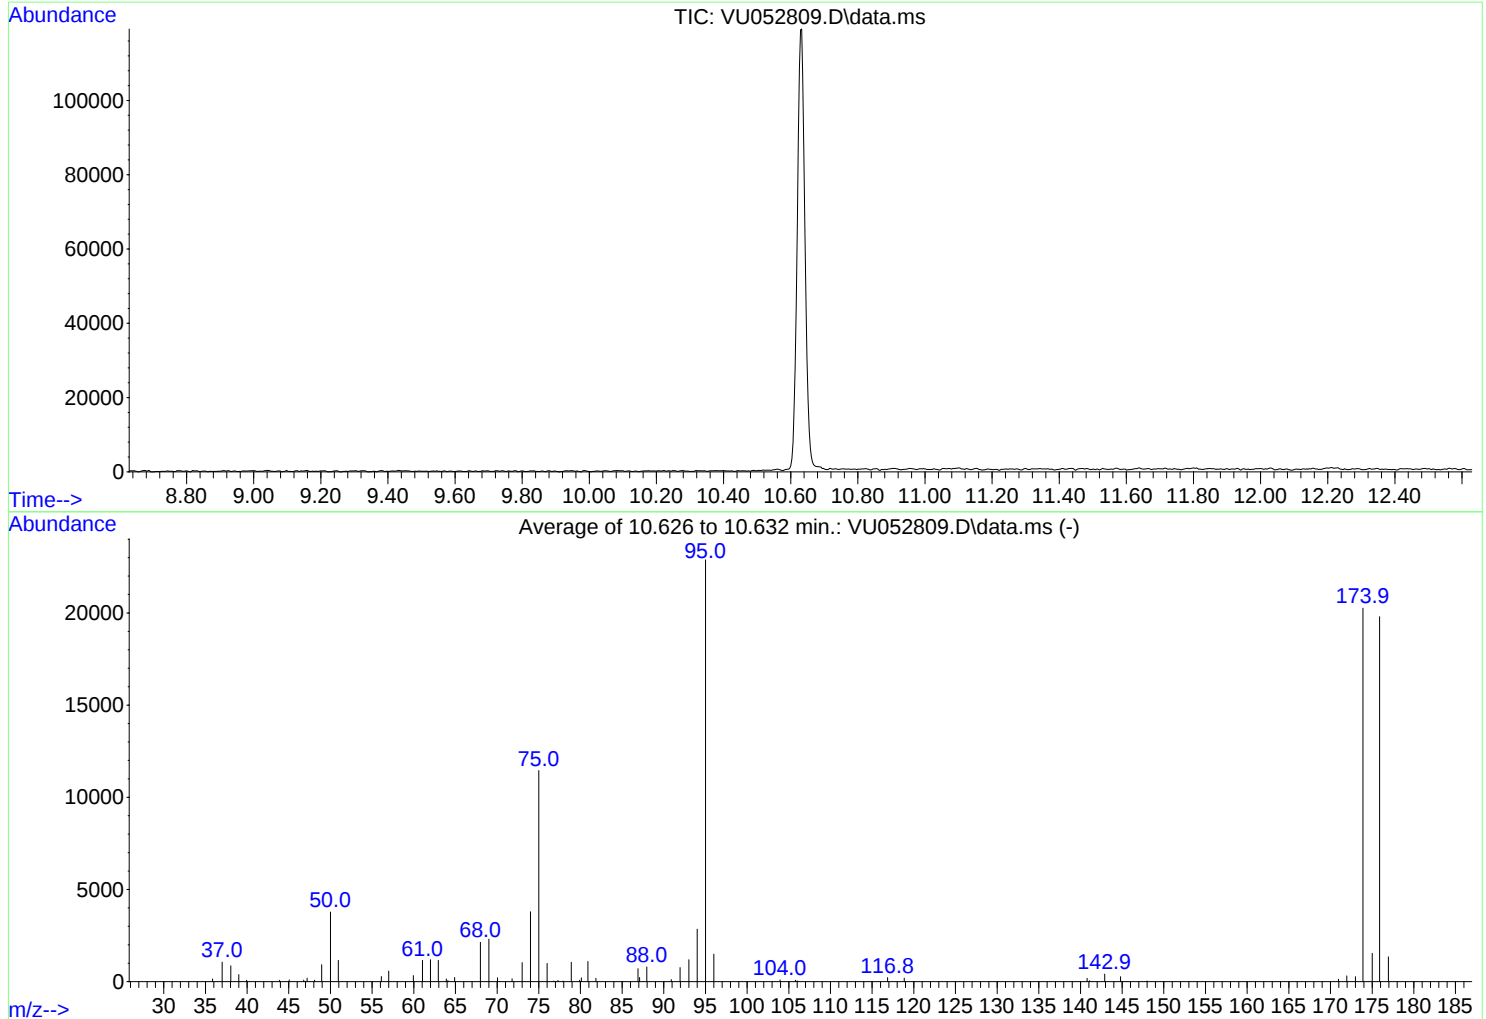

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	3772	PASS
75	95	30	80	50.0	11446	PASS
95	95	100	100	100.0	22880	PASS
96	95	5	9	6.5	1492	PASS
173	174	0.00	2	1.3	273	PASS
174	95	50	120	88.6	20261	PASS
175	174	5	9	7.6	1533	PASS
176	174	95	101	97.7	19795	PASS
177	176	5	9	6.8	1348	PASS

m/z	Abundance
35.90	349.0
37.80	126.0
39.90	114.0
43.80	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB153

m/z	Abundance
35.90	529.0
37.00	923.0
38.00	864.0
38.90	386.0
40.00	206.0
44.00	240.0
46.80	147.0
47.20	209.0
49.00	897.0
50.00	3478.0
50.90	1033.0
56.10	266.0
57.00	527.0
60.00	329.0
61.10	1114.0
62.00	1042.0
62.90	1065.0
63.90	215.0
64.90	200.0
68.00	1850.0
69.00	2091.0
70.10	202.0
71.80	145.0
73.00	954.0
74.00	3549.0
75.00	11003.0
76.00	875.0
77.30	106.0
77.90	110.0
78.90	967.0
79.90	224.0
80.90	1066.0
81.90	173.0
86.90	684.0
87.10	674.0
87.90	705.0
90.90	125.0
91.90	745.0
93.00	1111.0
94.00	2759.0
95.00	21696.0
96.00	1520.0
104.00	154.0
105.80	122.0
116.90	203.0
118.80	162.0
140.80	161.0
141.10	163.0
142.90	368.0
144.80	250.0
148.00	103.0
170.90	120.0
172.00	288.0
173.00	262.0
173.90	18528.0
175.00	1521.0
175.90	18288.0
177.00	1127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB153

m/z	Abundance
35.90	503.0
37.00	1121.0
38.00	900.0
39.00	397.0
40.00	200.0
44.00	219.0
45.10	119.0
47.20	212.0
48.10	111.0
49.00	941.0
50.00	3927.0
51.00	1179.0
56.10	286.0
57.00	591.0
60.00	334.0
61.00	1193.0
62.00	1220.0
63.00	1206.0
63.90	223.0
64.90	231.0
68.00	2182.0
69.00	2416.0
70.00	223.0
71.80	172.0
73.00	1089.0
74.00	3881.0
75.00	11853.0
76.00	1003.0
76.80	111.0
77.30	117.0
78.90	1080.0
80.10	310.0
80.90	1165.0
81.80	179.0
86.90	732.0
88.00	816.0
90.90	125.0
92.00	814.0
93.00	1245.0
94.00	2961.0
95.00	23504.0
96.00	1527.0
103.90	121.0
105.80	114.0
116.80	222.0
118.80	177.0
140.80	191.0
142.90	423.0
144.80	293.0
171.00	137.0
172.00	306.0
173.00	283.0
173.90	20832.0
175.00	1559.0
175.90	20336.0
176.90	1386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB153

m/z	Abundance
35.90	449.0
37.00	1132.0
38.10	817.0
39.10	356.0
40.00	169.0
44.00	213.0
45.00	160.0
46.80	109.0
47.20	149.0
48.10	114.0
48.90	917.0
50.00	3911.0
51.00	1245.0
56.10	285.0
57.00	608.0
59.90	315.0
61.00	1145.0
62.00	1295.0
63.00	1192.0
64.10	190.0
64.90	254.0
68.00	2366.0
69.00	2413.0
70.00	197.0
71.80	150.0
73.00	1068.0
74.00	3943.0
75.00	11481.0
76.00	1082.0
78.90	1102.0
80.10	315.0
80.90	1043.0
81.80	198.0
86.90	706.0
87.90	871.0
90.90	100.0
92.00	734.0
93.00	1221.0
94.00	2818.0
95.00	23440.0
96.00	1428.0
106.00	137.0
116.80	230.0
118.90	226.0
140.80	190.0
142.90	446.0
144.80	276.0
171.00	143.0
171.90	335.0
173.00	274.0
173.90	21424.0
175.00	1520.0
175.90	20760.0
176.90	1531.0

Instrument :
MSVOA_U
ClientSampleId :
BFB153