
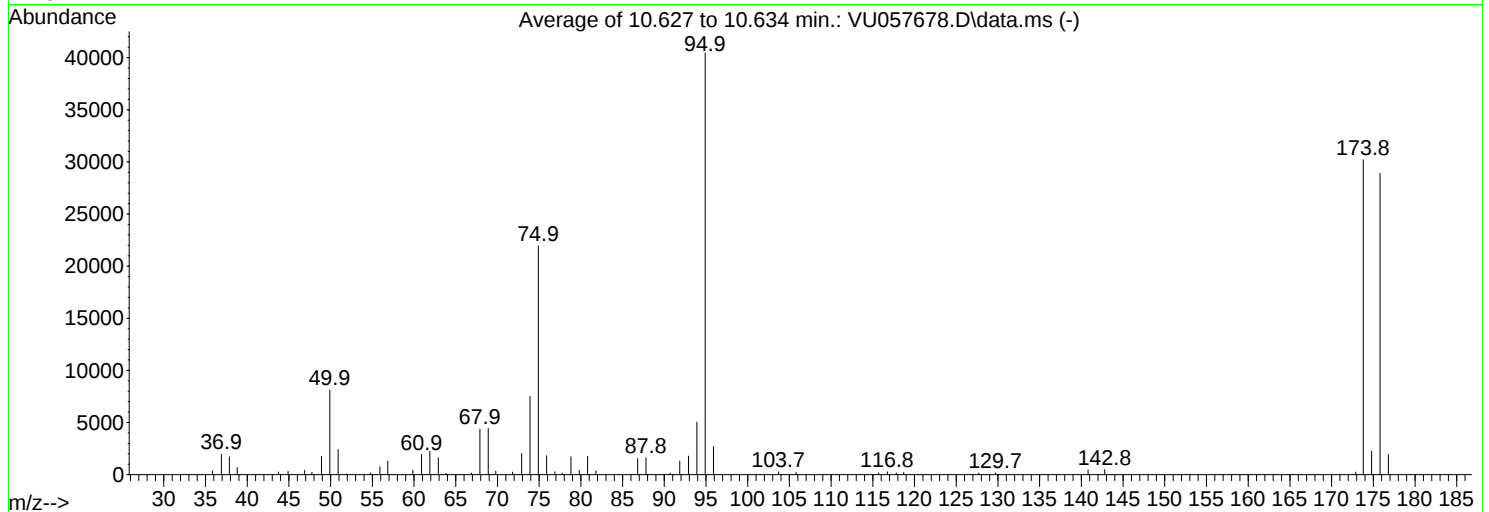


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012624\
Data File : VU057678.D
Acq On : 26 Jan 2024 08:42
Operator : MD/SY
Sample : BFB112
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB112

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012324WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jan 30 22:31:02 2024

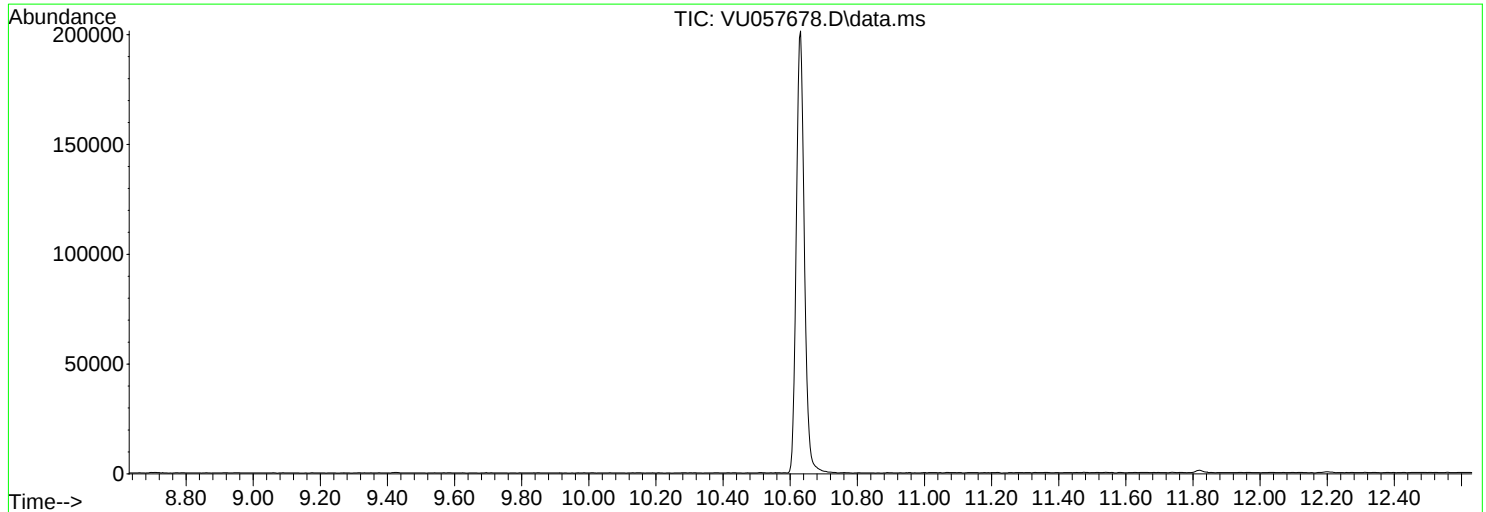

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	8121	PASS
75	95	30	80	54.2	21936	PASS
95	95	100	100	100.0	40459	PASS
96	95	5	9	6.7	2701	PASS
173	174	0.00	2	0.8	244	PASS
174	95	50	120	74.7	30213	PASS
175	174	5	9	7.5	2257	PASS
176	174	95	101	95.7	28899	PASS
177	176	5	9	6.7	1940	PASS

m/z	Abundance
39.80	348.0
43.70	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.80	387.0
36.90	1923.0
37.90	1743.0
38.80	688.0
39.80	300.0
43.80	396.0
44.90	345.0
46.90	479.0
47.70	224.0
48.90	1837.0
49.90	8308.0
50.90	2521.0
51.90	109.0
54.80	172.0
55.90	768.0
56.90	1426.0
59.80	491.0
60.90	2050.0
61.90	2290.0
62.90	1678.0
63.90	130.0
66.90	132.0
67.90	4583.0
68.90	4579.0
69.80	382.0
71.80	255.0
72.90	2044.0
73.90	7737.0
74.90	22448.0
75.90	1857.0
76.90	269.0
77.80	135.0
78.80	1765.0
79.80	412.0
80.80	1767.0
81.80	355.0
86.80	1695.0
87.80	1574.0
90.70	171.0
91.90	1246.0
92.90	1869.0
93.90	5139.0
94.90	41344.0
95.90	2870.0
96.90	107.0
103.70	247.0
105.80	238.0
115.60	168.0
116.70	278.0
117.80	180.0
118.70	228.0
127.70	167.0
129.70	168.0
140.80	485.0
142.80	510.0
172.90	230.0
173.80	29824.0
174.80	2350.0
175.80	28488.0
176.80	1911.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.80	382.0
36.90	2031.0
37.90	1740.0
38.80	706.0
39.80	311.0
43.80	412.0
44.90	317.0
46.90	454.0
47.70	247.0
48.90	1797.0
49.90	8335.0
50.90	2490.0
51.90	108.0
54.80	170.0
55.90	797.0
56.90	1342.0
59.80	444.0
60.90	1995.0
61.90	2321.0
62.90	1652.0
63.80	132.0
66.90	142.0
67.90	4505.0
68.90	4568.0
69.80	338.0
71.80	266.0
72.90	2109.0
73.90	7716.0
74.90	22560.0
75.90	1887.0
76.90	291.0
77.70	171.0
78.80	1772.0
79.80	419.0
80.80	1805.0
81.80	373.0
86.80	1583.0
87.80	1696.0
90.70	184.0
91.90	1336.0
92.90	1841.0
93.90	5189.0
94.90	41784.0
95.90	2776.0
103.70	268.0
105.80	228.0
115.70	164.0
116.80	287.0
117.80	171.0
118.70	235.0
127.70	160.0
129.70	173.0
140.80	452.0
142.80	504.0
172.90	246.0
173.80	31160.0
174.80	2338.0
175.80	29760.0
176.80	1993.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112

m/z	Abundance
35.90	349.0
36.90	1902.0
37.80	1628.0
38.80	661.0
39.80	318.0
43.80	385.0
44.90	286.0
46.90	379.0
47.80	242.0
48.90	1599.0
49.90	7719.0
50.90	2218.0
54.80	150.0
55.90	722.0
56.80	1150.0
59.90	354.0
60.90	1761.0
61.90	2104.0
62.90	1511.0
63.80	131.0
66.90	126.0
67.90	3990.0
68.90	4172.0
69.80	297.0
71.80	234.0
72.90	1953.0
73.90	7058.0
74.90	20800.0
75.90	1734.0
76.90	257.0
77.70	197.0
78.80	1642.0
79.80	393.0
80.80	1669.0
81.80	374.0
86.80	1358.0
87.80	1600.0
90.70	176.0
91.80	1268.0
92.90	1629.0
93.90	4757.0
94.90	38248.0
95.90	2458.0
103.70	252.0
105.80	188.0
115.80	158.0
116.80	249.0
117.80	150.0
118.70	226.0
127.70	139.0
129.70	156.0
140.80	382.0
142.80	451.0
172.90	255.0
173.80	29656.0
174.80	2084.0
175.80	28448.0
176.80	1915.0

Instrument :
MSVOA_U
ClientSampleId :
BFB112