


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU012720\
 Data File : VU036561.D
 Acq On : 27 Jan 2020 08:58
 Operator : JC/MD
 Sample : BFB30
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB602

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUTR012420WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 29 06:28:33 2020

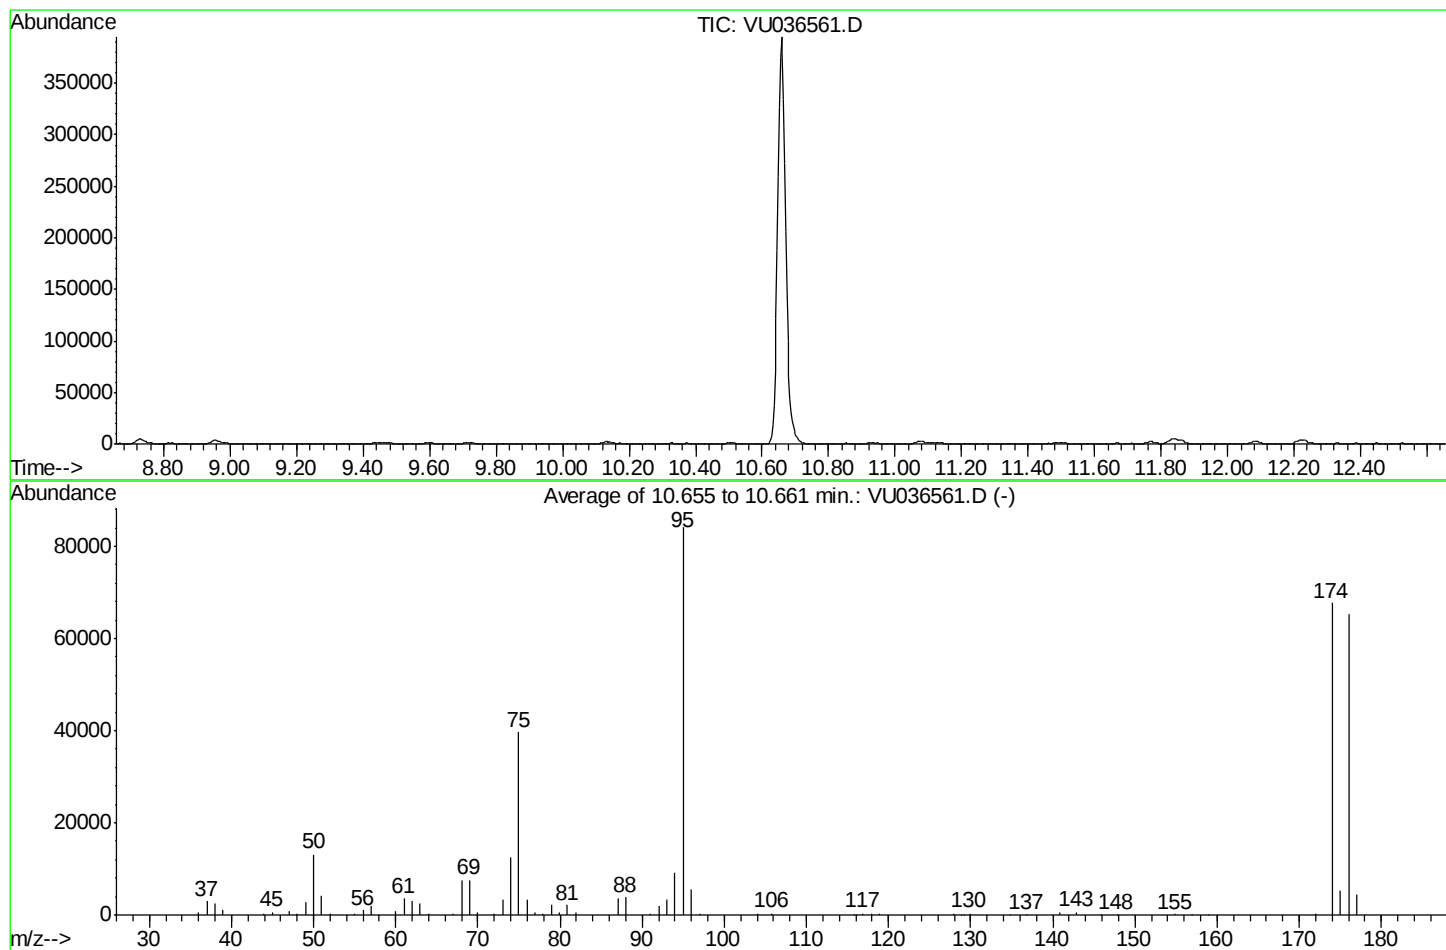

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	13159	PASS
75	95	30	80	47.2	39690	PASS
95	95	100	100	100.0	84106	PASS
96	95	5	9	6.6	5532	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.5	67741	PASS
175	174	5	9	7.6	5173	PASS
176	174	95	101	96.3	65208	PASS
177	176	5	9	6.6	4317	PASS

m/z	Abundance
43.90	299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	447.0
37.00	2961.0
38.00	2449.0
39.00	1027.0
43.90	651.0
44.90	609.0
47.00	940.0
48.00	384.0
49.00	2659.0
50.00	13178.0
51.00	4279.0
52.00	156.0
54.90	178.0
56.00	1095.0
57.00	1897.0
60.00	744.0
61.00	3598.0
62.00	3189.0
63.00	2546.0
64.00	190.0
66.90	235.0
68.00	7461.0
69.00	7472.0
70.00	471.0
72.00	374.0
73.00	3283.0
74.00	12514.0
75.00	39696.0
76.00	3257.0
77.00	522.0
77.90	360.0
78.90	2027.0
79.90	591.0
80.90	2124.0
81.90	465.0
87.00	3434.0
87.90	3616.0
90.90	252.0
92.00	2109.0
93.00	3129.0
94.00	9043.0
95.00	83128.0
96.00	5546.0
97.00	156.0
104.00	283.0
105.90	282.0
115.80	162.0
116.90	416.0
117.90	228.0
118.90	382.0
127.90	251.0
129.10	122.0
129.90	308.0
136.80	113.0
140.90	516.0
142.90	622.0
147.80	117.0
154.90	167.0
156.90	113.0
172.00	153.0
174.00	64808.0
175.00	5083.0
176.00	62440.0
177.00	4280.0
177.90	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	444.0
37.00	3088.0
37.90	2489.0
39.00	1036.0
43.90	679.0
45.00	659.0
47.00	941.0
48.00	389.0
49.00	2749.0
50.00	13599.0
51.00	4360.0
52.00	162.0
55.00	170.0
56.00	1098.0
57.00	1962.0
60.00	722.0
61.00	3669.0
62.00	3226.0
63.00	2600.0
63.90	223.0
66.90	285.0
68.00	7765.0
69.00	7786.0
70.00	497.0
72.00	362.0
73.00	3388.0
74.00	12771.0
75.00	40784.0
76.00	3294.0
77.00	541.0
77.90	385.0
78.90	2230.0
79.90	642.0
80.90	2248.0
81.90	462.0
87.00	3555.0
87.90	3920.0
91.00	273.0
92.00	2133.0
93.00	3419.0
94.00	9412.0
95.00	86560.0
96.00	5724.0
97.00	171.0
104.00	298.0
105.90	299.0
116.00	202.0
116.90	425.0
117.90	261.0
118.90	372.0
127.90	284.0
129.10	114.0
129.90	338.0
134.80	103.0
136.80	123.0
140.90	614.0
142.90	658.0
145.80	100.0
147.80	137.0
154.90	180.0
157.00	115.0
158.90	111.0
172.00	189.0
174.00	69888.0
175.00	5333.0
176.00	67304.0
177.00	4457.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602

m/z	Abundance
36.00	427.0
37.00	3004.0
38.00	2333.0
38.90	981.0
43.90	722.0
45.00	614.0
47.00	827.0
48.00	338.0
49.00	2637.0
50.00	12701.0
51.00	4016.0
52.00	162.0
55.00	171.0
56.00	1016.0
57.00	1804.0
60.00	657.0
61.00	3373.0
62.00	3125.0
63.00	2449.0
63.90	225.0
66.90	306.0
68.00	7481.0
69.00	7459.0
70.00	525.0
72.00	341.0
73.00	3183.0
74.00	12203.0
75.00	38592.0
76.00	3154.0
77.00	515.0
77.90	363.0
78.90	2145.0
79.90	608.0
80.90	2173.0
81.90	410.0
87.00	3481.0
88.00	3774.0
90.90	275.0
92.00	2019.0
93.00	3337.0
94.00	9089.0
95.00	82632.0
96.00	5328.0
97.00	179.0
104.00	274.0
105.80	278.0
116.00	230.0
116.90	367.0
118.00	263.0
118.90	348.0
127.90	294.0
128.80	102.0
129.90	319.0
134.80	103.0
136.80	115.0
140.90	642.0
142.90	640.0
145.70	101.0
147.80	153.0
154.90	175.0
158.90	102.0
171.90	206.0
174.00	68528.0
175.00	5104.0
176.00	65880.0
177.00	4215.0
177.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB602