


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012722\
 Data File : VU046858.D
 Acq On : 27 Jan 2022 08:54
 Operator : SY/MD
 Sample : BFB048
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB048

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR011822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jan 28 00:56:24 2022

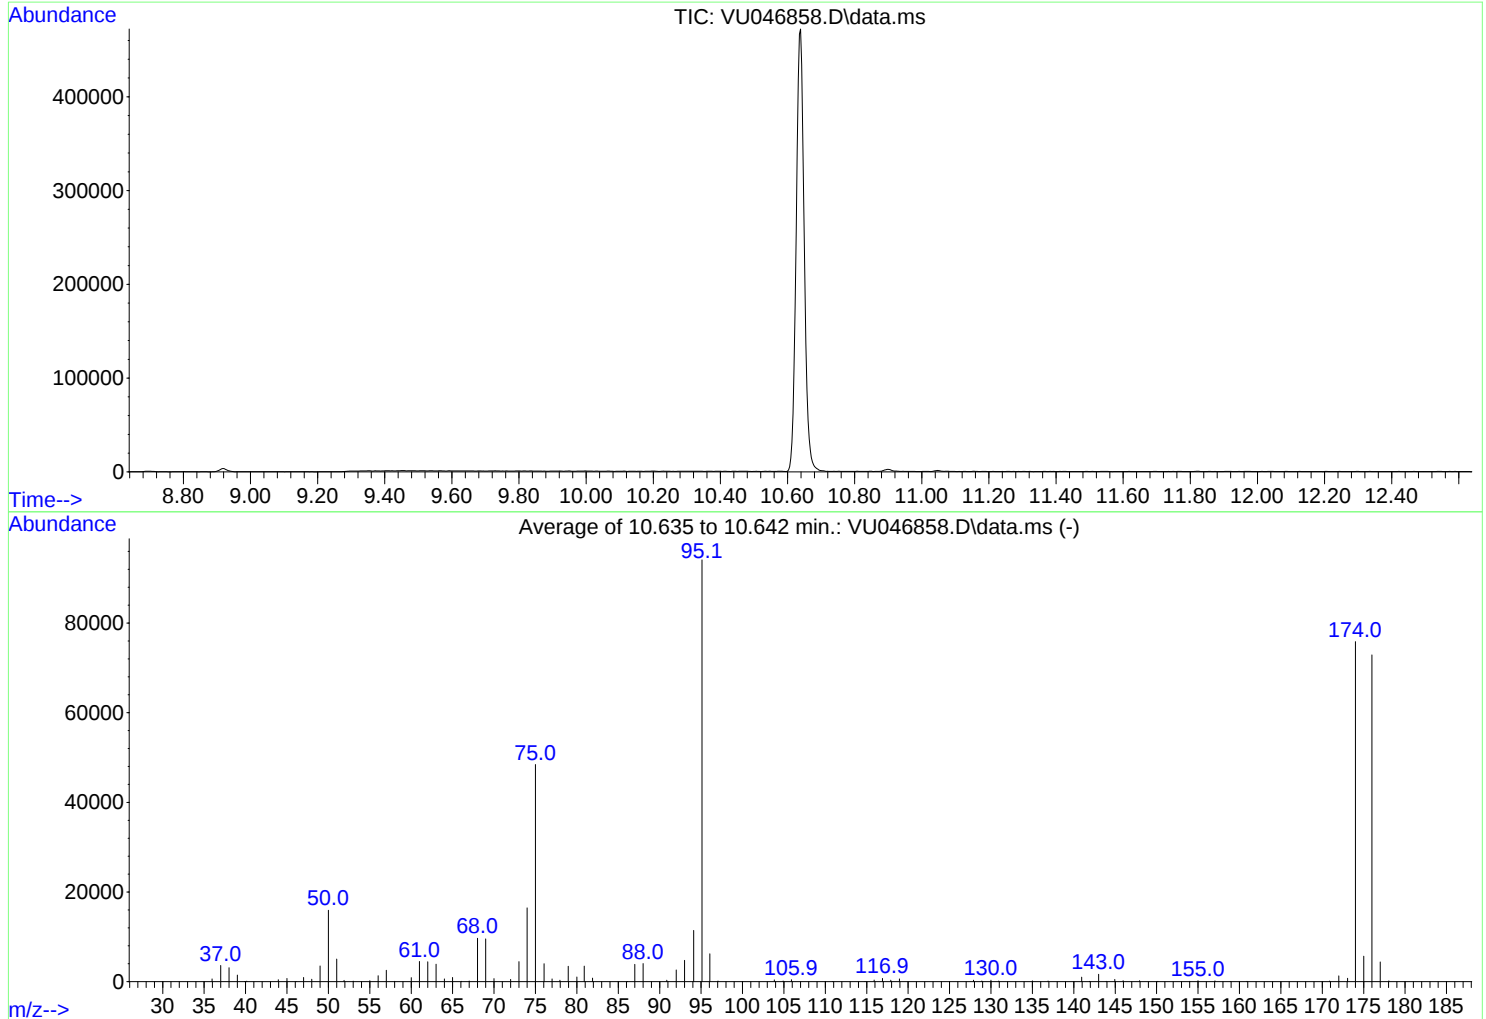

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	15923	PASS
75	95	30	80	51.5	48453	PASS
95	95	100	100	100.0	94107	PASS
96	95	5	9	6.6	6214	PASS
173	174	0.00	2	1.0	758	PASS
174	95	50	120	80.6	75872	PASS
175	174	5	9	7.5	5689	PASS
176	174	95	101	96.1	72896	PASS
177	176	5	9	6.0	4407	PASS

m/z	Abundance
35.90	247.0
38.00	117.0
43.90	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
36.00	873.0
37.00	3722.0
38.00	3399.0
39.00	1550.0
40.20	113.0
44.00	635.0
45.00	741.0
46.10	100.0
47.00	931.0
48.00	627.0
49.00	3576.0
50.00	16696.0
51.00	5293.0
51.90	323.0
53.00	124.0
55.00	220.0
56.00	1428.0
57.00	2610.0
60.00	905.0
61.00	4590.0
62.00	4718.0
63.00	3976.0
64.00	680.0
65.00	989.0
67.00	156.0
68.00	9986.0
69.00	9767.0
70.00	712.0
72.00	521.0
73.00	4790.0
74.00	16760.0
75.00	49264.0
76.10	4232.0
77.00	578.0
78.00	294.0
78.90	3694.0
80.00	1091.0
80.90	3562.0
81.90	854.0
87.00	4024.0
88.00	4109.0
90.90	330.0
92.00	2664.0
93.00	4884.0
94.10	11698.0
95.10	95952.0
96.00	6625.0
97.00	138.0
103.90	436.0
104.90	144.0
105.90	408.0
110.90	100.0
115.90	406.0
116.90	707.0
117.90	357.0
118.90	671.0
127.90	317.0
128.90	138.0
130.00	302.0
131.00	155.0
135.00	196.0
136.90	176.0
140.90	936.0
141.90	129.0
143.00	1703.0
143.90	102.0
144.90	506.0
145.90	209.0
147.90	180.0
154.00	102.0
155.00	246.0
157.10	218.0
160.90	137.0
170.90	171.0
172.00	1356.0
173.10	761.0
174.00	76464.0
175.00	5802.0
176.00	73256.0
177.00	4257.0
178.10	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
36.00	874.0
37.00	3730.0
38.00	3308.0
39.00	1525.0
40.00	116.0
40.30	122.0
44.00	610.0
45.00	763.0
47.00	975.0
48.00	566.0
49.00	3589.0
50.00	16440.0
51.00	5181.0
51.90	322.0
53.00	121.0
55.00	203.0
56.00	1420.0
57.00	2620.0
58.00	101.0
60.00	917.0
61.00	4644.0
62.00	4522.0
63.00	4017.0
64.00	603.0
65.00	892.0
66.10	100.0
67.00	162.0
68.00	10008.0
69.00	9803.0
70.00	694.0
72.00	515.0
73.00	4600.0
74.00	16984.0
75.00	50072.0
76.00	4115.0
77.00	650.0
78.00	341.0
79.00	3519.0
80.00	1110.0
80.90	3548.0
81.90	808.0
86.10	100.0
87.00	3997.0
88.00	4178.0
90.80	323.0
92.00	2688.0
93.00	4934.0
94.10	11815.0
95.10	96912.0
96.10	6401.0
97.10	152.0
103.80	408.0
104.90	137.0
105.90	465.0
115.90	367.0
116.90	734.0
117.90	356.0
118.90	631.0
127.90	346.0
128.90	135.0
130.00	345.0
130.90	151.0
135.00	199.0
136.90	156.0
141.00	974.0
141.90	117.0
143.00	1729.0
143.90	116.0
144.90	529.0
145.90	214.0
148.00	213.0
150.10	117.0
154.00	102.0
155.00	228.0
157.00	179.0
158.90	117.0
160.90	134.0
170.90	141.0
172.00	1345.0
173.00	777.0
174.00	78392.0
175.00	5853.0
176.00	75048.0
177.00	4557.0
178.00	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048

m/z	Abundance
36.00	844.0
37.00	3404.0
38.00	2937.0
39.00	1346.0
39.90	131.0
44.00	542.0
45.00	694.0
47.00	904.0
48.00	420.0
49.00	3340.0
50.00	14633.0
51.00	4654.0
51.90	271.0
53.00	121.0
55.00	196.0
56.00	1170.0
57.00	2339.0
58.00	105.0
60.00	822.0
61.00	4295.0
62.00	4038.0
63.00	3675.0
64.00	518.0
65.00	862.0
66.00	107.0
67.00	172.0
68.00	9038.0
69.00	9065.0
70.00	653.0
72.00	510.0
73.00	3961.0
74.00	15681.0
75.00	46024.0
76.00	3711.0
77.00	635.0
77.90	374.0
79.00	3085.0
80.00	960.0
80.90	3241.0
81.90	744.0
87.00	3583.0
88.00	3839.0
90.80	281.0
92.00	2487.0
93.00	4476.0
94.10	10716.0
95.10	89456.0
96.10	5617.0
97.10	167.0
103.90	328.0
104.90	123.0
105.90	425.0
114.80	107.0
115.90	306.0
116.90	721.0
117.90	305.0
119.00	561.0
127.90	324.0
128.90	130.0
130.00	356.0
130.90	153.0
135.00	171.0
136.90	146.0
141.00	1055.0
143.00	1538.0
145.00	482.0
146.00	180.0
148.00	217.0
150.20	129.0
155.00	217.0
157.00	141.0
171.00	100.0
172.00	1186.0
173.00	735.0
174.00	72760.0
175.00	5412.0
176.00	70384.0
177.00	4406.0
178.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB048