

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052837.D
 Acq On : 27 Jan 2023 11:31
 Operator : JC/MD
 Sample : 01295-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rVB	115398	137037	8.34%	1.343%
2	1.909	169	177	192	rVB	90658	124967	7.61%	1.225%
3	2.568	369	382	395	rBV4	269635	517000	31.47%	5.068%
4	2.793	438	452	469	rBV	124061	214292	13.04%	2.101%
5	2.990	509	513	515	rBV	465	339	0.02%	0.003%
6	3.035	523	527	528	rBV	1104	715	0.04%	0.007%
7	3.147	559	562	566	rVB	306	219	0.01%	0.002%
8	3.170	566	569	570	rBV2	451	236	0.01%	0.002%
9	3.311	604	613	617	rBV2	991	1594	0.10%	0.016%
10	3.459	656	659	666	rBV	498	575	0.04%	0.006%
11	3.488	666	668	671	rBV	130	104	0.01%	0.001%
12	3.539	682	684	688	rVB	308	129	0.01%	0.001%
13	3.562	688	691	694	rBV	165	112	0.01%	0.001%
14	3.581	694	697	700	rBV	306	250	0.02%	0.002%
15	3.729	739	743	747	rVB2	388	377	0.02%	0.004%
16	3.755	748	751	753	rBV	273	146	0.01%	0.001%
17	3.771	753	756	759	rBV	226	167	0.01%	0.002%
18	3.867	767	786	809	rBV	24129	56540	3.44%	0.554%
19	4.009	825	830	833	rBV	420	449	0.03%	0.004%
20	4.092	853	856	857	rBV	289	140	0.01%	0.001%
21	4.202	887	890	895	rVB2	202	207	0.01%	0.002%
22	4.234	895	900	901	rBV2	167	148	0.01%	0.001%
23	4.292	911	918	926	rBV2	399	796	0.05%	0.008%
24	4.375	941	944	947	rBV	399	378	0.02%	0.004%
25	4.414	954	956	959	rBV2	164	110	0.01%	0.001%
26	4.494	975	981	984	rVB	327	372	0.02%	0.004%
27	4.539	992	995	998	rBV2	382	285	0.02%	0.003%
28	4.620	998	1020	1023	rBV2	76915	136085	8.28%	1.334%
29	4.948	1119	1122	1125	rBB2	417	256	0.02%	0.003%
30	4.967	1125	1128	1130	rBV	267	209	0.01%	0.002%
31	5.057	1139	1156	1181	rBV	192443	436748	26.59%	4.281%
32	5.227	1207	1209	1212	rBV	165	128	0.01%	0.001%
33	5.260	1217	1219	1222	rBV	230	131	0.01%	0.001%
34	5.311	1222	1235	1245	rBV6	3046	7158	0.44%	0.070%
35	5.369	1249	1253	1254	rBV	589	451	0.03%	0.004%
36	5.398	1259	1262	1263	rBV	474	242	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052837.D
 Acq On : 27 Jan 2023 11:31
 Operator : JC/MD
 Sample : 01295-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.459	1278	1281	1283	rBV2	367	246	0.01%	0.002%
38	5.501	1291	1294	1297	rVV	189	155	0.01%	0.002%
39	5.581	1316	1319	1322	rBV	180	170	0.01%	0.002%
40	5.719	1341	1362	1382	rBV2	372606	1027612	62.56%	10.074%
41	5.954	1432	1435	1439	rBV2	281	260	0.02%	0.003%
42	6.025	1445	1457	1464	rBV4	1240	2396	0.15%	0.023%
43	6.083	1472	1475	1481	rBV2	275	288	0.02%	0.003%
44	6.147	1490	1495	1497	rBV2	306	286	0.02%	0.003%
45	6.244	1509	1525	1542	rBV	211032	398249	24.24%	3.904%
46	6.539	1590	1617	1649	rBV	861503	1642718	100.00%	16.103%
47	6.687	1649	1663	1680	rVV	231405	449794	27.38%	4.409%
48	6.861	1713	1717	1719	rBV	163	166	0.01%	0.002%
49	6.877	1719	1722	1724	rBV	241	184	0.01%	0.002%
50	6.989	1746	1757	1776	rVB4	4918	12840	0.78%	0.126%
51	7.070	1780	1782	1784	rBV2	170	109	0.01%	0.001%
52	7.186	1809	1818	1827	rBV3	1688	3225	0.20%	0.032%
53	7.311	1854	1857	1860	rBV	262	224	0.01%	0.002%
54	7.456	1898	1902	1903	rBV	199	160	0.01%	0.002%
55	7.491	1910	1913	1916	rVB2	265	185	0.01%	0.002%
56	7.562	1921	1935	1958	rBV	127461	224410	13.66%	2.200%
57	7.665	1964	1967	1969	rBV	508	337	0.02%	0.003%
58	7.678	1969	1971	1972	rBV	764	359	0.02%	0.004%
59	7.825	2013	2017	2024	rVB2	215	287	0.02%	0.003%
60	7.893	2024	2038	2055	rBV	477633	816524	49.71%	8.004%
61	8.051	2082	2087	2091	rBV4	425	442	0.03%	0.004%
62	8.176	2114	2126	2141	rBV2	87059	149807	9.12%	1.469%
63	8.298	2162	2164	2166	rBV2	179	117	0.01%	0.001%
64	8.481	2214	2221	2229	rVV5	3770	5481	0.33%	0.054%
65	8.549	2229	2242	2257	rVV	728449	1218764	74.19%	11.947%
66	8.629	2257	2267	2303	rVB2	225316	433336	26.38%	4.248%
67	8.925	2356	2359	2361	rBV2	470	297	0.02%	0.003%
68	9.034	2387	2393	2399	rVB4	1186	1573	0.10%	0.015%
69	9.060	2399	2401	2404	rVB2	226	121	0.01%	0.001%
70	9.083	2404	2408	2410	rBV2	202	135	0.01%	0.001%
71	9.186	2438	2440	2442	rBV	201	143	0.01%	0.001%
72	9.259	2460	2463	2464	rBV	208	113	0.01%	0.001%
73	9.369	2494	2497	2498	rBV	223	145	0.01%	0.001%
74	9.414	2499	2511	2533	rVV	297529	486744	29.63%	4.771%
75	9.568	2553	2559	2565	rBV4	732	1114	0.07%	0.011%
76	9.755	2611	2617	2627	rVB2	5733	8316	0.51%	0.082%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052837.D
 Acq On : 27 Jan 2023 11:31
 Operator : JC/MD
 Sample : 01295-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.076	2714	2717	2718	rBV	297	163	0.01%	0.002%
78	10.128	2728	2733	2742	rVB6	1276	1732	0.11%	0.017%
79	10.195	2749	2754	2756	rBV2	202	212	0.01%	0.002%
80	10.237	2765	2767	2769	rBV	210	116	0.01%	0.001%
81	10.340	2794	2799	2802	rBV2	464	453	0.03%	0.004%
82	10.430	2820	2827	2830	rBV2	219	278	0.02%	0.003%
83	10.636	2888	2891	2895	rVB	297	241	0.01%	0.002%
84	10.661	2895	2899	2900	rBV2	179	128	0.01%	0.001%
85	10.751	2914	2927	2943	rVB	319963	507213	30.88%	4.972%
86	10.877	2962	2966	2972	rBV3	581	809	0.05%	0.008%
87	10.948	2980	2988	2993	rBV2	383	553	0.03%	0.005%
88	10.983	2996	2999	3002	rBV2	236	158	0.01%	0.002%
89	11.038	3013	3016	3018	rBV2	288	206	0.01%	0.002%
90	11.420	3131	3135	3138	rBV	380	352	0.02%	0.003%
91	11.462	3145	3148	3152	rBV	481	462	0.03%	0.005%
92	11.636	3199	3202	3204	rBV	243	170	0.01%	0.002%
93	11.697	3218	3221	3225	rBV2	202	199	0.01%	0.002%
94	11.809	3243	3256	3277	rBV	270272	440929	26.84%	4.322%
95	12.057	3325	3333	3348	rVB2	10362	16620	1.01%	0.163%
96	12.189	3361	3374	3389	rBV	432279	702471	42.76%	6.886%
97	12.369	3427	3430	3433	rBV	235	197	0.01%	0.002%
98	12.504	3470	3472	3475	rBV2	210	175	0.01%	0.002%
99	12.999	3623	3626	3627	rBV	260	144	0.01%	0.001%
100	13.980	3929	3931	3937	rVB3	501	211	0.01%	0.002%




Sum of corrected areas: 10201116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052837.D
Acq On : 27 Jan 2023 11:31
Operator : JC/MD
Sample : 01295-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COLC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

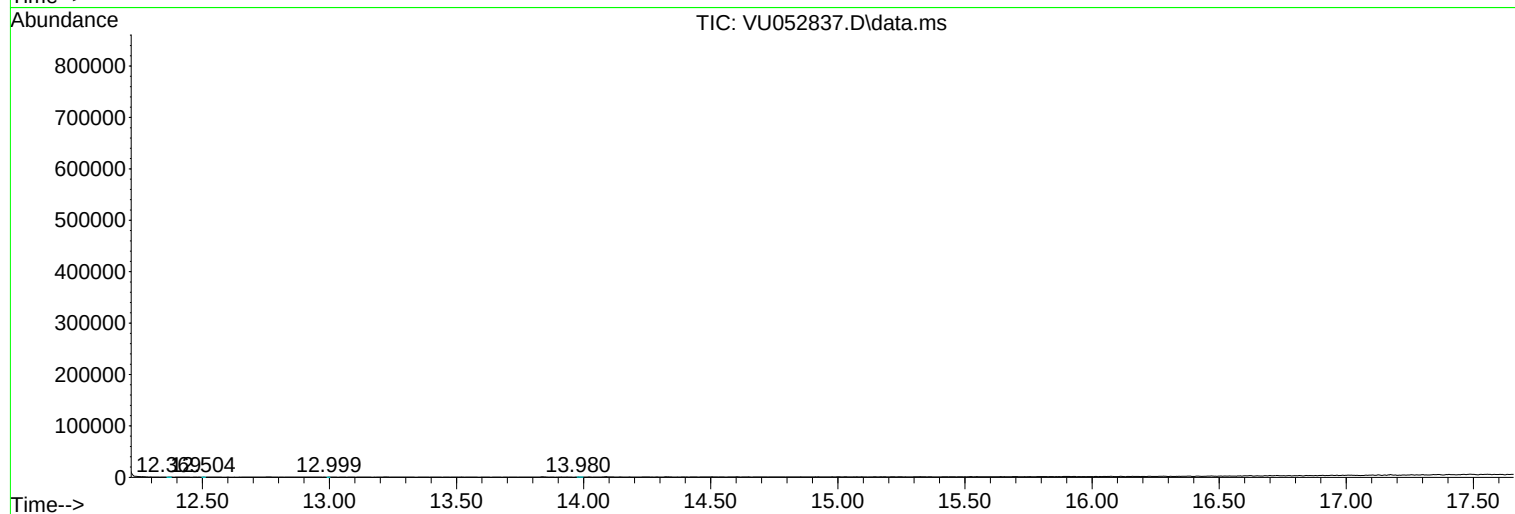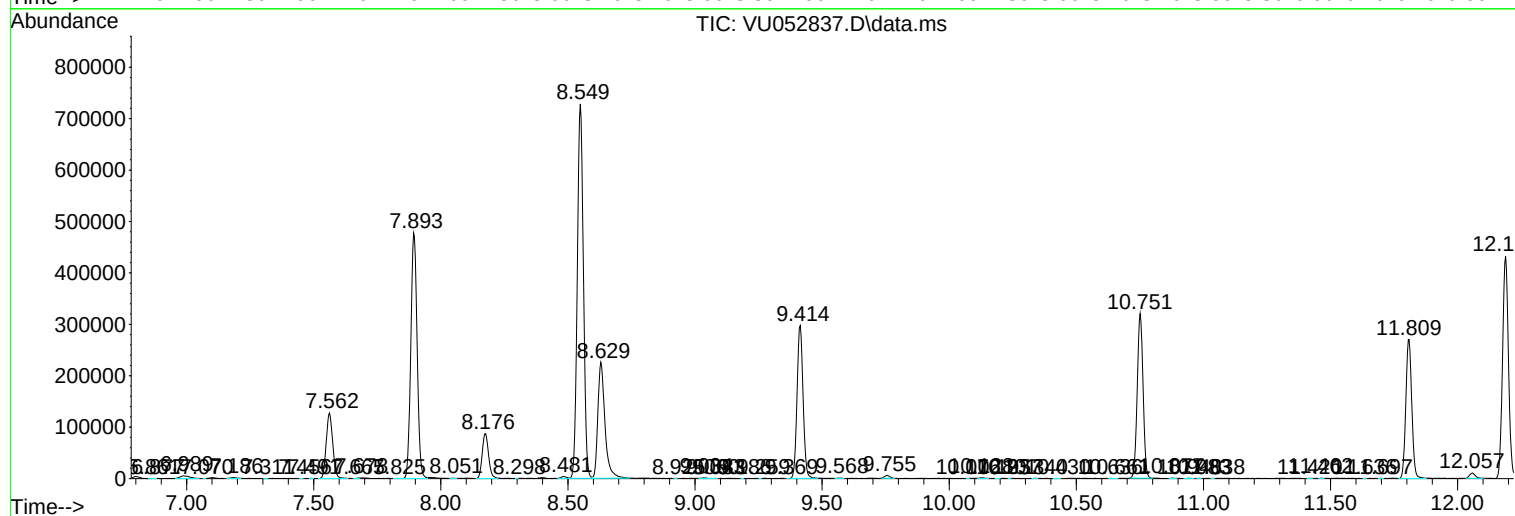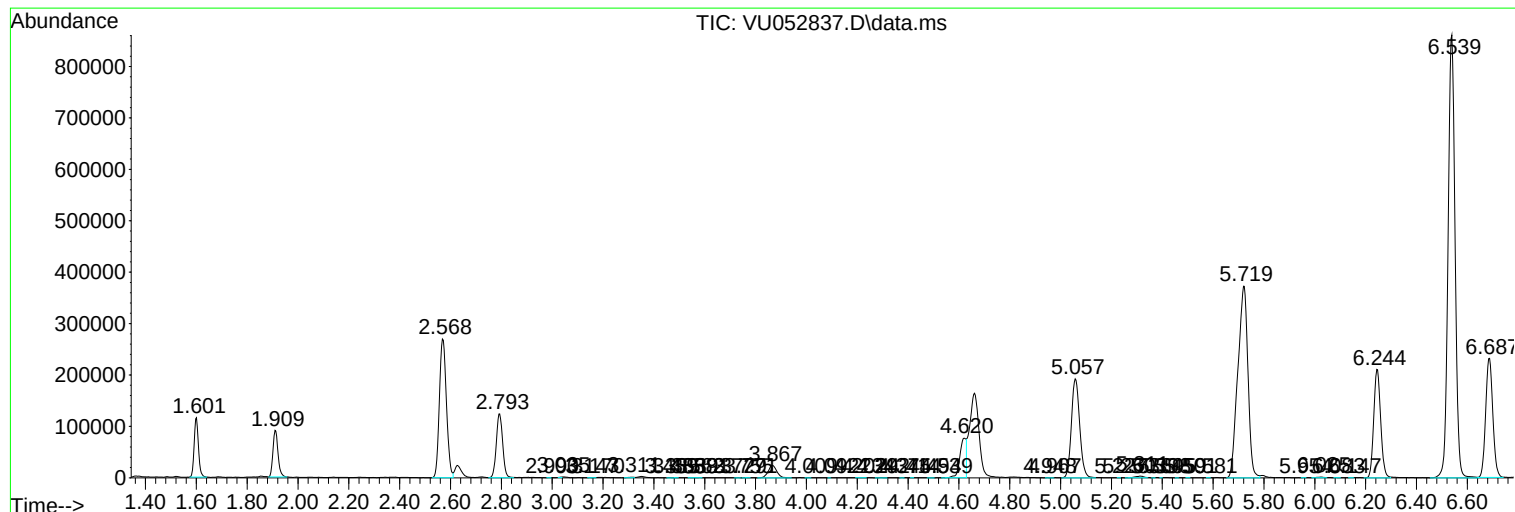

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052837.D
Acq On : 27 Jan 2023 11:31
Operator : JC/MD
Sample : 01295-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052837.D
Acq On : 27 Jan 2023 11:31
Operator : JC/MD
Sample : 01295-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc