

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052838.D
 Acq On : 27 Jan 2023 11:53
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rVB	110978	131432	2.77%	0.955%
2	1.909	169	177	194	rVB	95971	130238	2.75%	0.947%
3	2.491	355	358	360	rBV	449	285	0.01%	0.002%
4	2.568	369	382	398	rBV3	275669	523725	11.05%	3.807%
5	2.716	424	428	431	rBV3	604	525	0.01%	0.004%
6	2.758	438	441	444	rBV2	419	447	0.01%	0.003%
7	3.041	522	529	530	rBV3	726	792	0.02%	0.006%
8	3.102	545	548	550	rBV	335	234	0.00%	0.002%
9	3.189	574	575	580	rVB2	372	243	0.01%	0.002%
10	3.285	604	605	610	rVB	258	129	0.00%	0.001%
11	3.314	610	614	617	rBV2	419	416	0.01%	0.003%
12	3.353	618	626	641	rVB4	2738	5196	0.11%	0.038%
13	3.411	641	644	648	rBV	285	290	0.01%	0.002%
14	3.491	665	669	673	rBV2	240	282	0.01%	0.002%
15	3.546	682	686	689	rBV	296	320	0.01%	0.002%
16	3.639	712	715	721	rBV2	196	174	0.00%	0.001%
17	3.755	747	751	753	rBV	297	275	0.01%	0.002%
18	3.777	755	758	761	rBV	143	126	0.00%	0.001%
19	3.816	767	770	772	rVB2	282	182	0.00%	0.001%
20	3.864	772	785	799	rBV2	9199	19583	0.41%	0.142%
21	3.980	815	821	825	rBV2	220	274	0.01%	0.002%
22	4.028	833	836	837	rBV	201	129	0.00%	0.001%
23	4.154	872	875	877	rBV	259	183	0.00%	0.001%
24	4.218	889	895	899	rVB2	360	472	0.01%	0.003%
25	4.240	899	902	905	rBV	321	276	0.01%	0.002%
26	4.324	923	928	931	rBV	266	331	0.01%	0.002%
27	4.356	935	938	942	rVB2	312	205	0.00%	0.001%
28	4.401	949	952	955	rVB2	307	243	0.01%	0.002%
29	4.424	955	959	963	rBV2	368	452	0.01%	0.003%
30	4.465	969	972	979	rVB	408	523	0.01%	0.004%
31	4.504	979	984	986	rBV	181	187	0.00%	0.001%
32	4.658	1008	1032	1054	rBV3	279257	794796	16.77%	5.777%
33	4.919	1110	1113	1120	rVB2	253	301	0.01%	0.002%
34	4.964	1124	1127	1131	rBB3	284	163	0.00%	0.001%
35	4.986	1132	1134	1137	rBV2	173	129	0.00%	0.001%
36	5.057	1140	1156	1177	rBV	190088	419725	8.85%	3.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052838.D
 Acq On : 27 Jan 2023 11:53
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.250	1213	1216	1220	rVV	307	280	0.01%	0.002%
38	5.311	1220	1235	1255	rVV	34525	76049	1.60%	0.553%
39	5.430	1268	1272	1275	rBV2	208	204	0.00%	0.001%
40	5.719	1341	1362	1389	rBV2	373613	1017549	21.46%	7.396%
41	5.848	1399	1402	1404	rVB	287	138	0.00%	0.001%
42	5.935	1427	1429	1431	rBV	261	160	0.00%	0.001%
43	5.948	1431	1433	1434	rVV	257	131	0.00%	0.001%
44	5.973	1437	1441	1446	rVB2	216	202	0.00%	0.001%
45	6.012	1450	1453	1455	rBV2	271	149	0.00%	0.001%
46	6.070	1468	1471	1474	rBV2	331	332	0.01%	0.002%
47	6.157	1494	1498	1501	rVB	230	183	0.00%	0.001%
48	6.243	1511	1525	1554	rBV	263776	495433	10.45%	3.601%
49	6.356	1555	1560	1564	rVV2	407	431	0.01%	0.003%
50	6.536	1602	1616	1640	rBV	474391	877073	18.50%	6.375%
51	6.684	1649	1662	1685	rVB	229377	451232	9.52%	3.280%
52	7.067	1778	1781	1784	rBV2	189	172	0.00%	0.001%
53	7.186	1812	1818	1829	rVB5	1513	2653	0.06%	0.019%
54	7.243	1832	1836	1838	rBV3	286	184	0.00%	0.001%
55	7.282	1845	1848	1851	rBV2	283	243	0.01%	0.002%
56	7.317	1857	1859	1863	rBB	261	181	0.00%	0.001%
57	7.340	1864	1866	1868	rBV	244	137	0.00%	0.001%
58	7.362	1868	1873	1874	rBV2	196	146	0.00%	0.001%
59	7.562	1920	1935	1955	rBV	126947	221134	4.66%	1.607%
60	7.632	1955	1957	1961	rVB	512	342	0.01%	0.002%
61	7.652	1961	1963	1965	rBV	394	224	0.00%	0.002%
62	7.787	2002	2005	2010	rVB2	239	222	0.00%	0.002%
63	7.893	2023	2038	2057	rBV	473198	804713	16.98%	5.849%
64	8.092	2097	2100	2102	rVV2	218	130	0.00%	0.001%
65	8.134	2110	2113	2114	rBV	221	126	0.00%	0.001%
66	8.176	2114	2126	2142	rVV	90882	149403	3.15%	1.086%
67	8.256	2149	2151	2153	rBV2	373	140	0.00%	0.001%
68	8.427	2200	2204	2206	rBV	186	163	0.00%	0.001%
69	8.452	2209	2212	2213	rBV	617	312	0.01%	0.002%
70	8.549	2228	2242	2257	rBV	2879151	4740516	100.00%	34.456%
71	8.632	2258	2268	2297	rVB3	234275	454559	9.59%	3.304%
72	9.034	2390	2393	2395	rBV2	250	156	0.00%	0.001%
73	9.282	2463	2470	2479	rVB3	1444	2072	0.04%	0.015%
74	9.369	2493	2497	2498	rBV2	206	149	0.00%	0.001%
75	9.414	2498	2511	2534	rVV	375096	617475	13.03%	4.488%
76	9.529	2545	2547	2549	rBV3	503	276	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052838.D
 Acq On : 27 Jan 2023 11:53
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.571	2557	2560	2566	rVB3	491	465	0.01%	0.003%
78	9.652	2582	2585	2588	rBV	205	192	0.00%	0.001%
79	9.700	2597	2600	2602	rBV2	358	248	0.01%	0.002%
80	10.317	2787	2792	2795	rVB2	208	214	0.00%	0.002%
81	10.616	2882	2885	2889	rBV2	195	143	0.00%	0.001%
82	10.671	2900	2902	2904	rBV	215	147	0.00%	0.001%
83	10.751	2915	2927	2943	rBV	318216	513826	10.84%	3.735%
84	10.973	2993	2996	2999	rBV	303	289	0.01%	0.002%
85	10.989	2999	3001	3005	rVB	271	144	0.00%	0.001%
86	11.015	3005	3009	3014	rBV2	313	379	0.01%	0.003%
87	11.468	3145	3150	3154	rBV3	471	655	0.01%	0.005%
88	11.520	3160	3166	3173	rBV5	1447	1928	0.04%	0.014%
89	11.738	3231	3234	3236	rBV	235	197	0.00%	0.001%
90	11.806	3243	3255	3275	rBV	351725	559893	11.81%	4.069%
91	11.973	3304	3307	3312	rBV	430	505	0.01%	0.004%
92	12.057	3325	3333	3352	rVB2	12297	20502	0.43%	0.149%
93	12.189	3361	3374	3394	rBV	441069	708480	14.95%	5.149%
94	12.526	3476	3479	3482	rBV2	193	140	0.00%	0.001%
95	12.835	3572	3575	3581	rBV2	267	271	0.01%	0.002%
96	13.195	3684	3687	3690	rBV	255	170	0.00%	0.001%
97	13.211	3690	3692	3696	rBV2	285	213	0.00%	0.002%
98	13.446	3759	3765	3769	rVB2	296	295	0.01%	0.002%
99	13.716	3847	3849	3850	rBV	303	131	0.00%	0.001%
100	13.967	3923	3927	3929	rBV2	289	258	0.01%	0.002%




Sum of corrected areas: 13758342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052838.D
Acq On : 27 Jan 2023 11:53
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

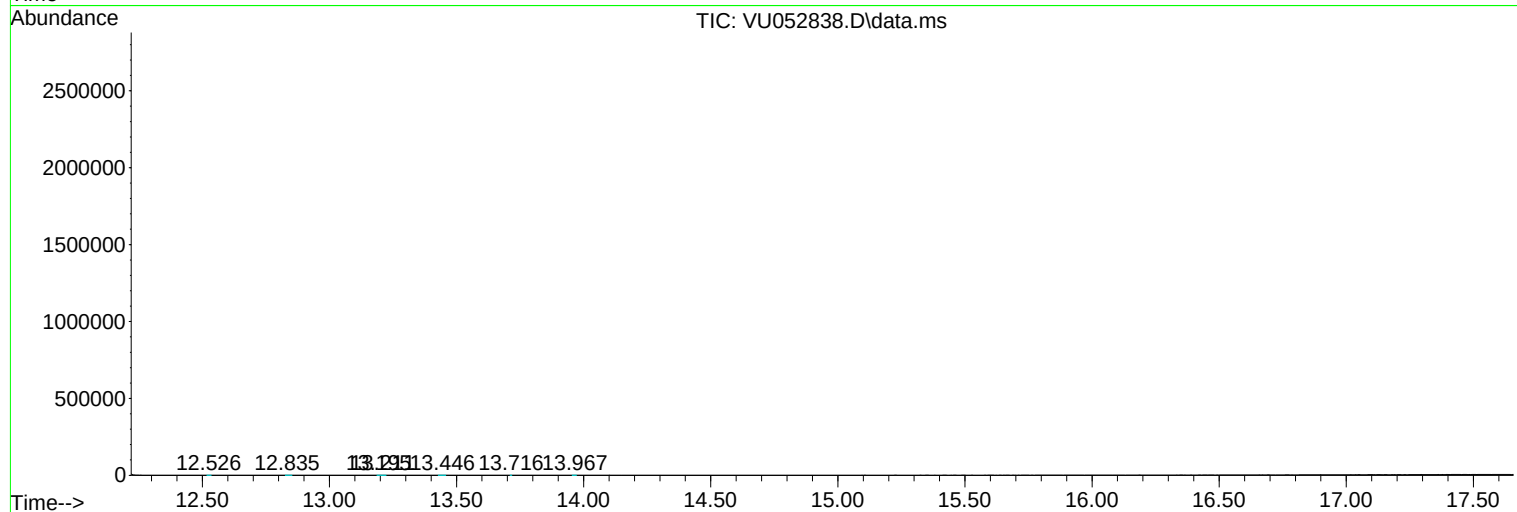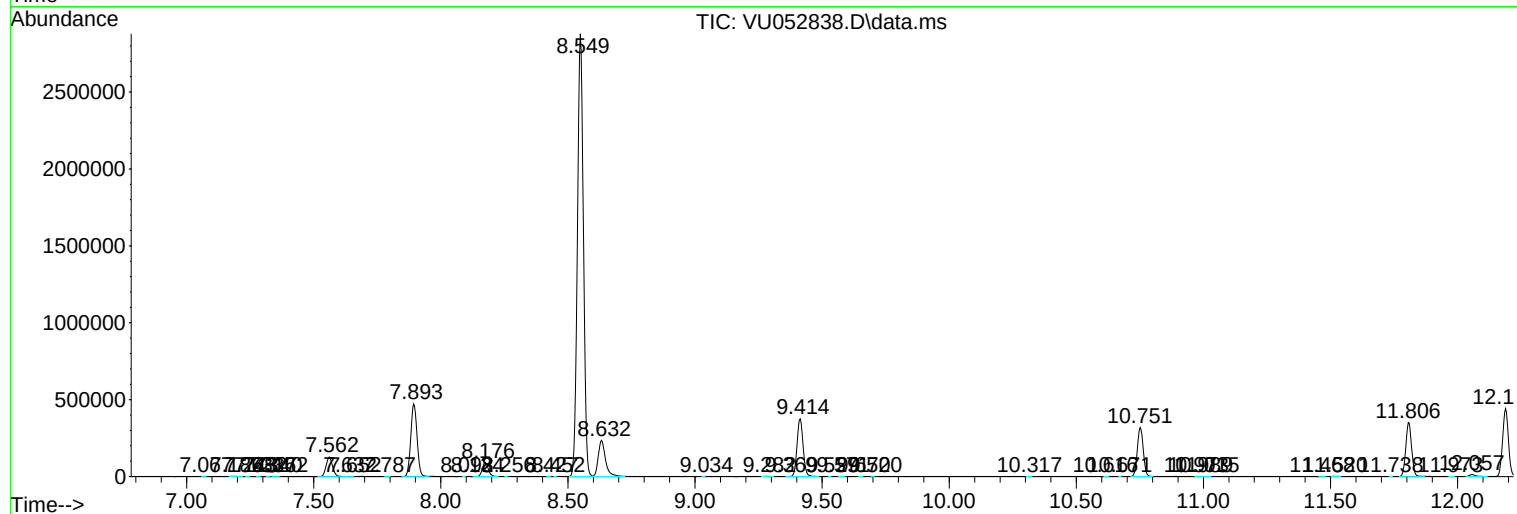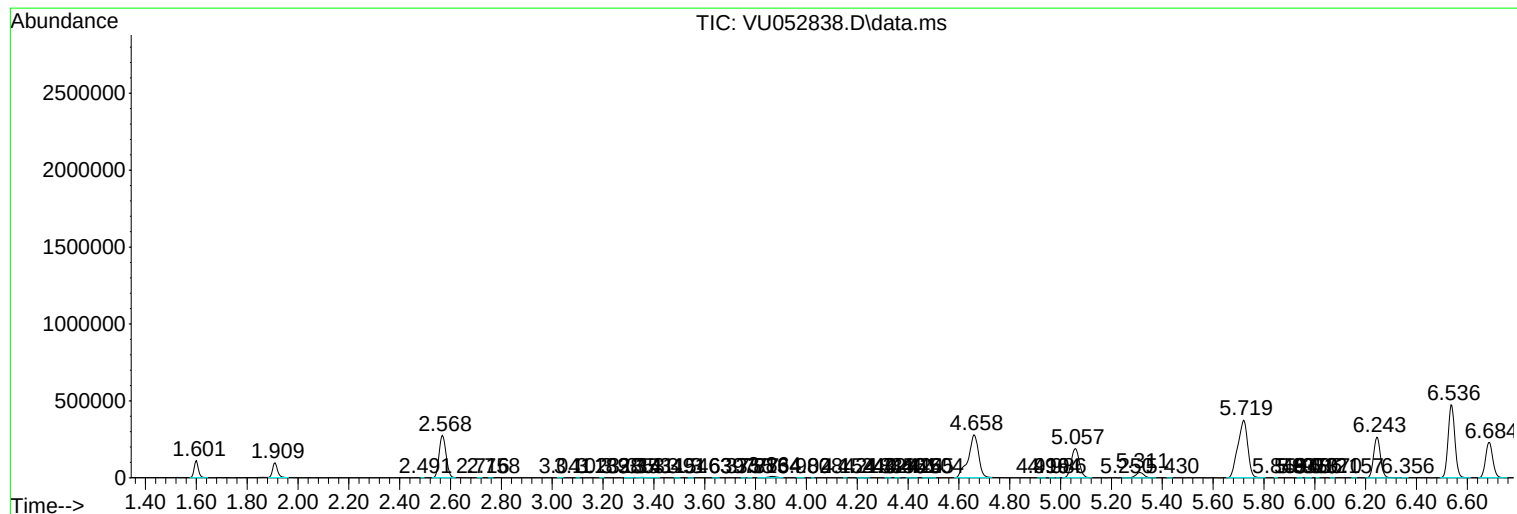

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052838.D
Acq On : 27 Jan 2023 11:53
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052838.D
Acq On : 27 Jan 2023 11:53
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc