

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052841.D
 Acq On : 27 Jan 2023 13:03
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COLC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rVB	93352	110714	2.62%	0.836%
2	1.913	170	178	195	rVB	82515	115605	2.74%	0.873%
3	2.568	368	382	399	rBV2	232093	443939	10.51%	3.354%
4	2.723	424	430	432	rBV4	461	511	0.01%	0.004%
5	2.797	444	453	461	rVB3	1381	2499	0.06%	0.019%
6	2.864	471	474	477	rBV2	156	136	0.00%	0.001%
7	3.044	523	530	539	rBV3	1606	2768	0.07%	0.021%
8	3.112	548	551	555	rVB2	191	137	0.00%	0.001%
9	3.138	555	559	561	rBV	220	195	0.00%	0.001%
10	3.221	582	585	590	rVB2	394	267	0.01%	0.002%
11	3.247	590	593	596	rVB2	287	180	0.00%	0.001%
12	3.273	597	601	602	rBV2	205	141	0.00%	0.001%
13	3.302	606	610	613	rBV3	397	368	0.01%	0.003%
14	3.353	619	626	634	rVB4	2257	3917	0.09%	0.030%
15	3.414	639	645	650	rBV2	288	420	0.01%	0.003%
16	3.591	695	700	705	rBV	267	320	0.01%	0.002%
17	3.777	755	758	763	rVB2	294	343	0.01%	0.003%
18	3.864	772	785	803	rBV2	8576	18959	0.45%	0.143%
19	3.974	814	819	820	rBV	337	323	0.01%	0.002%
20	4.015	829	832	834	rBV	175	148	0.00%	0.001%
21	4.083	848	853	856	rVB2	394	339	0.01%	0.003%
22	4.121	862	865	868	rBV	167	132	0.00%	0.001%
23	4.154	872	875	878	rBV	208	190	0.00%	0.001%
24	4.221	890	896	899	rVB2	408	427	0.01%	0.003%
25	4.244	900	903	905	rBV2	311	241	0.01%	0.002%
26	4.285	912	916	920	rBV2	294	290	0.01%	0.002%
27	4.308	920	923	926	rBV	232	174	0.00%	0.001%
28	4.465	968	972	976	rVB2	334	361	0.01%	0.003%
29	4.494	976	981	983	rBV2	291	261	0.01%	0.002%
30	4.530	989	992	995	rVB2	344	218	0.01%	0.002%
31	4.565	1000	1003	1006	rVB2	165	133	0.00%	0.001%
32	4.658	1009	1032	1069	rBV3	271626	773343	18.31%	5.842%
33	4.967	1123	1128	1130	rBV2	293	268	0.01%	0.002%
34	5.057	1140	1156	1176	rBV	179054	401459	9.50%	3.033%
35	5.311	1221	1235	1253	rBV	29465	67571	1.60%	0.510%
36	5.488	1282	1290	1292	rBV2	386	502	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052841.D
 Acq On : 27 Jan 2023 13:03
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	5.626	1331	1333	1335	rBB	263	119	0.00%	0.001%
38	5.719	1340	1362	1382	rBV2	354247	965510	22.86%	7.294%
39	5.928	1426	1427	1429	rBV2	349	125	0.00%	0.001%
40	5.993	1444	1447	1450	rBV2	279	159	0.00%	0.001%
41	6.035	1455	1460	1464	rBV4	436	502	0.01%	0.004%
42	6.083	1471	1475	1478	rBV2	217	187	0.00%	0.001%
43	6.102	1478	1481	1484	rVV2	455	349	0.01%	0.003%
44	6.244	1511	1525	1548	rBV	324531	608573	14.41%	4.597%
45	6.475	1593	1597	1602	rBB2	301	310	0.01%	0.002%
46	6.536	1602	1616	1642	rBV2	435213	814160	19.27%	6.151%
47	6.684	1649	1662	1686	rVB	223859	432411	10.24%	3.267%
48	6.793	1692	1696	1697	rBV	409	272	0.01%	0.002%
49	6.867	1715	1719	1722	rBV2	236	235	0.01%	0.002%
50	6.973	1749	1752	1755	rVB2	329	189	0.00%	0.001%
51	6.996	1755	1759	1761	rBV	172	168	0.00%	0.001%
52	7.179	1810	1816	1830	rVB5	1355	3146	0.07%	0.024%
53	7.231	1830	1832	1834	rBV5	262	176	0.00%	0.001%
54	7.243	1834	1836	1840	rBV2	262	158	0.00%	0.001%
55	7.295	1849	1852	1856	rBV2	229	222	0.01%	0.002%
56	7.398	1881	1884	1886	rBV	167	139	0.00%	0.001%
57	7.469	1904	1906	1911	rBV2	281	232	0.01%	0.002%
58	7.562	1922	1935	1954	rBV	122557	212548	5.03%	1.606%
59	7.832	2015	2019	2022	rVB2	220	177	0.00%	0.001%
60	7.893	2024	2038	2057	rBV	442629	749534	17.74%	5.662%
61	8.173	2113	2125	2146	rBV	85477	143774	3.40%	1.086%
62	8.285	2157	2160	2163	rBV3	359	235	0.01%	0.002%
63	8.395	2193	2194	2197	rBV	349	152	0.00%	0.001%
64	8.465	2209	2216	2228	rVB3	889	1806	0.04%	0.014%
65	8.549	2228	2242	2258	rBV	2569833	4223977	100.00%	31.910%
66	8.632	2258	2268	2297	rVB2	220213	435333	10.31%	3.289%
67	8.809	2321	2323	2326	rVB3	530	242	0.01%	0.002%
68	8.993	2375	2380	2382	rBV2	192	212	0.01%	0.002%
69	9.147	2422	2428	2432	rBV3	563	740	0.02%	0.006%
70	9.169	2433	2435	2439	rVB	250	143	0.00%	0.001%
71	9.282	2465	2470	2481	rVB4	1487	2430	0.06%	0.018%
72	9.324	2481	2483	2485	rBV	207	136	0.00%	0.001%
73	9.414	2497	2511	2534	rBV	469695	766470	18.15%	5.790%
74	9.604	2568	2570	2572	rBV	354	186	0.00%	0.001%
75	9.684	2592	2595	2598	rBV2	294	200	0.00%	0.002%
76	9.790	2627	2628	2631	rBV	277	174	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052841.D
 Acq On : 27 Jan 2023 13:03
 Operator : JC/MD
 Sample : 01295-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0LC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.838	2640	2643	2647	rBV2	307	307	0.01%	0.002%
78	10.063	2707	2713	2716	rBV2	292	331	0.01%	0.003%
79	10.301	2784	2787	2790	rBV	255	239	0.01%	0.002%
80	10.446	2829	2832	2835	rBV	234	185	0.00%	0.001%
81	10.517	2852	2854	2860	rBV	298	267	0.01%	0.002%
82	10.555	2864	2866	2869	rBV	298	210	0.00%	0.002%
83	10.751	2915	2927	2947	rVB	309774	495947	11.74%	3.747%
84	10.941	2983	2986	2990	rBV2	342	271	0.01%	0.002%
85	11.005	3003	3006	3009	rBV	182	122	0.00%	0.001%
86	11.195	3063	3065	3069	rBV2	171	160	0.00%	0.001%
87	11.269	3086	3088	3090	rBV	230	160	0.00%	0.001%
88	11.517	3160	3165	3166	rBV	883	693	0.02%	0.005%
89	11.806	3243	3255	3280	rBV	448786	710618	16.82%	5.368%
90	11.973	3305	3307	3308	rBV	303	119	0.00%	0.001%
91	12.057	3324	3333	3350	rBV2	12574	21916	0.52%	0.166%
92	12.189	3361	3374	3389	rBV	427769	689965	16.33%	5.212%
93	12.427	3445	3448	3449	rBV2	312	175	0.00%	0.001%
94	13.102	3655	3658	3663	rBV2	339	284	0.01%	0.002%
95	13.137	3665	3669	3670	rBV	253	170	0.00%	0.001%
96	13.298	3712	3719	3722	rBV2	348	437	0.01%	0.003%
97	13.562	3798	3801	3804	rBV	310	254	0.01%	0.002%
98	13.594	3808	3811	3813	rBV2	296	201	0.00%	0.002%
99	14.343	4042	4044	4048	rBV2	371	287	0.01%	0.002%
100	14.517	4095	4098	4100	rBV2	500	270	0.01%	0.002%




Sum of corrected areas: 13237198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052841.D
Acq On : 27 Jan 2023 13:03
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

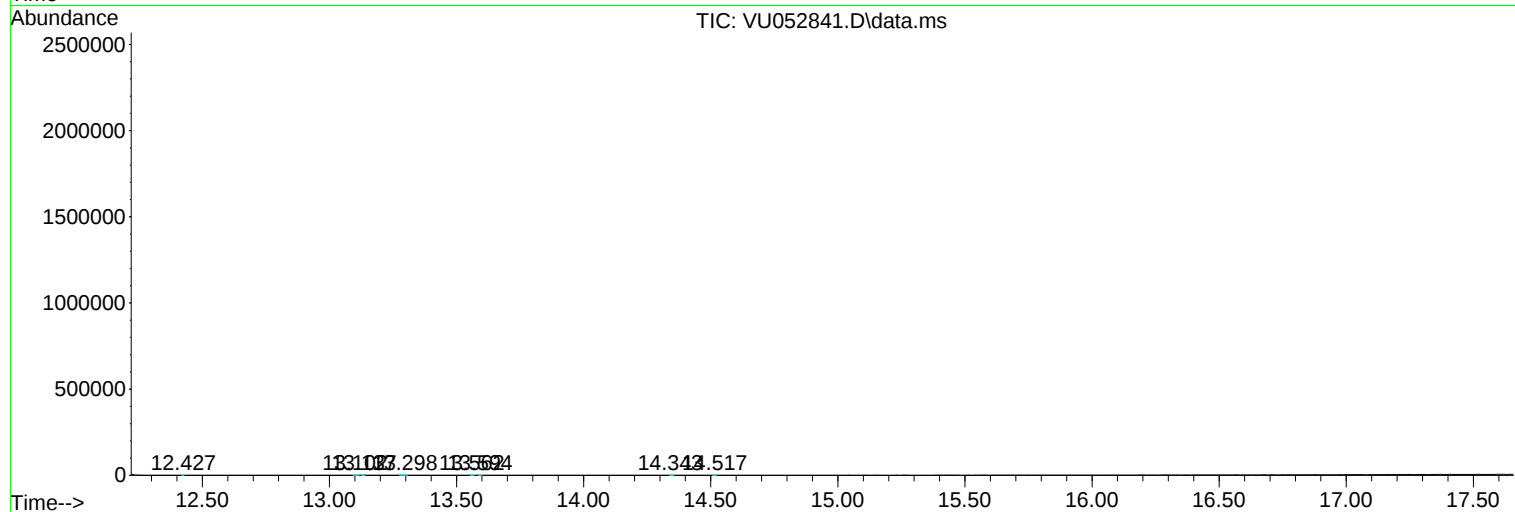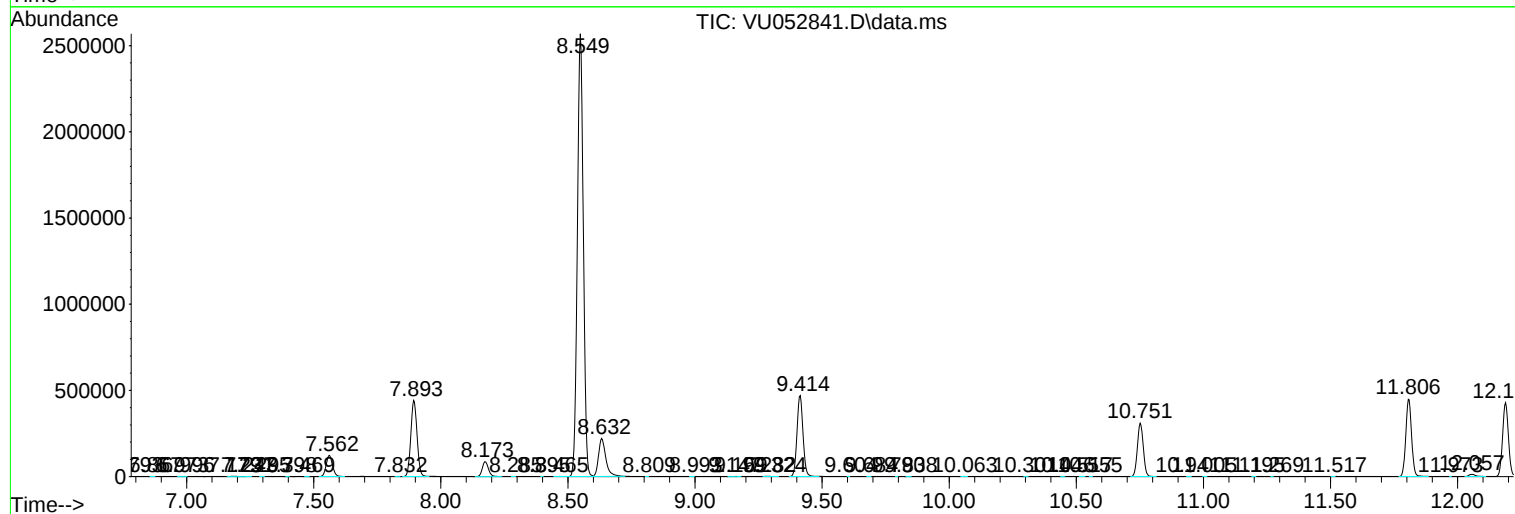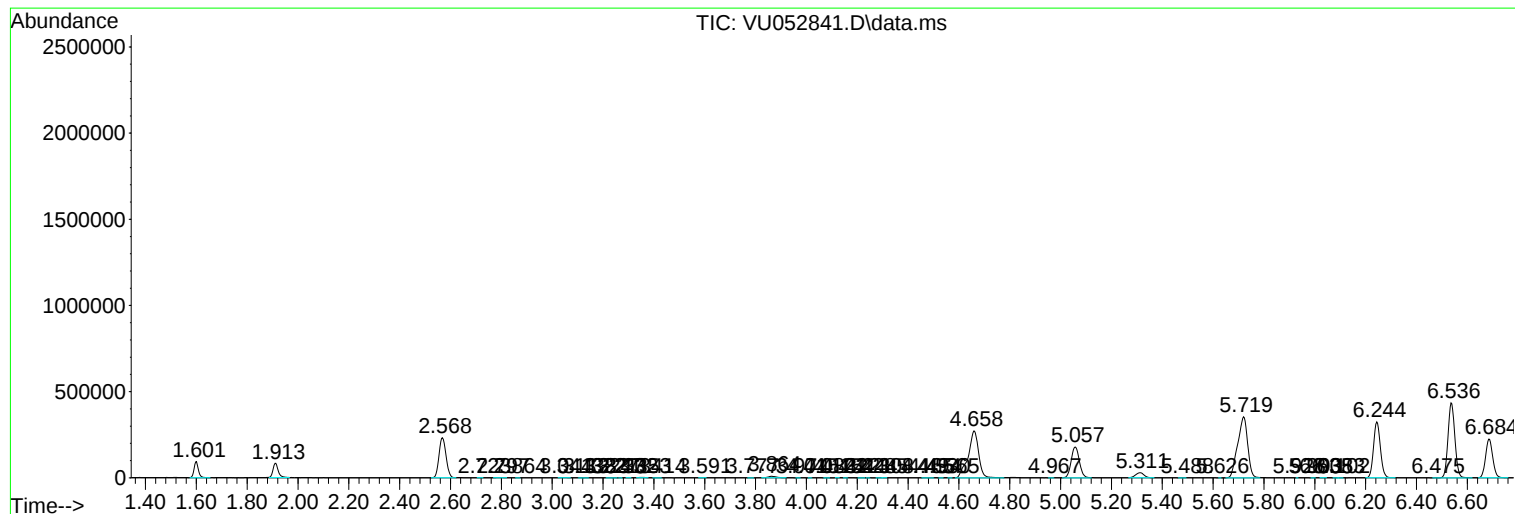

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052841.D
Acq On : 27 Jan 2023 13:03
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052841.D
Acq On : 27 Jan 2023 13:03
Operator : JC/MD
Sample : 01295-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0LC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc