

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052848.D
 Acq On : 27 Jan 2023 15:47
 Operator : JC/MD
 Sample : 01316-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	107167	129696	14.25%	1.821%
2	1.909	169	177	208	rVB	102923	151539	16.65%	2.127%
3	2.562	368	380	399	rBV	213251	348746	38.32%	4.895%
4	2.893	479	483	486	rBV2	295	230	0.03%	0.003%
5	2.980	506	510	512	rBV2	262	218	0.02%	0.003%
6	3.047	524	531	535	rBV4	768	943	0.10%	0.013%
7	3.121	549	554	555	rBV2	277	225	0.02%	0.003%
8	3.176	569	571	573	rBV2	295	204	0.02%	0.003%
9	3.228	581	587	590	rVB2	353	430	0.05%	0.006%
10	3.253	590	595	598	rBB2	330	285	0.03%	0.004%
11	3.282	599	604	605	rBV	341	297	0.03%	0.004%
12	3.321	613	616	618	rBV	249	190	0.02%	0.003%
13	3.514	668	676	679	rBV2	273	415	0.05%	0.006%
14	3.578	693	696	699	rVV	235	207	0.02%	0.003%
15	3.822	769	772	774	rBV	305	197	0.02%	0.003%
16	3.871	784	787	790	rVB	357	246	0.03%	0.003%
17	4.163	875	878	880	rBV2	276	218	0.02%	0.003%
18	4.195	886	888	894	rVV2	253	234	0.03%	0.003%
19	4.301	918	921	926	rVB	347	354	0.04%	0.005%
20	4.327	926	929	932	rBV	343	315	0.03%	0.004%
21	4.433	958	962	966	rBV2	387	436	0.05%	0.006%
22	4.456	966	969	973	rVV2	255	184	0.02%	0.003%
23	4.623	1009	1021	1045	rBV	63913	162151	17.82%	2.276%
24	4.916	1109	1112	1115	rBV2	278	227	0.02%	0.003%
25	5.002	1134	1139	1140	rBV	313	310	0.03%	0.004%
26	5.057	1140	1156	1179	rVV	175453	382262	42.00%	5.366%
27	5.215	1200	1205	1208	rBV	272	282	0.03%	0.004%
28	5.234	1208	1211	1216	rVB	216	218	0.02%	0.003%
29	5.282	1224	1226	1229	rBV2	627	478	0.05%	0.007%
30	5.324	1237	1239	1244	rVB2	332	262	0.03%	0.004%
31	5.366	1249	1252	1255	rBV	346	280	0.03%	0.004%
32	5.719	1342	1362	1384	rBV2	335019	910095	100.00%	12.775%
33	6.121	1484	1487	1490	rBV2	360	273	0.03%	0.004%
34	6.243	1511	1525	1544	rBV	323129	607154	66.71%	8.523%
35	6.504	1598	1606	1607	rBV	348	346	0.04%	0.005%
36	6.526	1608	1613	1617	rVV6	857	1085	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052848.D
 Acq On : 27 Jan 2023 15:47
 Operator : JC/MD
 Sample : 01316-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1690	rVB	239584	468154	51.44%	6.572%
38	6.899	1726	1729	1734	rVB3	398	459	0.05%	0.006%
39	6.925	1734	1737	1738	rBV2	321	210	0.02%	0.003%
40	7.028	1764	1769	1772	rBV	364	375	0.04%	0.005%
41	7.096	1786	1790	1796	rBV2	270	366	0.04%	0.005%
42	7.128	1797	1800	1804	rBV2	224	202	0.02%	0.003%
43	7.353	1866	1870	1873	rBV	261	228	0.03%	0.003%
44	7.378	1873	1878	1881	rVV	323	342	0.04%	0.005%
45	7.423	1889	1892	1895	rBV	425	347	0.04%	0.005%
46	7.494	1909	1914	1918	rVB2	196	238	0.03%	0.003%
47	7.562	1923	1935	1952	rBV	124648	220801	24.26%	3.099%
48	7.690	1970	1975	1976	rBV2	778	747	0.08%	0.010%
49	7.893	2025	2038	2060	rBV	467808	803329	88.27%	11.277%
50	8.176	2114	2126	2141	rBV	88927	147145	16.17%	2.066%
51	8.285	2157	2160	2162	rBV	366	232	0.03%	0.003%
52	8.314	2167	2169	2173	rVB2	400	240	0.03%	0.003%
53	8.385	2187	2191	2195	rBV2	404	357	0.04%	0.005%
54	8.404	2195	2197	2200	rVB2	364	195	0.02%	0.003%
55	8.427	2200	2204	2207	rBV	291	303	0.03%	0.004%
56	8.552	2235	2243	2250	rVB4	2948	4468	0.49%	0.063%
57	8.636	2256	2269	2311	rBV2	196686	384856	42.29%	5.402%
58	9.021	2387	2389	2394	rBV	168	200	0.02%	0.003%
59	9.169	2430	2435	2436	rBV	300	201	0.02%	0.003%
60	9.202	2442	2445	2448	rBV	270	238	0.03%	0.003%
61	9.276	2464	2468	2473	rVB2	293	339	0.04%	0.005%
62	9.311	2473	2479	2480	rBV	239	270	0.03%	0.004%
63	9.346	2486	2490	2493	rBV2	238	179	0.02%	0.003%
64	9.414	2498	2511	2531	rBV	407475	659293	72.44%	9.255%
65	9.739	2608	2612	2615	rBV2	193	219	0.02%	0.003%
66	9.787	2624	2627	2632	rVB2	272	263	0.03%	0.004%
67	9.857	2646	2649	2652	rVB	370	250	0.03%	0.004%
68	9.922	2666	2669	2674	rVB2	237	180	0.02%	0.003%
69	9.993	2687	2691	2695	rBV2	236	188	0.02%	0.003%
70	10.041	2702	2706	2712	rBV2	338	362	0.04%	0.005%
71	10.137	2731	2736	2742	rBV2	415	627	0.07%	0.009%
72	10.173	2743	2747	2750	rBV2	212	176	0.02%	0.002%
73	10.330	2792	2796	2799	rBV2	311	339	0.04%	0.005%
74	10.597	2874	2879	2880	rBV	338	298	0.03%	0.004%
75	10.751	2915	2927	2943	rBV2	296721	473086	51.98%	6.641%
76	10.893	2965	2971	2978	rVB3	1137	1406	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052848.D
 Acq On : 27 Jan 2023 15:47
 Operator : JC/MD
 Sample : 01316-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.198	3063	3066	3069	rBV2	260	206	0.02%	0.003%
78	11.240	3076	3079	3081	rBV	264	215	0.02%	0.003%
79	11.282	3089	3092	3096	rBV2	292	227	0.02%	0.003%
80	11.304	3096	3099	3104	rVV	352	283	0.03%	0.004%
81	11.398	3123	3128	3129	rBV	363	289	0.03%	0.004%
82	11.497	3156	3159	3162	rVV	279	175	0.02%	0.002%
83	11.629	3197	3200	3203	rBV2	302	266	0.03%	0.004%
84	11.806	3243	3255	3282	rBV	380285	603635	66.33%	8.473%
85	12.060	3328	3334	3344	rVB5	2878	4293	0.47%	0.060%
86	12.189	3362	3374	3396	rBV	396638	637522	70.05%	8.949%
87	12.761	3548	3552	3556	rBV4	684	709	0.08%	0.010%
88	12.870	3584	3586	3589	rBV2	324	185	0.02%	0.003%
89	12.960	3612	3614	3621	rVB	406	293	0.03%	0.004%
90	12.989	3621	3623	3627	rVB2	339	232	0.03%	0.003%
91	13.234	3697	3699	3702	rBV	401	278	0.03%	0.004%
92	13.346	3731	3734	3736	rBV2	285	215	0.02%	0.003%
93	13.565	3799	3802	3805	rBV	264	202	0.02%	0.003%
94	13.671	3833	3835	3839	rBV	310	198	0.02%	0.003%
95	13.738	3853	3856	3861	rVB	317	253	0.03%	0.004%
96	13.793	3870	3873	3875	rBV	391	220	0.02%	0.003%
97	13.989	3930	3934	3937	rBV2	286	248	0.03%	0.003%
98	14.227	4003	4008	4010	rBV2	246	243	0.03%	0.003%
99	14.336	4040	4042	4047	rBV2	348	264	0.03%	0.004%
100	15.555	4419	4421	4423	rBV2	487	248	0.03%	0.003%




Sum of corrected areas: 7123839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052848.D
Acq On : 27 Jan 2023 15:47
Operator : JC/MD
Sample : 01316-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

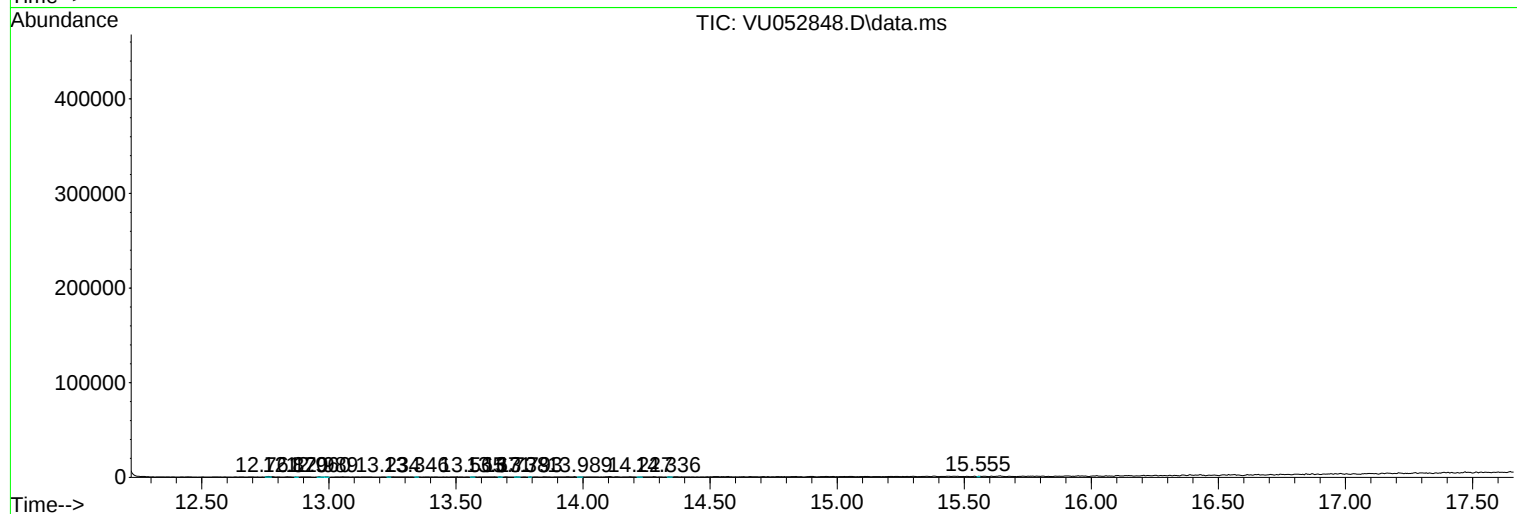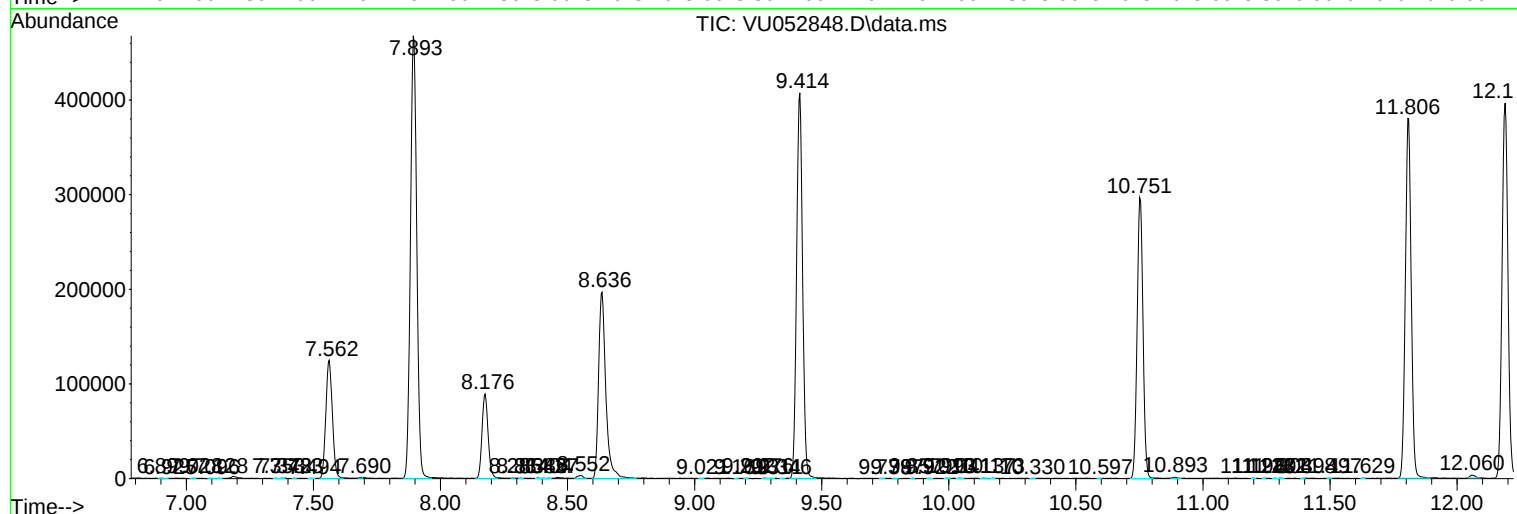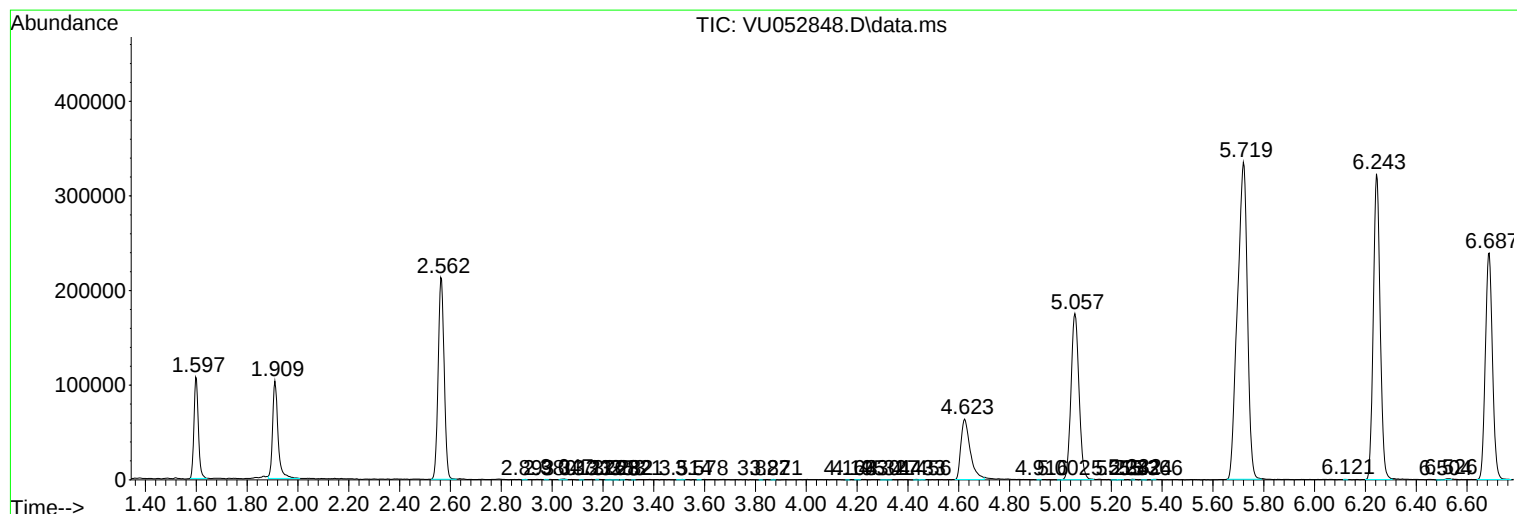

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052848.D
Acq On : 27 Jan 2023 15:47
Operator : JC/MD
Sample : 01316-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052848.D
Acq On : 27 Jan 2023 15:47
Operator : JC/MD
Sample : 01316-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------