

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052849.D
 Acq On : 27 Jan 2023 16:10
 Operator : JC/MD
 Sample : 01316-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052849.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	106841	127824	12.63%	1.810%
2	1.912	170	178	197	rVB	100578	140888	13.92%	1.994%
3	2.565	369	381	398	rBV	208170	338774	33.47%	4.796%
4	2.790	446	451	458	rBV3	520	758	0.07%	0.011%
5	2.841	464	467	471	rBV	243	213	0.02%	0.003%
6	2.899	481	485	489	rBV2	342	332	0.03%	0.005%
7	2.989	510	513	515	rBV	258	159	0.02%	0.002%
8	3.044	526	530	533	rBV2	373	324	0.03%	0.005%
9	3.205	577	580	583	rVB2	337	267	0.03%	0.004%
10	3.327	616	618	621	rBV	202	148	0.01%	0.002%
11	3.362	627	629	633	rVB2	322	225	0.02%	0.003%
12	3.417	643	646	650	rVV2	257	234	0.02%	0.003%
13	3.559	684	690	692	rBV	311	328	0.03%	0.005%
14	3.665	719	723	725	rBV	350	352	0.03%	0.005%
15	3.700	732	734	739	rBV	196	217	0.02%	0.003%
16	3.722	739	741	744	rVB	325	213	0.02%	0.003%
17	3.771	751	756	762	rBB2	352	412	0.04%	0.006%
18	3.803	762	766	767	rBV	246	158	0.02%	0.002%
19	4.002	825	828	831	rBV	223	183	0.02%	0.003%
20	4.092	853	856	859	rBV	336	311	0.03%	0.004%
21	4.134	865	869	874	rVB2	332	392	0.04%	0.006%
22	4.208	887	892	894	rBV	182	192	0.02%	0.003%
23	4.356	936	938	943	rBB	301	248	0.02%	0.004%
24	4.404	950	953	956	rBV	270	193	0.02%	0.003%
25	4.436	960	963	964	rBV	381	249	0.02%	0.004%
26	4.488	976	979	983	rBV2	205	191	0.02%	0.003%
27	4.623	1009	1021	1050	rBV	62411	162575	16.06%	2.301%
28	4.803	1073	1077	1081	rBV2	418	413	0.04%	0.006%
29	4.880	1094	1101	1103	rBV3	316	398	0.04%	0.006%
30	4.928	1113	1116	1119	rBV3	285	169	0.02%	0.002%
31	5.057	1140	1156	1176	rBV	188994	413042	40.81%	5.847%
32	5.285	1221	1227	1229	rBV3	434	488	0.05%	0.007%
33	5.719	1341	1362	1386	rBV2	371160	1012067	100.00%	14.327%
34	5.947	1430	1433	1436	rBV2	253	154	0.02%	0.002%
35	6.015	1451	1454	1455	rBV	314	158	0.02%	0.002%
36	6.243	1512	1525	1547	rBV	313801	582197	57.53%	8.242%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052849.D
 Acq On : 27 Jan 2023 16:10
 Operator : JC/MD
 Sample : 01316-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.449	1587	1589	1592	rVB2	292	180	0.02%	0.003%
38	6.468	1592	1595	1598	rBB	337	278	0.03%	0.004%
39	6.526	1608	1613	1617	rBV3	1091	1124	0.11%	0.016%
40	6.623	1640	1643	1645	rBV	351	226	0.02%	0.003%
41	6.684	1648	1662	1682	rBV	204424	390566	38.59%	5.529%
42	6.780	1688	1692	1695	rBV2	329	289	0.03%	0.004%
43	6.832	1705	1708	1713	rVB2	281	276	0.03%	0.004%
44	6.861	1714	1717	1720	rBV	182	183	0.02%	0.003%
45	6.938	1738	1741	1745	rBB	229	191	0.02%	0.003%
46	6.964	1746	1749	1752	rBV	308	252	0.02%	0.004%
47	7.041	1770	1773	1775	rBV	234	194	0.02%	0.003%
48	7.147	1804	1806	1809	rBV2	260	163	0.02%	0.002%
49	7.189	1812	1819	1829	rVB3	1281	2200	0.22%	0.031%
50	7.382	1875	1879	1882	rBV2	407	396	0.04%	0.006%
51	7.491	1910	1913	1916	rBV	185	174	0.02%	0.002%
52	7.562	1920	1935	1957	rBV2	104539	187231	18.50%	2.650%
53	7.652	1960	1963	1965	rBV	271	153	0.02%	0.002%
54	7.738	1987	1990	1994	rBV	224	209	0.02%	0.003%
55	7.800	2005	2009	2011	rBV	275	226	0.02%	0.003%
56	7.893	2025	2038	2063	rBV	394304	683616	67.55%	9.677%
57	8.076	2092	2095	2100	rBV3	466	363	0.04%	0.005%
58	8.176	2114	2126	2142	rBV	76060	126360	12.49%	1.789%
59	8.336	2174	2176	2179	rVB	267	167	0.02%	0.002%
60	8.356	2179	2182	2188	rVB2	183	204	0.02%	0.003%
61	8.401	2193	2196	2200	rVB2	469	330	0.03%	0.005%
62	8.433	2203	2206	2208	rBV	324	278	0.03%	0.004%
63	8.517	2229	2232	2236	rBV2	323	314	0.03%	0.004%
64	8.552	2236	2243	2250	rVB4	2667	3904	0.39%	0.055%
65	8.632	2256	2268	2301	rBV2	192016	373456	36.90%	5.287%
66	8.934	2358	2362	2365	rBV2	293	259	0.03%	0.004%
67	8.954	2365	2368	2371	rVB	434	316	0.03%	0.004%
68	8.973	2371	2374	2377	rBV2	299	323	0.03%	0.005%
69	9.044	2391	2396	2402	rVB3	372	290	0.03%	0.004%
70	9.070	2402	2404	2407	rBV	171	150	0.01%	0.002%
71	9.198	2440	2444	2446	rBV2	294	226	0.02%	0.003%
72	9.414	2498	2511	2537	rBV	401711	652722	64.49%	9.240%
73	9.545	2549	2552	2553	rBV2	405	270	0.03%	0.004%
74	9.590	2563	2566	2571	rBV	435	545	0.05%	0.008%
75	9.732	2608	2610	2616	rVB2	213	193	0.02%	0.003%
76	9.758	2616	2618	2622	rBV2	159	153	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052849.D
 Acq On : 27 Jan 2023 16:10
 Operator : JC/MD
 Sample : 01316-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44J2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	9.841	2638	2644	2648	rBV2	294	336	0.03%	0.005%
78	10.214	2757	2760	2763	rBV2	243	220	0.02%	0.003%
79	10.275	2775	2779	2782	rBV	314	330	0.03%	0.005%
80	10.417	2816	2823	2826	rBV	363	490	0.05%	0.007%
81	10.465	2835	2838	2840	rBV	236	170	0.02%	0.002%
82	10.513	2850	2853	2856	rBV	296	223	0.02%	0.003%
83	10.606	2879	2882	2885	rBV2	351	269	0.03%	0.004%
84	10.664	2895	2900	2901	rBV2	219	193	0.02%	0.003%
85	10.751	2915	2927	2942	rBV	312697	500059	49.41%	7.079%
86	11.806	3243	3255	3275	rBV	415061	653959	64.62%	9.258%
87	12.057	3325	3333	3345	rBV2	11419	19149	1.89%	0.271%
88	12.188	3362	3374	3394	rBV	418919	670523	66.25%	9.492%
89	12.764	3548	3553	3555	rBV3	695	684	0.07%	0.010%
90	13.272	3708	3711	3715	rBV	287	294	0.03%	0.004%
91	13.513	3783	3786	3789	rBV	270	206	0.02%	0.003%
92	13.581	3806	3807	3810	rBV	250	174	0.02%	0.002%
93	13.693	3839	3842	3846	rBV	311	275	0.03%	0.004%
94	13.950	3919	3922	3924	rBV	373	183	0.02%	0.003%
95	14.143	3978	3982	3983	rBV	337	215	0.02%	0.003%
96	14.314	4032	4035	4037	rBV2	279	172	0.02%	0.002%
97	14.693	4151	4153	4157	rVB2	478	276	0.03%	0.004%
98	14.809	4185	4189	4194	rBV3	678	754	0.07%	0.011%
99	14.915	4219	4222	4224	rBV2	373	298	0.03%	0.004%
100	15.050	4262	4264	4265	rBV	403	179	0.02%	0.003%




Sum of corrected areas: 7064027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052849.D
Acq On : 27 Jan 2023 16:10
Operator : JC/MD
Sample : 01316-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

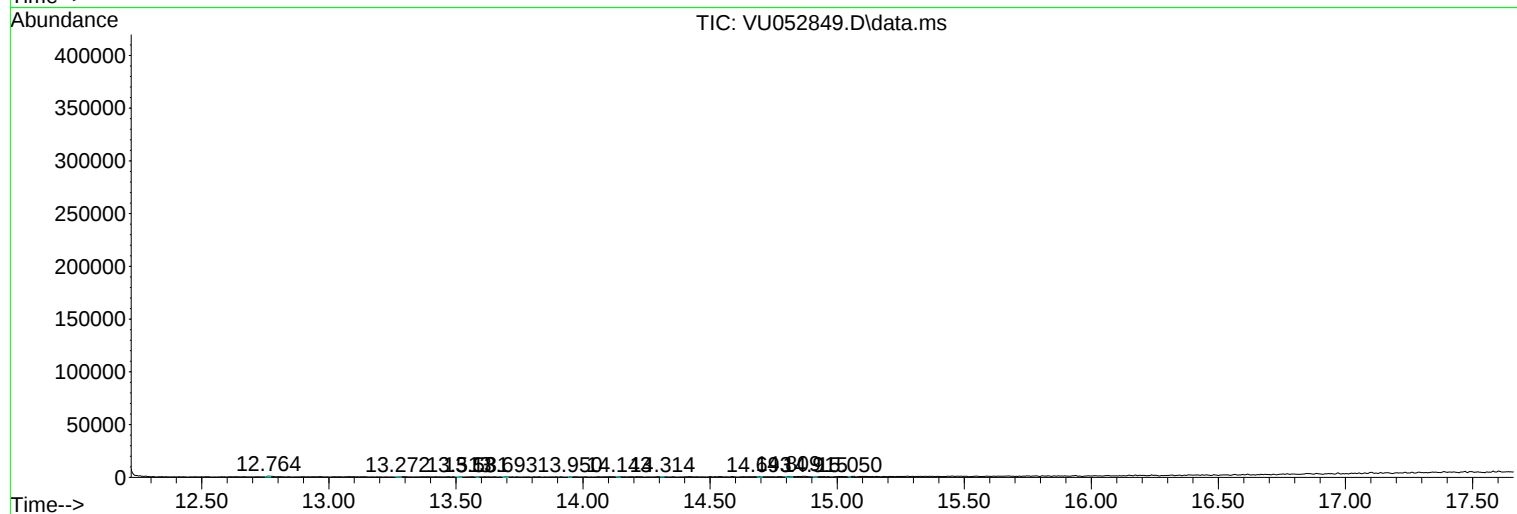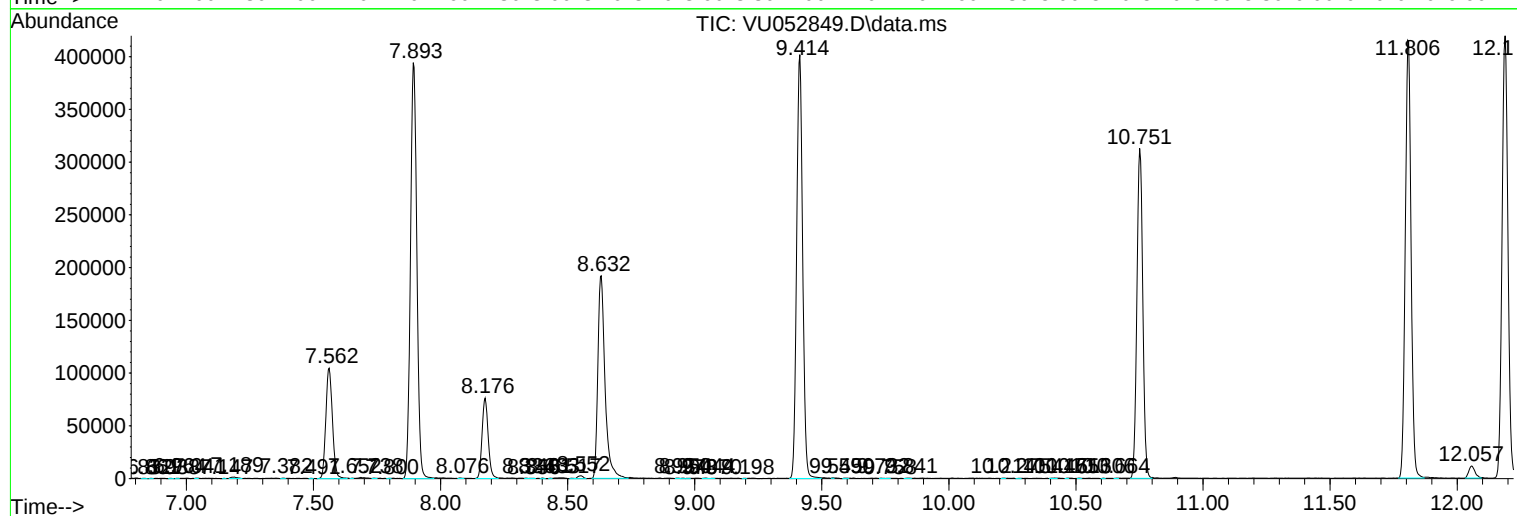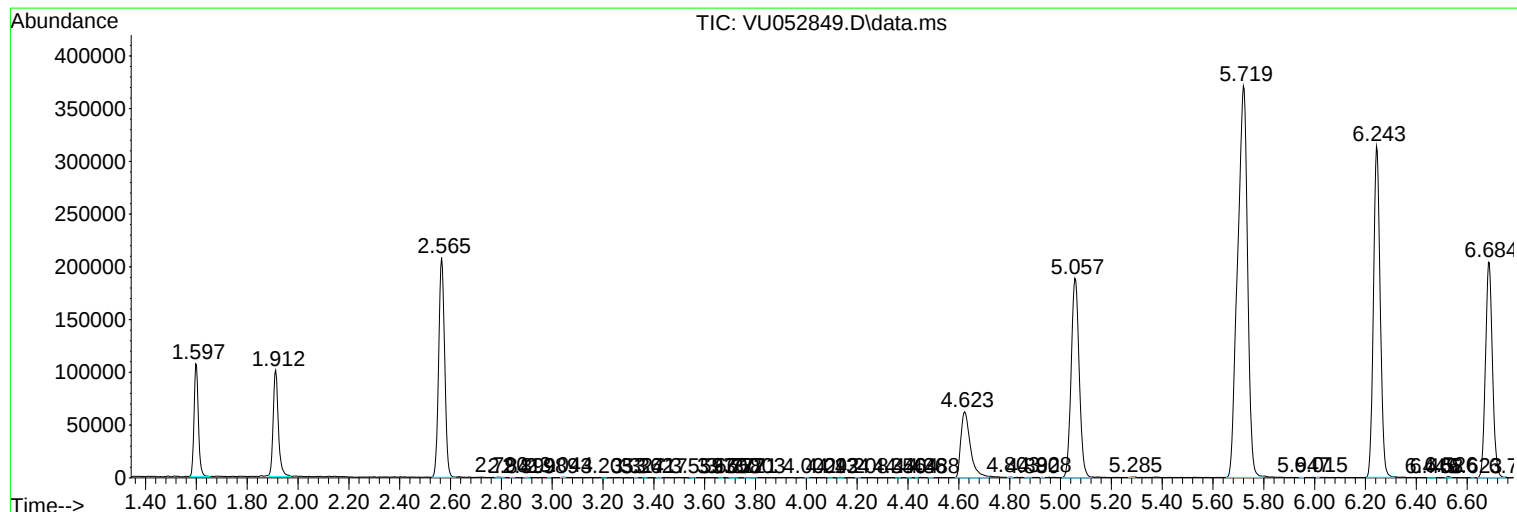

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052849.D
Acq On : 27 Jan 2023 16:10
Operator : JC/MD
Sample : 01316-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052849.D
Acq On : 27 Jan 2023 16:10
Operator : JC/MD
Sample : 01316-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc