

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052853.D
 Acq On : 27 Jan 2023 17:42
 Operator : JC/MD
 Sample : 01314-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	97	rVB2	127664	157332	0.34%	0.211%
2	1.909	170	177	194	rVB	99878	138297	0.30%	0.185%
3	2.565	369	381	398	rBV2	225732	376925	0.81%	0.505%
4	3.044	521	530	540	rBV2	4684	8693	0.02%	0.012%
5	3.099	545	547	550	rBV2	397	268	0.00%	0.000%
6	3.353	618	626	642	rVB2	12944	24079	0.05%	0.032%
7	3.632	709	713	715	rBV	240	198	0.00%	0.000%
8	3.658	719	721	725	rVV2	244	185	0.00%	0.000%
9	3.687	728	730	733	rBB	316	190	0.00%	0.000%
10	3.716	734	739	742	rBB2	276	267	0.00%	0.000%
11	3.742	745	747	750	rBB	334	220	0.00%	0.000%
12	3.870	775	787	795	rVV3	1900	4030	0.01%	0.005%
13	3.957	809	814	819	rBB2	308	344	0.00%	0.000%
14	3.986	819	823	825	rBV	250	195	0.00%	0.000%
15	4.054	840	844	846	rBV	275	259	0.00%	0.000%
16	4.102	854	859	861	rBV	238	201	0.00%	0.000%
17	4.160	872	877	881	rBV	206	219	0.00%	0.000%
18	4.234	896	900	904	rBV2	377	406	0.00%	0.001%
19	4.285	912	916	920	rBV	317	363	0.00%	0.000%
20	4.388	945	948	950	rBV	319	230	0.00%	0.000%
21	4.417	954	957	959	rBV2	314	206	0.00%	0.000%
22	4.462	969	971	974	rBB	297	180	0.00%	0.000%
23	4.661	1004	1033	1061	rBV2	854566	2059685	4.40%	2.760%
24	4.960	1122	1126	1130	rVB2	375	263	0.00%	0.000%
25	4.993	1133	1136	1138	rBV2	223	190	0.00%	0.000%
26	5.057	1141	1156	1177	rBV	172913	382332	0.82%	0.512%
27	5.285	1221	1227	1228	rBV3	996	637	0.00%	0.001%
28	5.369	1249	1253	1257	rBV	524	609	0.00%	0.001%
29	5.494	1288	1292	1296	rBV2	311	290	0.00%	0.000%
30	5.610	1322	1328	1332	rBV2	354	456	0.00%	0.001%
31	5.719	1340	1362	1396	rBV3	334559	944082	2.02%	1.265%
32	5.960	1433	1437	1443	rBV	353	531	0.00%	0.001%
33	6.121	1484	1487	1490	rBV2	371	224	0.00%	0.000%
34	6.243	1511	1525	1545	rBV	293722	557197	1.19%	0.747%
35	6.388	1566	1570	1573	rBV2	403	321	0.00%	0.000%
36	6.404	1573	1575	1578	rBV2	307	207	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052853.D
 Acq On : 27 Jan 2023 17:42
 Operator : JC/MD
 Sample : 01314-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.539	1599	1617	1649	rBV	7306628	13451447	28.76%	18.023%
38	6.687	1652	1663	1686	rVB	210911	410035	0.88%	0.549%
39	7.144	1802	1805	1809	rBV2	257	204	0.00%	0.000%
40	7.185	1809	1818	1825	rBV5	1427	2490	0.01%	0.003%
41	7.311	1851	1857	1858	rBV	316	237	0.00%	0.000%
42	7.353	1864	1870	1872	rBV	282	347	0.00%	0.000%
43	7.401	1881	1885	1888	rBB2	328	290	0.00%	0.000%
44	7.427	1889	1893	1897	rBB2	328	281	0.00%	0.000%
45	7.449	1897	1900	1901	rBV	304	188	0.00%	0.000%
46	7.484	1907	1911	1914	rBV2	316	263	0.00%	0.000%
47	7.562	1923	1935	1955	rVV	128838	220476	0.47%	0.295%
48	7.681	1968	1972	1975	rBV3	793	769	0.00%	0.001%
49	7.893	2024	2038	2054	rBV	479475	820526	1.75%	1.099%
50	8.041	2081	2084	2086	rBV	287	189	0.00%	0.000%
51	8.108	2101	2105	2106	rBV3	315	216	0.00%	0.000%
52	8.176	2115	2126	2143	rBV	91959	151928	0.32%	0.204%
53	8.269	2151	2155	2157	rBV3	602	418	0.00%	0.001%
54	8.455	2208	2213	2214	rBV2	699	538	0.00%	0.001%
55	8.552	2236	2243	2253	rVB7	1727	2974	0.01%	0.004%
56	8.632	2256	2268	2300	rBV2	233416	443640	0.95%	0.594%
57	8.989	2376	2379	2383	rBV2	323	272	0.00%	0.000%
58	9.356	2487	2493	2497	rBV2	230	305	0.00%	0.000%
59	9.414	2497	2511	2515	rBV	439529	708415	1.51%	0.949%
60	9.594	2562	2567	2577	rVB3	5906	7893	0.02%	0.011%
61	9.687	2593	2596	2603	rVB2	997	1013	0.00%	0.001%
62	9.880	2653	2656	2659	rBV2	232	224	0.00%	0.000%
63	9.938	2670	2674	2676	rBV2	283	243	0.00%	0.000%
64	10.060	2708	2712	2715	rBV	238	230	0.00%	0.000%
65	10.095	2719	2723	2724	rBV	339	238	0.00%	0.000%
66	10.134	2732	2735	2738	rBV2	225	188	0.00%	0.000%
67	10.192	2746	2753	2761	rBV2	298	497	0.00%	0.001%
68	10.352	2799	2803	2808	rBV	238	283	0.00%	0.000%
69	10.414	2819	2822	2826	rBV2	282	256	0.00%	0.000%
70	10.484	2839	2844	2848	rBV2	217	232	0.00%	0.000%
71	10.696	2901	2910	2912	rBV	349	515	0.00%	0.001%
72	10.751	2915	2927	2941	rVV	294367	464075	0.99%	0.622%
73	10.825	2947	2950	2952	rBV2	340	186	0.00%	0.000%
74	10.886	2964	2969	2970	rBV3	892	616	0.00%	0.001%
75	11.008	3002	3007	3010	rVV2	273	281	0.00%	0.000%
76	11.098	3030	3035	3041	rVB4	500	581	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052853.D
 Acq On : 27 Jan 2023 17:42
 Operator : JC/MD
 Sample : 01314-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	11.365	3115	3118	3122	rBV2	207	218	0.00%	0.000%
78	11.462	3144	3148	3151	rBV2	496	448	0.00%	0.001%
79	11.687	3212	3218	3222	rBV2	372	456	0.00%	0.001%
80	11.741	3222	3235	3245	rBV	238377	373889	0.80%	0.501%
81	11.831	3245	3263	3290	rVB2	3285724	5737071	12.27%	7.687%
82	12.057	3325	3333	3345	rBV4	4624	8097	0.02%	0.011%
83	12.214	3361	3382	3417	rBV	28366987	46763571	100.00%	62.658%
84	12.616	3504	3507	3510	rBV2	568	475	0.00%	0.001%
85	12.806	3562	3566	3570	rVB2	515	456	0.00%	0.001%
86	12.889	3588	3592	3594	rBV3	1054	902	0.00%	0.001%
87	12.963	3608	3615	3625	rVB2	6977	9868	0.02%	0.013%
88	13.143	3662	3671	3681	rBV6	3896	7693	0.02%	0.010%
89	13.204	3681	3690	3701	rVV	13407	22190	0.05%	0.030%
90	13.278	3711	3713	3716	rBV3	274	187	0.00%	0.000%
91	13.323	3719	3727	3737	rVB5	3631	5535	0.01%	0.007%
92	13.494	3778	3780	3782	rBV5	303	188	0.00%	0.000%
93	13.748	3856	3859	3862	rBV	382	280	0.00%	0.000%
94	13.835	3874	3886	3904	rBV	171786	269251	0.58%	0.361%
95	14.327	4023	4039	4049	rBV3	34987	56270	0.12%	0.075%
96	14.426	4066	4070	4072	rBV	339	254	0.00%	0.000%
97	14.465	4078	4082	4084	rBV2	264	255	0.00%	0.000%
98	14.548	4105	4108	4110	rBV2	424	287	0.00%	0.000%
99	14.741	4166	4168	4171	rBV2	402	229	0.00%	0.000%
100	16.089	4580	4587	4596	rVB2	14883	21197	0.05%	0.028%




Sum of corrected areas: 74633577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052853.D
Acq On : 27 Jan 2023 17:42
Operator : JC/MD
Sample : 01314-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

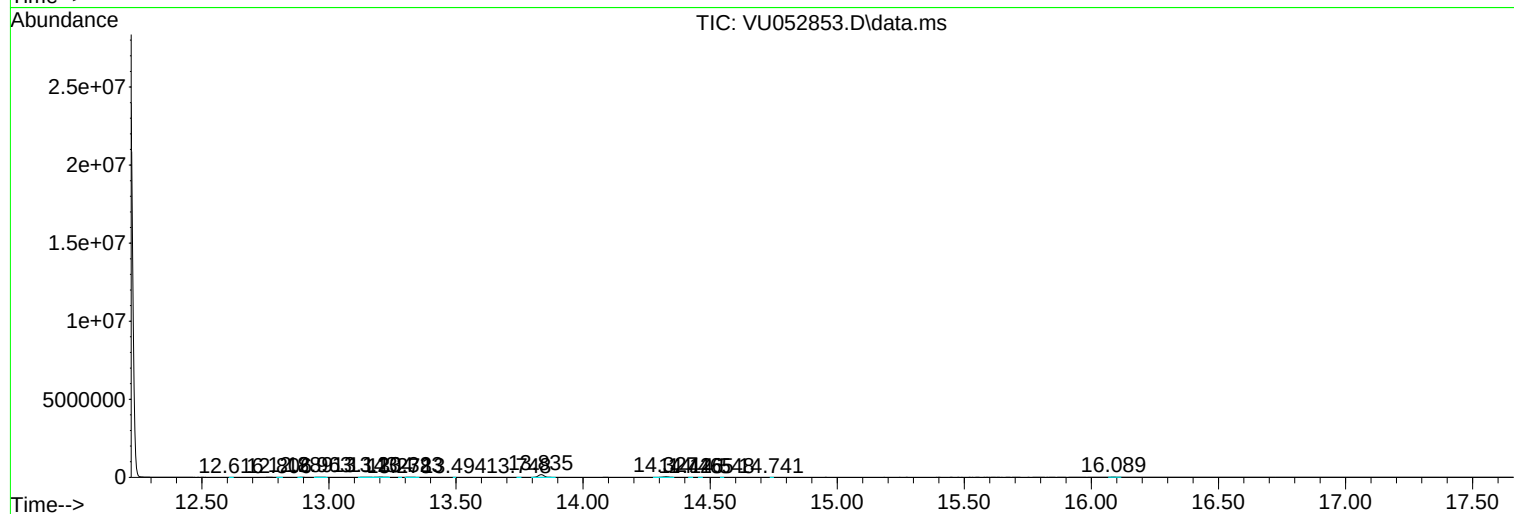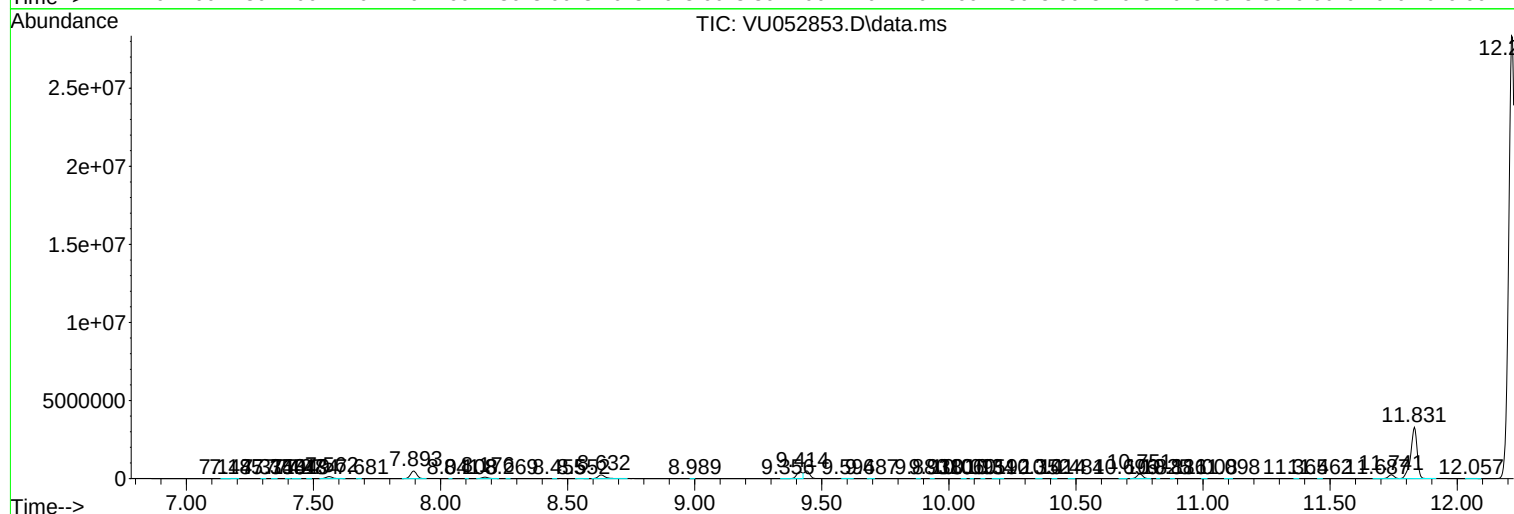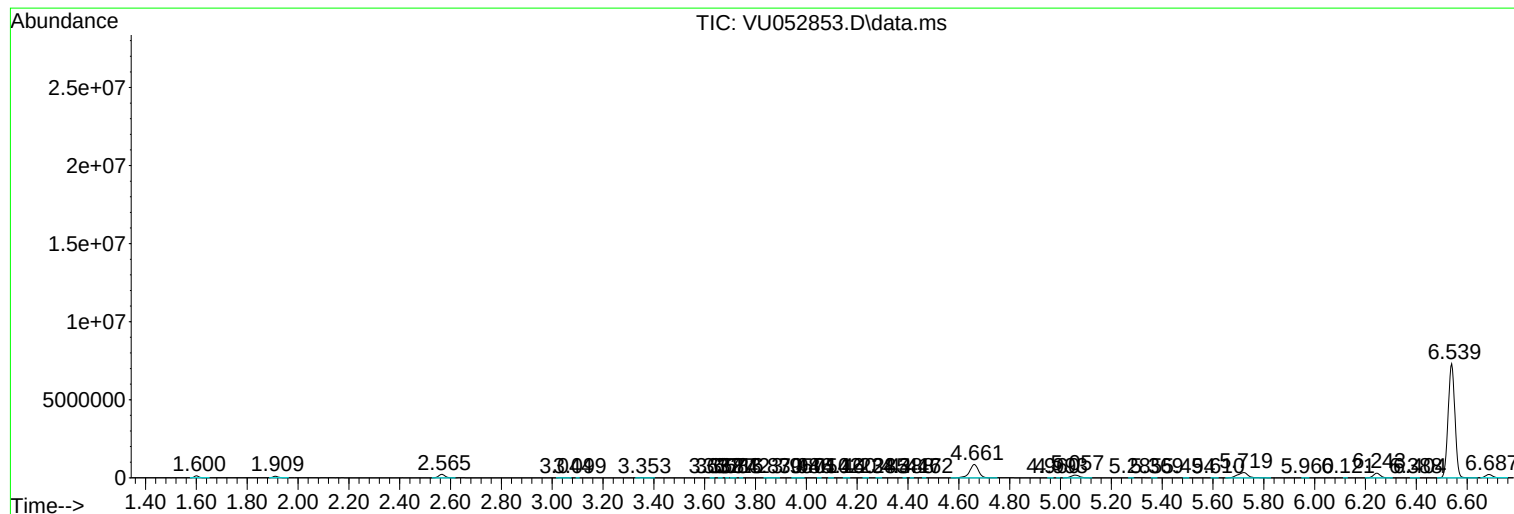

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052853.D
Acq On : 27 Jan 2023 17:42
Operator : JC/MD
Sample : 01314-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052853.D
Acq On : 27 Jan 2023 17:42
Operator : JC/MD
Sample : 01314-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc