

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052857.D
 Acq On : 27 Jan 2023 19:16
 Operator : JC/MD
 Sample : 01316-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

Signal : TIC: VU052857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	94686	115704	13.32%	1.693%
2	1.906	169	176	194	rVB	108339	148094	17.05%	2.166%
3	2.520	364	367	368	rBV	299	160	0.02%	0.002%
4	2.565	368	381	399	rVV	212085	349590	40.24%	5.114%
5	3.044	522	530	540	rBV4	2111	3545	0.41%	0.052%
6	3.578	693	696	698	rBV2	290	230	0.03%	0.003%
7	3.694	728	732	734	rBV	323	270	0.03%	0.004%
8	3.748	743	749	752	rBV	248	270	0.03%	0.004%
9	3.877	785	789	792	rBV	336	276	0.03%	0.004%
10	4.022	829	834	837	rBV	366	374	0.04%	0.005%
11	4.041	837	840	843	rBV	284	217	0.02%	0.003%
12	4.150	871	874	876	rBV	221	158	0.02%	0.002%
13	4.343	931	934	936	rBV2	198	154	0.02%	0.002%
14	4.620	1008	1020	1046	rBV	75220	191763	22.08%	2.805%
15	5.057	1137	1156	1177	rBV2	166816	365014	42.02%	5.340%
16	5.205	1198	1202	1204	rVB	341	188	0.02%	0.003%
17	5.279	1222	1225	1227	rBV	304	218	0.03%	0.003%
18	5.362	1246	1251	1252	rBV2	350	343	0.04%	0.005%
19	5.424	1264	1270	1274	rVB2	215	246	0.03%	0.004%
20	5.469	1281	1284	1286	rBV	350	272	0.03%	0.004%
21	5.526	1299	1302	1306	rVV	187	211	0.02%	0.003%
22	5.629	1330	1334	1337	rVB2	311	267	0.03%	0.004%
23	5.719	1341	1362	1384	rBV2	319676	868685	100.00%	12.707%
24	5.922	1420	1425	1431	rBV2	353	516	0.06%	0.008%
25	6.012	1450	1453	1456	rVB2	332	246	0.03%	0.004%
26	6.038	1459	1461	1464	rBV	334	242	0.03%	0.004%
27	6.160	1496	1499	1502	rBV2	302	251	0.03%	0.004%
28	6.243	1512	1525	1547	rBV	282581	530286	61.04%	7.757%
29	6.337	1552	1554	1558	rVB2	423	226	0.03%	0.003%
30	6.436	1580	1585	1590	rVB2	235	267	0.03%	0.004%
31	6.475	1595	1597	1600	rBV2	257	184	0.02%	0.003%
32	6.510	1603	1608	1609	rBV2	255	185	0.02%	0.003%
33	6.536	1609	1616	1625	rVV8	2148	4365	0.50%	0.064%
34	6.629	1643	1645	1648	rBV	301	250	0.03%	0.004%
35	6.687	1648	1663	1686	rVB	200820	389109	44.79%	5.692%
36	6.780	1687	1692	1694	rBV	271	266	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052857.D
 Acq On : 27 Jan 2023 19:16
 Operator : JC/MD
 Sample : 01316-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.803	1696	1699	1706	rVV3	584	526	0.06%	0.008%
38	6.973	1748	1752	1754	rBV2	276	224	0.03%	0.003%
39	6.989	1755	1757	1762	rVB2	337	254	0.03%	0.004%
40	7.028	1765	1769	1772	rBV2	282	326	0.04%	0.005%
41	7.102	1789	1792	1795	rBV2	310	246	0.03%	0.004%
42	7.186	1811	1818	1829	rVB3	1925	2758	0.32%	0.040%
43	7.243	1833	1836	1839	rBV	283	225	0.03%	0.003%
44	7.272	1841	1845	1848	rVB2	255	218	0.03%	0.003%
45	7.317	1856	1859	1861	rBV2	306	232	0.03%	0.003%
46	7.504	1914	1917	1921	rBV2	297	288	0.03%	0.004%
47	7.562	1923	1935	1953	rVV	104812	183375	21.11%	2.682%
48	7.687	1970	1974	1979	rBV3	950	1076	0.12%	0.016%
49	7.710	1979	1981	1986	rVB2	463	363	0.04%	0.005%
50	7.777	1996	2002	2007	rVB2	262	295	0.03%	0.004%
51	7.893	2022	2038	2059	rBV	402454	683333	78.66%	9.996%
52	8.047	2080	2086	2090	rBV2	406	483	0.06%	0.007%
53	8.102	2100	2103	2107	rBV2	323	300	0.03%	0.004%
54	8.176	2113	2126	2147	rBV	74339	126712	14.59%	1.854%
55	8.292	2156	2162	2165	rBV2	493	617	0.07%	0.009%
56	8.346	2175	2179	2181	rBV2	328	258	0.03%	0.004%
57	8.517	2229	2232	2235	rBV2	433	396	0.05%	0.006%
58	8.546	2239	2241	2247	rVB2	512	383	0.04%	0.006%
59	8.632	2256	2268	2304	rBV2	189387	373423	42.99%	5.463%
60	8.848	2330	2335	2336	rBV	225	161	0.02%	0.002%
61	9.086	2405	2409	2412	rBV2	323	283	0.03%	0.004%
62	9.144	2424	2427	2430	rBV2	263	185	0.02%	0.003%
63	9.173	2433	2436	2438	rBV	239	177	0.02%	0.003%
64	9.250	2457	2460	2462	rBV2	278	219	0.03%	0.003%
65	9.292	2470	2473	2476	rVB2	341	281	0.03%	0.004%
66	9.311	2476	2479	2482	rBV	299	252	0.03%	0.004%
67	9.414	2497	2511	2531	rBV	392037	642461	73.96%	9.398%
68	9.610	2568	2572	2577	rVB	313	324	0.04%	0.005%
69	9.690	2593	2597	2601	rBV2	350	448	0.05%	0.007%
70	9.735	2608	2611	2613	rBV2	316	215	0.02%	0.003%
71	10.079	2716	2718	2721	rVB	277	178	0.02%	0.003%
72	10.259	2771	2774	2777	rBV2	353	301	0.03%	0.004%
73	10.314	2787	2791	2796	rVB2	331	405	0.05%	0.006%
74	10.343	2797	2800	2803	rBV2	343	323	0.04%	0.005%
75	10.616	2877	2885	2887	rBV	341	398	0.05%	0.006%
76	10.668	2897	2901	2904	rVB	219	209	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052857.D
 Acq On : 27 Jan 2023 19:16
 Operator : JC/MD
 Sample : 01316-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44H1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2944	rVB	310274	494035	56.87%	7.227%
78	10.870	2959	2964	2967	rBV2	247	307	0.04%	0.004%
79	10.980	2995	2998	3000	rBV2	245	156	0.02%	0.002%
80	11.044	3012	3018	3020	rBV	299	306	0.04%	0.004%
81	11.060	3020	3023	3025	rBV	221	178	0.02%	0.003%
82	11.243	3073	3080	3082	rBV	238	312	0.04%	0.005%
83	11.375	3116	3121	3124	rBV2	227	185	0.02%	0.003%
84	11.459	3143	3147	3150	rBV2	207	168	0.02%	0.002%
85	11.478	3150	3153	3156	rBV	266	171	0.02%	0.003%
86	11.745	3233	3236	3239	rBV	389	274	0.03%	0.004%
87	11.806	3243	3255	3277	rBV	398895	634590	73.05%	9.283%
88	12.189	3361	3374	3393	rBV	428244	705424	81.21%	10.319%
89	12.324	3412	3416	3420	rBV5	604	536	0.06%	0.008%
90	12.918	3599	3601	3604	rBV2	228	182	0.02%	0.003%
91	13.102	3653	3658	3661	rBV2	269	321	0.04%	0.005%
92	13.320	3723	3726	3729	rBV	301	223	0.03%	0.003%
93	13.590	3806	3810	3814	rVB2	350	311	0.04%	0.005%
94	13.783	3867	3870	3874	rBV	261	255	0.03%	0.004%
95	13.857	3889	3893	3897	rBV3	375	432	0.05%	0.006%
96	13.912	3907	3910	3912	rBV2	357	258	0.03%	0.004%
97	14.047	3949	3952	3957	rBV3	330	294	0.03%	0.004%
98	14.533	4100	4103	4107	rBV	418	418	0.05%	0.006%
99	14.578	4113	4117	4121	rVB3	349	306	0.04%	0.004%
100	14.735	4162	4166	4170	rBV3	556	605	0.07%	0.009%




Sum of corrected areas: 6836020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052857.D
Acq On : 27 Jan 2023 19:16
Operator : JC/MD
Sample : 01316-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

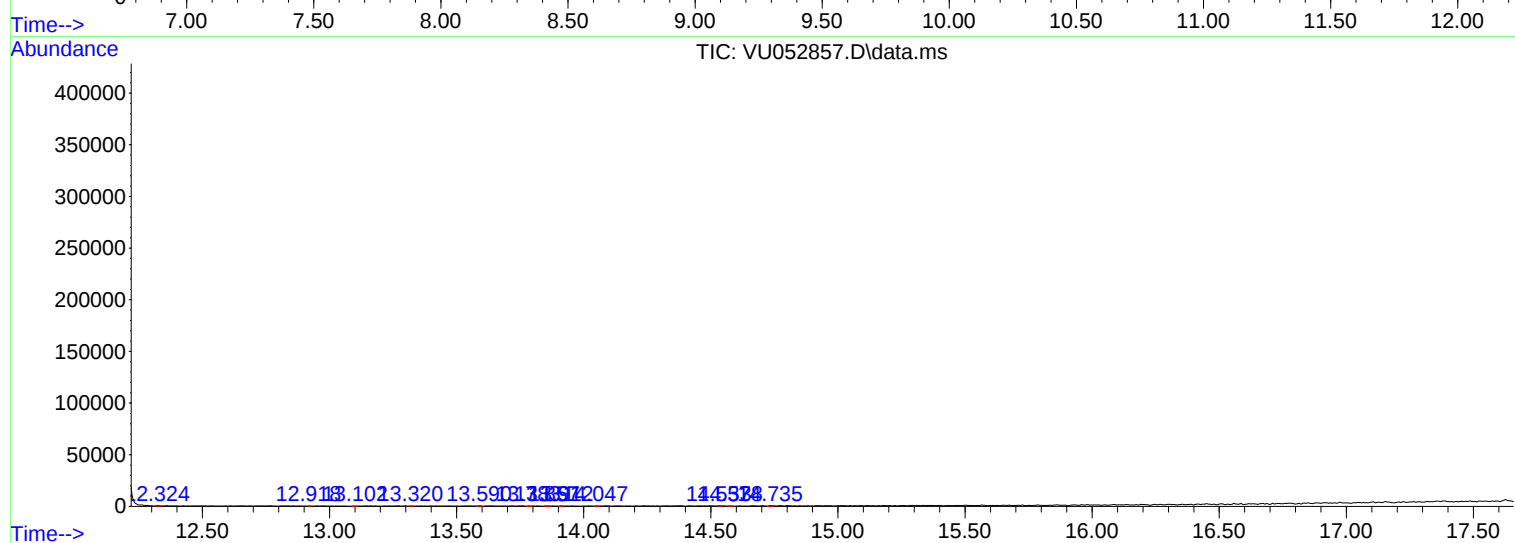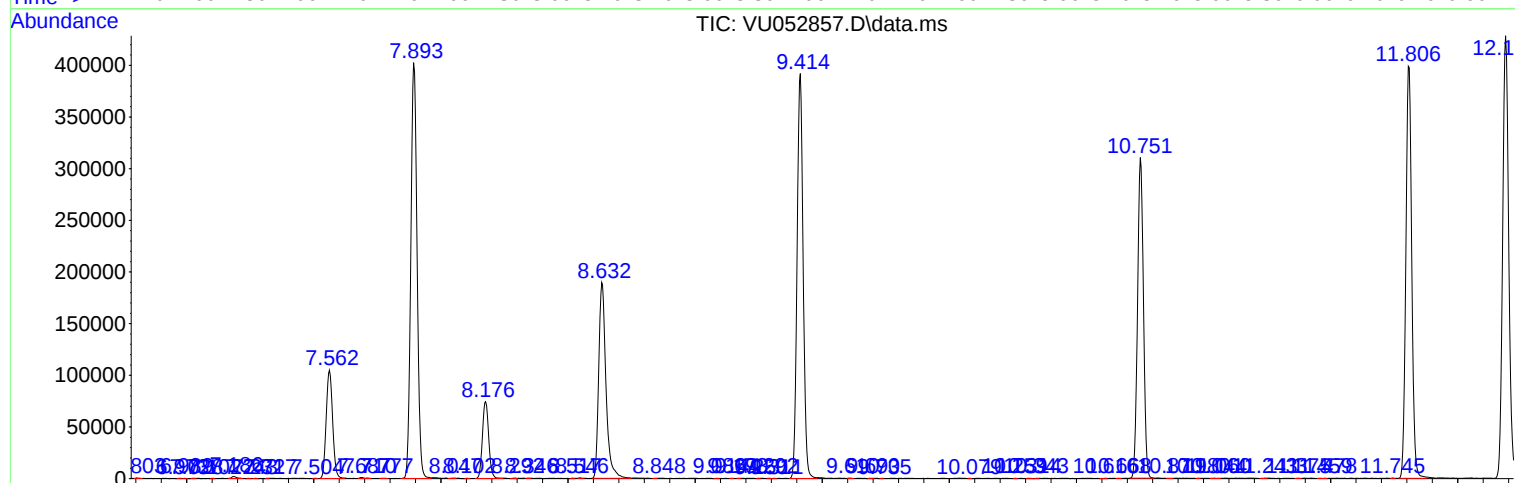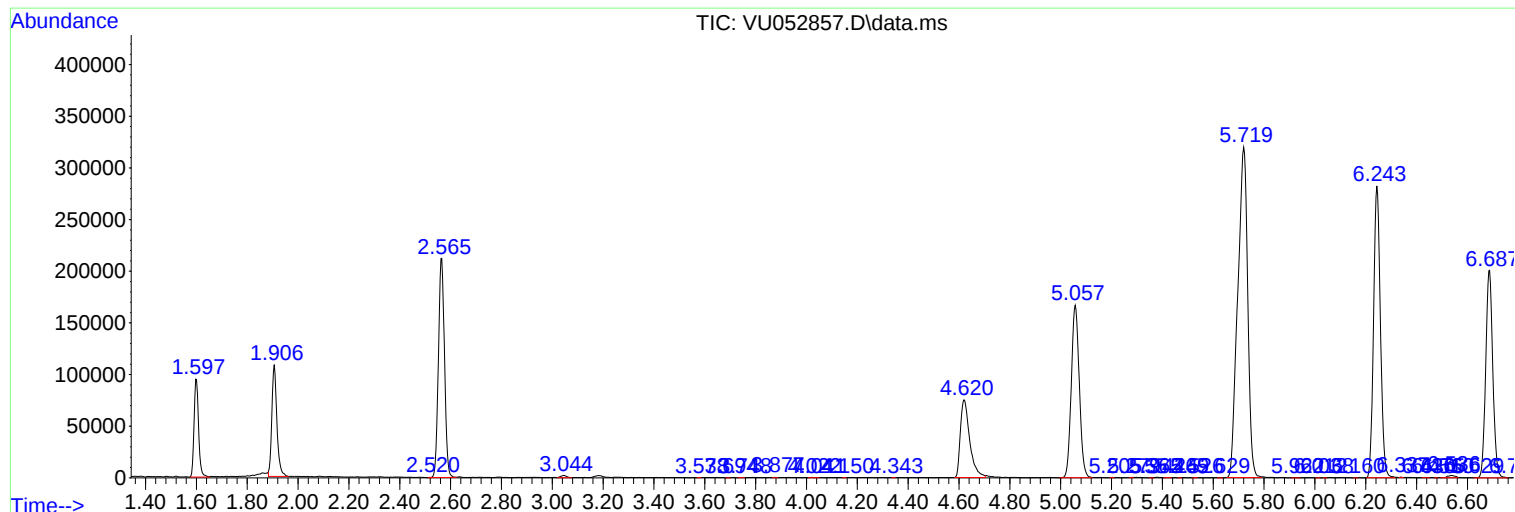

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052857.D
Acq On : 27 Jan 2023 19:16
Operator : JC/MD
Sample : 01316-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052857.D
Acq On : 27 Jan 2023 19:16
Operator : JC/MD
Sample : 01316-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------