

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052858.D
 Acq On : 27 Jan 2023 19:39
 Operator : JC/MD
 Sample : 01314-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M

Title : VOC Analysis

Signal : TIC: VU052858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	99	rBV	90524	108866	12.73%	1.673%
2	1.906	169	176	196	rVB	100753	139374	16.30%	2.142%
3	2.565	369	381	398	rVB	210414	341937	39.98%	5.255%
4	2.720	425	429	433	rBV	706	609	0.07%	0.009%
5	3.044	522	530	538	rBV3	1726	2901	0.34%	0.045%
6	3.453	650	657	660	rBV2	413	601	0.07%	0.009%
7	3.498	668	671	675	rBV2	317	323	0.04%	0.005%
8	3.591	697	700	703	rBV2	202	204	0.02%	0.003%
9	3.617	705	708	711	rBV3	369	262	0.03%	0.004%
10	4.064	843	847	850	rBV	196	178	0.02%	0.003%
11	4.321	924	927	929	rBV2	247	170	0.02%	0.003%
12	4.478	970	976	981	rVB2	263	365	0.04%	0.006%
13	4.507	981	985	988	rBV2	253	259	0.03%	0.004%
14	4.572	999	1005	1007	rBV2	275	314	0.04%	0.005%
15	4.620	1008	1020	1055	rVV	76023	197677	23.11%	3.038%
16	4.893	1102	1105	1108	rBV3	309	241	0.03%	0.004%
17	4.909	1108	1110	1113	rVB2	464	240	0.03%	0.004%
18	4.929	1114	1116	1119	rBV	316	247	0.03%	0.004%
19	4.977	1127	1131	1135	rBB	361	331	0.04%	0.005%
20	5.057	1135	1156	1174	rBV	162774	356962	41.74%	5.486%
21	5.163	1186	1189	1191	rBV2	306	185	0.02%	0.003%
22	5.205	1198	1202	1203	rBV2	295	205	0.02%	0.003%
23	5.279	1218	1225	1228	rBV3	825	874	0.10%	0.013%
24	5.314	1234	1236	1241	rBB2	257	190	0.02%	0.003%
25	5.340	1241	1244	1248	rBV2	281	274	0.03%	0.004%
26	5.469	1278	1284	1289	rBB2	279	378	0.04%	0.006%
27	5.494	1289	1292	1296	rBB2	251	220	0.03%	0.003%
28	5.568	1312	1315	1318	rBV	306	229	0.03%	0.004%
29	5.636	1330	1336	1340	rBV2	347	481	0.06%	0.007%
30	5.720	1340	1362	1383	rBV2	312690	855297	100.00%	13.145%
31	6.035	1457	1460	1465	rVV2	224	168	0.02%	0.003%
32	6.060	1465	1468	1472	rVB2	276	234	0.03%	0.004%
33	6.125	1486	1488	1494	rVB3	396	319	0.04%	0.005%
34	6.192	1505	1509	1512	rBV	378	324	0.04%	0.005%
35	6.244	1512	1525	1543	rBV	271591	513617	60.05%	7.893%
36	6.353	1555	1559	1564	rBV3	310	314	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052858.D
 Acq On : 27 Jan 2023 19:39
 Operator : JC/MD
 Sample : 01314-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

37	6.488	1598	1601	1602	rBV	302	180	0.02%	0.003%
38	6.533	1610	1615	1624	rVB6	1739	2535	0.30%	0.039%
39	6.684	1649	1662	1680	rVV	195835	376305	44.00%	5.783%
40	6.771	1686	1689	1691	rBV	341	188	0.02%	0.003%
41	6.803	1695	1699	1703	rVB2	433	426	0.05%	0.007%
42	6.822	1703	1705	1709	rVB2	289	206	0.02%	0.003%
43	6.973	1745	1752	1755	rBV2	389	526	0.06%	0.008%
44	7.019	1761	1766	1769	rBV2	291	334	0.04%	0.005%
45	7.182	1811	1817	1819	rBV2	1119	1125	0.13%	0.017%
46	7.401	1882	1885	1888	rVB	235	183	0.02%	0.003%
47	7.433	1891	1895	1899	rVB2	262	258	0.03%	0.004%
48	7.456	1899	1902	1905	rBV	326	306	0.04%	0.005%
49	7.498	1910	1915	1917	rBV2	279	246	0.03%	0.004%
50	7.562	1922	1935	1951	rBV2	102652	179208	20.95%	2.754%
51	7.687	1969	1974	1977	rBV2	876	771	0.09%	0.012%
52	7.752	1988	1994	1997	rBV2	310	426	0.05%	0.007%
53	7.893	2025	2038	2055	rBV	395076	665053	77.76%	10.221%
54	8.073	2090	2094	2098	rVB3	470	501	0.06%	0.008%
55	8.176	2111	2126	2143	rBV	74714	125703	14.70%	1.932%
56	8.295	2159	2163	2168	rBV2	378	423	0.05%	0.007%
57	8.343	2176	2178	2182	rBV	382	333	0.04%	0.005%
58	8.366	2182	2185	2189	rVB3	444	390	0.05%	0.006%
59	8.391	2189	2193	2198	rBB2	318	331	0.04%	0.005%
60	8.430	2198	2205	2210	rBV2	281	374	0.04%	0.006%
61	8.520	2229	2233	2239	rVB2	319	327	0.04%	0.005%
62	8.552	2239	2243	2246	rBV2	415	391	0.05%	0.006%
63	8.633	2256	2268	2297	rBV2	187715	362722	42.41%	5.574%
64	8.838	2330	2332	2335	rVB	322	195	0.02%	0.003%
65	8.906	2349	2353	2356	rVB2	359	262	0.03%	0.004%
66	8.938	2359	2363	2367	rBV2	323	404	0.05%	0.006%
67	8.986	2373	2378	2380	rBV2	216	244	0.03%	0.004%
68	9.192	2440	2442	2447	rVB2	360	323	0.04%	0.005%
69	9.234	2450	2455	2456	rBV	260	263	0.03%	0.004%
70	9.311	2473	2479	2484	rBV2	415	612	0.07%	0.009%
71	9.414	2498	2511	2530	rBV	386788	630176	73.68%	9.685%
72	9.678	2586	2593	2597	rBV2	378	446	0.05%	0.007%
73	9.703	2597	2601	2603	rBV2	248	180	0.02%	0.003%
74	9.993	2689	2691	2693	rBV	297	188	0.02%	0.003%
75	10.044	2703	2707	2709	rBV	180	171	0.02%	0.003%
76	10.157	2739	2742	2747	rBV2	339	395	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052858.D
 Acq On : 27 Jan 2023 19:39
 Operator : JC/MD
 Sample : 01314-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis

77	10.269	2774	2777	2782	rBV2	275	287	0.03%	0.004%
78	10.539	2857	2861	2869	rVB2	243	308	0.04%	0.005%
79	10.751	2914	2927	2943	rBV	277263	441795	51.65%	6.790%
80	10.880	2963	2967	2970	rBV2	503	486	0.06%	0.007%
81	11.118	3038	3041	3045	rBV2	231	247	0.03%	0.004%
82	11.395	3124	3127	3132	rBV2	294	259	0.03%	0.004%
83	11.520	3163	3166	3171	rBV2	228	212	0.02%	0.003%
84	11.623	3196	3198	3202	rVB	360	203	0.02%	0.003%
85	11.645	3203	3205	3207	rBV	302	168	0.02%	0.003%
86	11.658	3207	3209	3215	rVV2	330	356	0.04%	0.005%
87	11.710	3218	3225	3227	rBV	325	353	0.04%	0.005%
88	11.806	3243	3255	3273	rBV	362701	573007	67.00%	8.806%
89	12.140	3353	3359	3361	rBV2	261	281	0.03%	0.004%
90	12.189	3361	3374	3396	rBV	376749	606033	70.86%	9.314%
91	12.337	3417	3420	3428	rBV2	385	403	0.05%	0.006%
92	13.079	3644	3651	3656	rBV	532	620	0.07%	0.010%
93	13.446	3758	3765	3767	rBV	370	487	0.06%	0.007%
94	13.488	3776	3778	3781	rVB	424	196	0.02%	0.003%
95	13.713	3845	3848	3850	rBV2	436	291	0.03%	0.004%
96	13.748	3857	3859	3863	rBV2	458	281	0.03%	0.004%
97	14.285	4019	4026	4028	rBV2	331	328	0.04%	0.005%
98	14.623	4129	4131	4137	rBV	375	376	0.04%	0.006%
99	14.693	4151	4153	4156	rBV2	258	223	0.03%	0.003%
100	14.861	4202	4205	4210	rBV5	625	668	0.08%	0.010%




Sum of corrected areas: 6506868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052858.D
Acq On : 27 Jan 2023 19:39
Operator : JC/MD
Sample : 01314-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

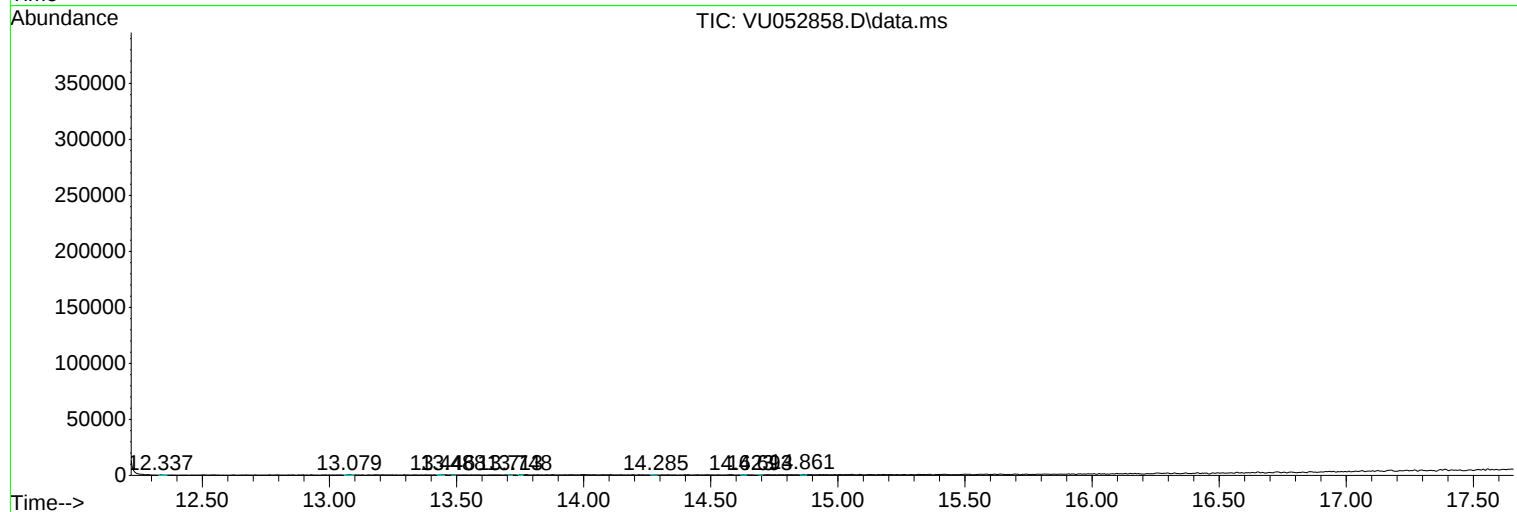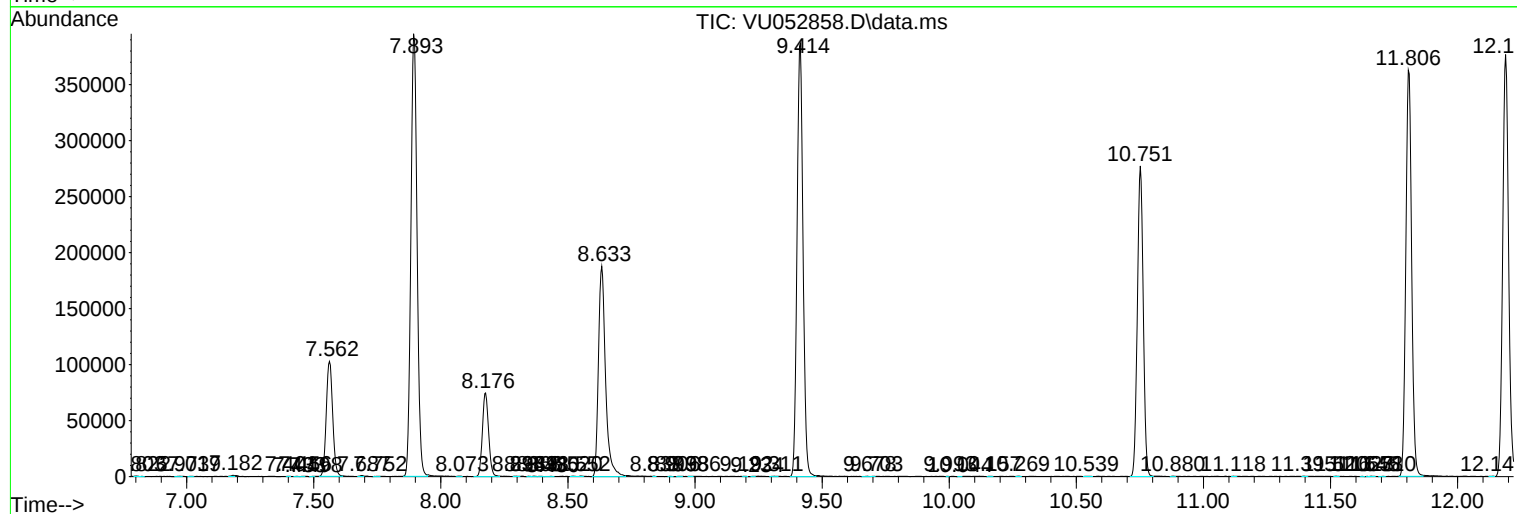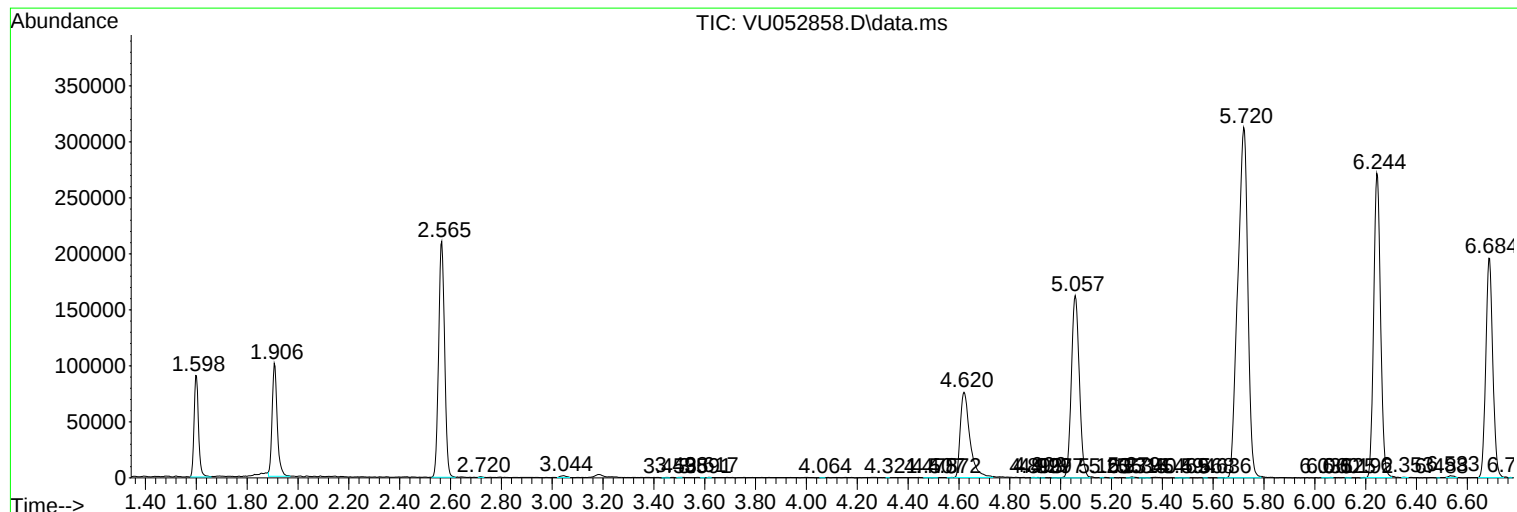

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052858.D
Acq On : 27 Jan 2023 19:39
Operator : JC/MD
Sample : 01314-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
Data File : VU052858.D
Acq On : 27 Jan 2023 19:39
Operator : JC/MD
Sample : 01314-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------