
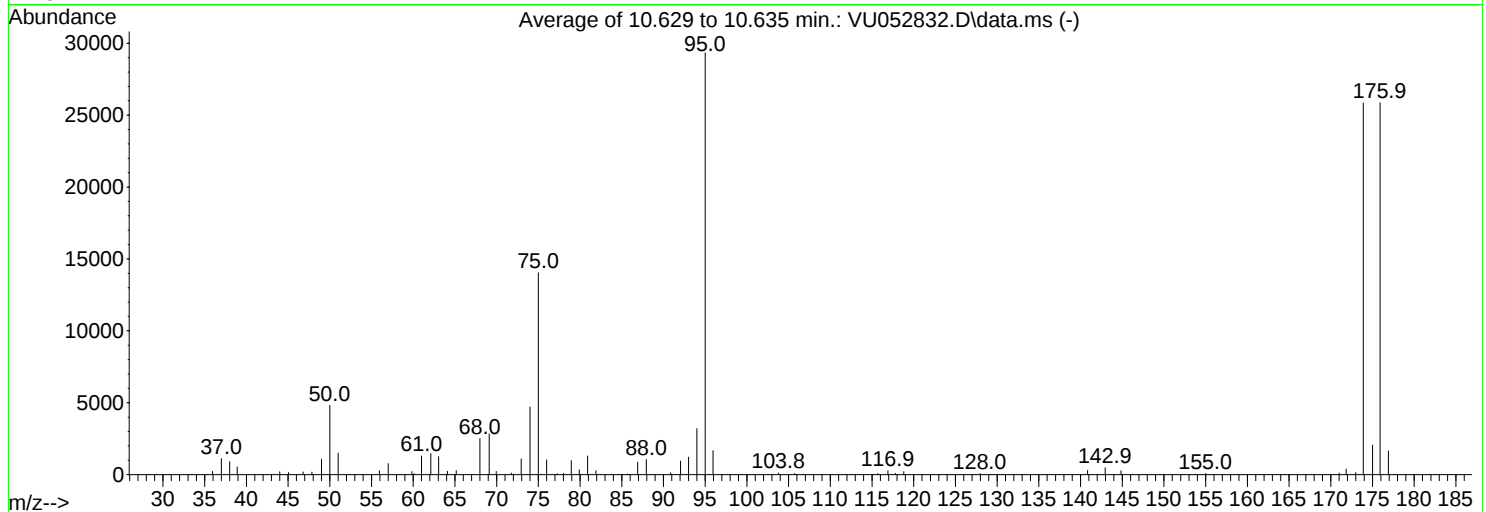


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012723\
 Data File : VU052832.D
 Acq On : 27 Jan 2023 09:03
 Operator : JC/MD
 Sample : BFB154
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB154

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM012623WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 01 00:53:48 2023

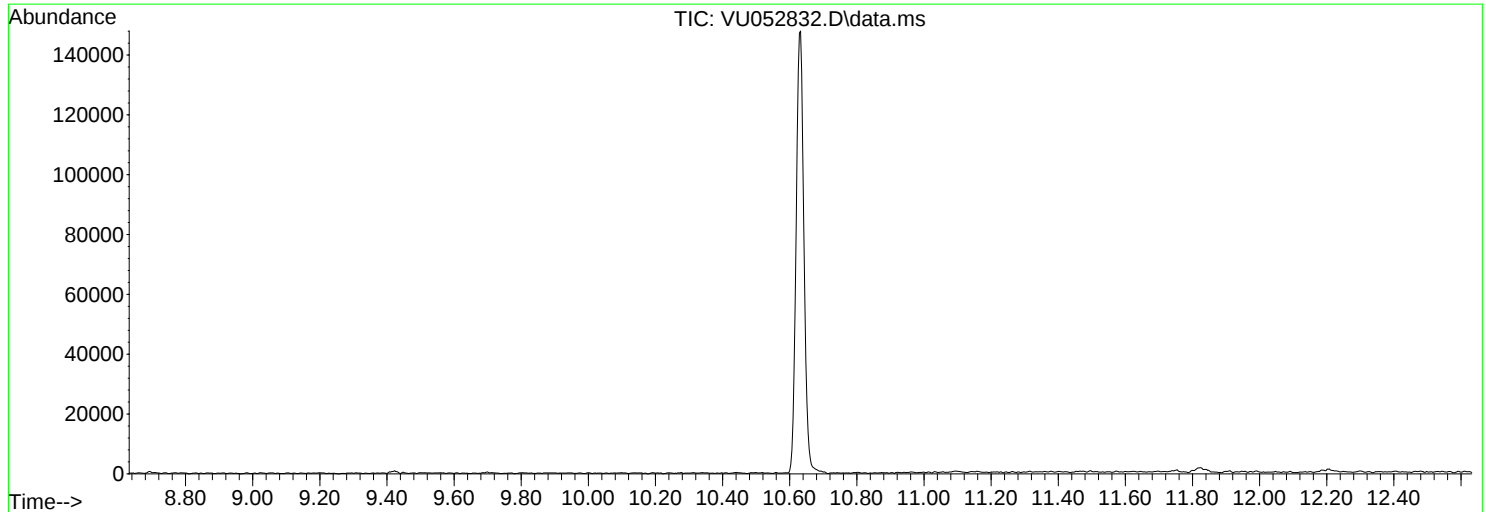

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	4818	PASS
75	95	30	80	47.9	14046	PASS
95	95	100	100	100.0	29333	PASS
96	95	5	9	5.7	1670	PASS
173	174	0.00	2	0.6	149	PASS
174	95	50	120	88.1	25848	PASS
175	174	5	9	8.0	2056	PASS
176	174	95	101	100.0	25859	PASS
177	176	5	9	6.4	1646	PASS

m/z	Abundance
39.90	178.0
44.00	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
36.00	194.0
37.00	1117.0
38.00	1037.0
38.90	499.0
40.00	153.0
44.00	332.0
45.00	140.0
46.80	166.0
47.90	171.0
49.00	1080.0
50.00	4942.0
51.00	1608.0
55.90	279.0
57.00	769.0
59.80	345.0
61.00	1377.0
62.10	1451.0
63.00	1410.0
64.10	263.0
65.10	296.0
68.00	2495.0
69.10	2940.0
70.00	258.0
71.70	172.0
73.00	1213.0
74.00	4896.0
75.00	14563.0
76.00	1201.0
78.00	140.0
78.90	994.0
79.90	335.0
80.90	1237.0
81.90	279.0
85.70	120.0
86.90	959.0
87.90	1096.0
90.80	109.0
92.00	919.0
93.00	1283.0
94.00	3394.0
95.00	30184.0
95.90	1771.0
103.90	118.0
115.70	116.0
116.90	290.0
118.80	238.0
127.90	132.0
140.80	308.0
142.90	458.0
144.90	264.0
155.00	105.0
171.00	170.0
171.80	374.0
173.90	26280.0
175.00	2112.0
175.90	26528.0
176.90	1681.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
35.90	236.0
37.00	1152.0
38.00	916.0
38.90	553.0
40.00	131.0
44.00	379.0
45.00	141.0
46.80	184.0
47.80	193.0
49.00	1090.0
50.00	5019.0
51.00	1539.0
56.00	263.0
57.00	796.0
59.90	286.0
61.00	1345.0
62.10	1509.0
63.00	1287.0
64.10	252.0
65.10	282.0
68.00	2598.0
69.10	2909.0
70.00	220.0
71.80	166.0
73.00	1082.0
74.00	4879.0
75.00	14491.0
76.00	988.0
77.30	101.0
78.00	113.0
79.00	987.0
79.90	351.0
80.90	1330.0
81.90	274.0
86.90	853.0
88.00	1097.0
90.90	121.0
92.00	1003.0
93.00	1229.0
94.00	3285.0
95.00	30552.0
96.00	1705.0
103.80	105.0
105.80	131.0
115.70	102.0
116.90	267.0
117.80	126.0
118.80	212.0
128.00	114.0
140.80	303.0
143.00	501.0
144.80	275.0
155.00	116.0
171.00	162.0
171.90	406.0
173.90	26568.0
175.00	2135.0
175.90	26880.0
176.90	1707.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
35.90	245.0
37.00	1055.0
38.00	778.0
38.90	541.0
40.00	131.0
44.00	355.0
45.10	154.0
46.80	209.0
47.80	171.0
49.00	1022.0
50.00	4494.0
51.00	1326.0
56.00	298.0
57.00	742.0
60.10	206.0
61.00	1193.0
62.10	1435.0
63.10	1065.0
64.10	194.0
65.20	253.0
68.00	2481.0
69.10	2669.0
69.90	181.0
72.00	150.0
72.90	966.0
74.00	4358.0
75.00	13084.0
76.00	868.0
77.20	110.0
79.00	951.0
79.90	315.0
80.90	1331.0
81.90	278.0
86.90	790.0
88.00	958.0
90.90	157.0
92.10	905.0
93.00	1115.0
94.00	2920.0
95.00	27264.0
96.00	1535.0
103.70	108.0
105.70	123.0
116.90	259.0
117.80	129.0
118.80	185.0
140.90	271.0
143.00	485.0
144.80	288.0
171.90	389.0
173.00	448.0
173.90	24696.0
175.00	1922.0
175.90	24168.0
176.90	1549.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154