




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063052.D
Acq On : 28 Jan 2025 06:56
Operator : MD/SY
Sample : Q1195-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2968

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 01/30/2025
Supervised By :Semsettin Yesilyurt 01/30/2025

Quant Time: Jan 29 08:21:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

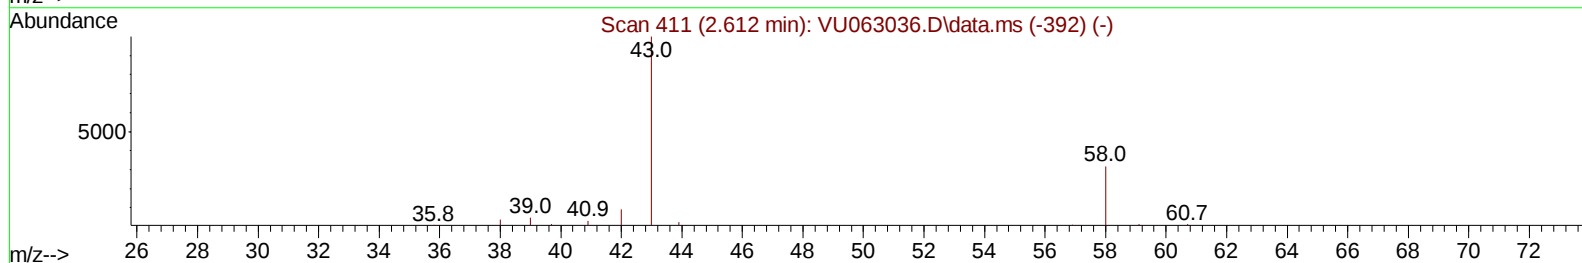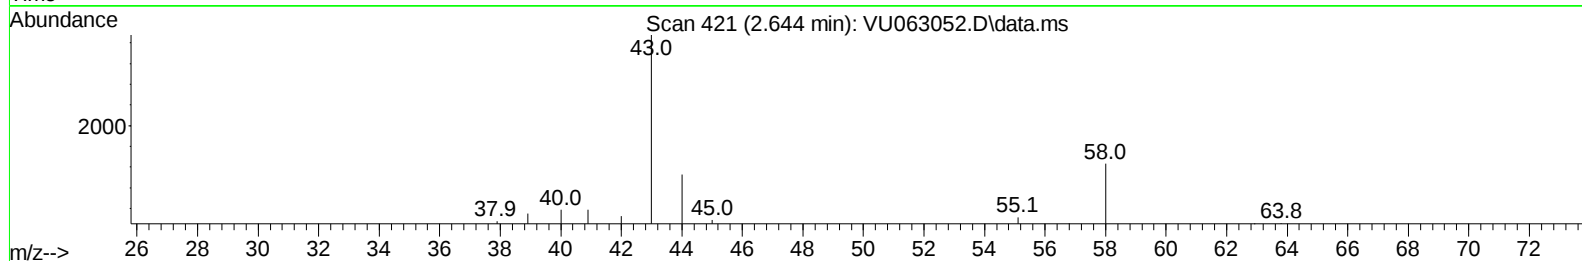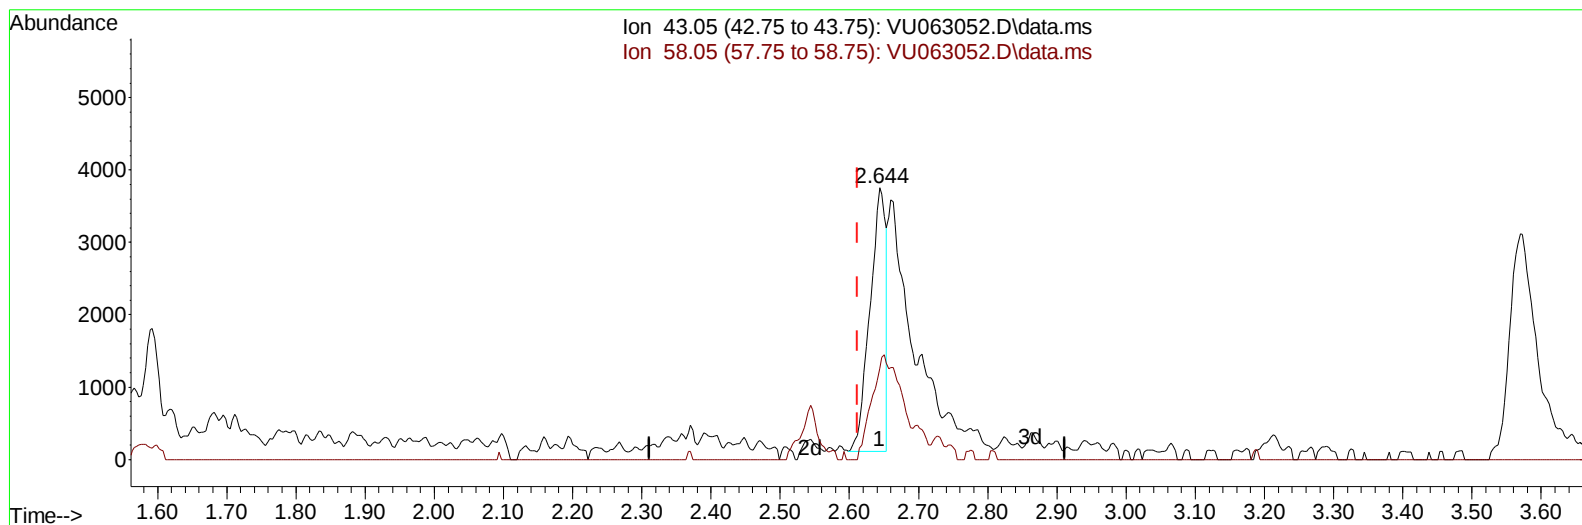

TIC: VU063052.D\data.ms

(13) Acetone (T)

2.644min (+ 0.032) 6.98 ug/L

response 5797

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	73.07#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063052.D
Acq On : 28 Jan 2025 06:56
Operator : MD/SY
Sample : Q1195-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2968

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 01/30/2025
Supervised By :Semsettin Yesilyurt 01/30/2025

Quant Time: Jan 29 08:21:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

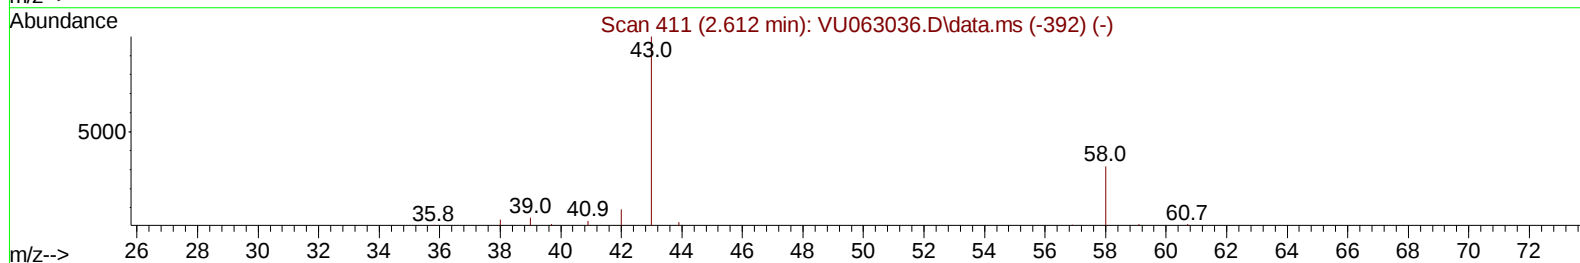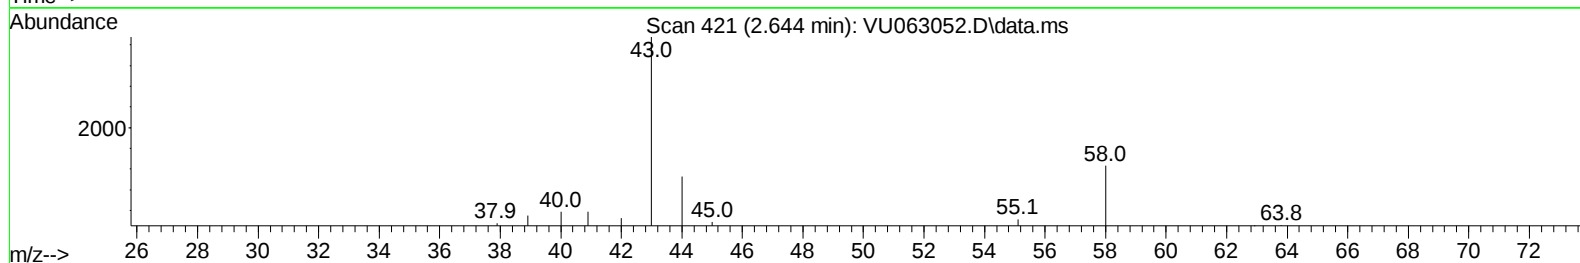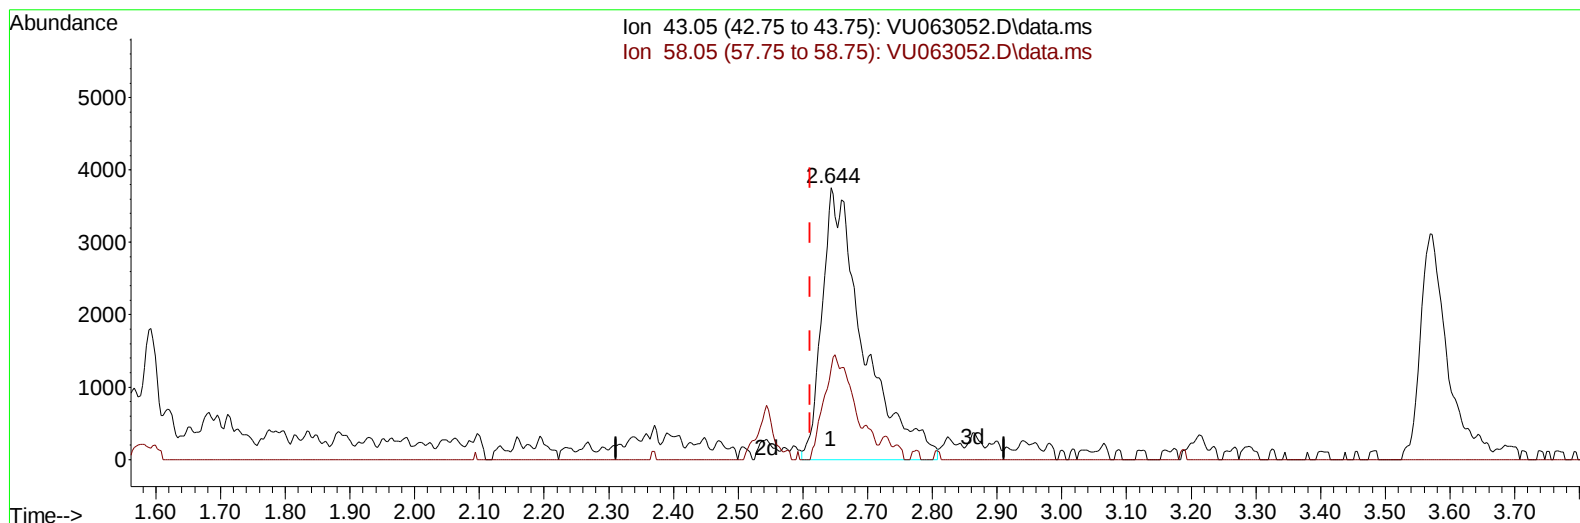

TIC: VU063052.D\data.ms

(13) Acetone (T)

2.644min (+ 0.032) 20.08 ug/L m

response 16680

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	25.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
 Data File : VU063052.D
 Acq On : 28 Jan 2025 06:56
 Operator : MD/SY
 Sample : Q1195-17
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2968

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 01/30/2025
 Supervised By :Semsettin Yesilyurt 01/30/2025

Quant Time: Jan 29 08:21:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 08:16:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.235	114	123133	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.405	117	246296	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	58045	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	45631	10.309	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 206.200%#			
7) Chloroethane-d5	1.901	69	26323	7.832	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 156.600%#			
11) 1,1-Dichloroethene-d2	2.557	65	25754	9.729	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 194.600%#			
20) 2-Butanone-d5	4.631	46	90527	70.466	ug/L	0.03
Spiked Amount 50.000	Range 40 - 130		Recovery = 140.940%#			
24) Chloroform-d	5.039	84	98946	5.627	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 112.600%			
26) 1,2-Dichloroethane-d4	5.692	65	46518	4.635	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 92.600%			
32) Benzene-d6	5.714	84	135045	2.399	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 48.000%#			
36) 1,2-Dichloropropane-d6	6.682	67	72031	5.026	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 100.600%			
41) Toluene-d8	7.888	98	239205	4.299	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 86.000%			
43) trans-1,3-Dichloroprop...	8.171	79	38099	4.294	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 85.800%			
46) 2-Hexanone-d5	8.624	63	156786	70.828	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 141.660%#			
56) 1,1,2,2-Tetrachloroeth...	10.743	84	21331	1.568	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 31.400%#			
66) 1,2-Dichlorobenzene-d4	12.183	152	45464	4.376	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 87.600%			
Target Compounds						
						Qvalue
13) Acetone	2.644	43	16680m	20.080	ug/L	
14) Carbon disulfide	2.782	76	14068	0.858	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063052.D
Acq On : 28 Jan 2025 06:56
Operator : MD/SY
Sample : Q1195-17
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2968

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 01/30/2025
Supervised By :Semsettin Yesilyurt 01/30/2025

Quant Time: Jan 29 08:21:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

