

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
 Data File : VU063019.D
 Acq On : 27 Jan 2025 16:31
 Operator : MD/SY
 Sample : Q1191-06
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44W6

Quant Time: Jan 29 07:28:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 07:27:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	113406	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.406	117	107809	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	52275	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	13898	3.409	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.200%
7) Chloroethane-d5	1.901	69	12376	3.998	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.000%
11) 1,1-Dichloroethene-d2	2.554	65	9721	3.987	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.800%
20) 2-Butanone-d5	4.605	46	58357	49.321	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.640%
24) Chloroform-d	5.046	84	67415	4.163	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
26) 1,2-Dichloroethane-d4	5.689	65	40874	4.422	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.400%
32) Benzene-d6	5.714	84	106891	4.339	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	6.676	67	30167	4.809	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.200%
41) Toluene-d8	7.888	98	100148	4.111	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	8.174	79	16312	4.200	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.621	63	45390	46.844	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.680%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	27109	4.551	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.000%
66) 1,2-Dichlorobenzene-d4	12.184	152	42595	4.552	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.000%
Target Compounds					Qvalue	
13) Acetone	2.612	43	10392	13.583	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063019.D
Acq On : 27 Jan 2025 16:31
Operator : MD/SY
Sample : Q1191-06
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44W6


Quant Time: Jan 29 07:28:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 07:27:08 2025
Response via : Initial Calibration

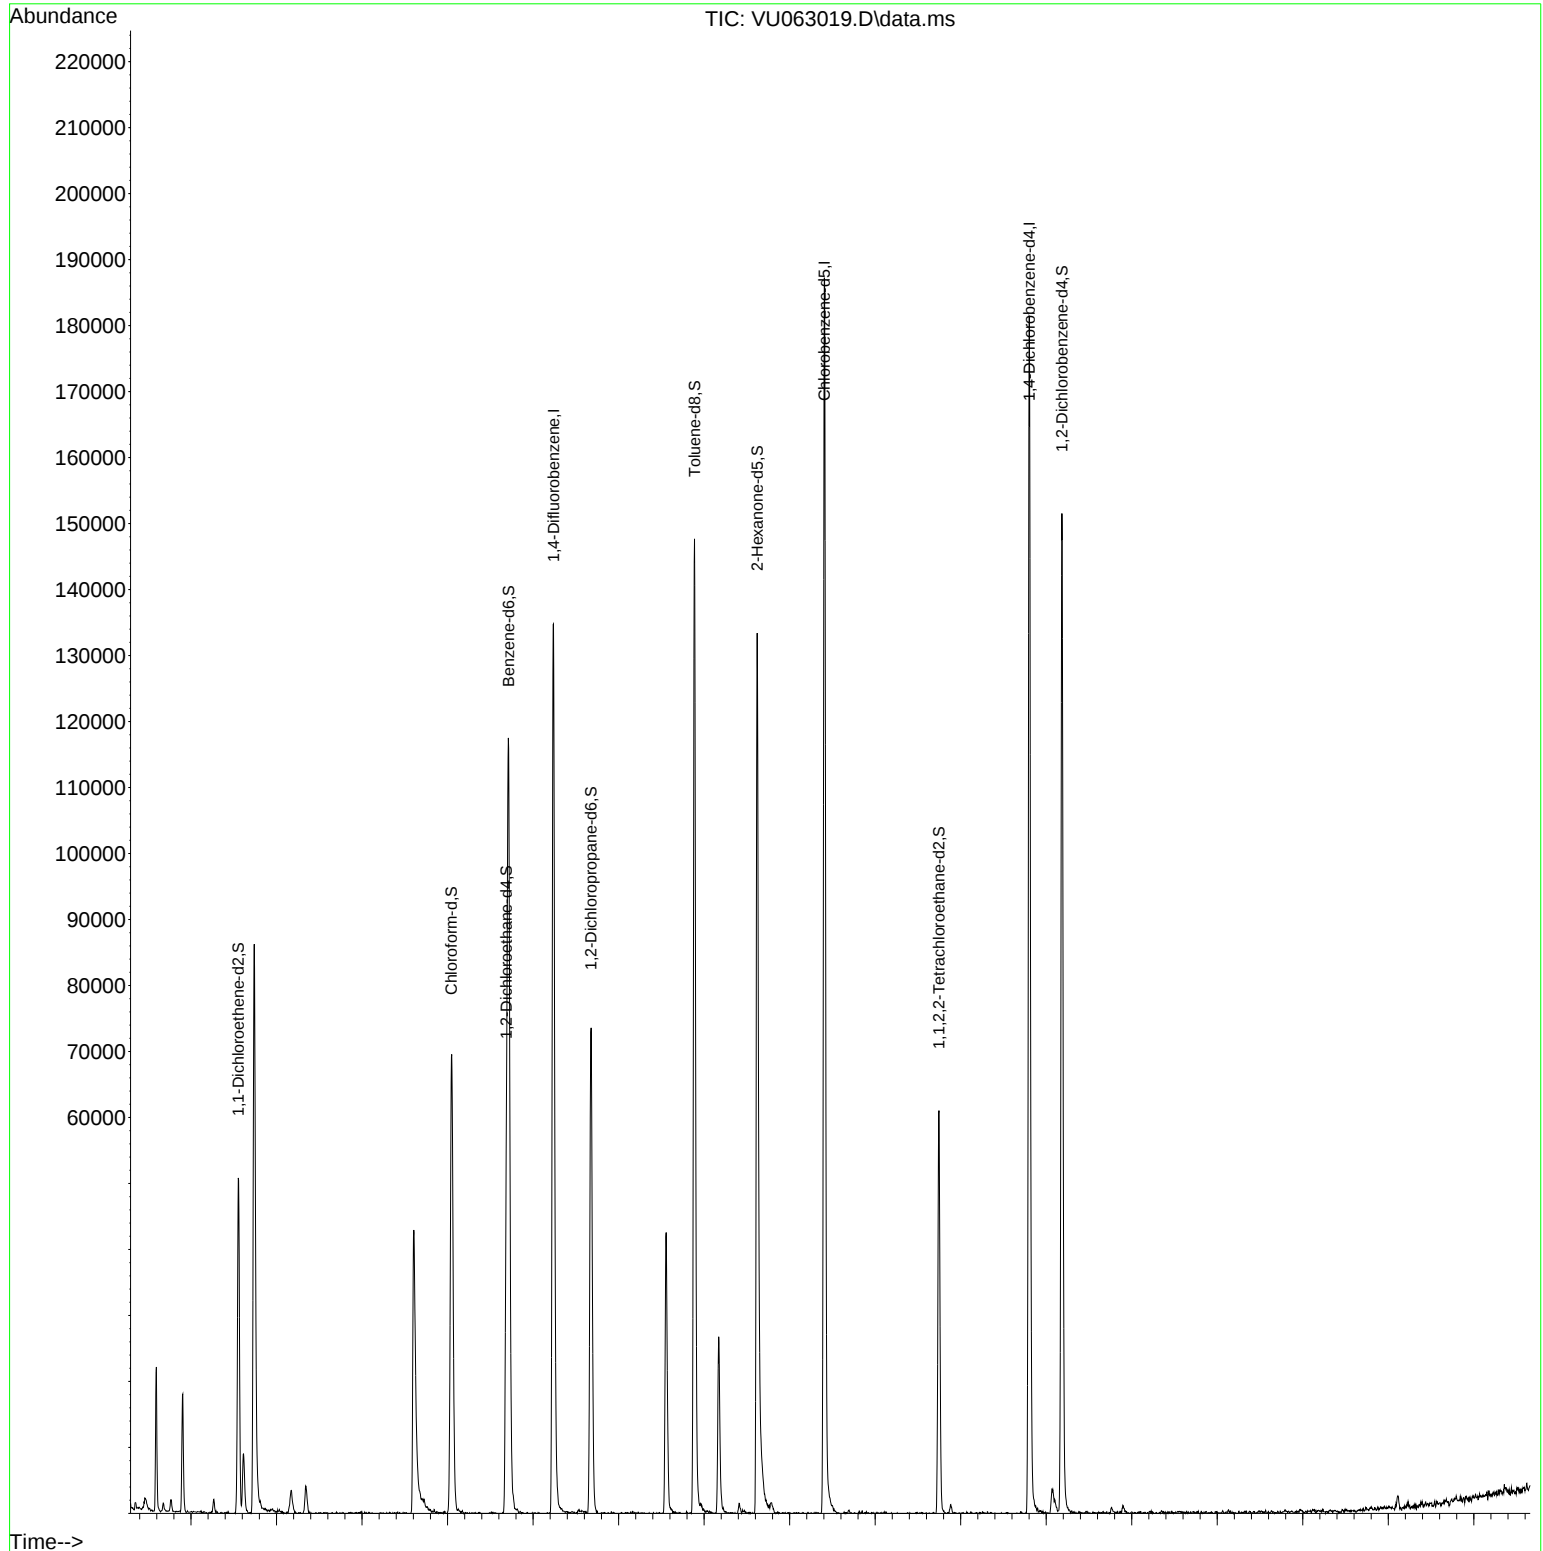

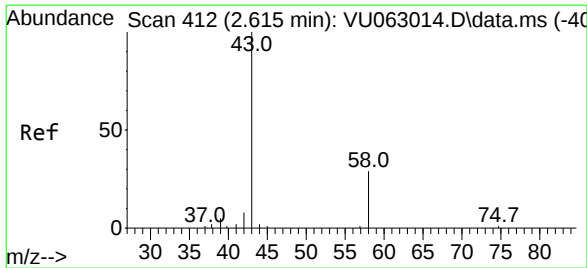

#13
Acetone
Concen: 13.583 ug/L
RT: 2.612 min Scan# 41
Delta R.T. -0.003 min
Lab File: VU063019.D
Acq: 27 Jan 2025 16:31

Instrument :
MSVOA_U
ClientSampleId :
A44W6

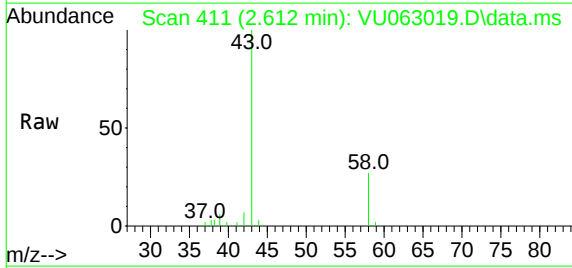

Tgt Ion: 43 Resp: 10392
Ion Ratio Lower Upper
43 100
58 30.9 0.0 64.4

