

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
 Data File : VU063026.D
 Acq On : 27 Jan 2025 19:24
 Operator : MD/SY
 Sample : Q1192-07
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A44W2

Quant Time: Jan 29 07:30:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 07:27:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	103450	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	102170	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	49436	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.593	65	16966	4.562	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.200%
7) Chloroethane-d5	1.904	69	11980	4.243	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.800%
11) 1,1-Dichloroethene-d2	2.557	65	8406	3.780	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	4.605	46	46281	42.879	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.760%
24) Chloroform-d	5.049	84	56203	3.805	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.000%
26) 1,2-Dichloroethane-d4	5.689	65	39941	4.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.715	84	97843	4.191	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.800%
36) 1,2-Dichloropropane-d6	6.679	67	29528	4.967	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.400%
41) Toluene-d8	7.888	98	98441	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	8.174	79	15960	4.337	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.621	63	49932	54.376	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.760%
56) 1,1,2,2-Tetrachloroeth...	10.743	84	29801	5.279	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.600%
66) 1,2-Dichlorobenzene-d4	12.184	152	42463	4.798	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.000%
Target Compounds					Qvalue	
13) Acetone	2.615	43	9156	13.119	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063026.D
Acq On : 27 Jan 2025 19:24
Operator : MD/SY
Sample : Q1192-07
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A44W2


Quant Time: Jan 29 07:30:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 07:27:08 2025
Response via : Initial Calibration

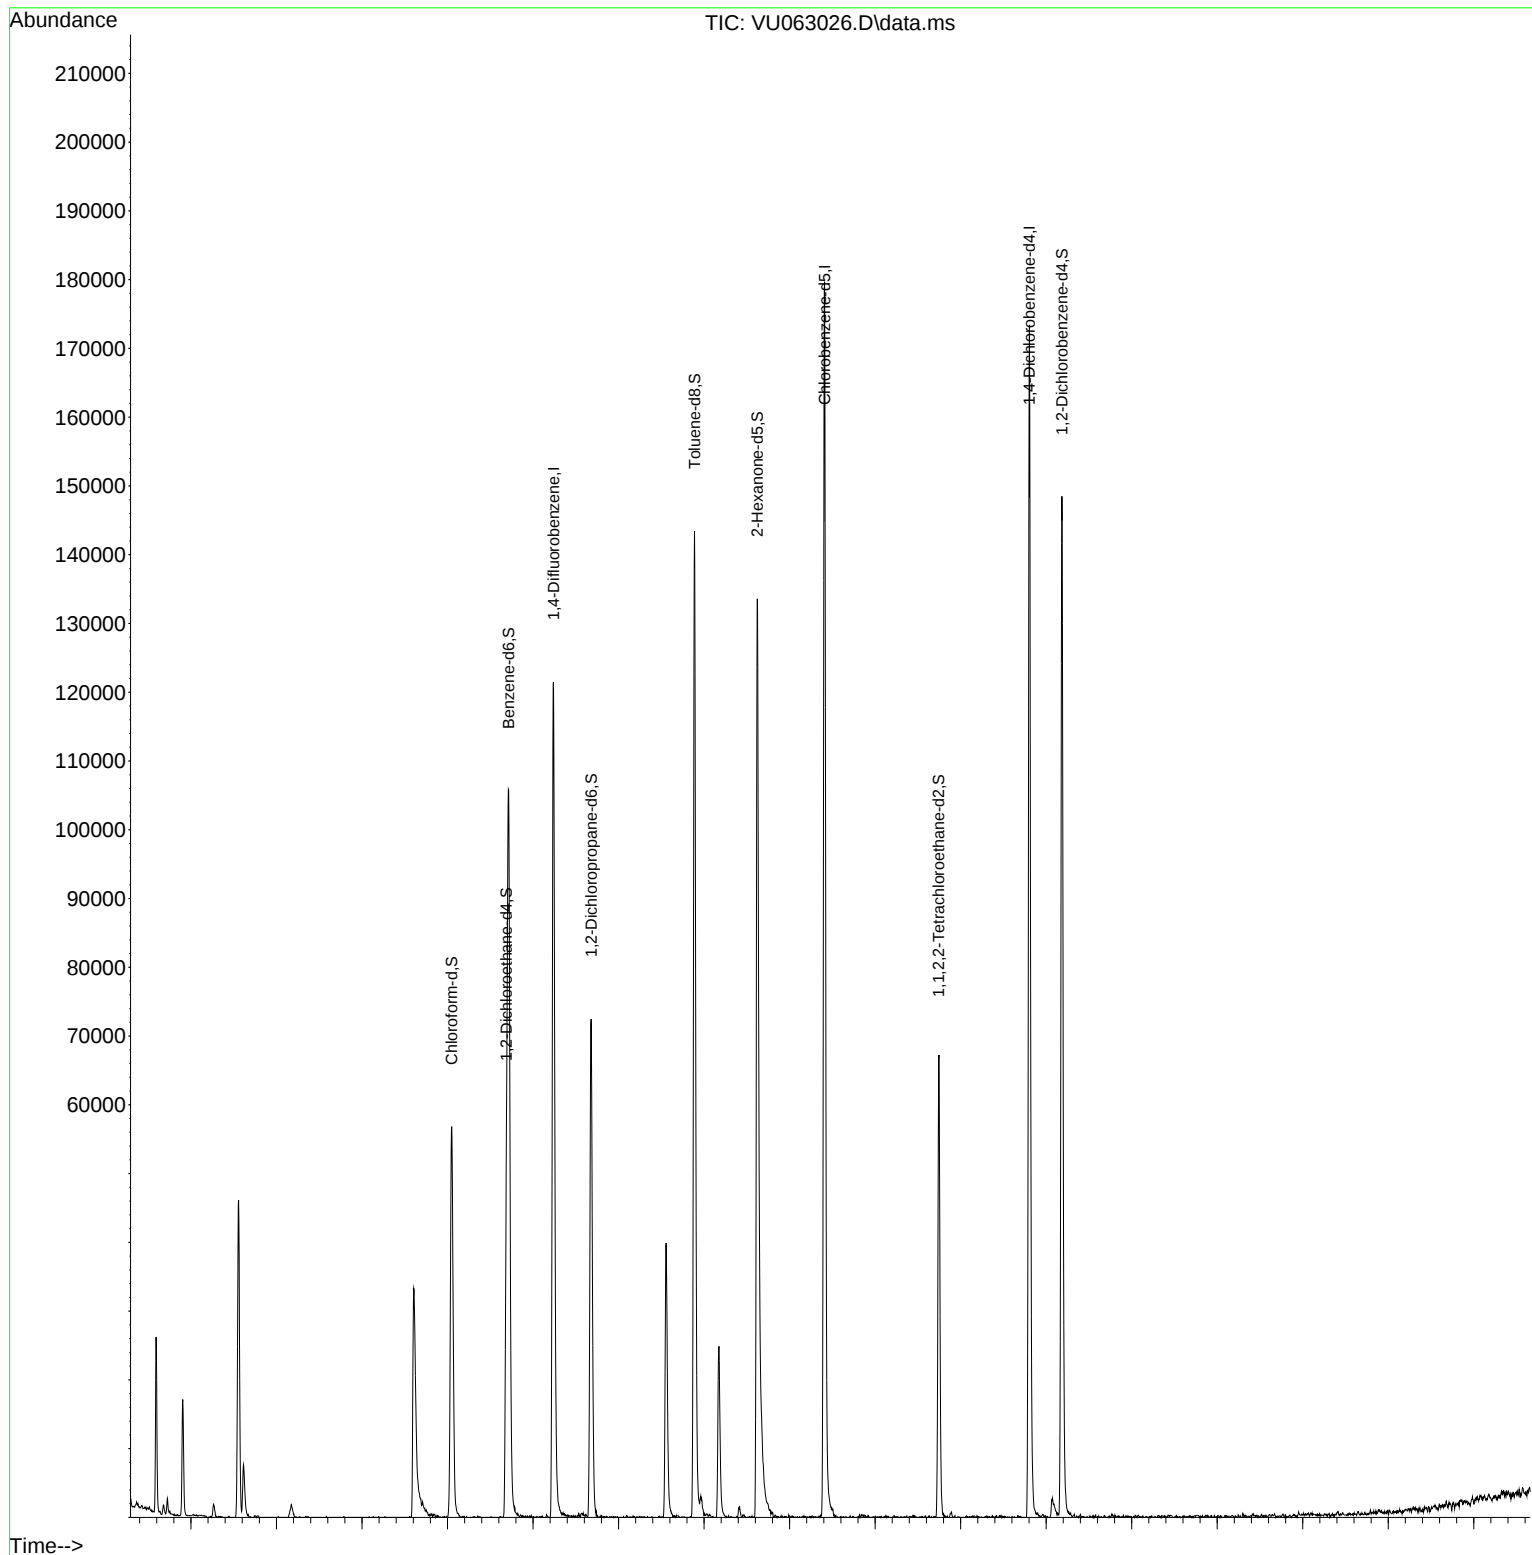

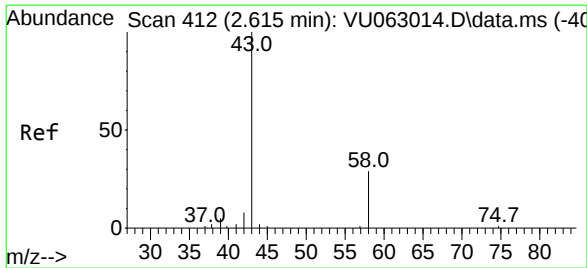

#13
 Acetone
 Concen: 13.119 ug/L
 RT: 2.615 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU063026.D
 Acq: 27 Jan 2025 19:24

Instrument :
 MSVOA_U
 ClientSampleId :
 A44W2

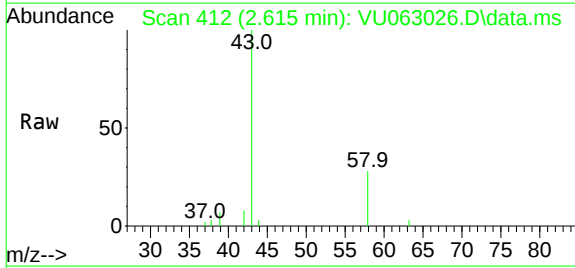

Tgt Ion: 43 Resp: 9156
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 64.4

