

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
 Data File : VU063037.D
 Acq On : 28 Jan 2025 00:46
 Operator : MD/SY
 Sample : VU0127WBL02
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK152

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU063037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.464	43	54	80	rBV	19579	42236	14.78%	1.663%
2	1.596	87	95	104	rVB	23778	26712	9.35%	1.052%
3	1.905	183	191	204	rBV	21233	26312	9.21%	1.036%
4	2.557	383	394	411	rBB	57523	92851	32.50%	3.656%
5	3.175	575	586	599	rBB2	2934	6085	2.13%	0.240%
6	4.605	1020	1031	1058	rBV	36550	89817	31.44%	3.536%
7	5.049	1154	1169	1189	rBV	62596	142746	49.96%	5.620%
8	5.711	1357	1375	1402	rBV3	106205	285711	100.00%	11.250%
9	6.239	1527	1539	1562	rBV	113760	217850	76.25%	8.578%
10	6.679	1664	1676	1701	rBB	66365	128488	44.97%	5.059%
11	7.554	1939	1948	1967	rBV	36402	66155	23.15%	2.605%
12	7.888	2040	2052	2070	rBV	139242	242336	84.82%	9.542%
13	8.171	2130	2140	2153	rBV	23898	40713	14.25%	1.603%
14	8.621	2270	2280	2307	rBV2	106009	221943	77.68%	8.739%
15	9.406	2513	2524	2547	rBV	155914	267390	93.59%	10.528%
16	10.743	2930	2940	2958	rBV2	57573	95759	33.52%	3.770%
17	11.804	3258	3270	3295	rBV	156843	273192	95.62%	10.757%
18	12.184	3377	3388	3406	rBV2	149243	255531	89.44%	10.061%
19	14.100	3975	3984	3992	rBV3	1619	3031	1.06%	0.119%
20	15.476	4405	4412	4423	rBV3	3709	5690	1.99%	0.224%
21	16.229	4638	4646	4652	rBV2	6888	9205	3.22%	0.362%




Sum of corrected areas: 2539753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063037.D
Acq On : 28 Jan 2025 00:46
Operator : MD/SY
Sample : VU0127WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

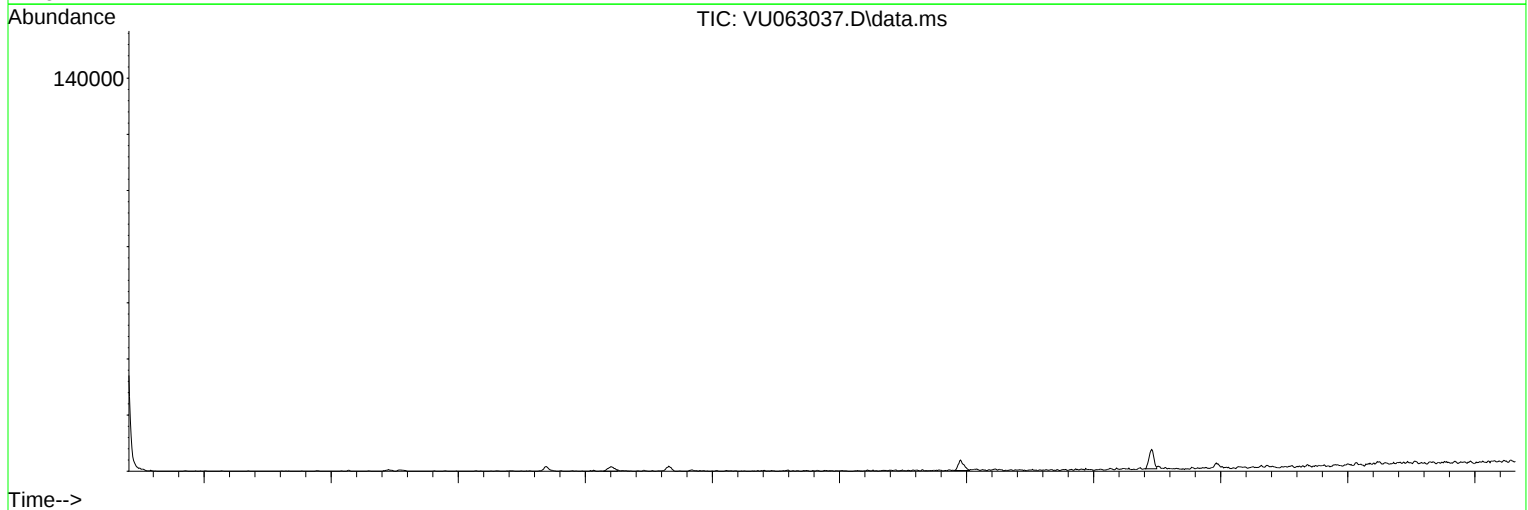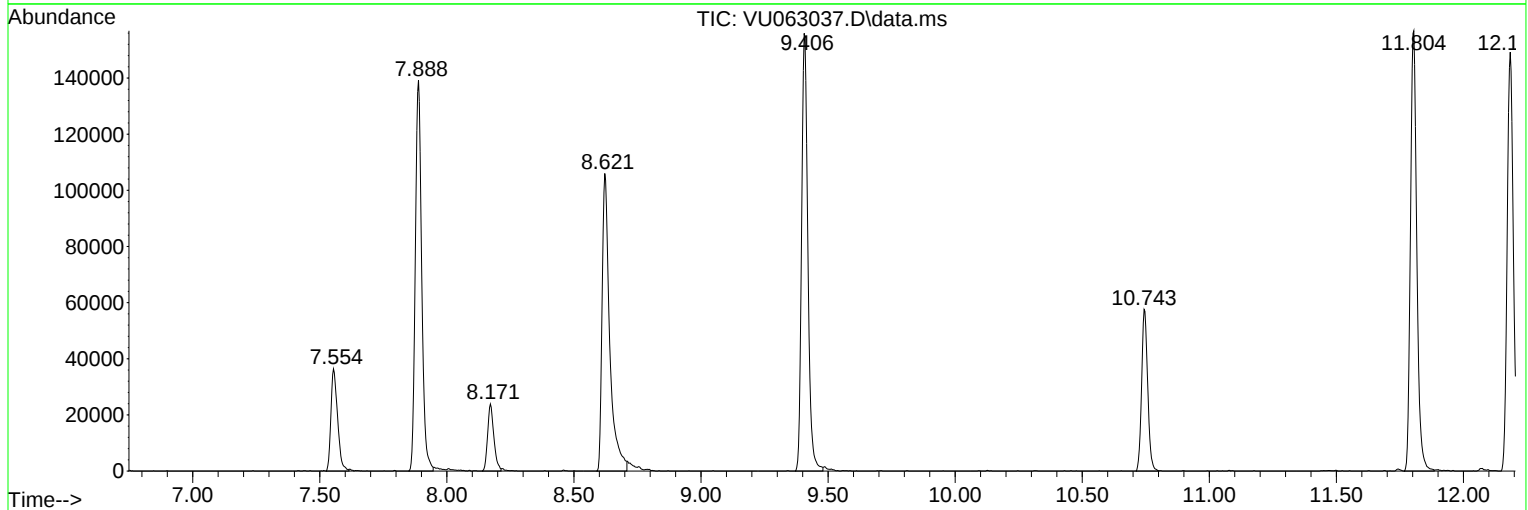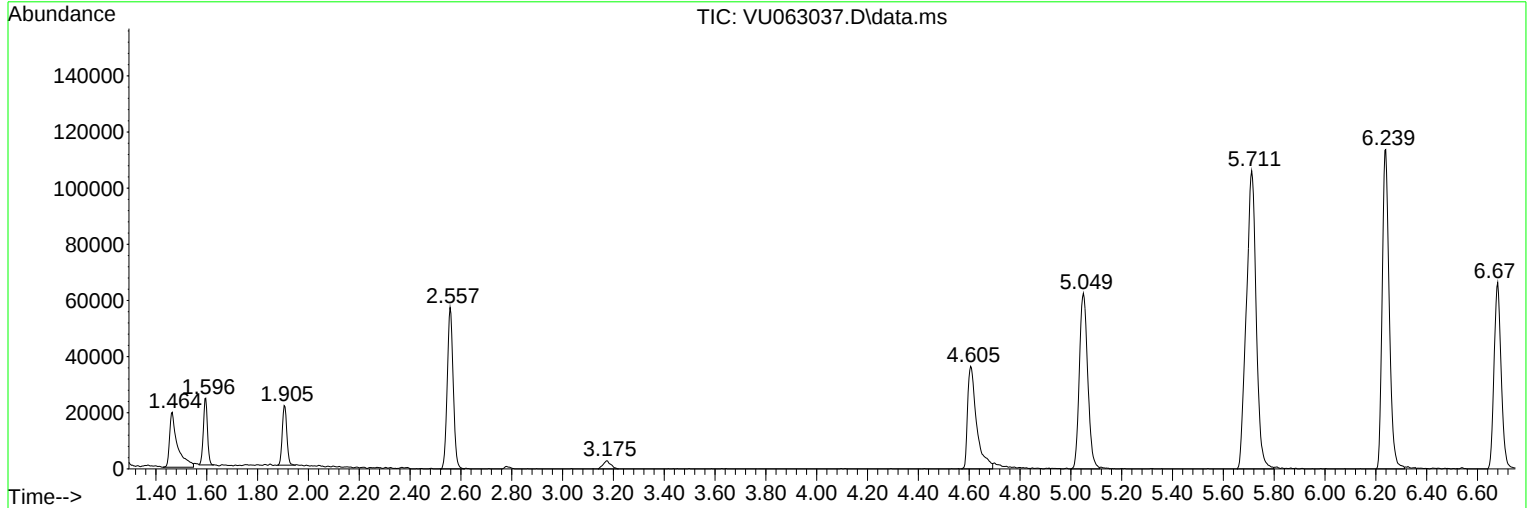

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063037.D
Acq On : 28 Jan 2025 00:46
Operator : MD/SY
Sample : VU0127WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063037.D
Acq On : 28 Jan 2025 00:46
Operator : MD/SY
Sample : VU0127WBL02
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
