
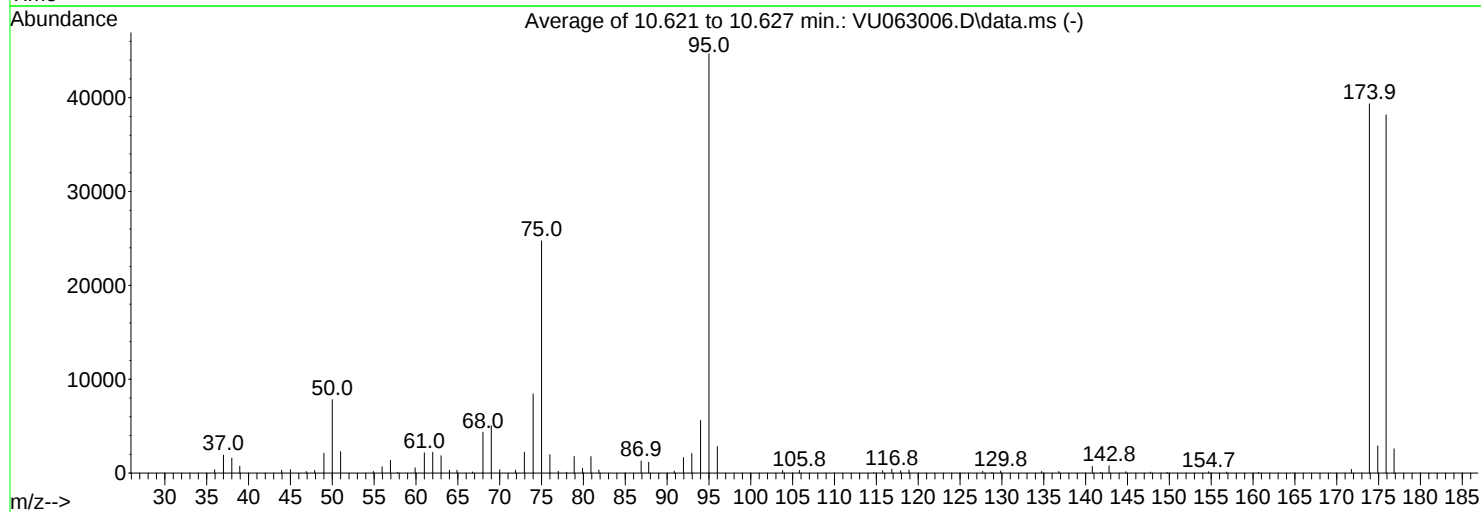


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012725\
Data File : VU063006.D
Acq On : 27 Jan 2025 08:20
Operator : MD/SY
Sample : BFB068
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB068

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 30 07:33:13 2025

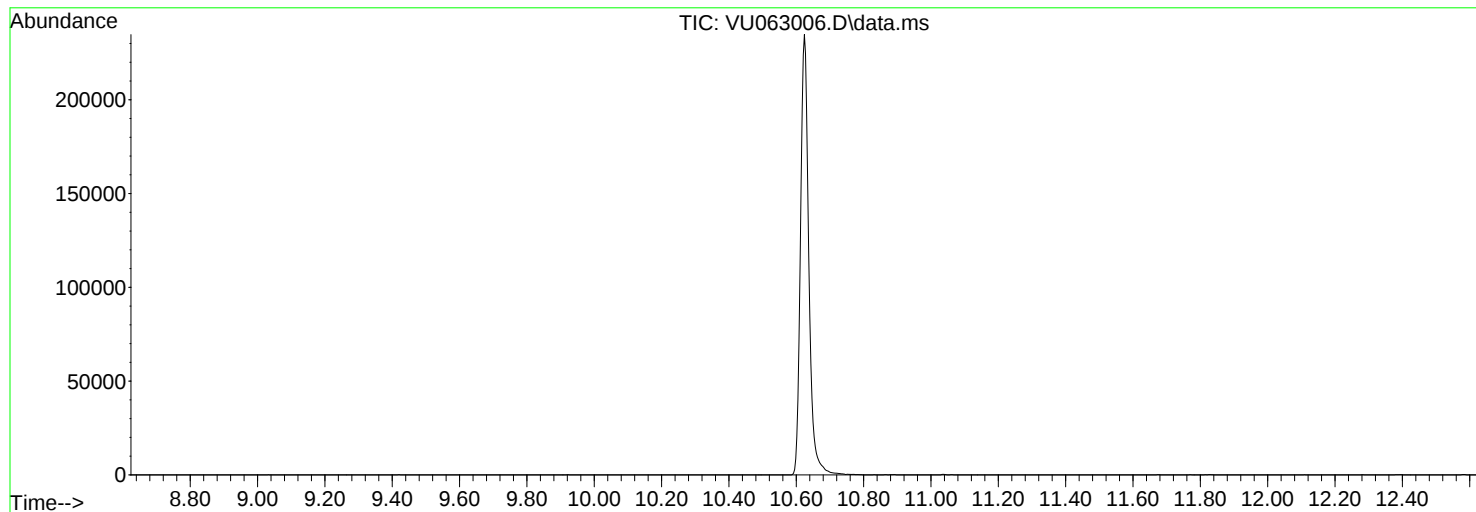

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	7814	PASS
75	95	30	80	55.4	24739	PASS
95	95	100	100	100.0	44680	PASS
96	95	5	9	6.3	2825	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.1	39341	PASS
175	174	5	9	7.3	2890	PASS
176	174	95	101	97.0	38173	PASS
177	176	5	9	6.8	2586	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB068

m/z	Abundance
35.90	378.0
37.00	1985.0
38.00	1677.0
39.00	711.0
44.00	279.0
45.00	390.0
47.00	113.0
47.90	285.0
49.00	2064.0
50.00	7854.0
51.00	2187.0
54.90	164.0
56.00	694.0
57.00	1412.0
59.90	511.0
61.00	2040.0
62.00	2308.0
63.00	1792.0
64.00	324.0
64.90	328.0
66.80	104.0
68.00	4420.0
69.00	5127.0
70.00	359.0
71.90	257.0
72.90	2143.0
74.00	8333.0
75.00	24712.0
76.00	2022.0
77.00	175.0
78.90	1712.0
79.90	554.0
80.90	1674.0
81.90	421.0
86.90	1238.0
87.80	1215.0
90.90	190.0
91.90	1547.0
92.90	2103.0
94.00	5587.0
95.00	44088.0
96.00	2794.0
103.80	301.0
105.80	245.0
114.70	101.0
115.80	276.0
116.90	389.0
117.90	217.0
118.90	306.0
127.70	217.0
129.80	226.0
134.70	111.0
136.70	157.0
140.80	652.0
141.80	129.0
142.80	815.0
144.80	161.0
147.70	100.0
149.80	125.0
154.70	165.0
156.90	111.0
171.80	374.0
173.90	38136.0
174.90	2899.0
175.90	36752.0
176.90	2650.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
36.00	364.0
37.00	1974.0
38.00	1629.0
38.90	754.0
44.00	322.0
45.00	385.0
46.90	160.0
47.90	295.0
49.00	2193.0
50.00	8022.0
51.00	2338.0
54.90	197.0
56.00	689.0
57.00	1427.0
57.80	100.0
59.90	591.0
61.00	2238.0
62.00	2242.0
63.00	1912.0
64.00	283.0
64.90	323.0
66.80	131.0
68.00	4420.0
69.00	5225.0
70.00	377.0
71.90	294.0
72.90	2307.0
74.00	8759.0
75.00	25416.0
76.00	2022.0
77.00	183.0
78.00	135.0
78.90	1855.0
79.90	540.0
80.90	1824.0
81.90	320.0
86.90	1313.0
87.80	1179.0
90.90	235.0
91.90	1726.0
92.90	2160.0
94.00	5733.0
95.00	46024.0
96.00	2875.0
103.80	279.0
105.80	305.0
115.80	253.0
116.80	441.0
117.90	271.0
118.90	341.0
127.70	185.0
128.80	123.0
129.80	231.0
134.80	186.0
136.80	168.0
140.80	784.0
141.80	122.0
142.80	790.0
144.80	155.0
147.80	112.0
149.70	111.0
154.70	154.0
156.80	130.0
160.60	107.0
171.70	400.0
173.90	40584.0
174.90	2994.0
175.90	39320.0
176.90	2661.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	315.0
37.00	1807.0
38.00	1480.0
38.90	770.0
43.90	302.0
45.00	326.0
46.80	229.0
47.90	270.0
49.00	2125.0
50.00	7565.0
51.00	2312.0
54.90	175.0
55.90	630.0
56.90	1219.0
57.80	108.0
59.90	580.0
61.00	2195.0
62.00	2080.0
63.00	1829.0
64.00	265.0
64.90	284.0
66.70	118.0
68.00	4225.0
69.00	4796.0
70.00	328.0
71.90	358.0
73.00	2233.0
74.00	8225.0
75.00	24088.0
76.00	1858.0
77.00	199.0
78.00	140.0
78.90	1752.0
79.90	468.0
80.90	1794.0
81.70	240.0
86.90	1319.0
87.80	1062.0
90.80	222.0
92.00	1680.0
93.00	1996.0
94.00	5500.0
95.00	43928.0
96.00	2805.0
103.80	254.0
105.80	324.0
115.70	232.0
116.80	432.0
117.90	272.0
118.90	337.0
127.70	157.0
128.80	124.0
129.90	241.0
134.80	221.0
136.90	203.0
140.80	719.0
142.80	745.0
144.80	134.0
147.80	128.0
154.70	128.0
156.80	123.0
160.70	114.0
171.70	397.0
173.90	39304.0
174.90	2778.0
175.90	38448.0
176.80	2446.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068