


tert-Butyl Alcohol

Response Ratio

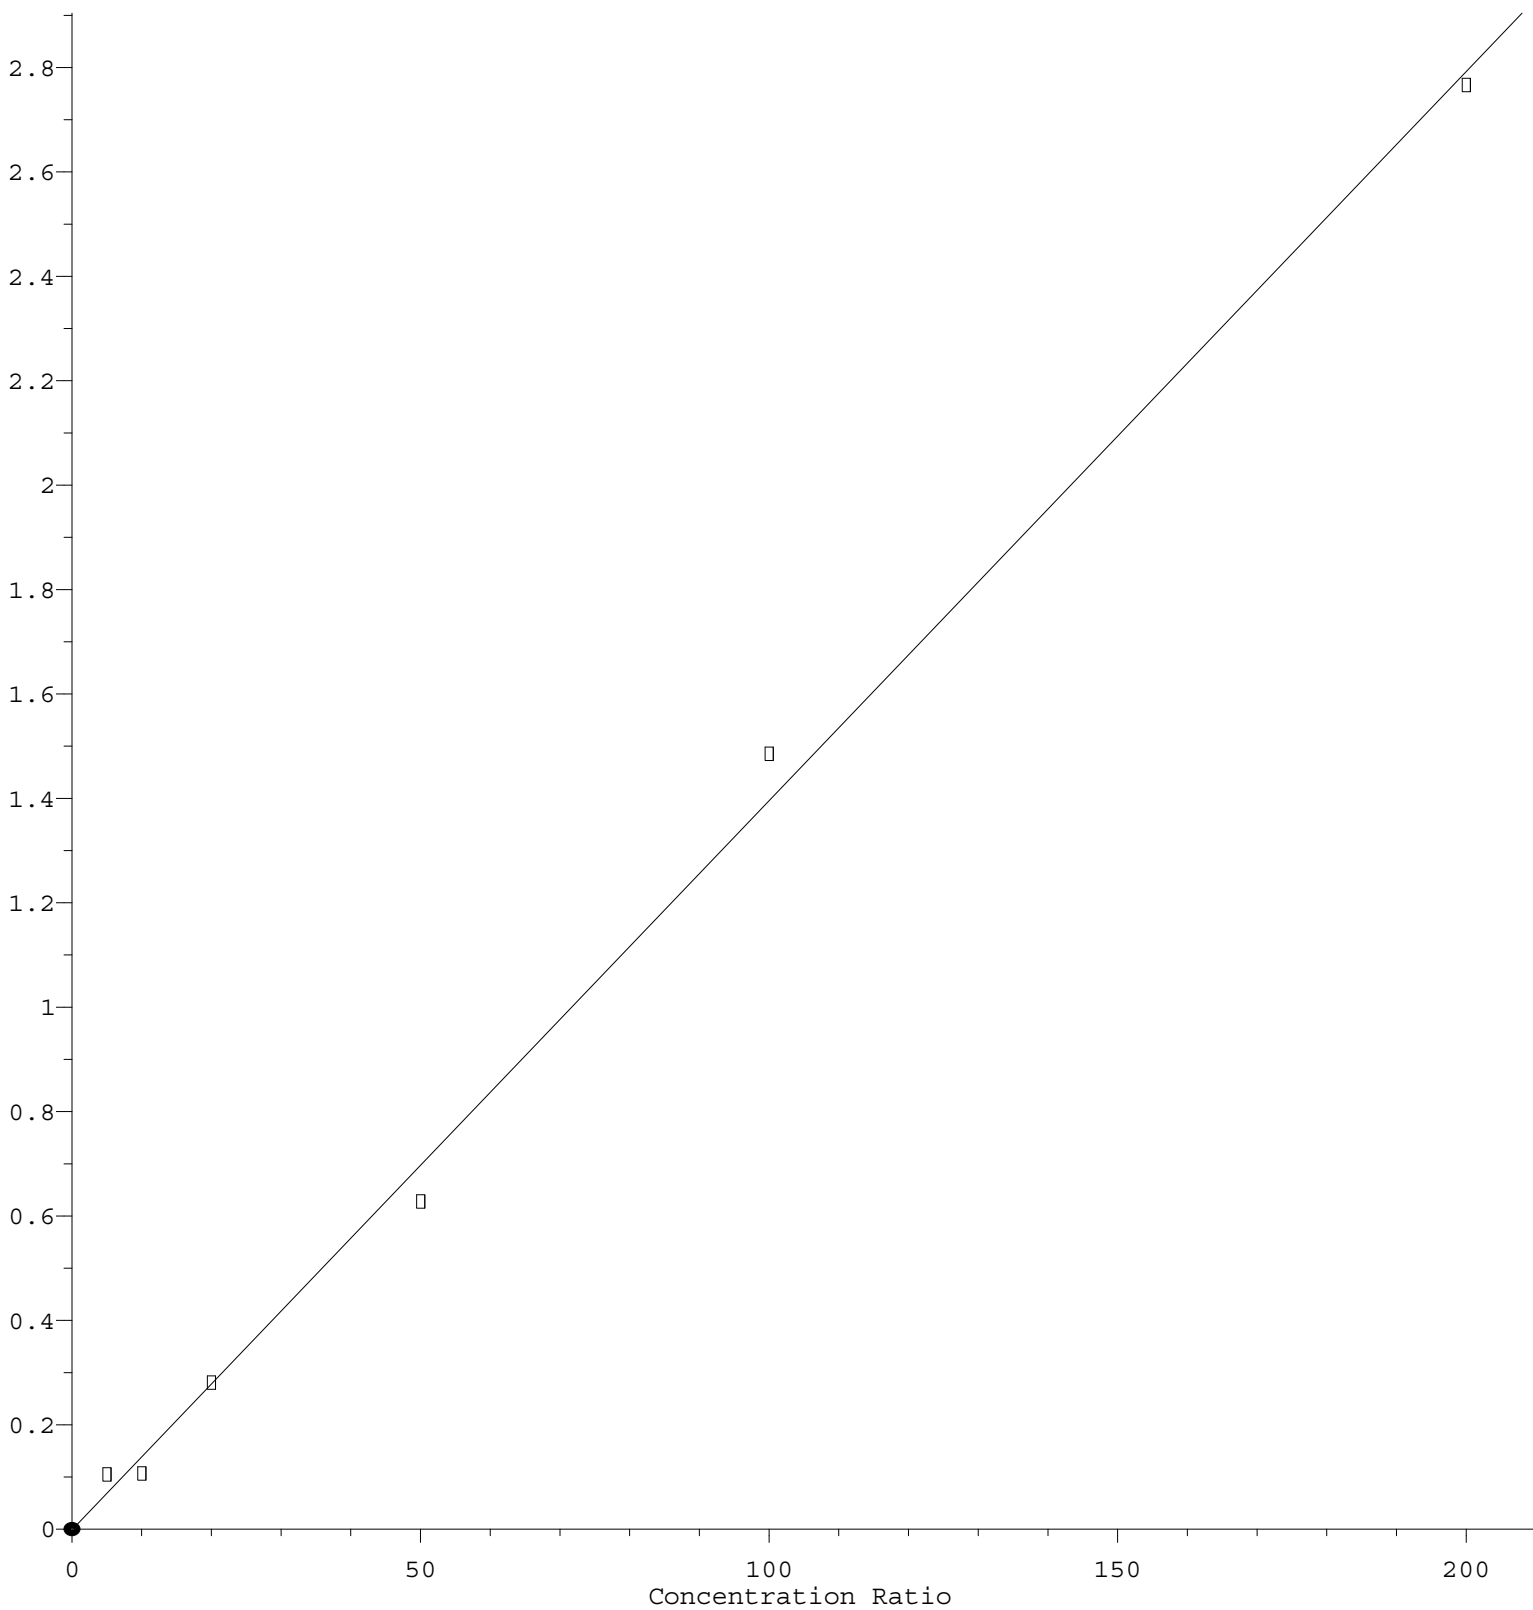

$$\text{Response} = 1.397\text{e-}002 * \text{Amt} - 1.251\text{e-}003$$


Coef of Det (r^2) = 0.997137 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U012821DW.M

Calibration Table Last Updated: Fri Jan 29 09:59:59 2021

Methacrylonitrile

Response Ratio

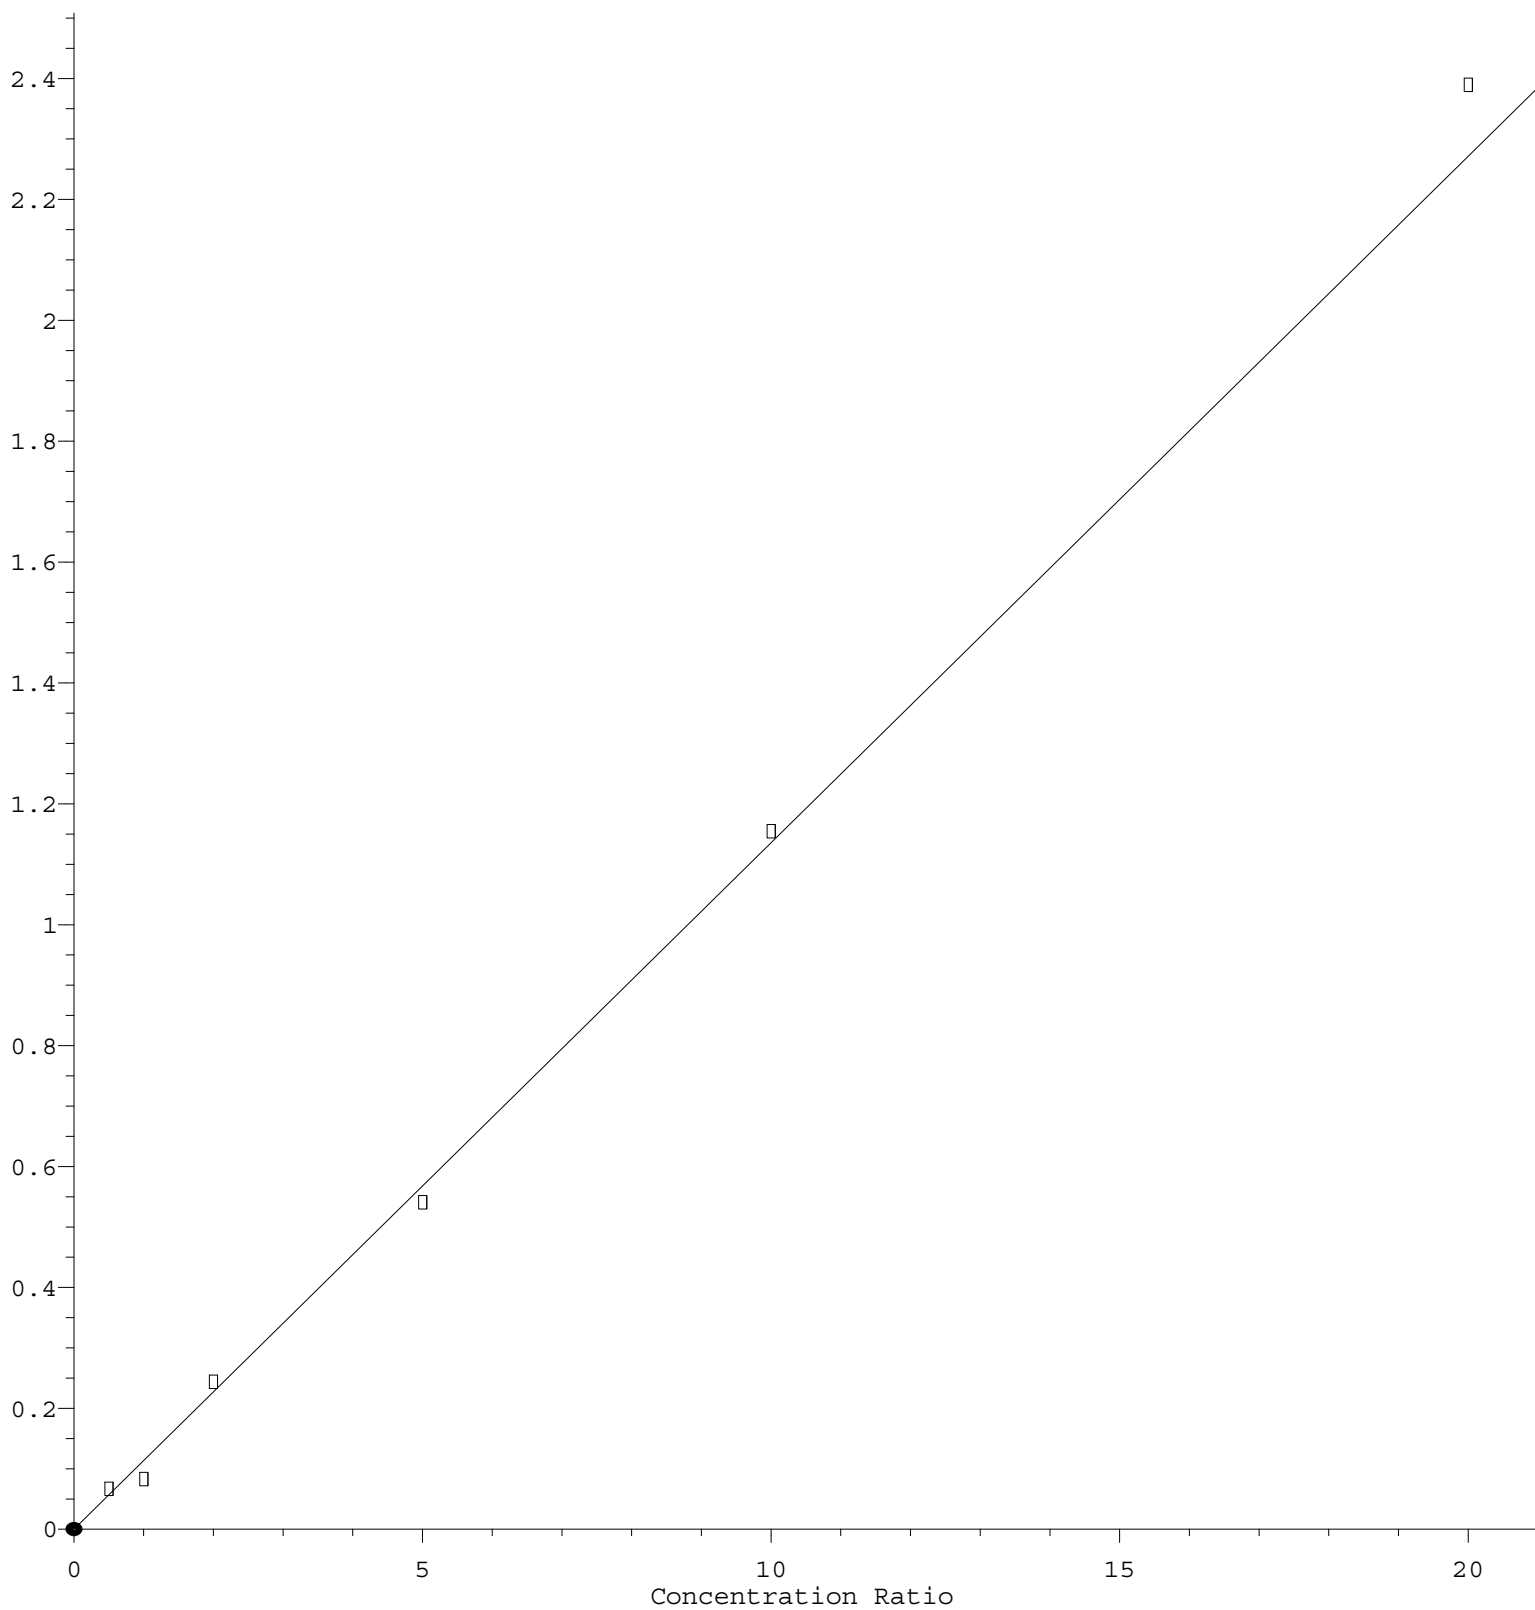

$$\text{Response} = 1.136\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 15.154% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U012821DW.M

Calibration Table Last Updated: Fri Jan 29 09:59:59 2021

Tetrahydrofuran

Response Ratio

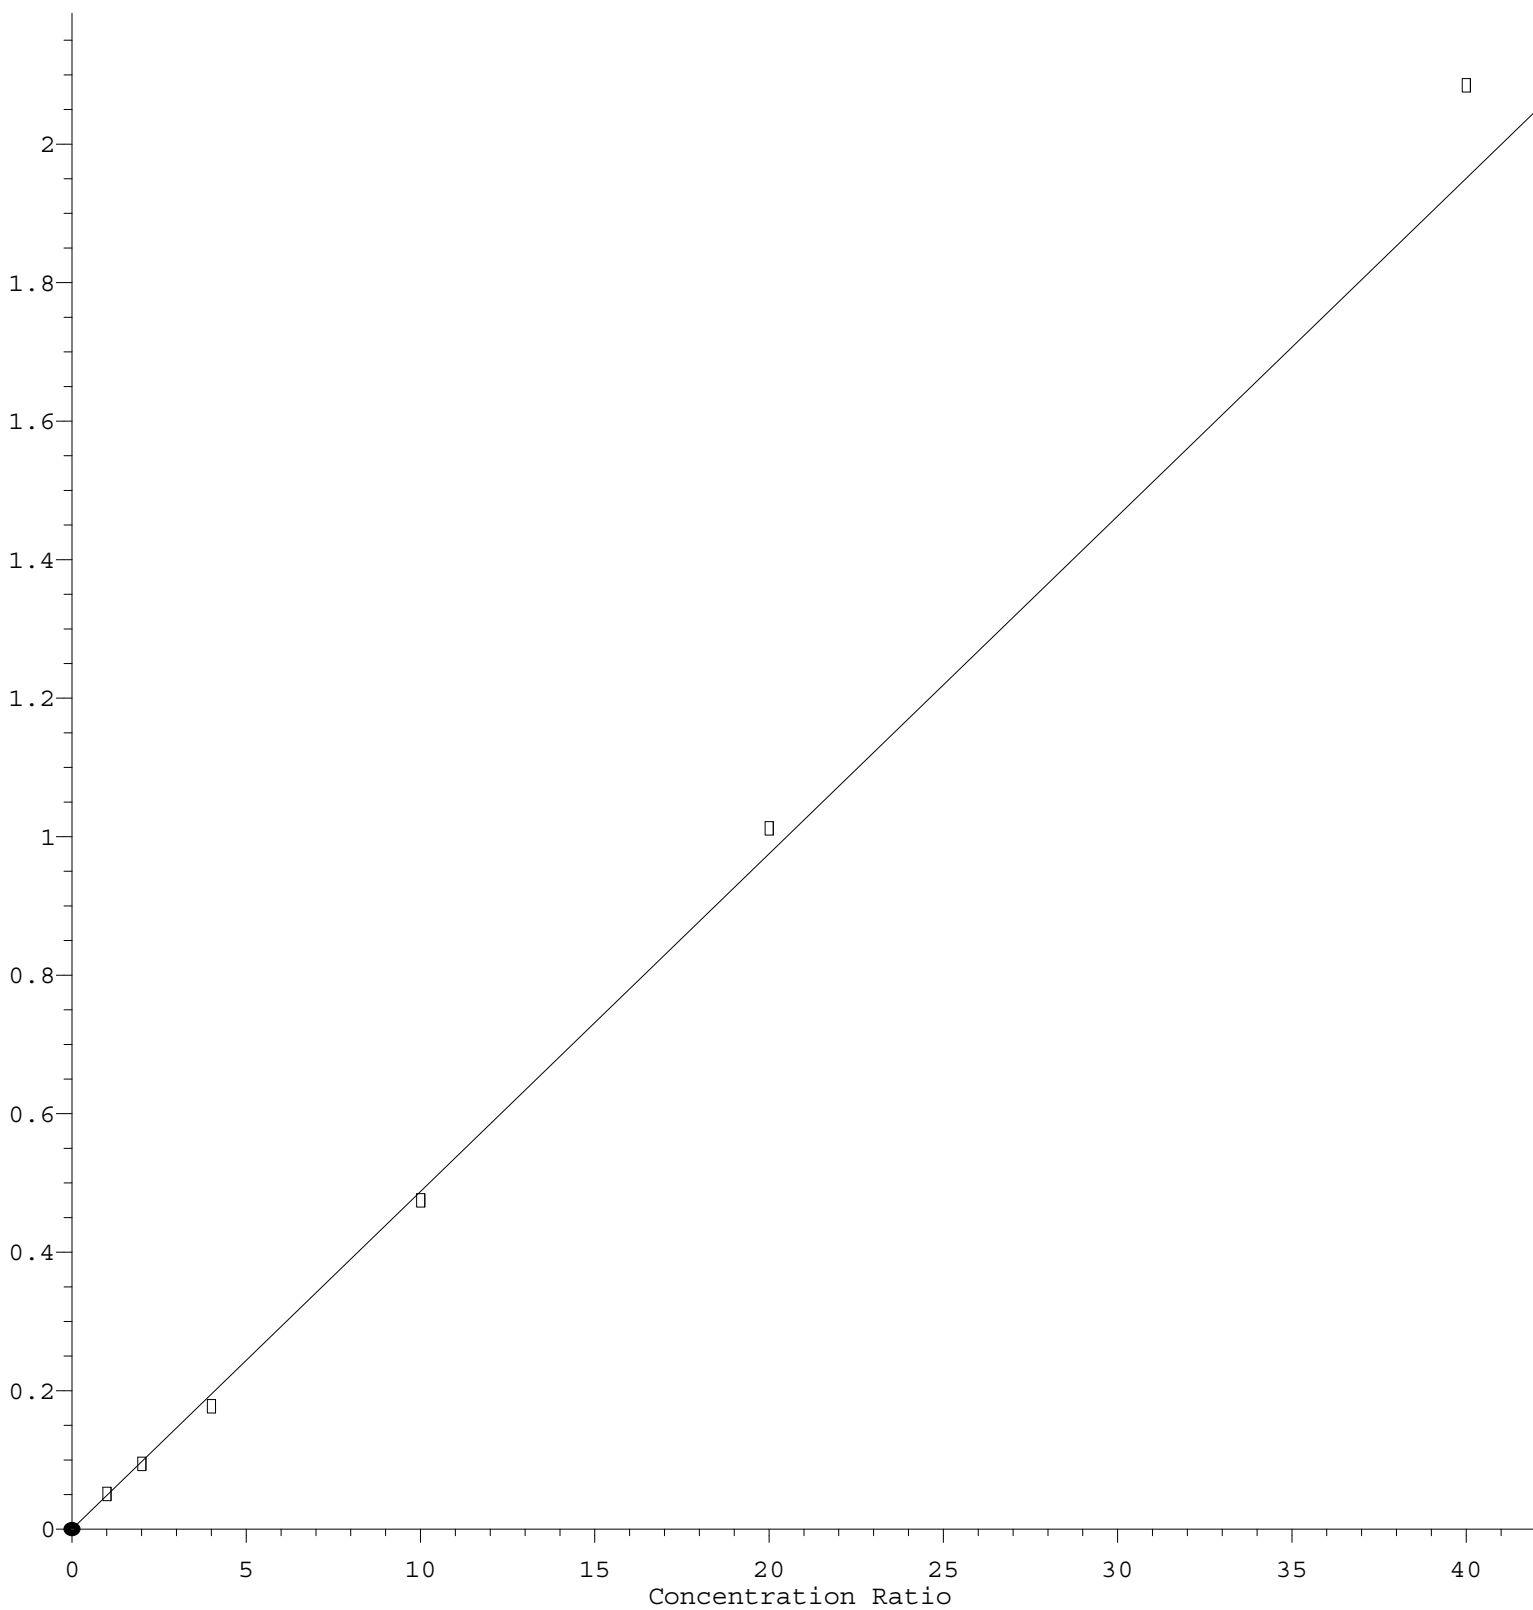

$$\text{Response} = 4.876\text{e-}002 * \text{Amt}$$


RF Rel Std Dev = 5.984% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U012821DW.M

Calibration Table Last Updated: Fri Jan 29 09:59:59 2021

Nitrobenzene

Response Ratio

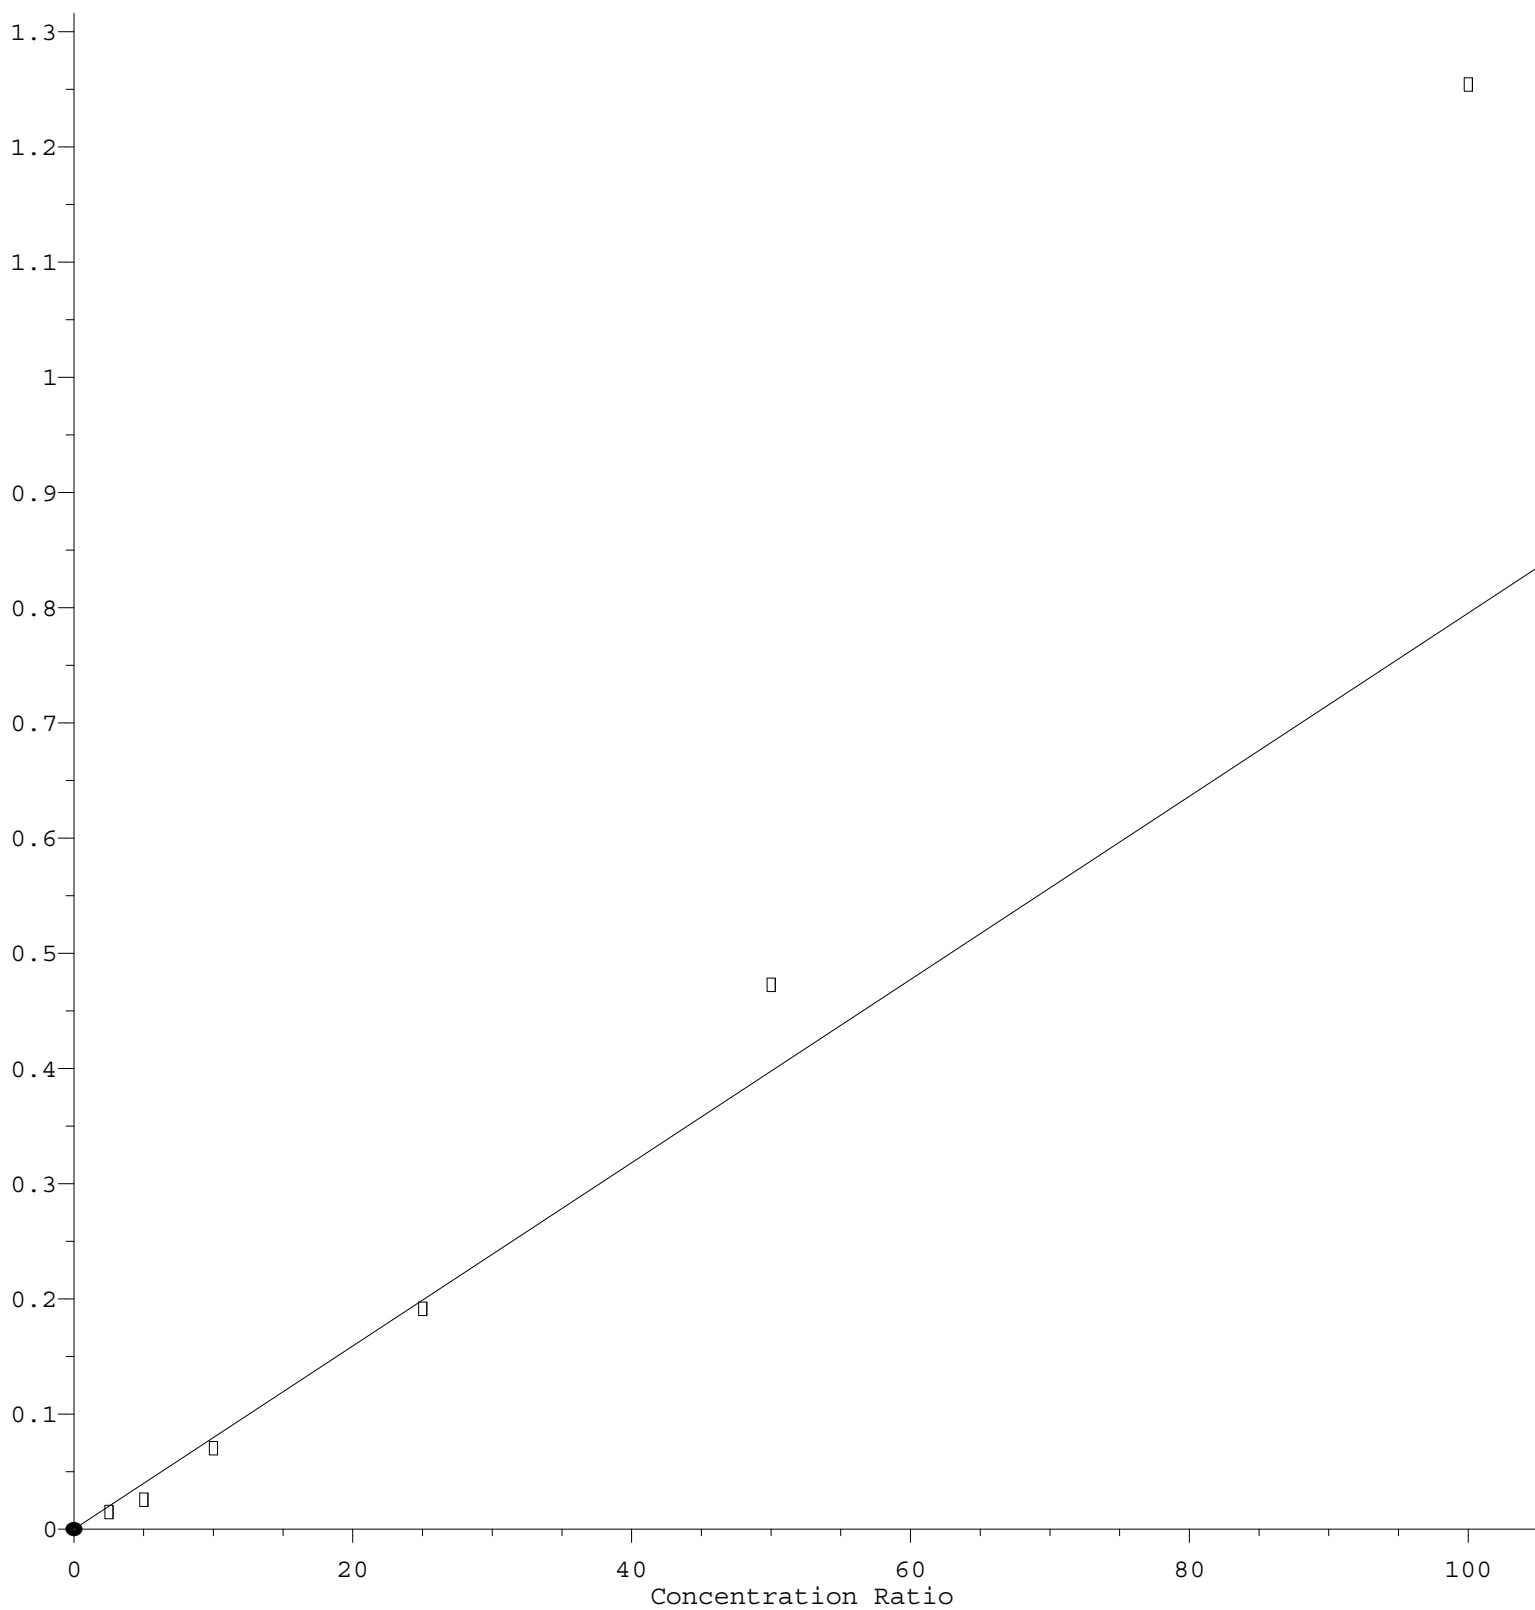

$$\text{Response} = 7.954\text{e-}003 * \text{Amt}$$

RF Rel Std Dev = 33.911% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\524U012821DW.M

Calibration Table Last Updated: Fri Jan 29 09:59:59 2021