




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063064.D
Acq On : 28 Jan 2025 13:53
Operator : MD/SY
Sample : Q1195-13DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2963DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/29/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 29 09:05:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

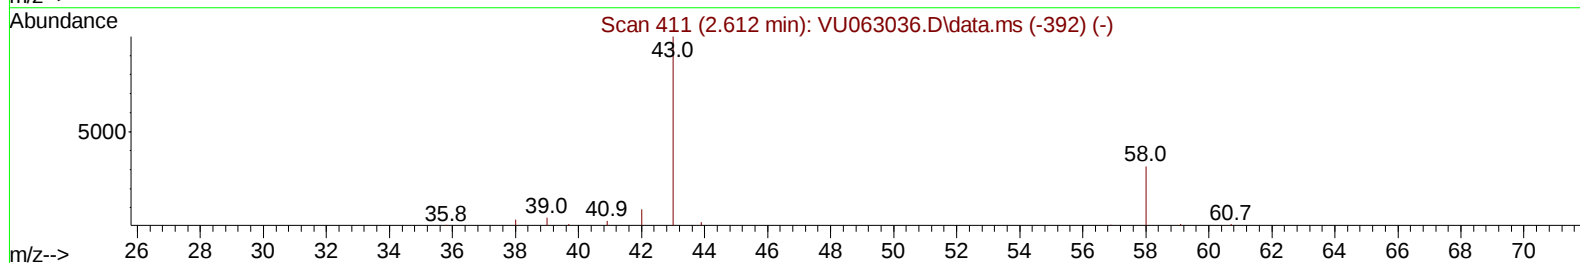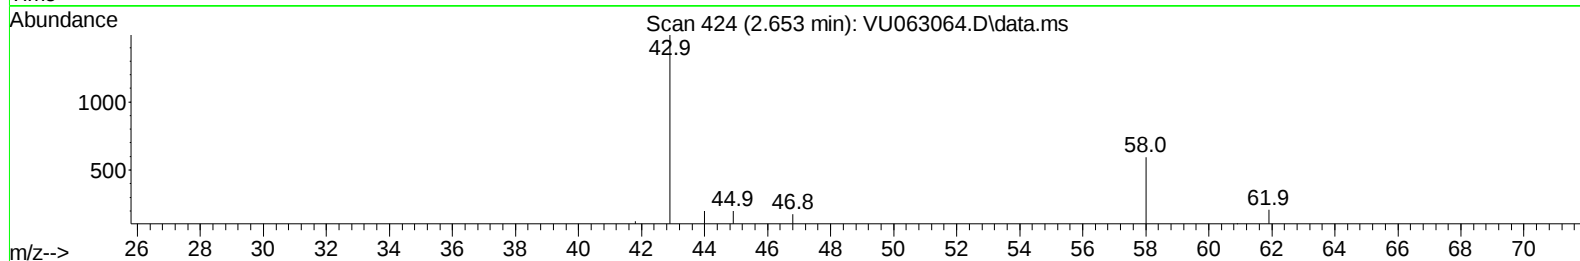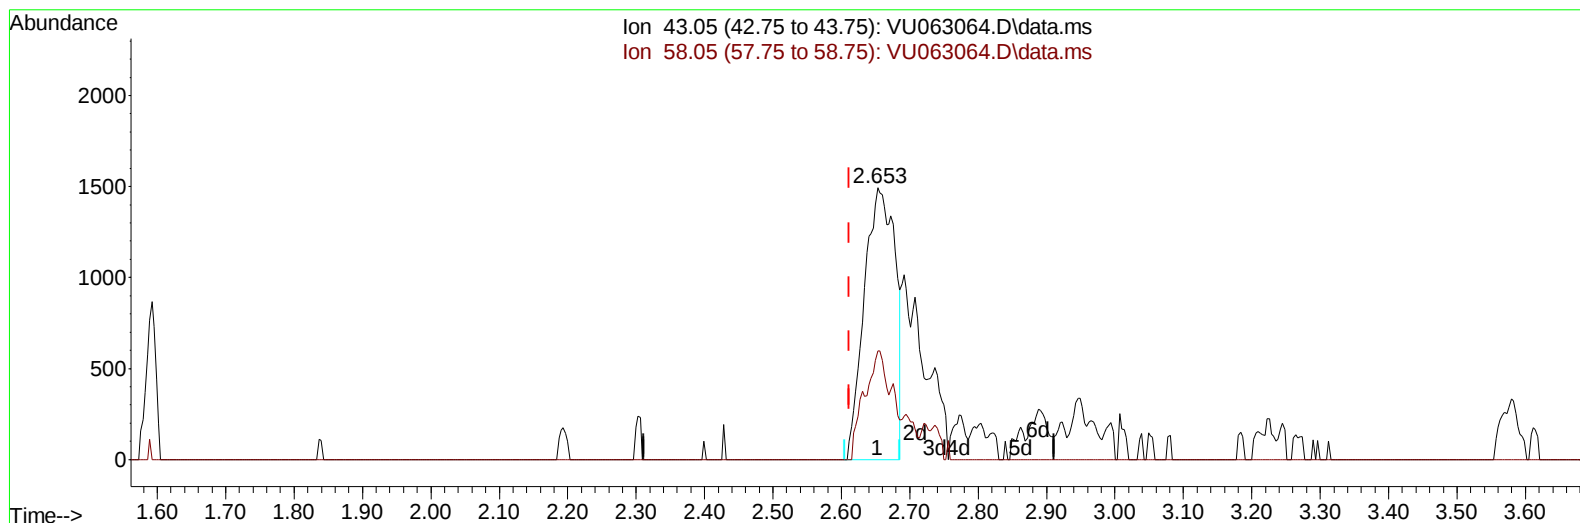

TIC: VU063064.D\data.ms

(13) Acetone (T)

2.653min (+ 0.042) 5.91 ug/L

response 4648

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	28.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063064.D
Acq On : 28 Jan 2025 13:53
Operator : MD/SY
Sample : Q1195-13DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2963DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/29/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 29 09:05:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

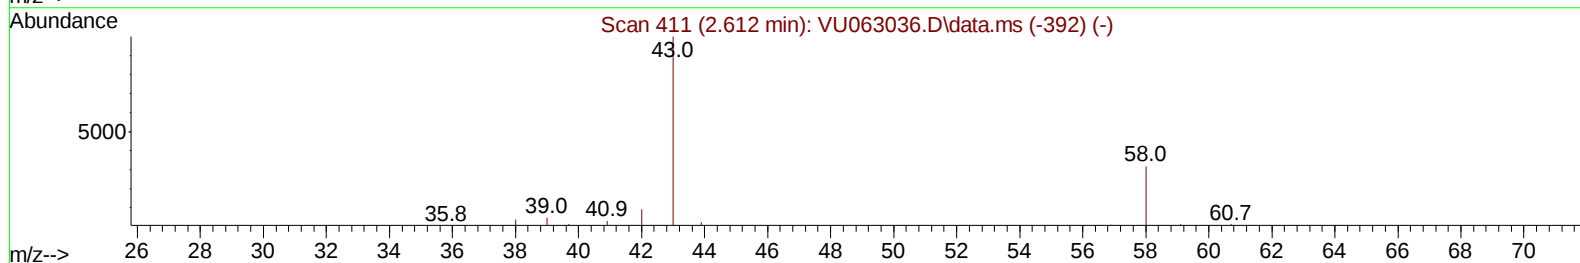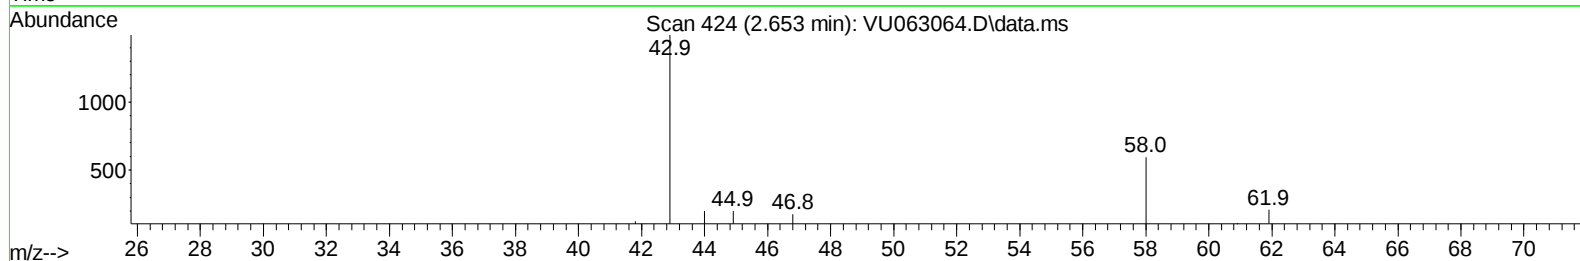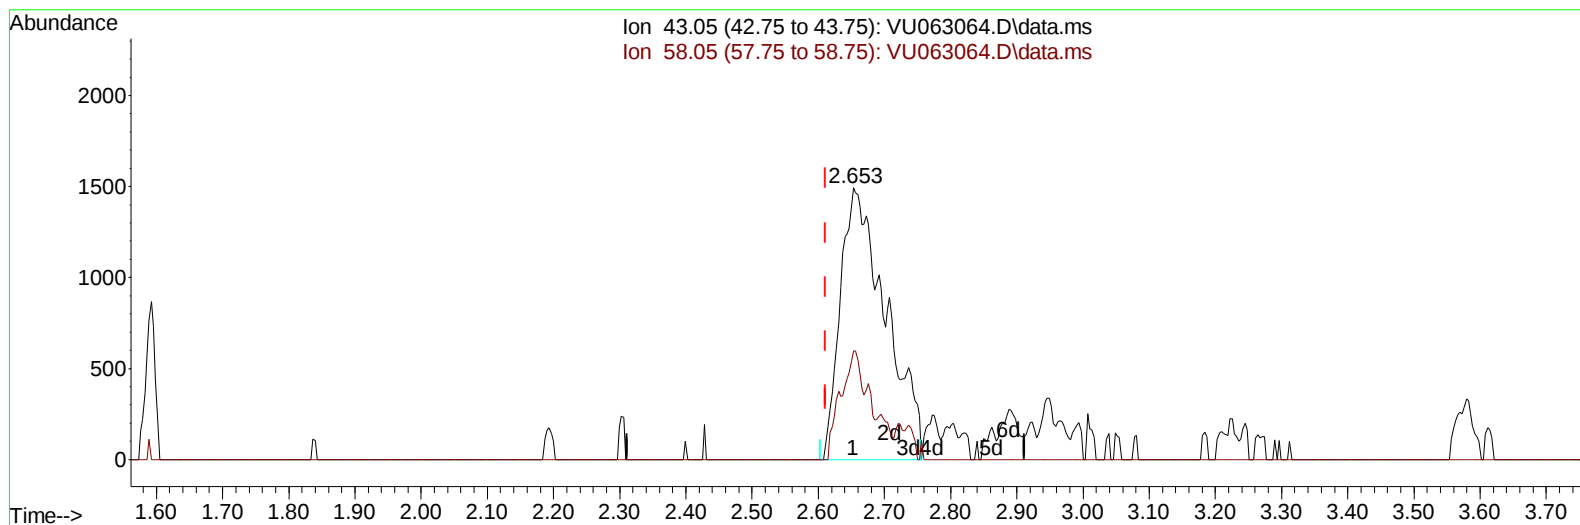

TIC: VU063064.D\data.ms

(13) Acetone (T)

2.653min (+ 0.042) 8.98 ug/L m

response 7062

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.20	18.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
 Data File : VU063064.D
 Acq On : 28 Jan 2025 13:53
 Operator : MD/SY
 Sample : Q1195-13DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2963DL

Manual IntegrationsAPPROVED

Quant Time: Jan 29 09:05:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 08:16:38 2025
 Response via : Initial Calibration

Reviewed By :John Carlone 01/29/2025
 Supervised By :Mahesh Dadoda 01/30/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	116614	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	109745	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	65212	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	14077	3.358	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.901	69	13823	4.343	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	86.800%	
11) 1,1-Dichloroethene-d2	2.550	65	10074	4.018	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	80.400%	
20) 2-Butanone-d5	4.631	46	62164	51.093	ug/L	0.03
Spiked Amount 50.000	Range 40	- 130	Recovery	=	102.180%	
24) Chloroform-d	5.049	84	75144	4.513	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	90.200%	
26) 1,2-Dichloroethane-d4	5.692	65	43342	4.560	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	91.200%	
32) Benzene-d6	5.714	84	119472	4.764	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.676	67	28836	4.516	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	90.400%	
41) Toluene-d8	7.888	98	113060	4.560	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	91.200%	
43) trans-1,3-Dichloroprop...	8.171	79	19061	4.822	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	96.400%	
46) 2-Hexanone-d5	8.624	63	55206	55.970	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	111.940%	
56) 1,1,2,2-Tetrachloroeth...	10.743	84	32697	5.393	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	107.800%	
66) 1,2-Dichlorobenzene-d4	12.183	152	52317	4.482	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	89.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.653	43	7062m	8.977	ug/L	
14) Carbon disulfide	2.782	76	2881	0.186	ug/L	99
40) 4-Methyl-2-pentanone	7.791	43	4299	1.490	ug/L #	74
42) Toluene	7.958	91	36053	1.141	ug/L	93
47) Tetrachloroethene	8.544	164	56955	7.248	ug/L	95
52) Ethylbenzene	9.563	91	13607	0.369	ug/L	97
53) m,p-Xylene	9.682	106	14589	1.026	ug/L	99
54) o-Xylene	10.093	106	8752	0.672	ug/L	92
63) 1,2,4-Trimethylbenzene	11.460	105	11396	0.333	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063064.D
Acq On : 28 Jan 2025 13:53
Operator : MD/SY
Sample : Q1195-13DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2963DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 01/29/2025
Supervised By :Mahesh Dadoda 01/30/2025

Quant Time: Jan 29 09:05:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

