

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
 Data File : VU063070.D
 Acq On : 28 Jan 2025 16:28
 Operator : MD/SY
 Sample : Q1174-18
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2952

Quant Time: Jan 29 09:32:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 08:16:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	109988	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	116676	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	58578	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	14454	3.656	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.200%
7) Chloroethane-d5	1.904	69	12289	4.094	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.800%
11) 1,1-Dichloroethene-d2	2.554	65	8734	3.694	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.800%
20) 2-Butanone-d5	4.608	46	56486	49.224	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.440%
24) Chloroform-d	5.049	84	64907	4.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	5.692	65	39762	4.435	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%
32) Benzene-d6	5.714	84	100789	3.780	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.600%
36) 1,2-Dichloropropane-d6	6.676	67	28206	4.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.000%
41) Toluene-d8	7.888	98	105022	3.984	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.171	79	17396	4.139	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.800%
46) 2-Hexanone-d5	8.621	63	53056	50.595	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.180%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	32031	4.969	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%
66) 1,2-Dichlorobenzene-d4	12.183	152	51246	4.887	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.800%
Target Compounds					Qvalue	
13) Acetone	2.615	43	7664	10.329	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063070.D
Acq On : 28 Jan 2025 16:28
Operator : MD/SY
Sample : Q1174-18
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2952


Quant Time: Jan 29 09:32:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

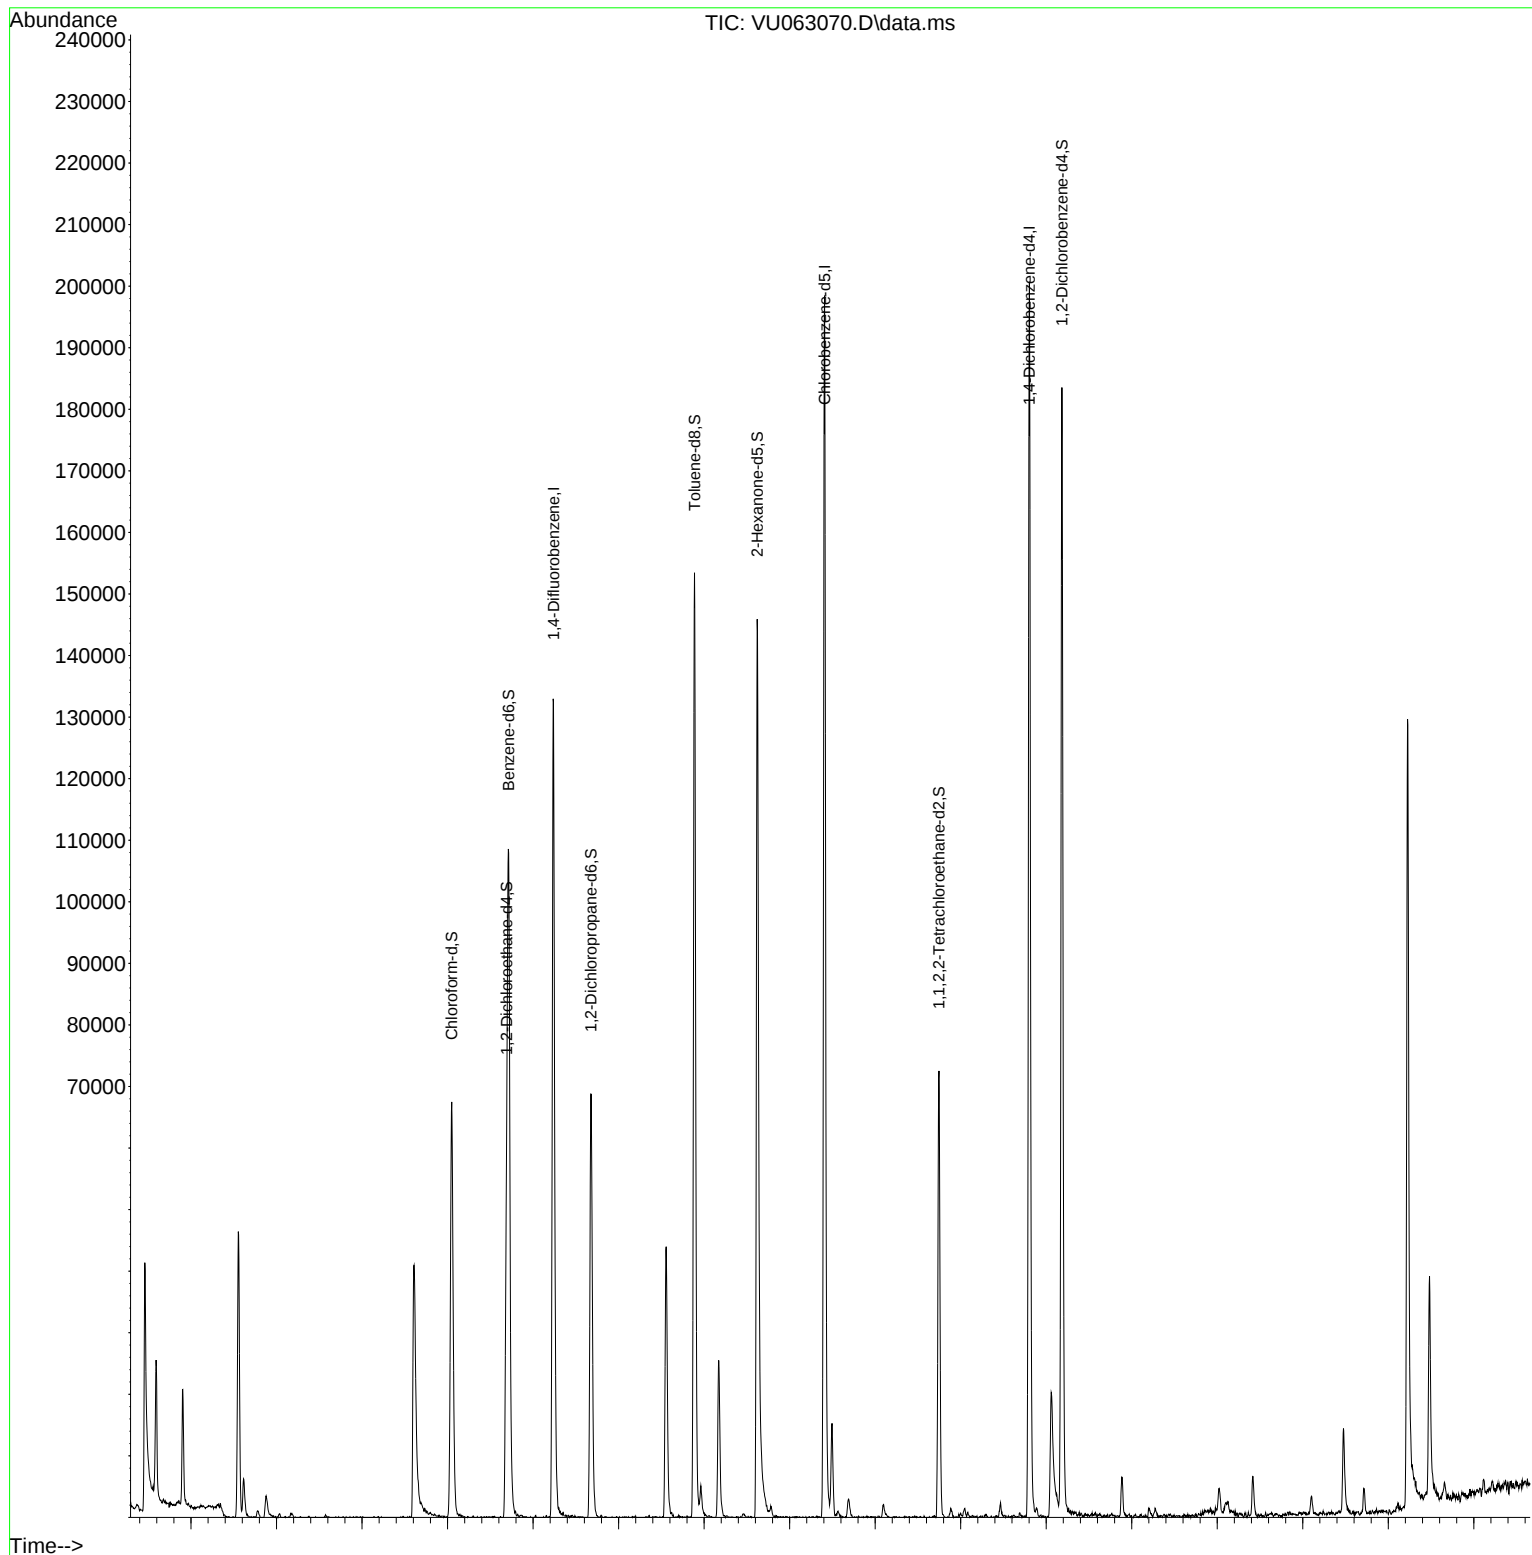

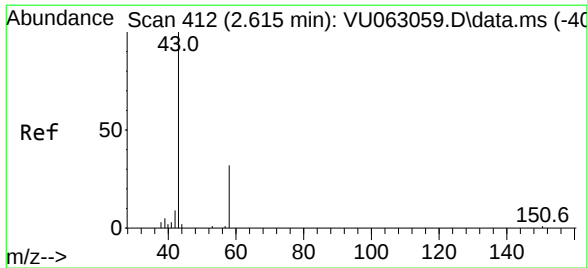

#13
 Acetone
 Concen: 10.329 ug/L
 RT: 2.615 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU063070.D
 Acq: 28 Jan 2025 16:28

Instrument :
 MSVOA_U
 ClientSampleId :
 E2952

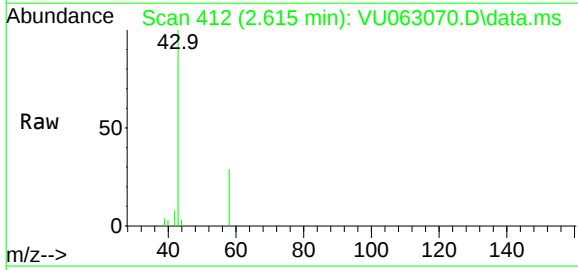

Tgt Ion: 43 Resp: 7664
 Ion Ratio Lower Upper
 43 100
 58 26.1 0.0 64.4

