

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
 Data File : VU063076.D
 Acq On : 28 Jan 2025 18:58
 Operator : MD/SY
 Sample : Q1195-18
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E2969

Quant Time: Jan 29 09:47:59 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jan 29 08:16:38 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	103491	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	105449	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	61531	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	13256	3.563	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.200%
7) Chloroethane-d5	1.904	69	10685	3.783	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.600%
11) 1,1-Dichloroethene-d2	2.554	65	8134	3.656	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	4.608	46	54271	50.262	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.520%
24) Chloroform-d	5.049	84	58348	3.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.000%
26) 1,2-Dichloroethane-d4	5.689	65	35741	4.237	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.800%
32) Benzene-d6	5.714	84	91420	3.794	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.800%
36) 1,2-Dichloropropane-d6	6.676	67	24600	4.009	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.200%
41) Toluene-d8	7.888	98	93142	3.909	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.200%
43) trans-1,3-Dichloroprop...	8.171	79	15474	4.074	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.621	63	51332	54.162	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.320%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	28667	4.921	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	12.184	152	50344	4.571	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.400%
Target Compounds					Qvalue	
13) Acetone	2.615	43	7793	11.162	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063076.D
Acq On : 28 Jan 2025 18:58
Operator : MD/SY
Sample : Q1195-18
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E2969

Quant Time: Jan 29 09:47:59 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jan 29 08:16:38 2025
Response via : Initial Calibration

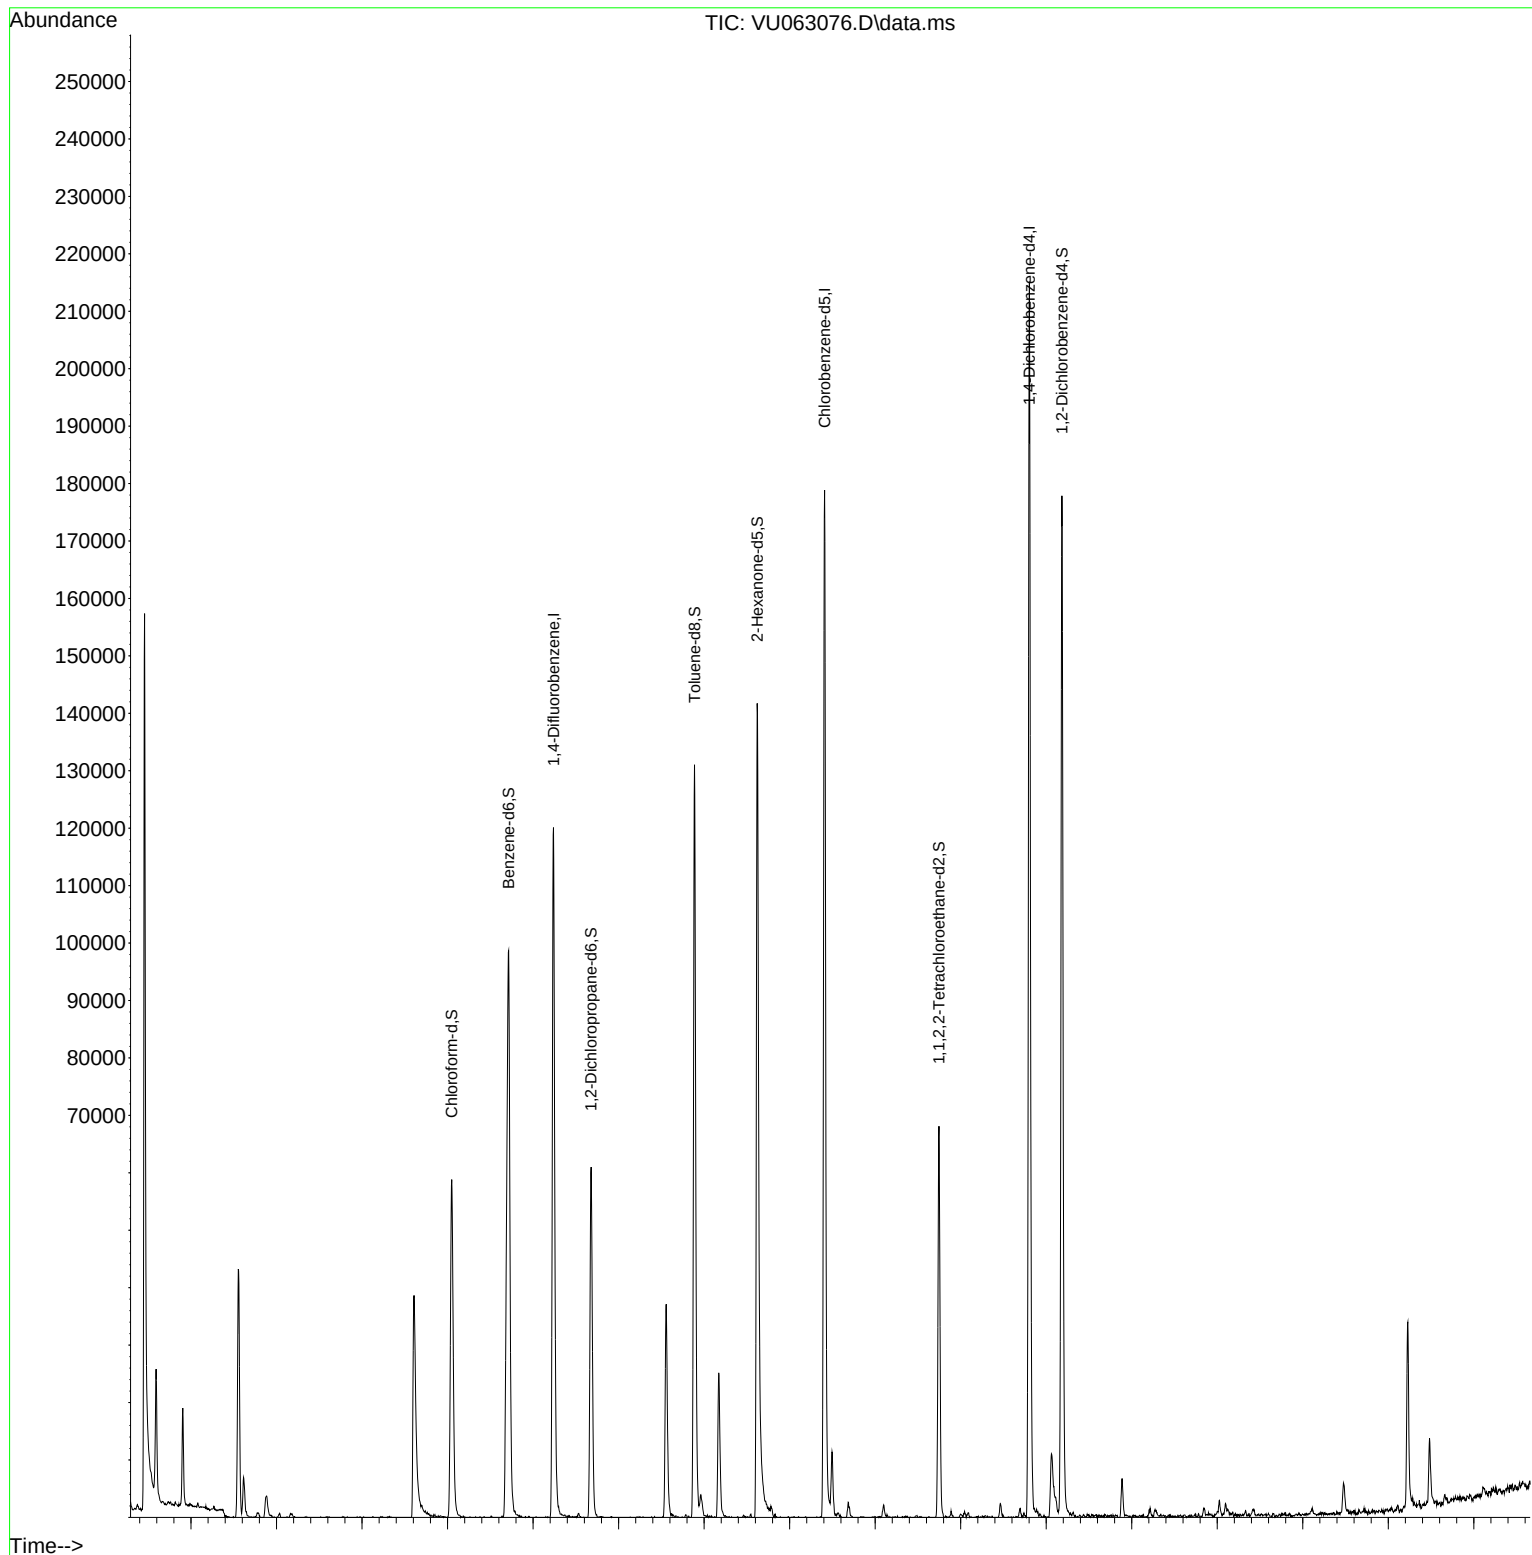

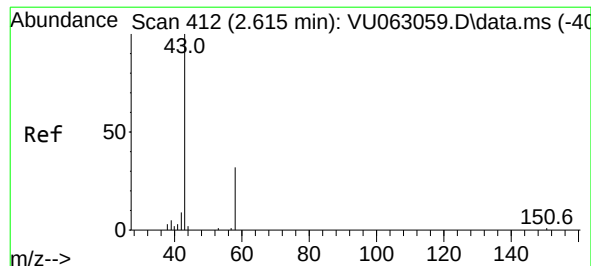

#13
 Acetone
 Concen: 11.162 ug/L
 RT: 2.615 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU063076.D
 Acq: 28 Jan 2025 18:58

Instrument :
 MSVOA_U
 ClientSampleId :
 E2969

Tgt Ion: 43 Resp: 7793
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 64.4

