
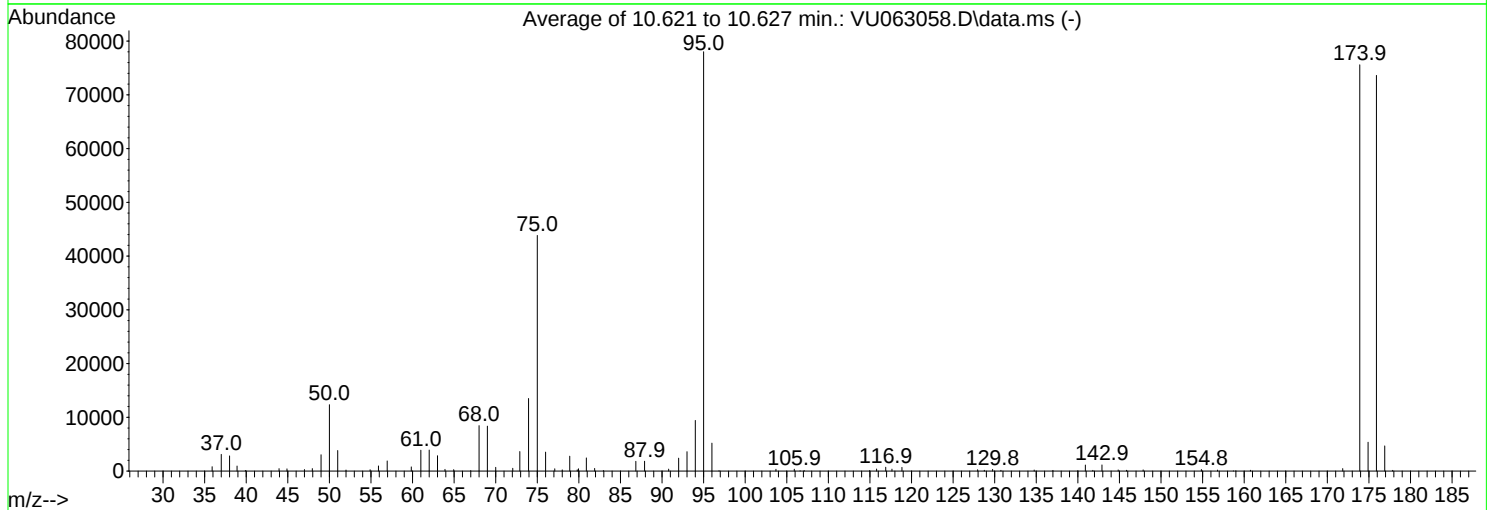


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU012825\
Data File : VU063058.D
Acq On : 28 Jan 2025 10:00
Operator : MD/SY
Sample : BFB069
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB069

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR012725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jan 30 07:33:13 2025

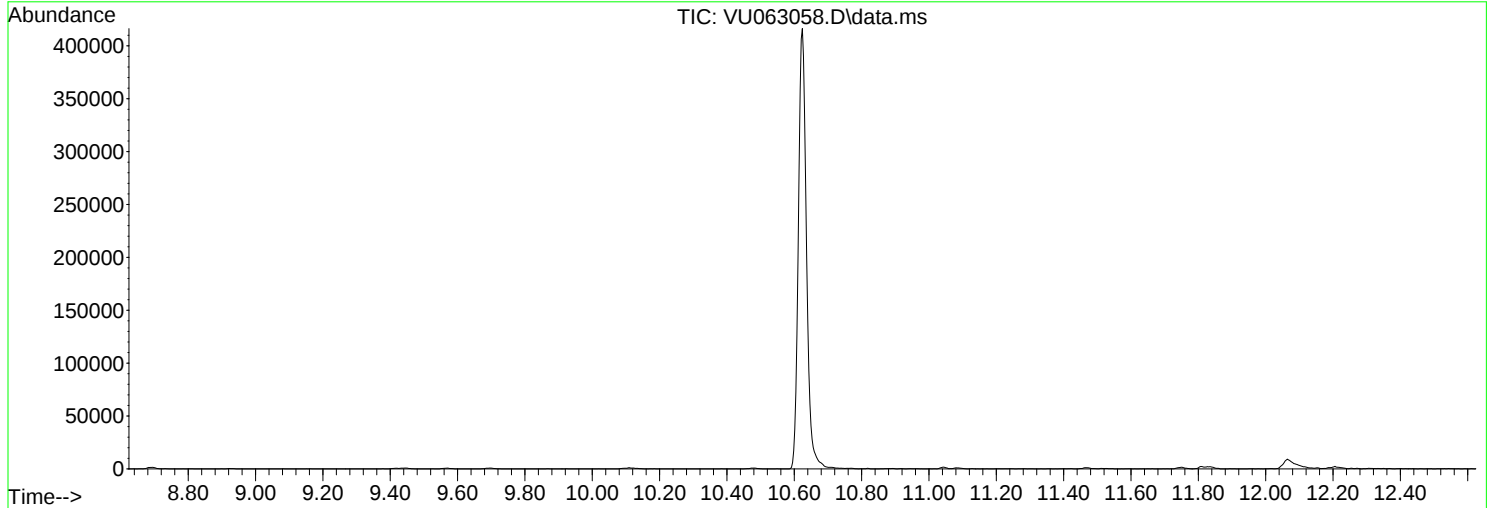

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	12355	PASS
75	95	30	80	56.2	43843	PASS
95	95	100	100	100.0	78024	PASS
96	95	5	9	6.7	5196	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.9	75592	PASS
175	174	5	9	7.1	5366	PASS
176	174	95	101	97.4	73621	PASS
177	176	5	9	6.4	4679	PASS

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB069

m/z	Abundance
35.90	831.0
37.00	3317.0
38.00	2773.0
38.90	931.0
39.90	102.0
44.00	384.0
44.80	438.0
47.00	301.0
48.00	490.0
49.00	3186.0
50.00	12784.0
51.00	3851.0
52.00	204.0
54.90	283.0
55.90	955.0
56.90	1973.0
59.80	696.0
61.00	3845.0
62.00	4083.0
63.00	2973.0
63.80	381.0
65.00	299.0
68.00	8481.0
69.00	8351.0
70.00	623.0
72.10	455.0
72.90	3736.0
74.00	13742.0
75.00	44928.0
76.00	3613.0
77.10	438.0
78.00	255.0
78.90	2664.0
79.80	712.0
80.90	2546.0
81.90	461.0
83.00	147.0
86.80	1699.0
87.90	1861.0
90.80	370.0
92.00	2533.0
93.00	3632.0
94.00	9736.0
95.00	78304.0
96.00	5073.0
96.80	117.0
103.70	394.0
105.90	292.0
106.60	101.0
114.90	129.0
115.80	376.0
116.90	692.0
117.70	344.0
118.90	657.0
128.00	258.0
128.80	146.0
129.70	352.0
130.70	157.0
134.70	198.0
136.90	159.0
140.90	1195.0
141.80	129.0
142.90	1136.0
144.80	253.0
145.80	156.0
147.80	280.0
154.80	288.0
156.70	184.0
159.00	114.0
160.70	138.0
171.80	443.0
173.90	75128.0
174.90	5177.0
175.90	73128.0
176.90	4635.0
177.80	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	836.0
37.00	3220.0
38.00	2925.0
38.90	994.0
39.90	124.0
44.00	470.0
44.90	407.0
46.90	294.0
47.90	490.0
49.00	3118.0
50.00	12697.0
51.00	3884.0
52.00	215.0
54.90	244.0
55.90	969.0
57.00	1930.0
59.90	800.0
61.00	3992.0
62.00	4036.0
63.00	2940.0
63.90	295.0
64.90	274.0
68.00	8718.0
69.00	8499.0
70.00	745.0
72.00	534.0
72.90	3805.0
74.00	13796.0
75.00	44944.0
76.00	3555.0
77.10	447.0
78.00	231.0
78.90	2917.0
80.00	688.0
80.90	2464.0
81.90	488.0
82.90	119.0
86.90	1874.0
87.90	1908.0
90.80	400.0
92.00	2458.0
93.00	3644.0
94.00	9756.0
95.00	80520.0
96.00	5389.0
96.90	112.0
103.70	353.0
105.90	364.0
106.60	100.0
107.10	107.0
115.00	112.0
115.80	416.0
116.90	784.0
117.70	391.0
118.80	721.0
127.90	254.0
128.80	149.0
129.70	315.0
130.80	138.0
134.70	216.0
137.00	118.0
140.00	132.0
140.90	1153.0
141.80	139.0
142.90	1150.0
144.80	225.0
145.90	149.0
147.80	229.0
154.90	310.0
156.80	182.0
160.80	167.0
171.80	479.0
173.90	77984.0
174.90	5479.0
175.90	75808.0
176.90	4824.0
177.80	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	776.0
37.00	2781.0
38.00	2767.0
38.90	898.0
39.90	125.0
43.90	524.0
45.00	400.0
47.10	256.0
47.90	417.0
49.00	2810.0
50.00	11585.0
51.00	3729.0
52.00	176.0
54.90	225.0
55.90	964.0
57.00	1767.0
59.90	837.0
61.00	3815.0
62.00	3608.0
63.00	2657.0
64.00	289.0
64.90	236.0
67.00	215.0
68.00	8173.0
69.00	8242.0
70.00	722.0
72.00	563.0
72.90	3367.0
73.90	12996.0
75.00	41656.0
76.00	3420.0
77.10	408.0
78.00	192.0
78.90	2734.0
79.90	612.0
80.90	2338.0
81.90	525.0
86.90	1870.0
87.90	1729.0
90.80	339.0
92.00	2220.0
93.00	3540.0
94.00	8776.0
95.00	75248.0
96.00	5127.0
103.70	289.0
105.90	388.0
107.10	142.0
115.80	372.0
116.90	672.0
117.60	374.0
118.80	682.0
127.90	244.0
128.70	148.0
129.80	276.0
130.70	135.0
134.80	195.0
137.10	106.0
140.90	1027.0
141.80	150.0
142.90	1135.0
144.90	176.0
145.90	157.0
147.90	180.0
154.90	294.0
156.90	188.0
158.70	110.0
160.80	157.0
171.90	470.0
173.90	73664.0
174.90	5442.0
175.90	71928.0
176.90	4577.0
177.90	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069