


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU012919\
Data File : VU029302.D
Acq On : 29 Jan 2019 15:23
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U012919DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Jan 30 09:13:14 2019

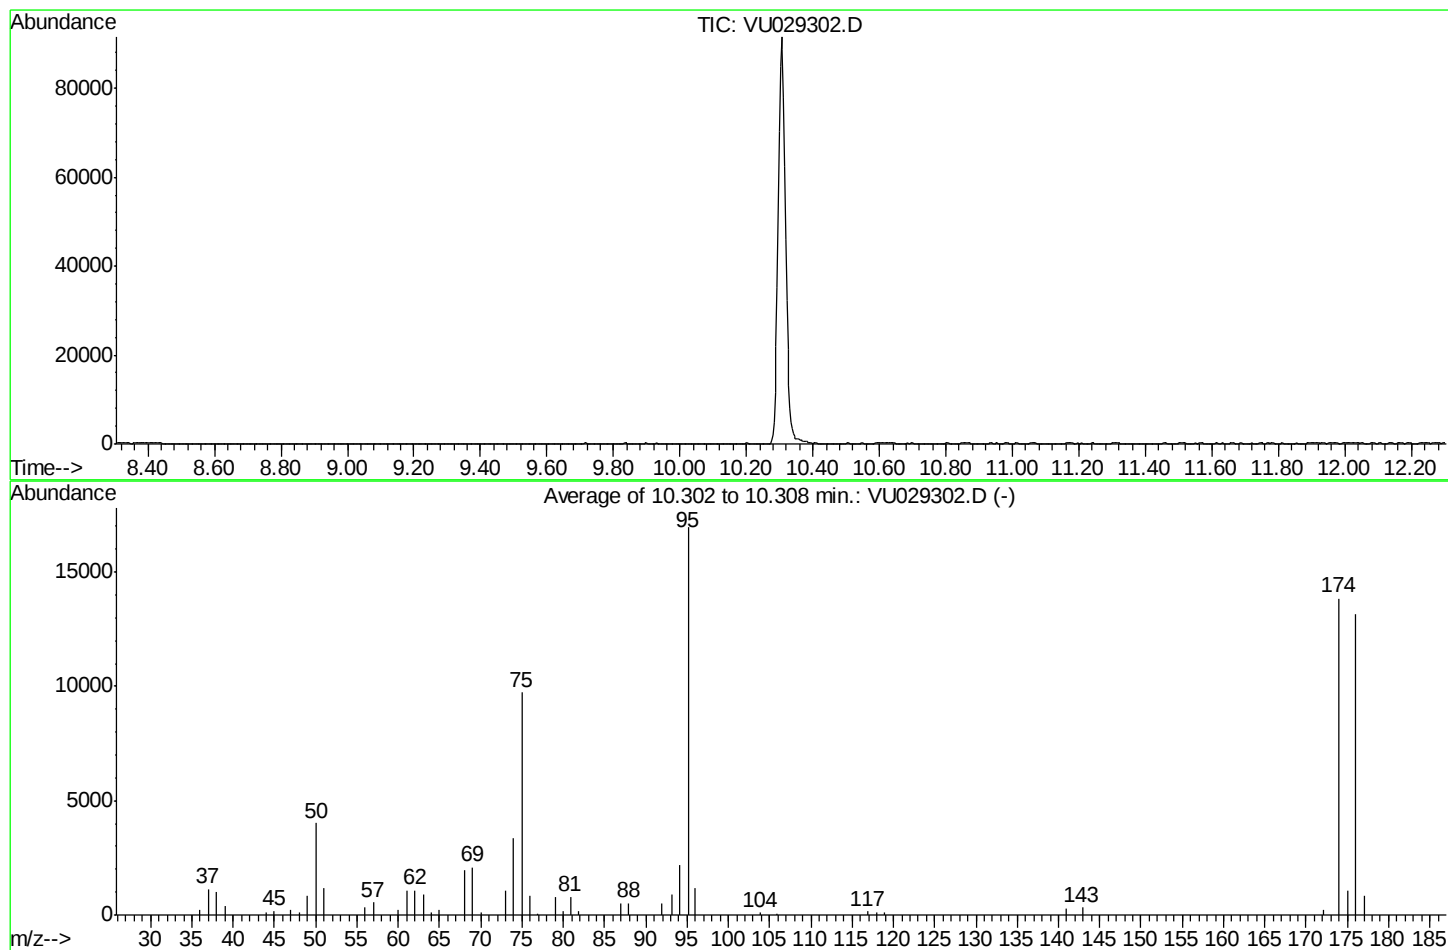

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	4019	PASS
75	95	30	60	57.4	9726	PASS
95	95	100	100	100.0	16951	PASS
96	95	5	9	6.8	1157	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.6	13838	PASS
175	174	5	9	7.7	1061	PASS
176	174	95	101	95.1	13155	PASS
177	176	5	9	6.6	869	PASS