

Data File : VU036602.D
Acq On : 29 Jan 2020 18:57
Operator : JC/MD
Sample : L1271-04
Misc : 5.10g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GASZ5

Quant Time: Jan 30 02:52:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 30 02:48:11 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	298786	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	292509	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	165163	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	83458	37.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.58%
7) Chloroethane-d5	1.89	69	21084	10.98	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	21.96%#
11) 1,1-Dichloroethene-d2	2.56	63	111367	30.78	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.56%
21) 2-Butanone-d5	4.69	46	116299	87.55	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.55%
24) Chloroform-d	5.11	84	149450	40.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.56%
26) 1,2-Dichloroethane-d4	5.74	65	97233	42.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.14%
32) Benzene-d6	5.76	84	347334	42.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.42%
36) 1,2-Dichloropropane-d6	6.73	67	109242	42.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.22%
41) Toluene-d8	7.93	98	341819	43.18	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.36%
43) trans-1,3-Dichloropropene-	8.21	79	53883	44.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.38%
47) 2-Hexanone-d5	8.68	63	138313	116.33	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.33%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	182676	48.46	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.92%
64) 1,2-Dichlorobenzene-d4	12.21	152	150887	42.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.14%

Target Compounds


						Qvalue
15) Methyl Acetate	2.99	43	1895	0.943	ug/L	91
35) Methylcyclohexane	6.73	83	25116	6.690	ug/L #	21
37) 1,2-Dichloropropane	6.73	63	10783	4.851	ug/L #	87
39) cis-1,3-Dichloropropene	7.60	75	3017	0.842	ug/L #	62
42) Toluene	8.00	91	22710	2.389	ug/L	97
52) Ethylbenzene	9.60	91	24904	2.392	ug/L	97
53) m,p-Xylene	9.72	106	110306	27.159	ug/L	99
54) o-xylene	10.13	106	108615	26.810	ug/L	99
55) Styrene	10.14	104	104691	15.924	ug/L	94
59) 1,2,3-Trichloropropane	11.83	75	18266	6.079	ug/L	88
66) 1,2-Dibromo-3-chloropropan	12.99	75	3120	3.440	ug/L #	6
69) Naphthalene	14.10	128	4454001	561.152	ug/L	99
70) 1,2,3-Trichlorobenzene	14.37	180	4958	1.754	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU036602.D
Acq On : 29 Jan 2020 18:57
Operator : JC/MD
Sample : L1271-04
Misc : 5.10g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GASZ5

Quant Time: Jan 30 02:52:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM012920WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 30 02:48:11 2020
Response via : Initial Calibration




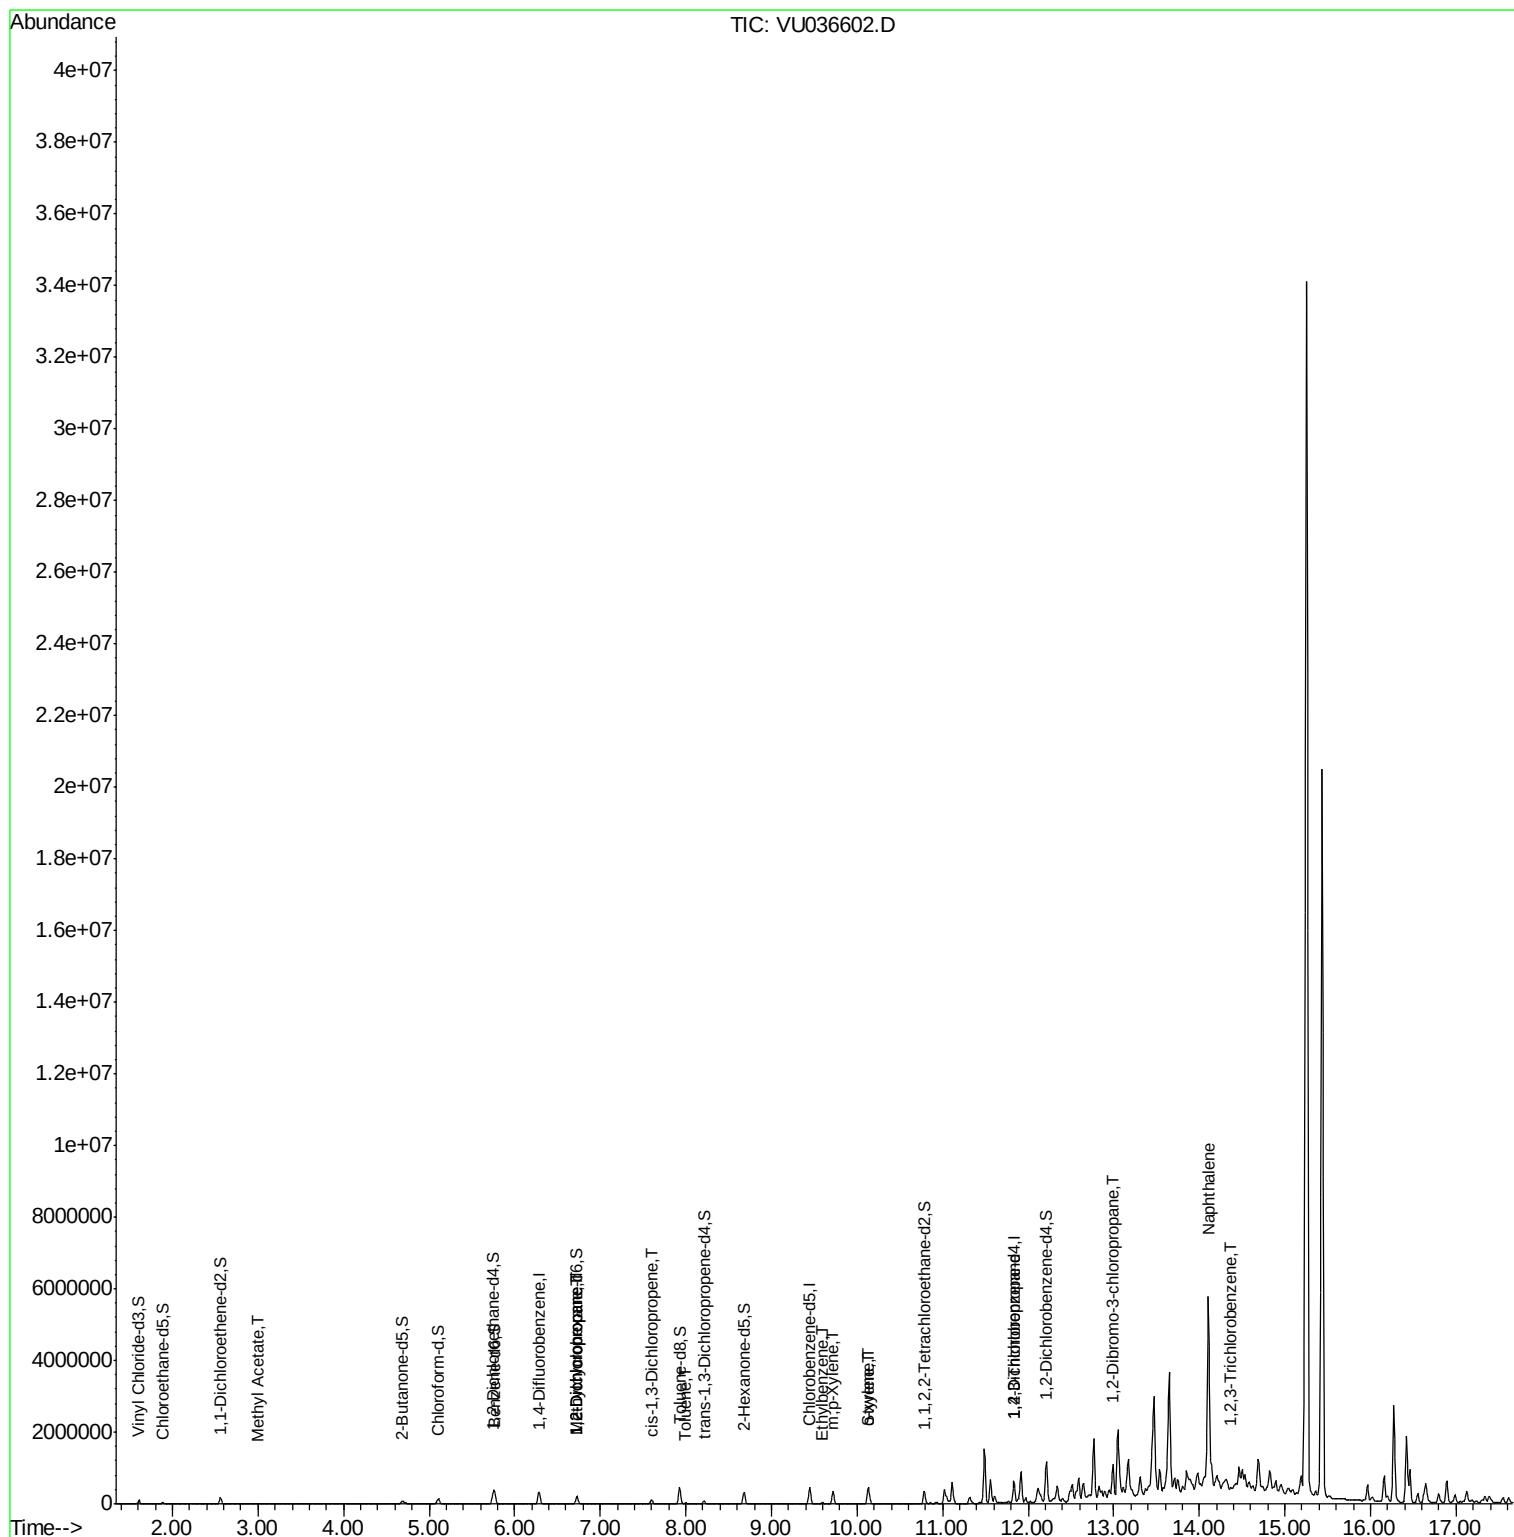


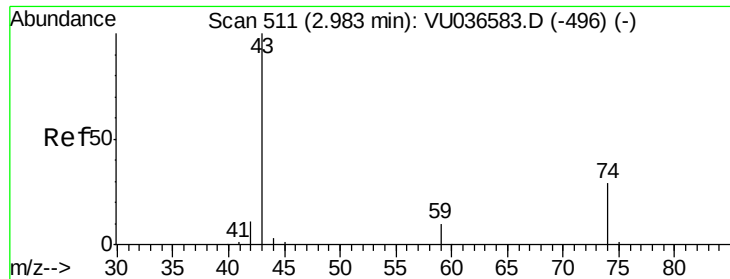

#15
Methyl Acetate
Concen: 0.943 ug/L
RT: 2.99 min Scan# 514
Delta R.T. 0.01 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57




Instrument :
MSVOA_U
ClientSampleId :
GASZ5


Tgt Ion: 43 Resp: 1895
Ion Ratio Lower Upper
43 100
74 24.5 23.3 34.9

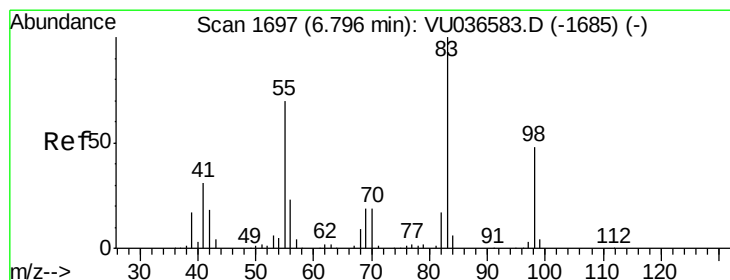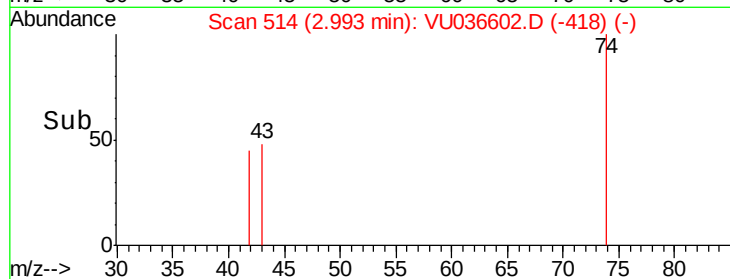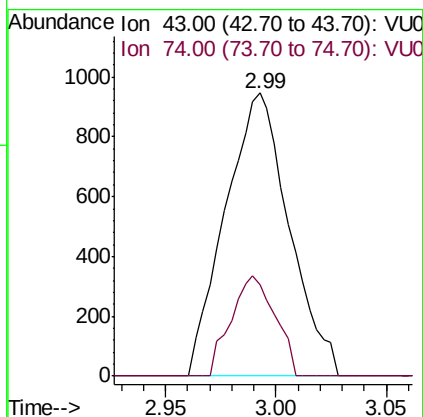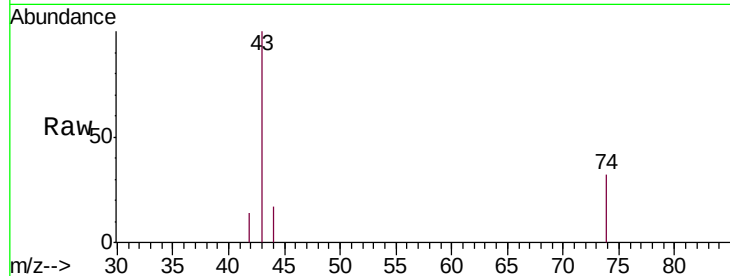

#35
Methylcyclohexane
Concen: 6.690 ug/L
RT: 6.73 min Scan# 1675
Delta R.T. -0.07 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57

Tgt Ion: 83 Resp: 25116
Ion Ratio Lower Upper
83 100
55 0.0 56.1 84.1#
98 1.2 37.5 56.3#


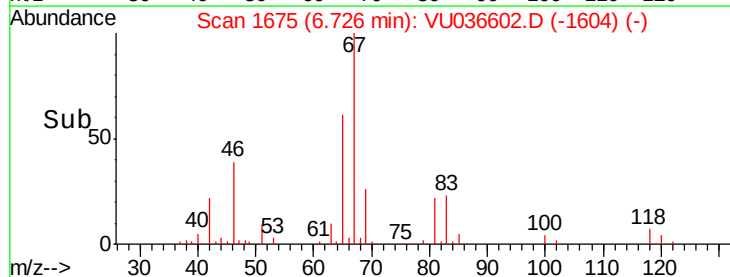
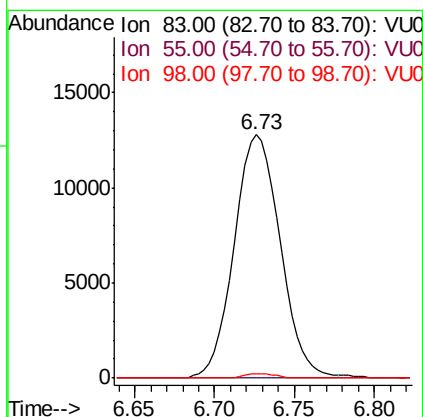
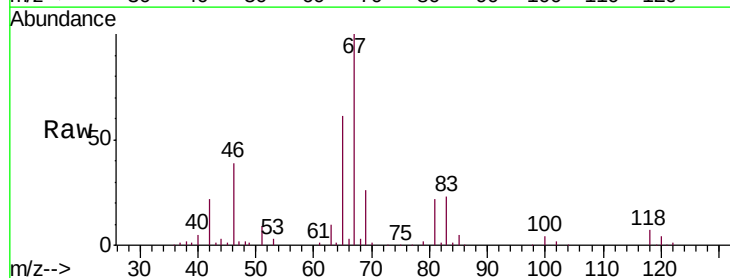


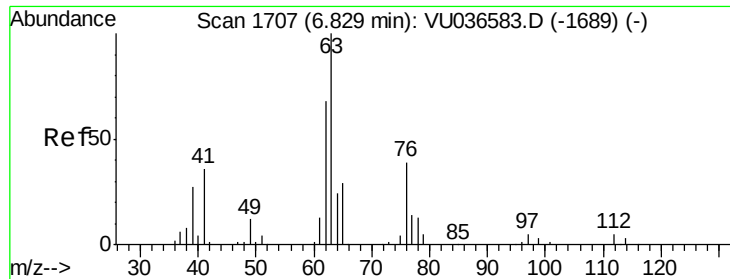

#37
 1,2-Dichloropropane
 Concen: 4.851 ug/L
 RT: 6.73 min Scan# 1676
 Delta R.T. -0.10 min
 Lab File: VU036602.D
 Acq: 29 Jan 2020 18:57




Instrument :
 MSVOA_U
 ClientSampleId :
 GASZ5


Tgt Ion: 63 Resp: 10783
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.4 5.2#

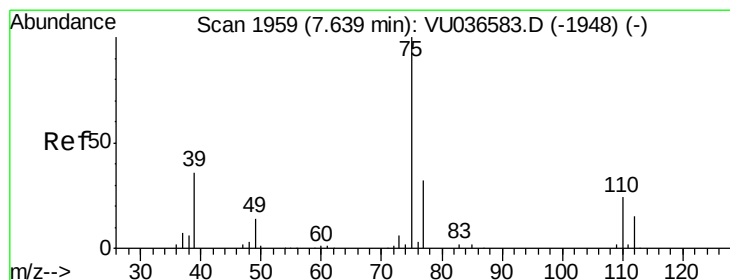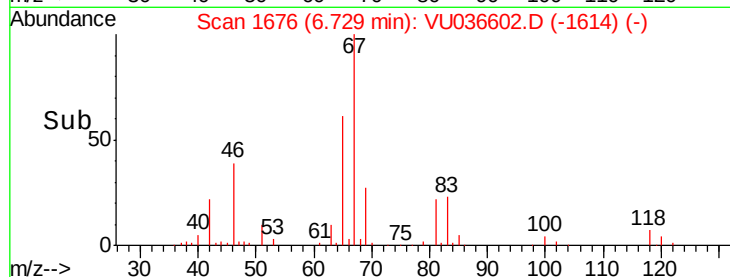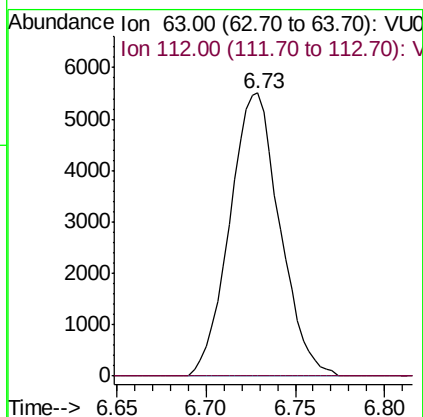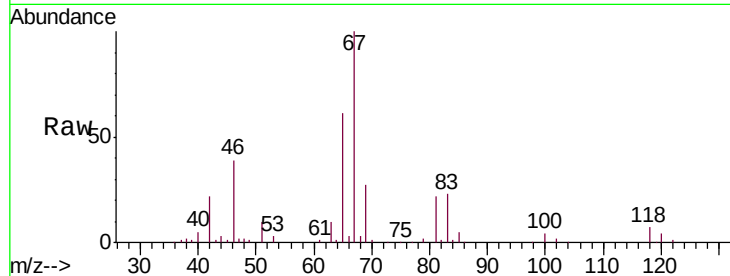

#39
 cis-1,3-Dichloropropene
 Concen: 0.842 ug/L
 RT: 7.60 min Scan# 1947
 Delta R.T. -0.04 min
 Lab File: VU036602.D
 Acq: 29 Jan 2020 18:57

Tgt Ion: 75 Resp: 3017
 Ion Ratio Lower Upper
 75 100
 77 53.3 22.5 41.9#

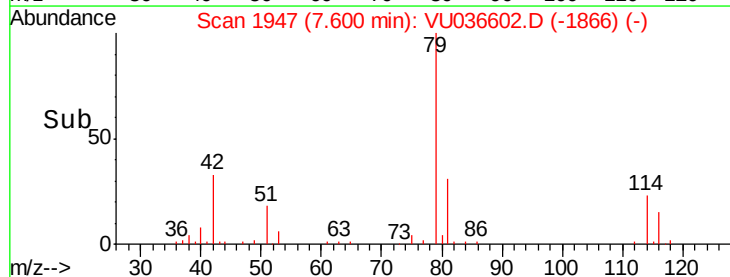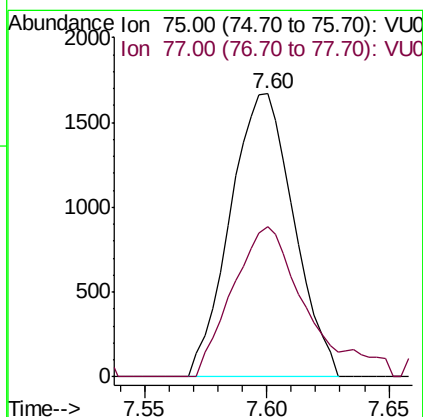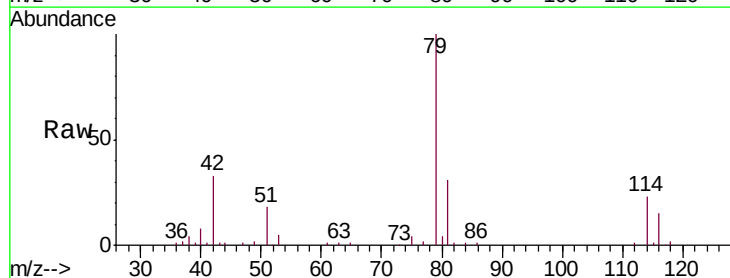

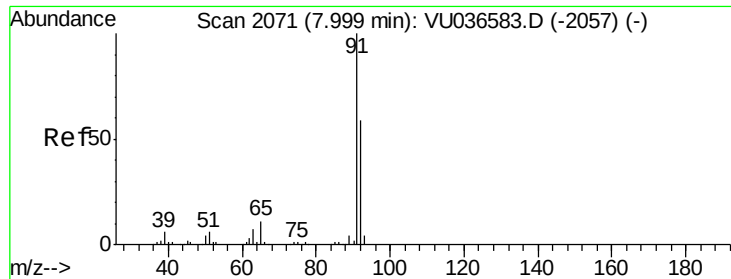

#42

Toluene

Concen: 2.389 ug/L

RT: 8.00 min Scan# 2071

Delta R.T. 0.00 min

Lab File: VU036602.D

Acq: 29 Jan 2020 18:57

Instrument :

MSVOA_U

ClientSampled :


GASZ5

Tgt Ion: 91 Resp: 22710




Ion Ratio Lower Upper

91 100

92 54.7 39.9 74.1

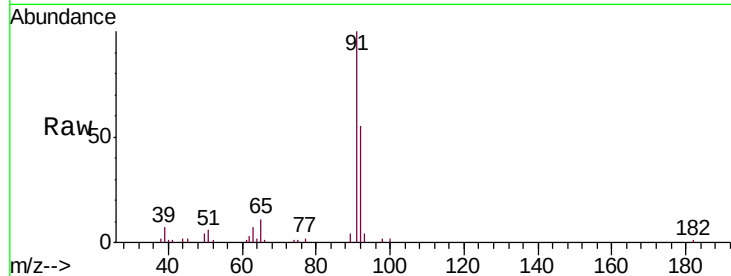

Abundance Ion 91.00 (90.70 to 91.70): VU036602.D (-1978) (-)

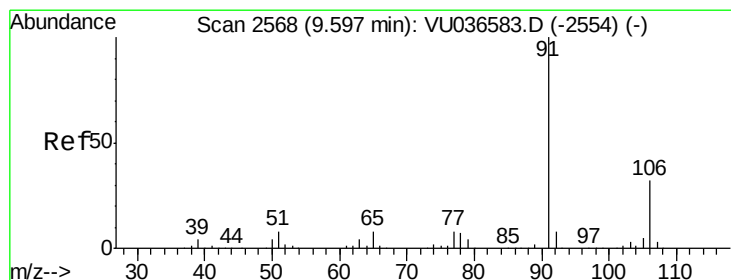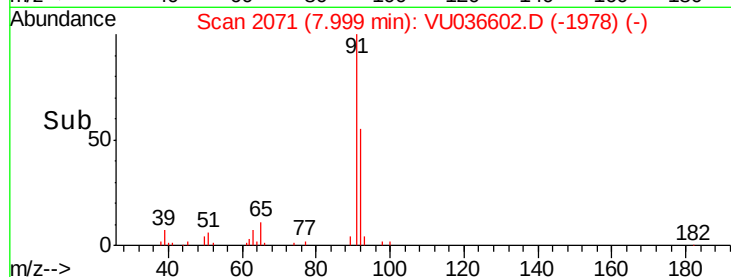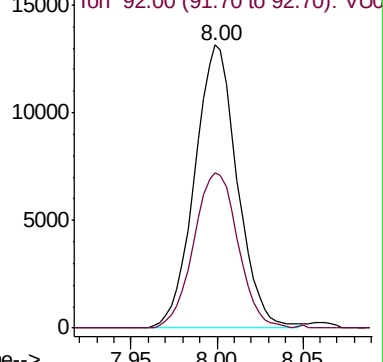

#52

Ethylbenzene

Concen: 2.392 ug/L

RT: 9.60 min Scan# 2568

Delta R.T. 0.00 min

Lab File: VU036602.D


Acq: 29 Jan 2020 18:57

Tgt Ion: 91 Resp: 24904



Ion Ratio Lower Upper


91 100

106 30.7 22.6 42.0

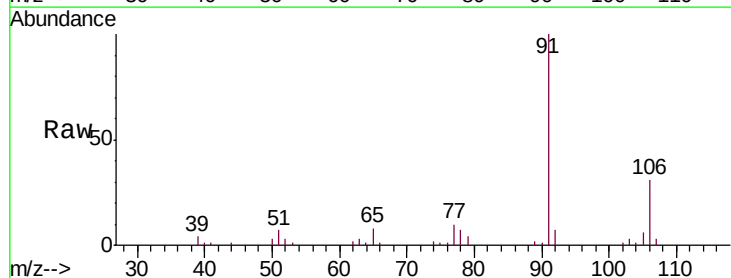

Abundance Ion 91.00 (90.70 to 91.70): VU036602.D (-2475) (-)

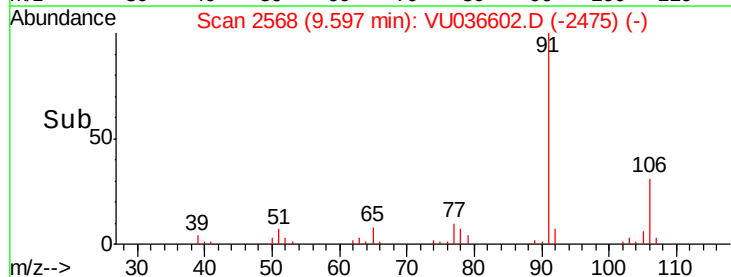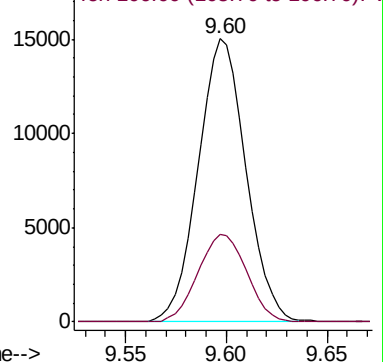


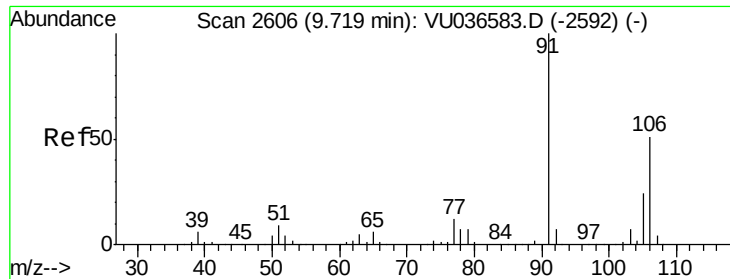




#53
m,p-Xylene
Concen: 27.159 ug/L
RT: 9.72 min Scan# 2606
Delta R.T. 0.00 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57

Instrument :
MSVOA_U
ClientSampled :
GASZ5

Tgt Ion:106 Resp: 110306
Ion Ratio Lower Upper
106 100
91 198.0 139.4 259.0

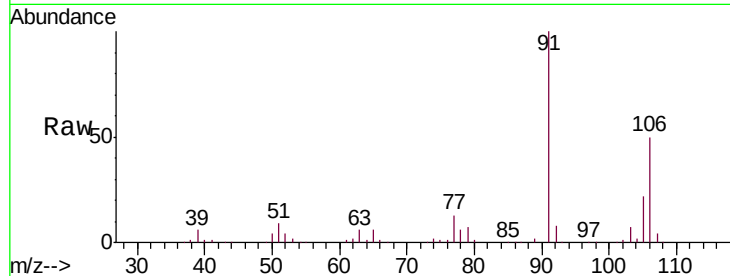


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0

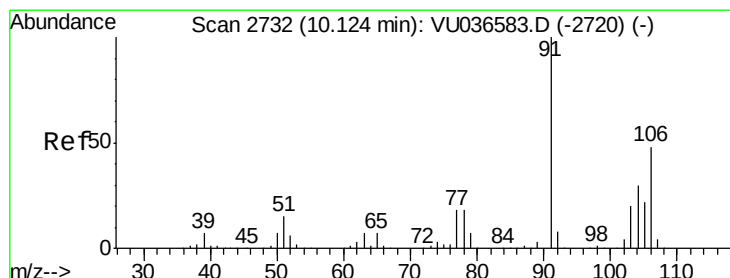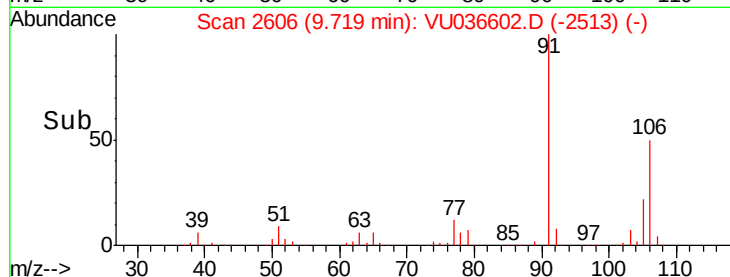
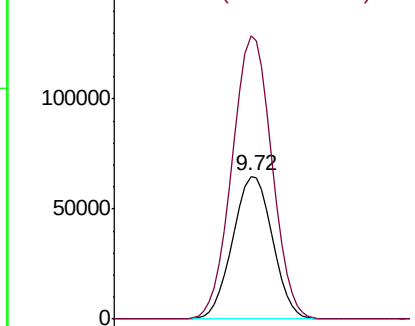



#54
o-xylene
Concen: 26.810 ug/L
RT: 10.13 min Scan# 2733
Delta R.T. 0.00 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57

Tgt Ion:106 Resp: 108615
Ion Ratio Lower Upper
106 100
91 209.8 145.9 271.1

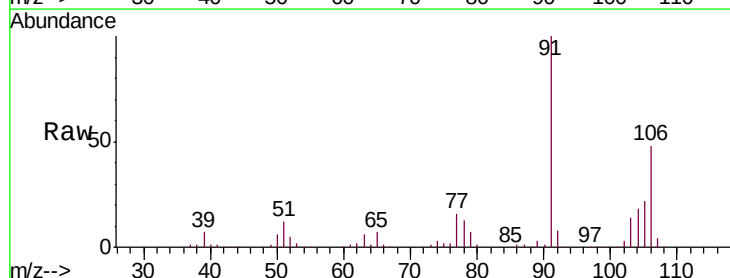

Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0



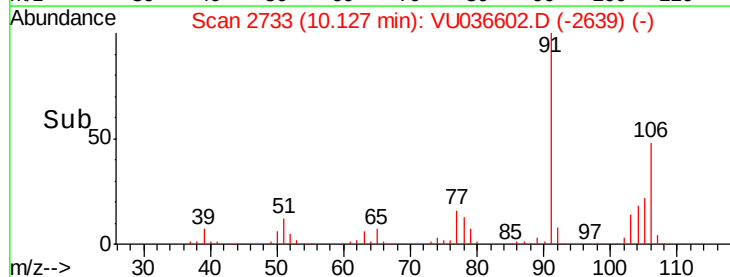
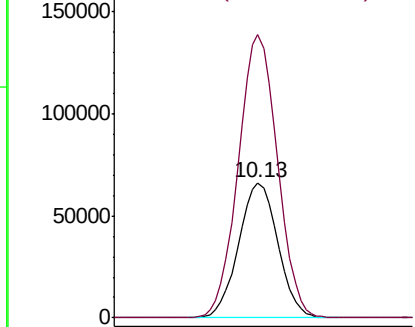


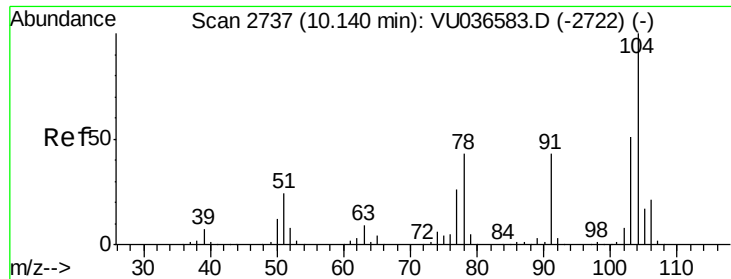

#55
Styrene
Concen: 15.924 ug/L
RT: 10.14 min Scan# 2738
Delta R.T. 0.00 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57




Instrument :
MSVOA_U
ClientSampled :
GASZ5


Tgt Ion:104 Resp: 104691
Ion Ratio Lower Upper
104 100
78 46.9 30.1 55.9

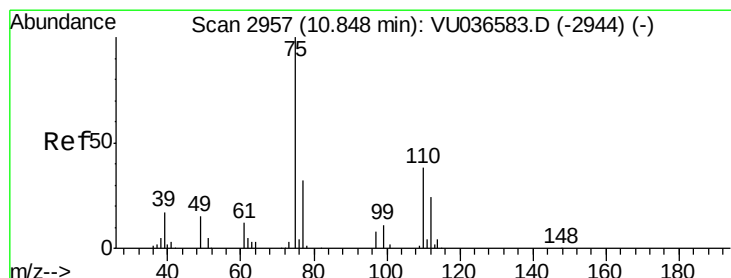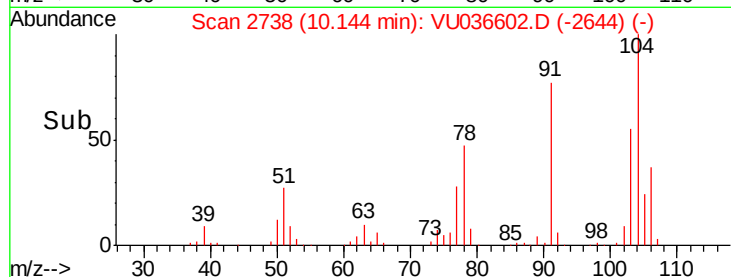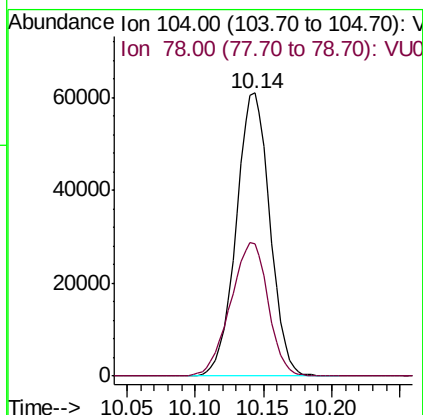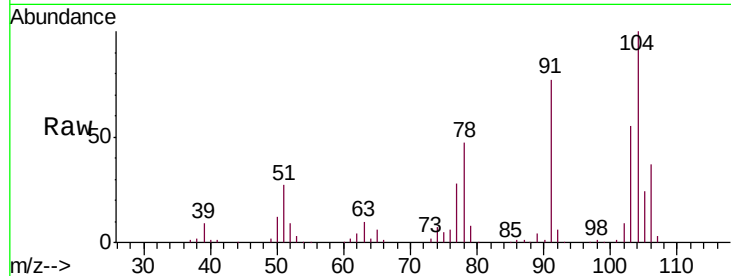

#59
1,2,3-Trichloropropane
Concen: 6.079 ug/L
RT: 11.83 min Scan# 3264
Delta R.T. 0.99 min
Lab File: VU036602.D
Acq: 29 Jan 2020 18:57

Tgt Ion: 75 Resp: 18266
Ion Ratio Lower Upper
75 100
77 39.2 26.2 39.2


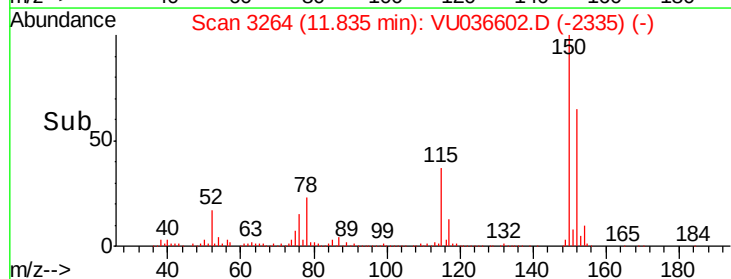
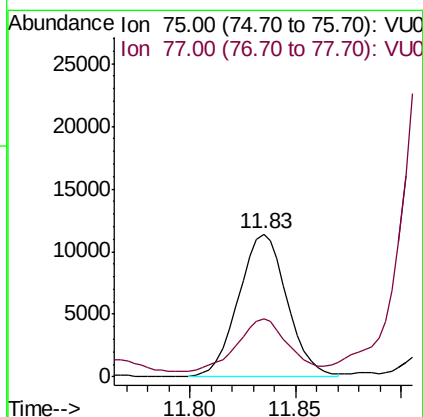
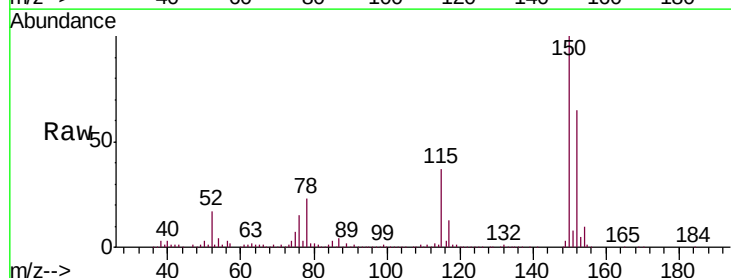


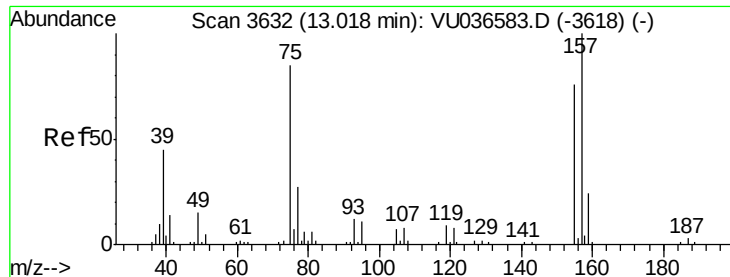

#66
 1,2-Dibromo-3-chloropropane
 Concen: 3.440 ug/L
 RT: 12.99 min Scan# 3624
 Delta R.T. -0.03 min
 Lab File: VU036602.D
 Acq: 29 Jan 2020 18:57




Instrument :
 MSVOA_U
 ClientSampleId :
 GASZ5


Tgt Ion: 75 Resp: 3120
 Ion Ratio Lower Upper
 75 100
 155 19.7 73.4 110.2#
 157 0.0 96.8 145.2#

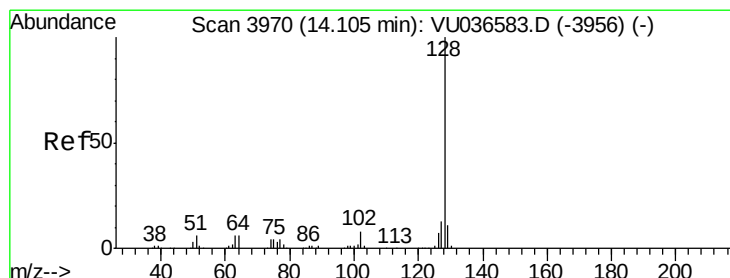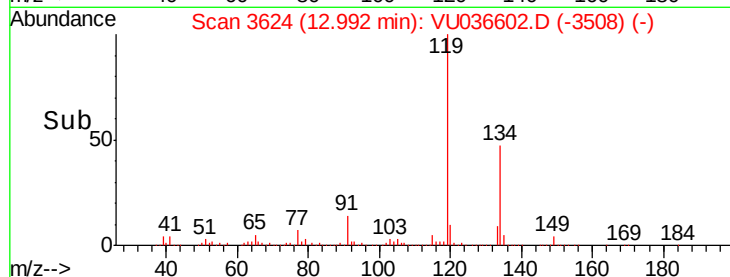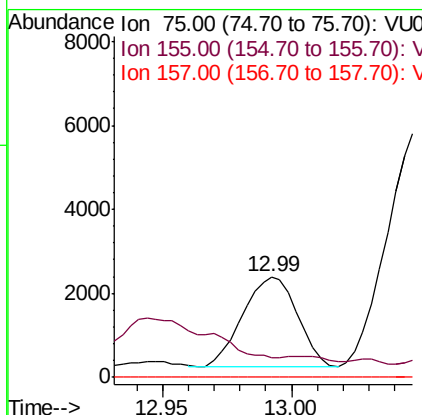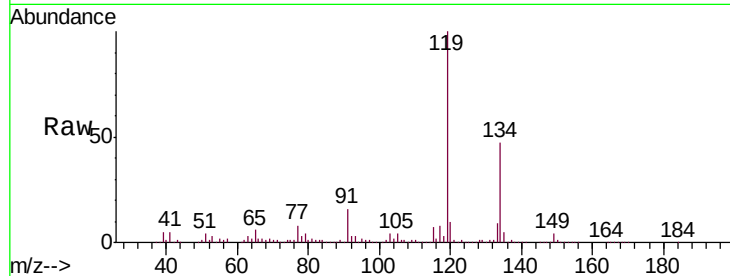

#69
 Naphthalene
 Concen: 561.152 ug/L
 RT: 14.10 min Scan# 3970
 Delta R.T. 0.00 min
 Lab File: VU036602.D
 Acq: 29 Jan 2020 18:57

Tgt Ion: 128 Resp: 4454001
 Ion Ratio Lower Upper
 128 100
 127 13.2 10.6 15.8
 129 11.5 8.6 12.8

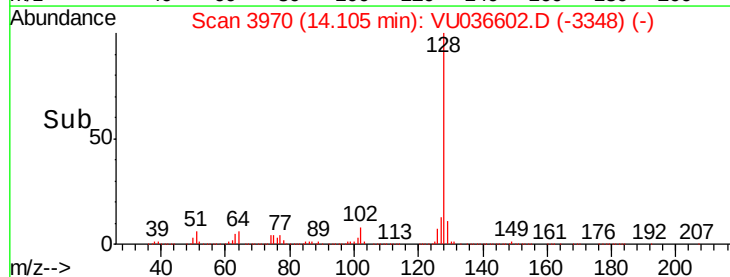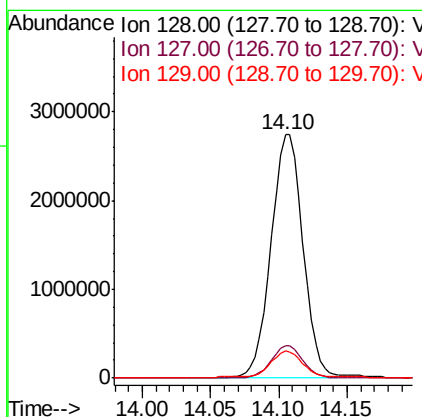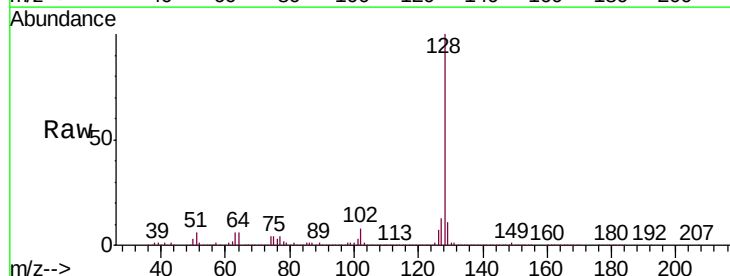


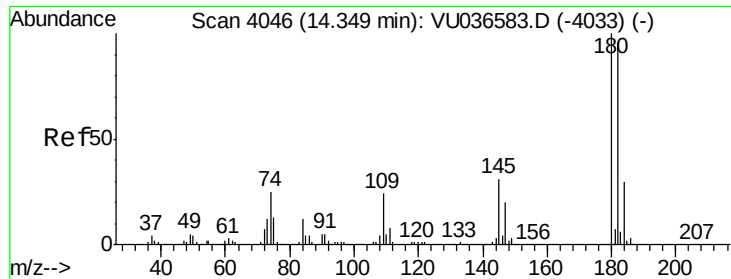

#70
 1,2,3-Trichlorobenzene
 Concen: 1.754 ug/L
 RT: 14.37 min Scan# 4052
 Delta R.T. 0.02 min
 Lab File: VU036602.D
 Acq: 29 Jan 2020 18:57

Instrument :
 MSVOA_U
 ClientSampleId :
 GASZ5

Tgt Ion:180 Resp: 4958
 Ion Ratio Lower Upper
 180 100
 182 12.0 76.1 114.1#
 145 590.2 25.4 38.2#

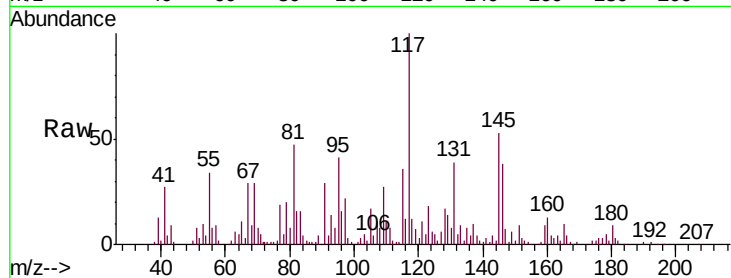

Abundance Ion 180.00 (179.70 to 180.70): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 145.00 (144.70 to 145.70): V

